

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101218\
 Data File : PL040983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2018 18:54
 Operator : AJ\SJ
 Sample : J5199-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 01:10:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.479	4.106	116.9E6	59628671	21.335	21.385
28)	SA Decachlor...	8.231	9.239	104.6E6	50519019	20.122	19.537
Target Compounds							
5)	MB Aldrin	0.000	5.616	0	1417966	N.D.	0.470 #
6)	B beta-BHC	4.420f	4.995f	8929145	9246037	2.814	5.769 #
7)	B delta-BHC	0.000	5.152	0	624825	N.D.	0.190 #
13)	MA Dieldrin	5.754	0.000	3012566	0	0.476	N.D. #
16)	A 4,4'-DDD	0.000	6.918f	0	5505198	N.D.	2.628 #
17)	MA 4,4'-DDT	6.394	0.000	1453565	0	0.319	N.D. #
19)	B Endosulfa...	6.684	0.000	1784370	0	0.351	N.D. #
23)	Chlordane-1	4.420	5.152	8929145	624825	34.987	5.059 #
24)	Chlordane-2	0.000	5.616	0	1417966	N.D.	11.466 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101218\
Data File : PL040983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2018 18:54
Operator : AJ\SJ
Sample : J5199-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 01:10:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

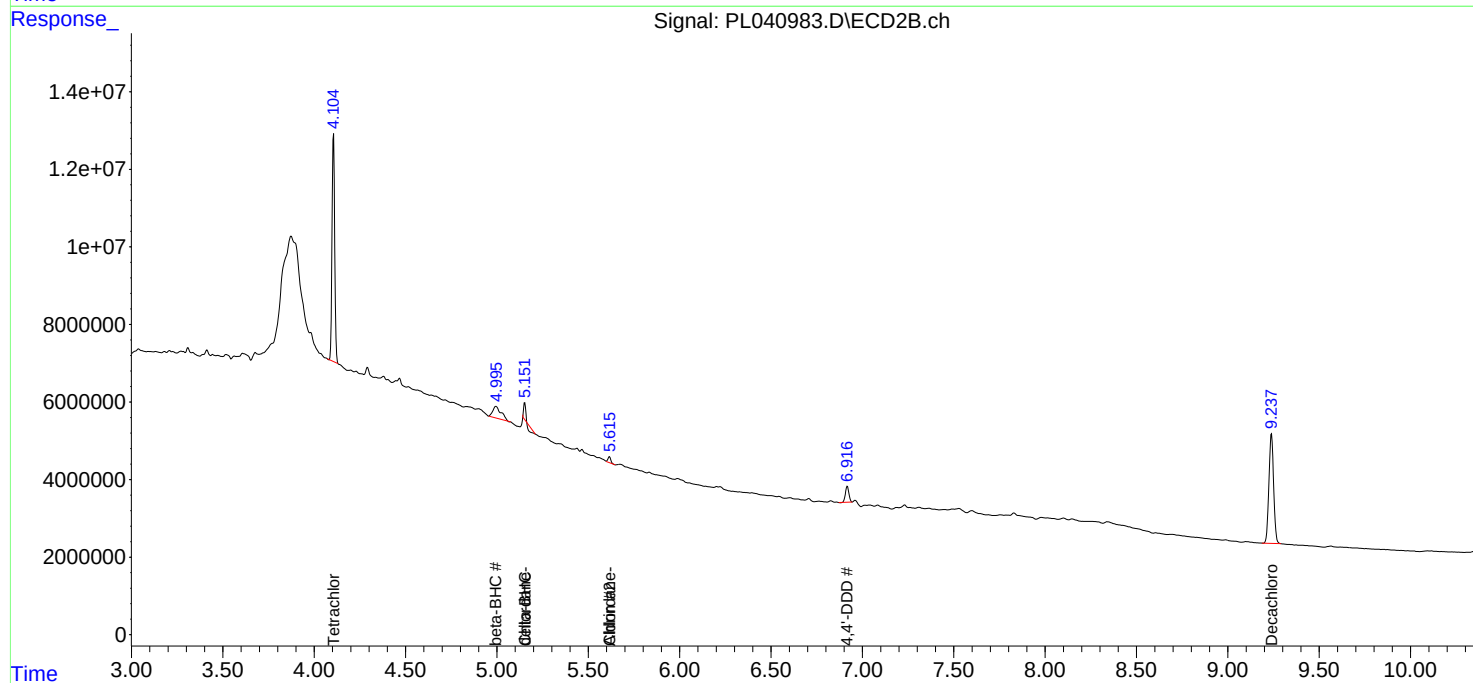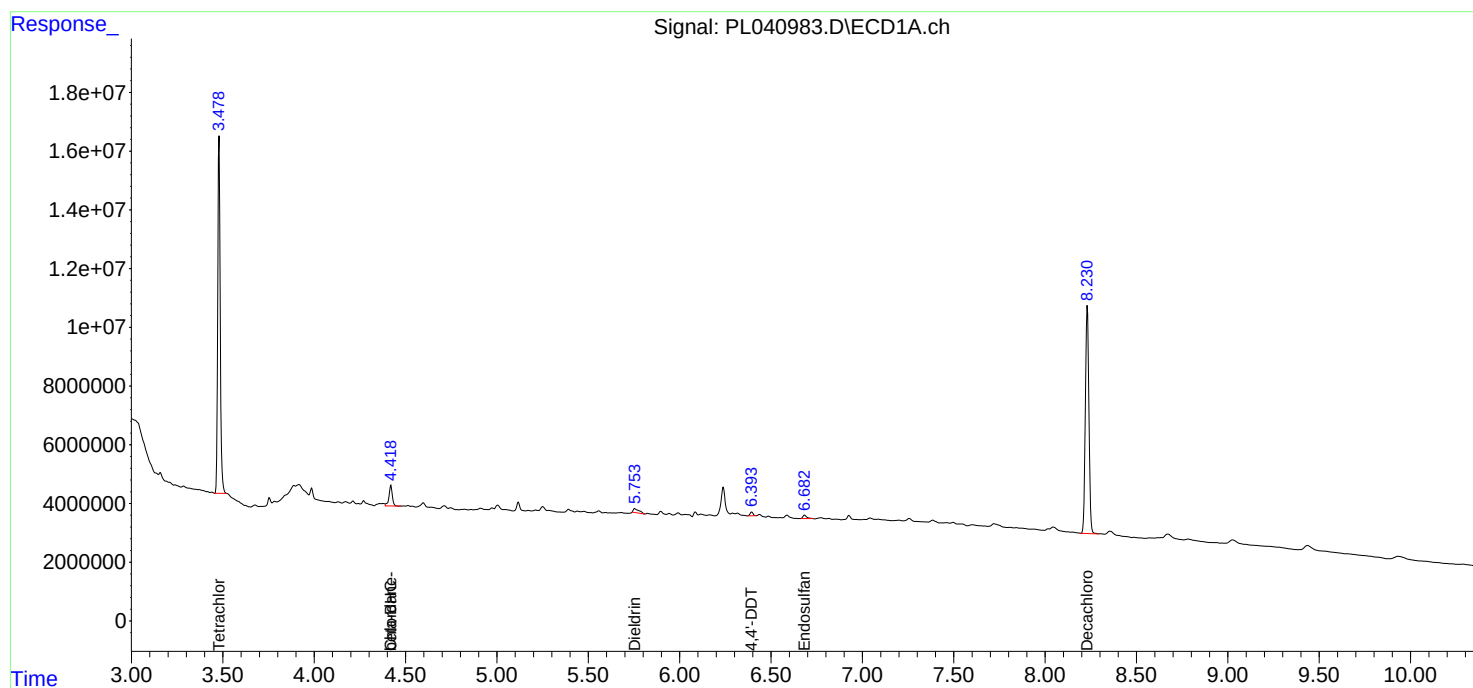


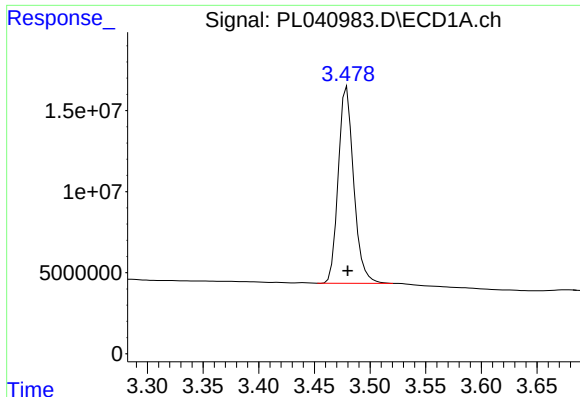

#1 Tetrachloro-m-xylene


R.T.: 3.479 min
Delta R.T.: 0.000 min
Response: 116932552
Conc: 21.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

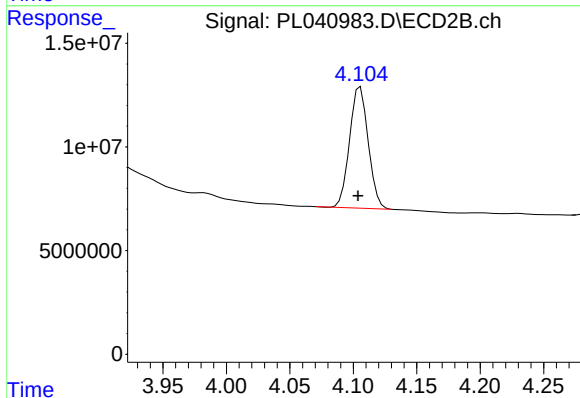


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: 0.002 min
Response: 59628671
Conc: 21.39 ng/ml

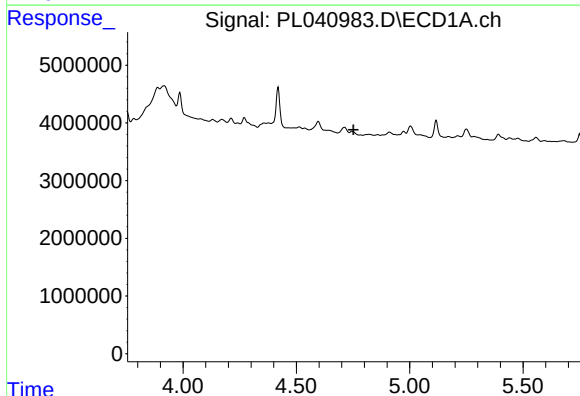


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.752 min
Response: 0
Conc: N.D.

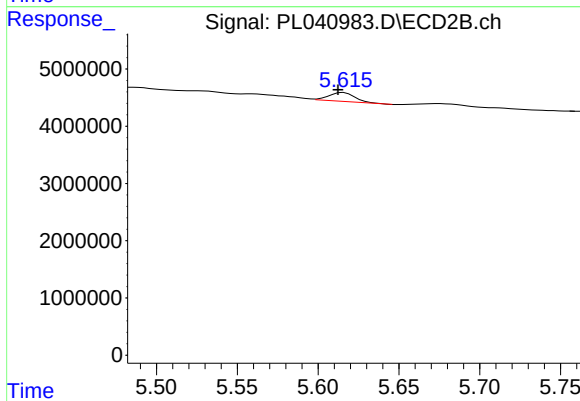

#5 Aldrin


R.T.: 5.616 min
Delta R.T.: 0.003 min
Response: 1417966
Conc: 0.47 ng/ml

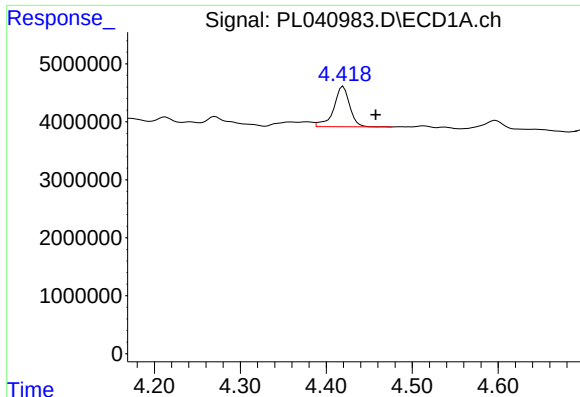

#6 beta-BHC


R.T.: 4.420 min
Delta R.T.: -0.038 min
Response: 8929145
Conc: 2.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

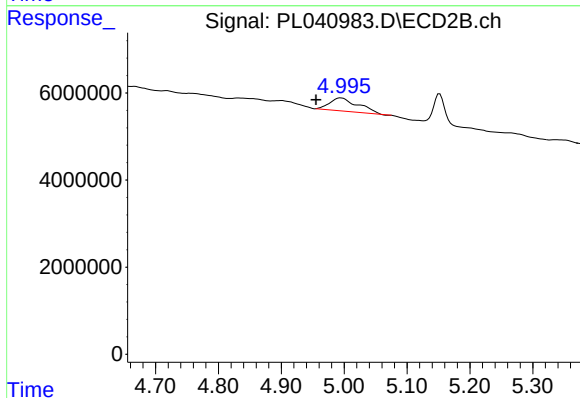


#6 beta-BHC

R.T.: 4.995 min
Delta R.T.: 0.040 min
Response: 9246037
Conc: 5.77 ng/ml

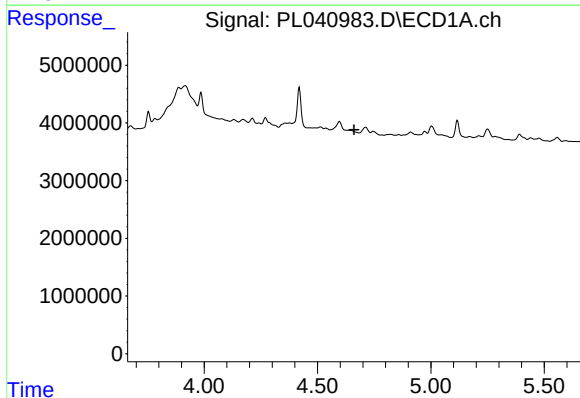


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.662 min
Response: 0
Conc: N.D.

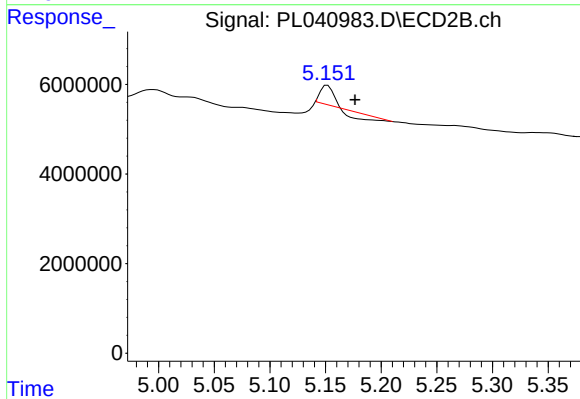

#7 delta-BHC


R.T.: 5.152 min
Delta R.T.: -0.025 min
Response: 624825
Conc: 0.19 ng/ml

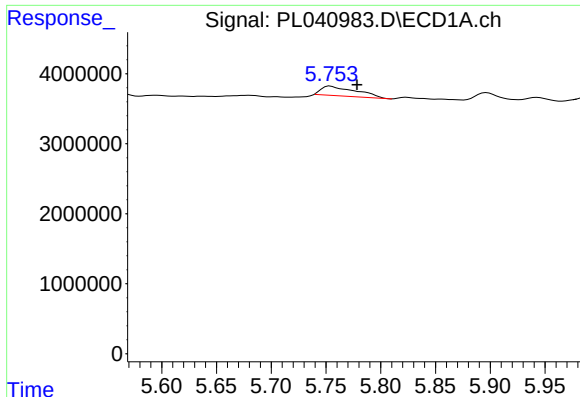

#13 Dieldrin


R.T.: 5.754 min
Delta R.T.: -0.024 min
Response: 3012566
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

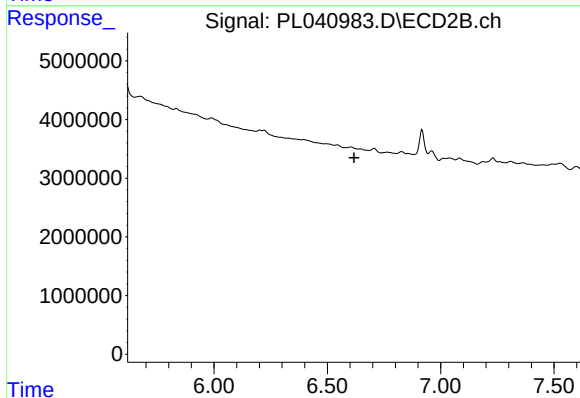


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.618 min
Response: 0
Conc: N.D.

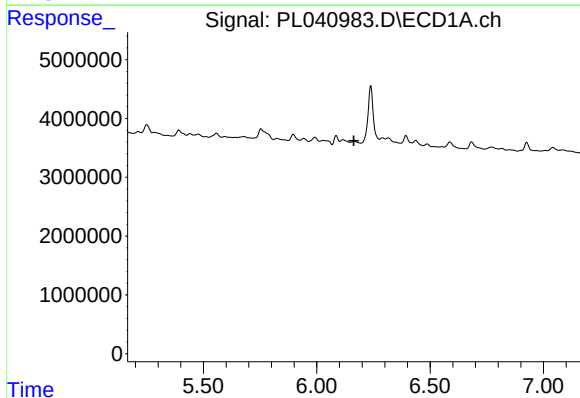


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.163 min
Response: 0
Conc: N.D.

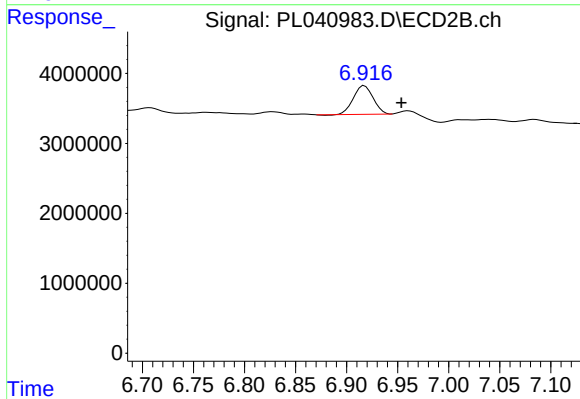

#16 4,4'-DDD


R.T.: 6.918 min
Delta R.T.: -0.036 min
Response: 5505198
Conc: 2.63 ng/ml

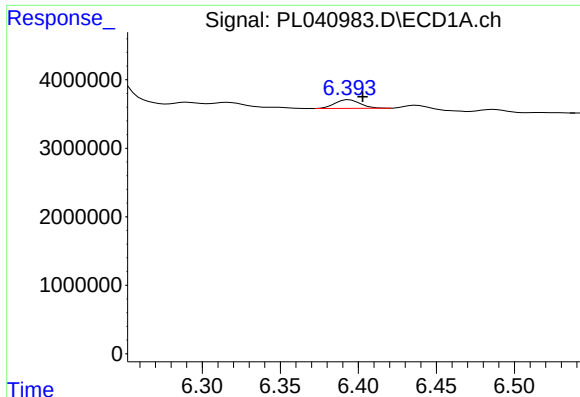

#17 4,4'-DDT


R.T.: 6.394 min
Delta R.T.: -0.009 min
Response: 1453565
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

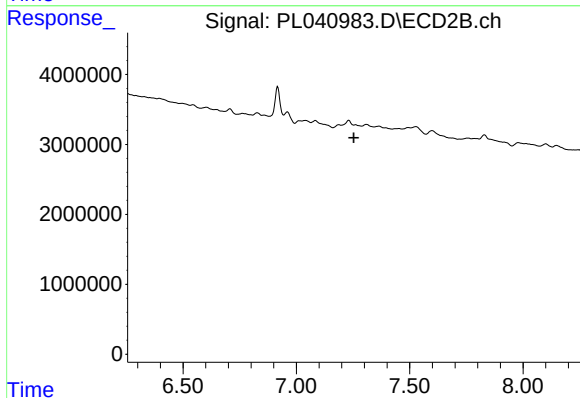


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.254 min
Response: 0
Conc: N.D.

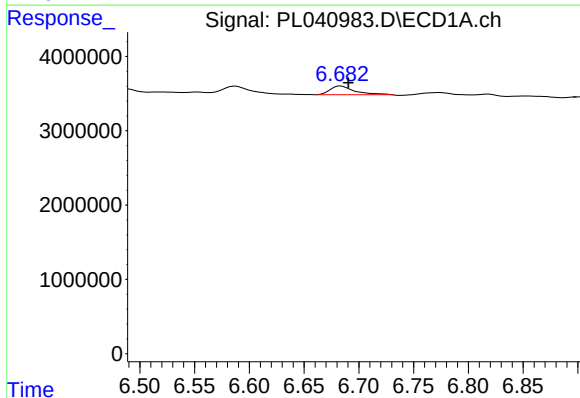


#19 Endosulfan Sulfate

R.T.: 6.684 min
Delta R.T.: -0.007 min
Response: 1784370
Conc: 0.35 ng/ml

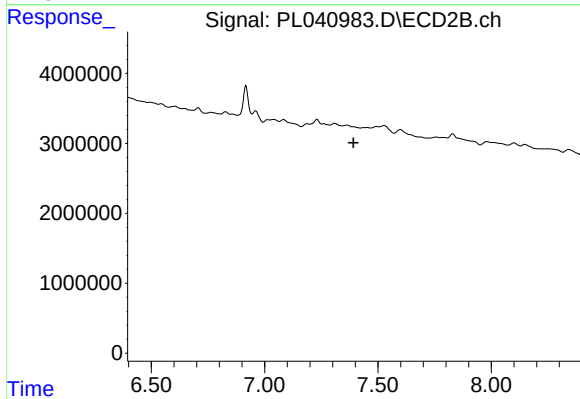

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

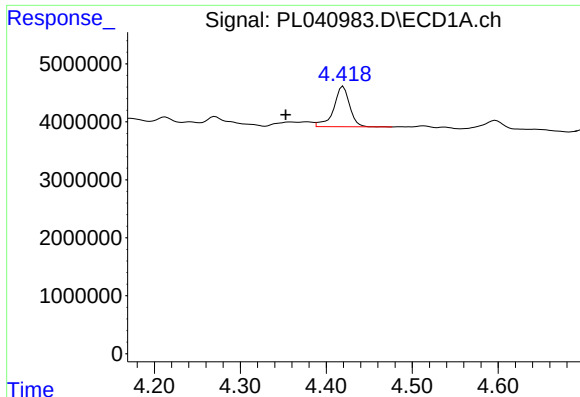

#23 Chlordane-1


R.T.: 4.420 min
Delta R.T.: 0.067 min
Response: 8929145
Conc: 34.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

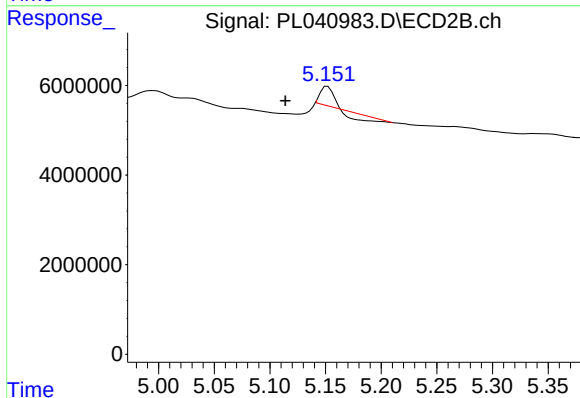


#23 Chlordane-1

R.T.: 5.152 min
Delta R.T.: 0.038 min
Response: 624825
Conc: 5.06 ng/ml

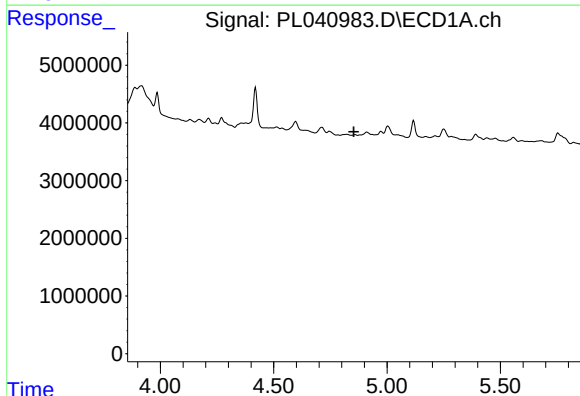


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.854 min
Response: 0
Conc: N.D.

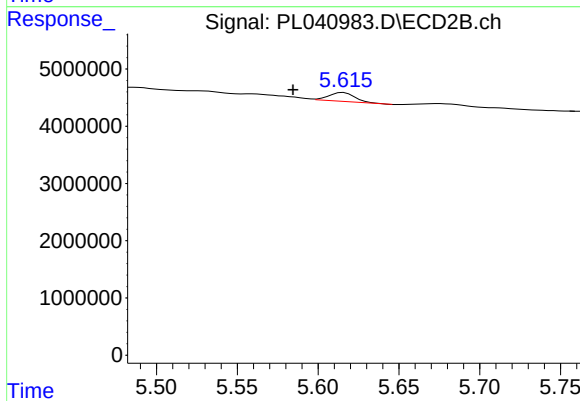

#24 Chlordane-2

R.T.: 5.616 min
Delta R.T.: 0.031 min
Response: 1417966
Conc: 11.47 ng/ml

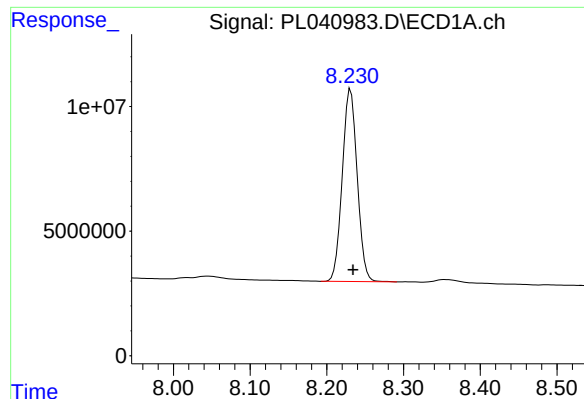

#28 Decachlorobiphenyl


R.T.: 8.231 min

Delta R.T.: -0.003 min

Response: 104627291

Conc: 20.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

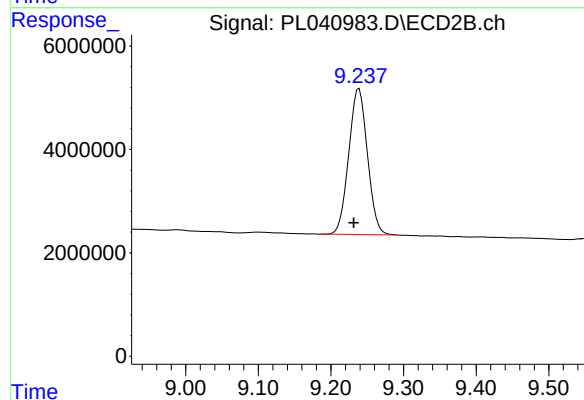

#28 Decachlorobiphenyl

R.T.: 9.239 min

Delta R.T.: 0.007 min

Response: 50519019

Conc: 19.54 ng/ml