

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101219\
 Data File : PL053260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2019 01:15
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 03:11:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
6) B	beta-BHC	0.000	4.903	0	5584750	N.D. 3.553 #
8) B	Heptachlo...	0.000	5.919	0	73927325	N.D. 22.058 #
10) B	gamma-Chl...	0.000	6.166	0	1830084	N.D. 0.541 #
13) MA	Dieldrin	5.864	0.000	39770199	0	3.081 N.D. #
14) MA	Endrin	6.134	6.753	10018834	19679156	0.880 7.087 #
15) B	Endosulfa...	0.000	6.975	0	24097727	N.D. 8.122 #
17) MA	4,4'-DDT	0.000	7.185	0	7990212	N.D. 3.070 #
18) B	Endrin al...	0.000	7.088	0	9373436	N.D. 3.822 #
24)	Chlordane-2	4.962f	0.000	88470252	0	222.686 N.D. #
25)	Chlordane-3	0.000	6.166	0	1830084	N.D. 4.202 #
27)	Chlordane-5	0.000	7.052	0	15099560	N.D. 171.179 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101219\
Data File : PL053260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2019 01:15
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 03:11:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

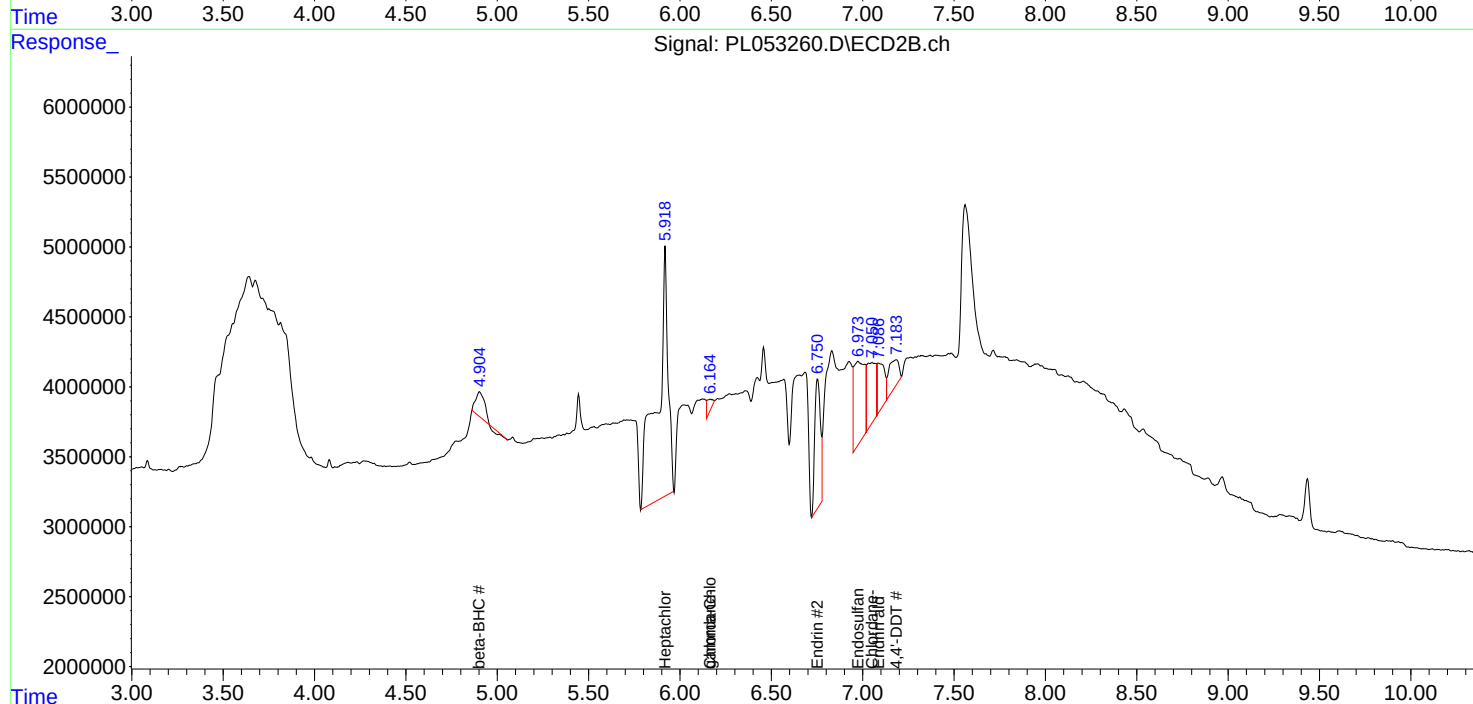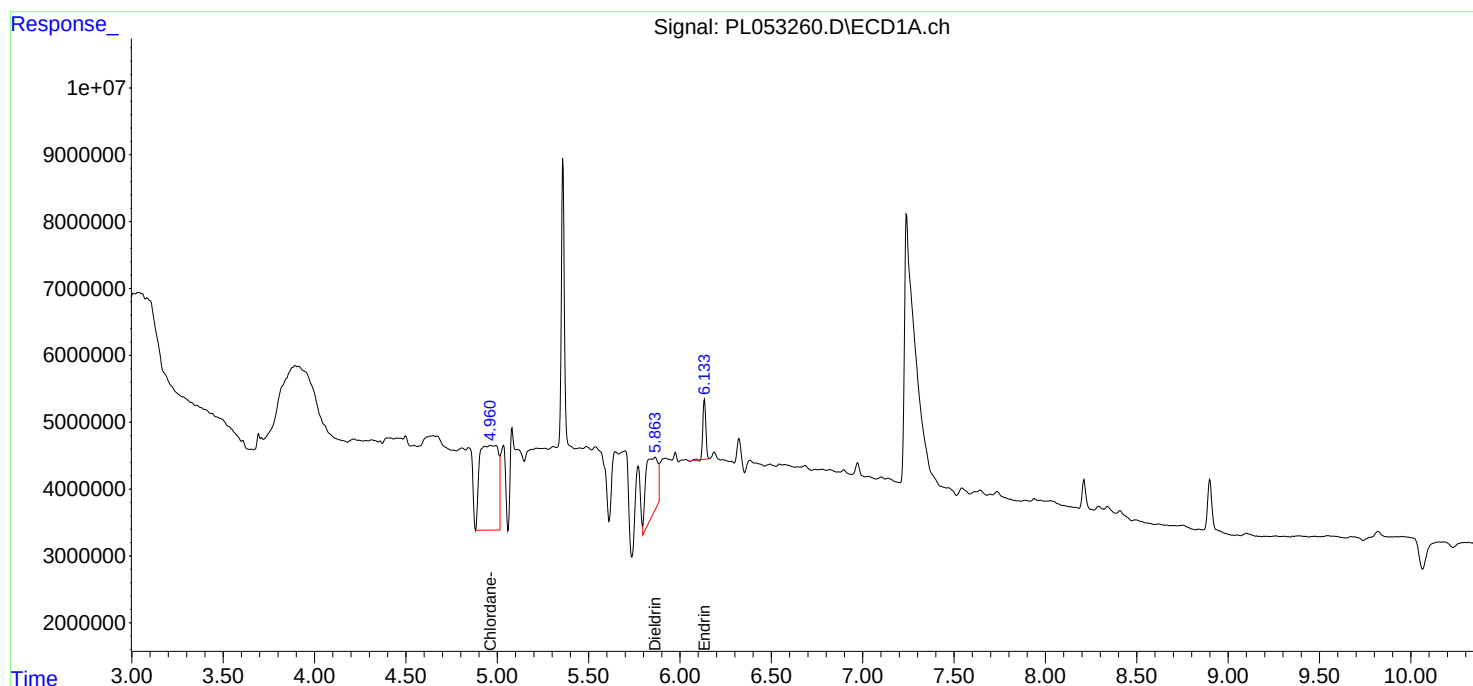


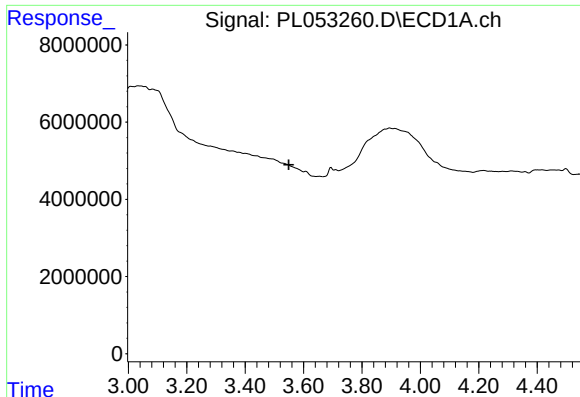

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

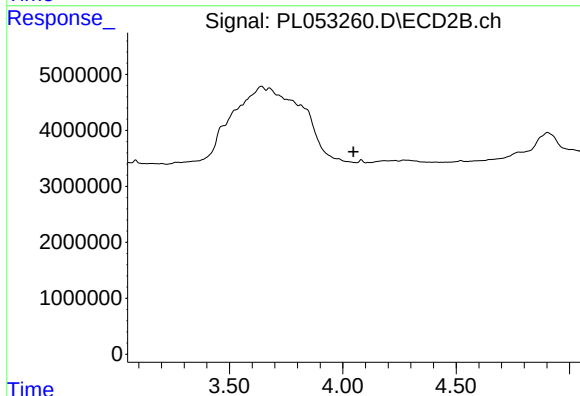


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.047 min
Response: 0
Conc: N.D.

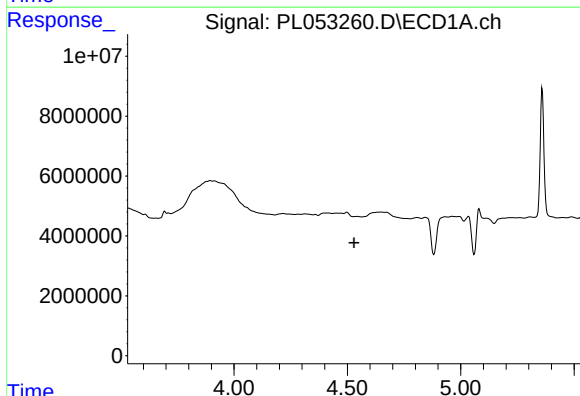


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.530 min
Response: 0
Conc: N.D.

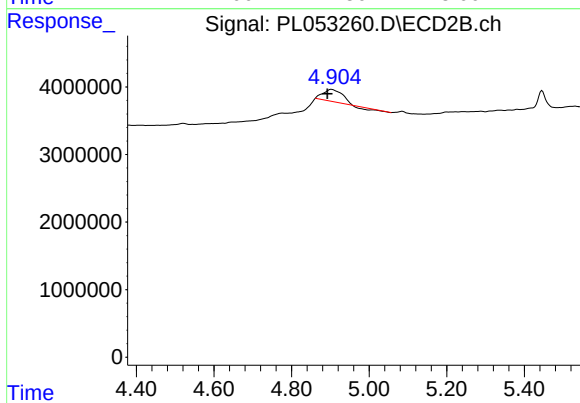

#6 beta-BHC


R.T.: 4.903 min
Delta R.T.: 0.011 min
Response: 5584750
Conc: 3.55 ng/ml

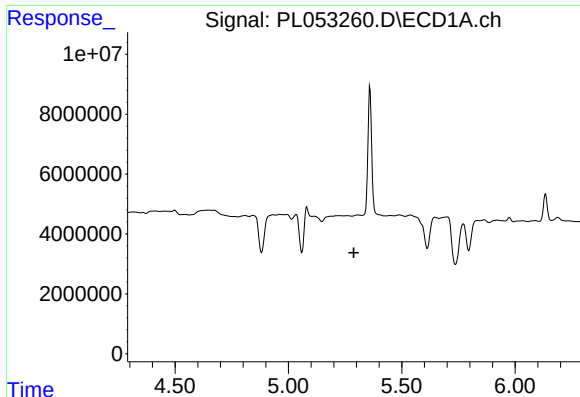

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

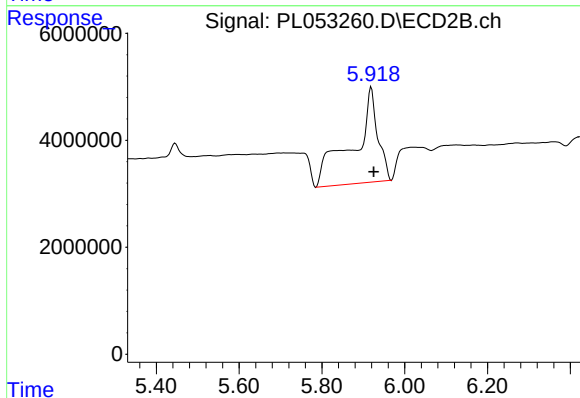


#8 Heptachlor epoxide

R.T.: 5.919 min
Delta R.T.: -0.006 min
Response: 73927325
Conc: 22.06 ng/ml

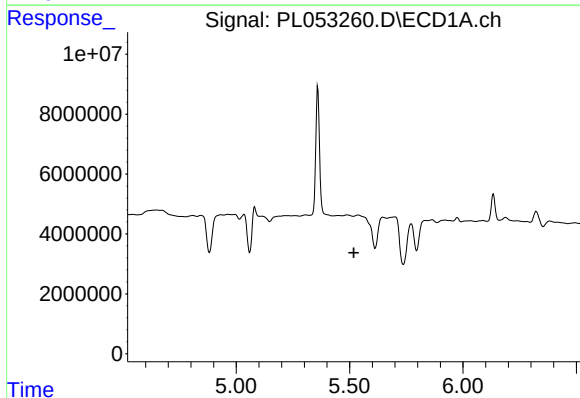


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

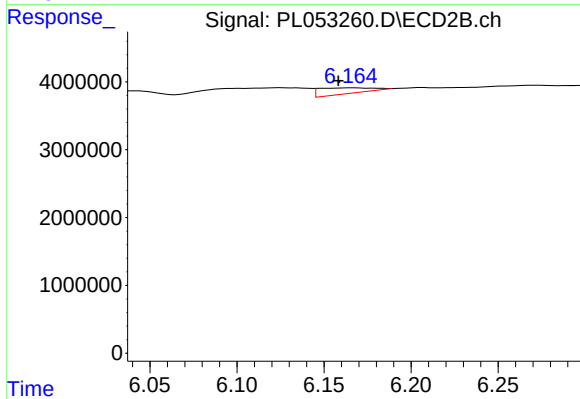

#10 gamma-Chlordane


R.T.: 6.166 min
Delta R.T.: 0.008 min
Response: 1830084
Conc: 0.54 ng/ml

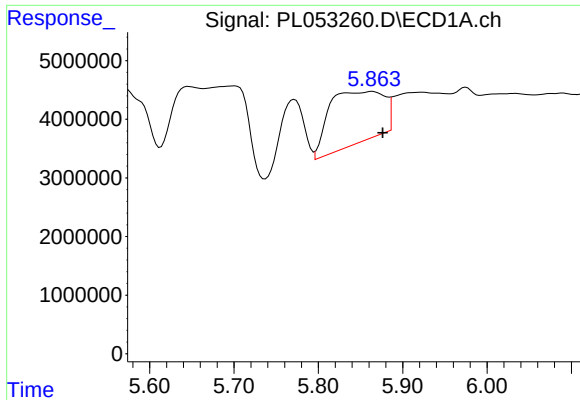

#13 Dieldrin


R.T.: 5.864 min
Delta R.T.: -0.012 min
Response: 39770199
Conc: 3.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

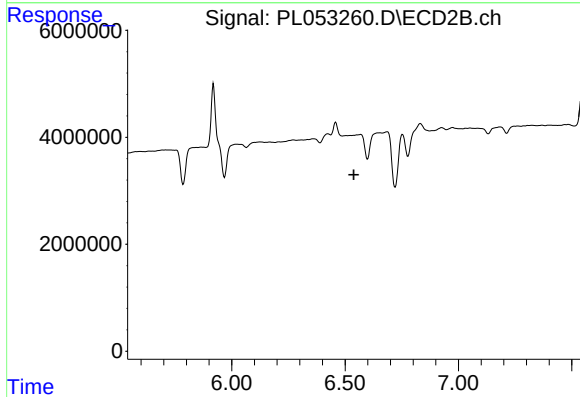


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.538 min
Response: 0
Conc: N.D.

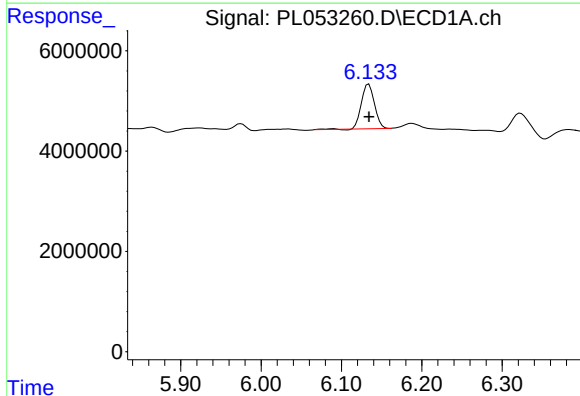


#14 Endrin

R.T.: 6.134 min
Delta R.T.: 0.000 min
Response: 10018834
Conc: 0.88 ng/ml

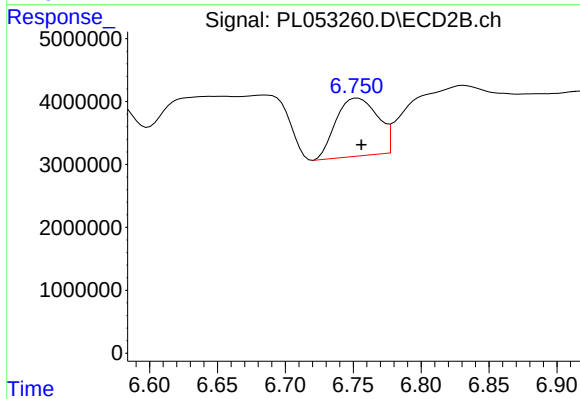

#14 Endrin


R.T.: 6.753 min
Delta R.T.: -0.003 min
Response: 19679156
Conc: 7.09 ng/ml

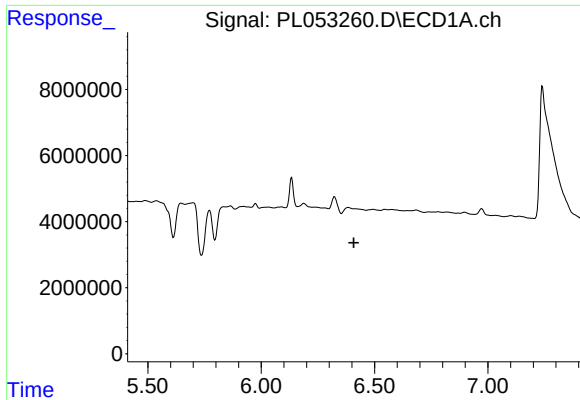

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

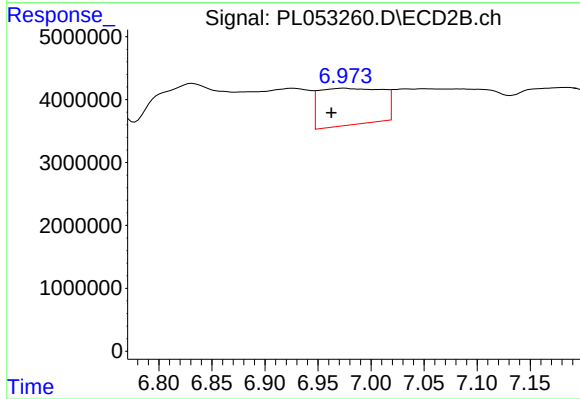


#15 Endosulfan II

R.T.: 6.975 min
Delta R.T.: 0.012 min
Response: 24097727
Conc: 8.12 ng/ml

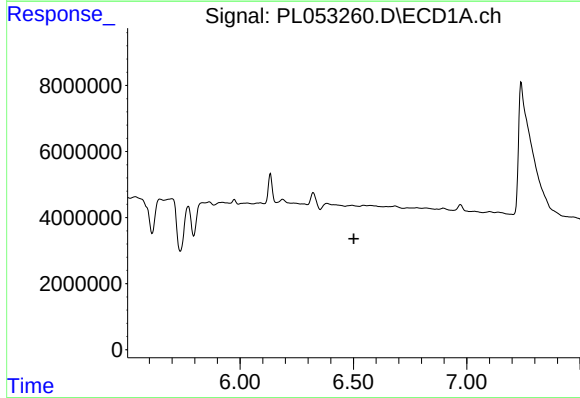


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.502 min
Response: 0
Conc: N.D.

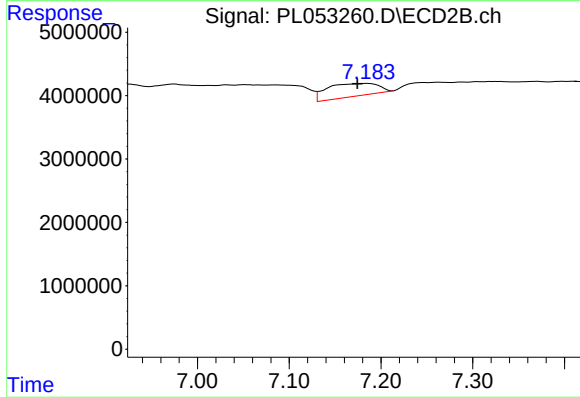

#17 4,4'-DDT


R.T.: 7.185 min
Delta R.T.: 0.011 min
Response: 7990212
Conc: 3.07 ng/ml

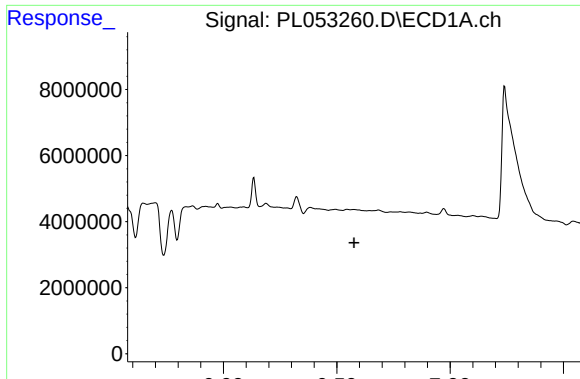

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

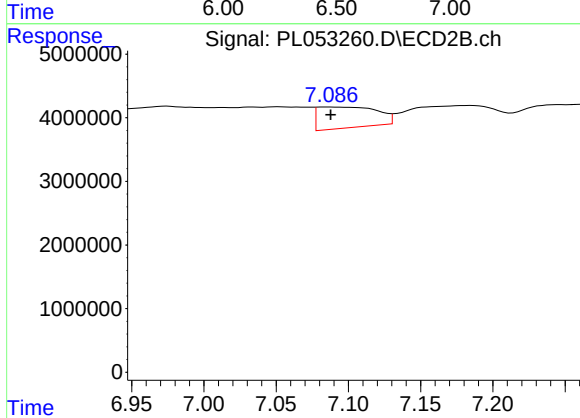


#18 Endrin aldehyde

R.T.: 7.088 min
Delta R.T.: 0.000 min
Response: 9373436
Conc: 3.82 ng/ml

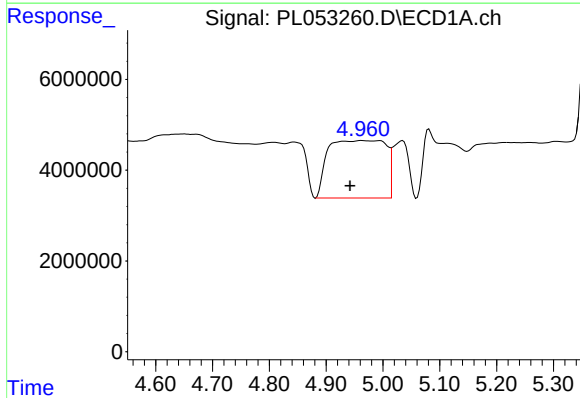


#24 Chlordane-2

R.T.: 4.962 min
Delta R.T.: 0.020 min
Response: 88470252
Conc: 222.69 ng/ml

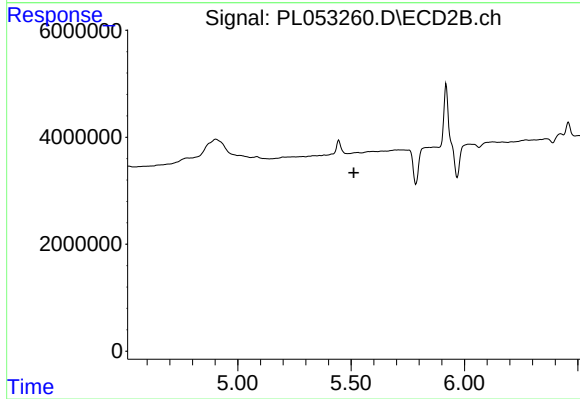

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.512 min
Response: 0
Conc: N.D.

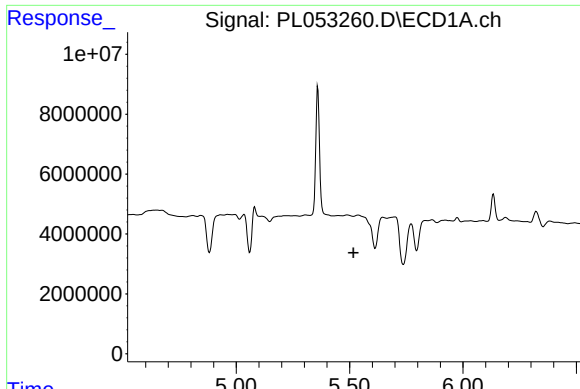

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

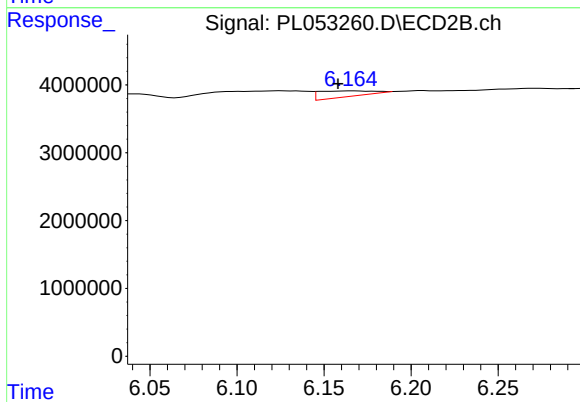


#25 Chlordane-3

R.T.: 6.166 min
Delta R.T.: 0.008 min
Response: 1830084
Conc: 4.20 ng/ml

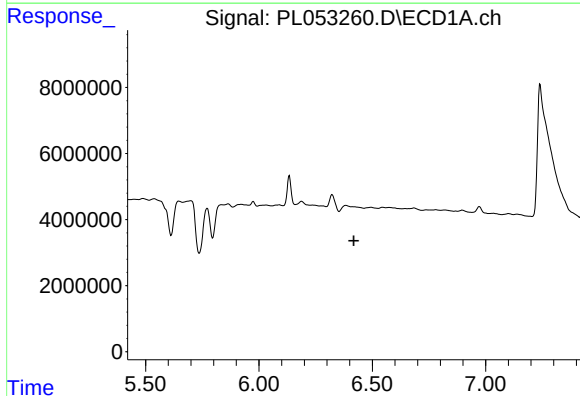


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.418 min
Response: 0
Conc: N.D.

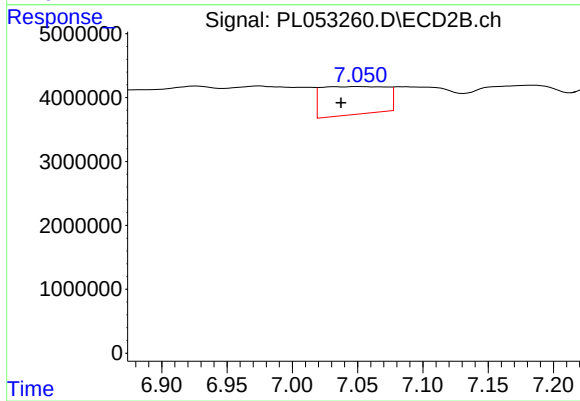

#27 Chlordane-5


R.T.: 7.052 min
Delta R.T.: 0.014 min
Response: 15099560
Conc: 171.18 ng/ml

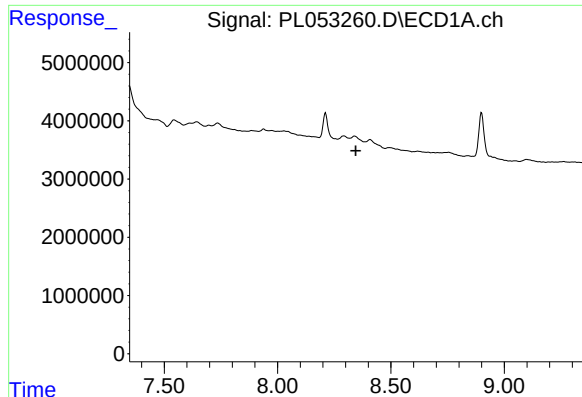

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

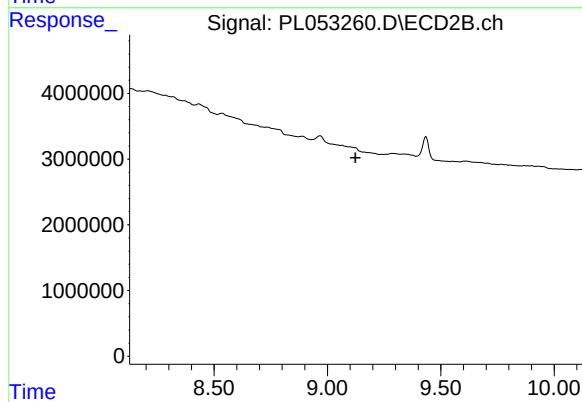

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.124 min
Response: 0
Conc: N.D.