

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101219\
 Data File : PL053285.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2019 07:03
 Operator : SG\AJ
 Sample : K5266-13
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AMENDED-COMPOSITE-A

Manual Integrations
 APPROVED

Ankita
 10/14/2019 3:00:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 00:40:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	4.046	198.5E6	44407621	19.959	16.538
28)	SA Decachlor...	8.335	9.125	176.1E6	54080547	17.577	18.434
Target Compounds							
10)	B gamma-Chl...	5.525	6.165	20085873	17928282	1.494m	5.299 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101219\
Data File : PL053285.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2019 07:03
Operator : SG\AJ
Sample : K5266-13
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
AMENDED-COMPOSITE-A


Manual Integrations
APPROVED

Ankita
10/14/2019 3:00:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 00:40:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

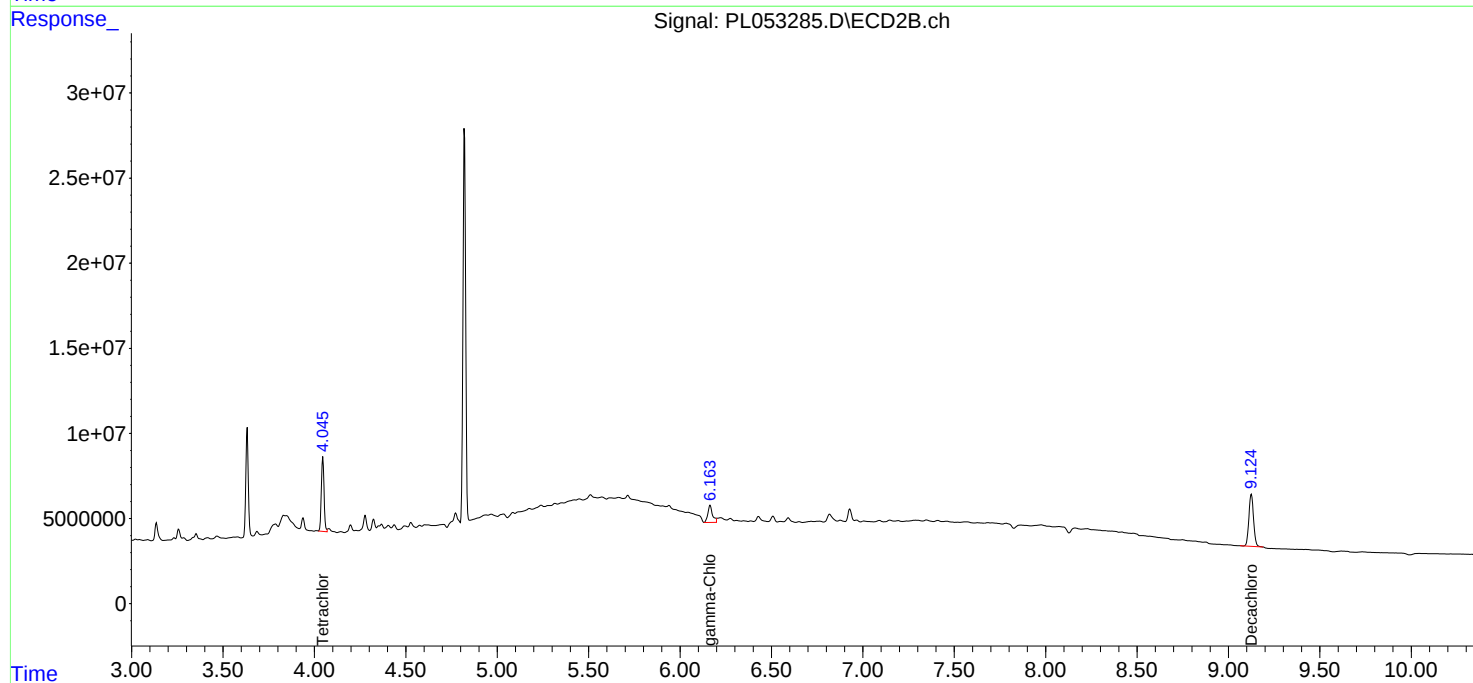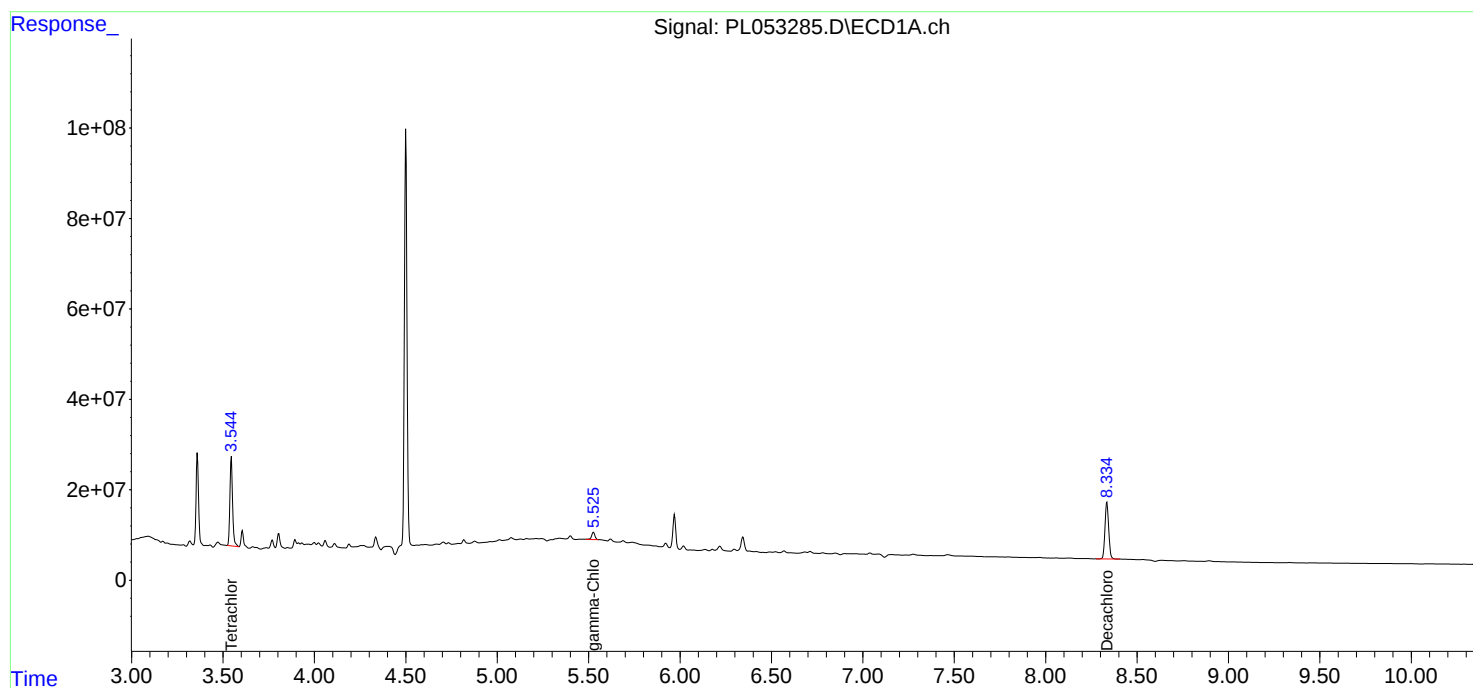

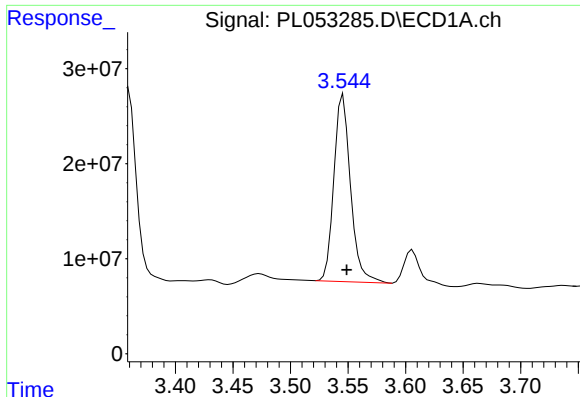


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.003 min
Response: 198527397
Conc: 19.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
AMENDED-COMPOSITE-A


Manual Integrations
APPROVED

Ankita
10/14/2019 3:00:13 PM

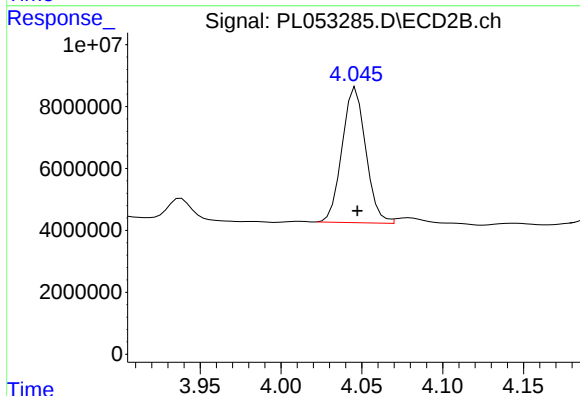


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 44407621
Conc: 16.54 ng/ml

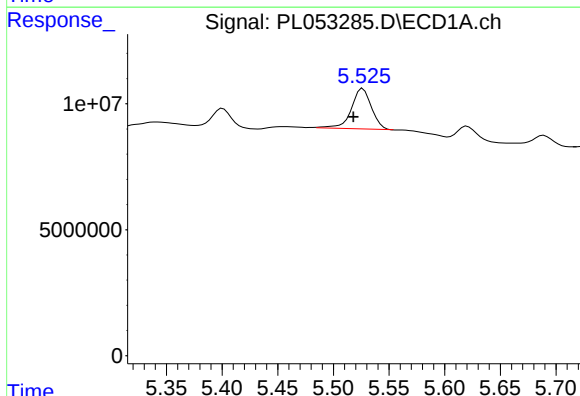


#10 gamma-Chlordane

R.T.: 5.525 min
Delta R.T.: 0.007 min
Response: 20085873
Conc: 1.49 ng/ml m

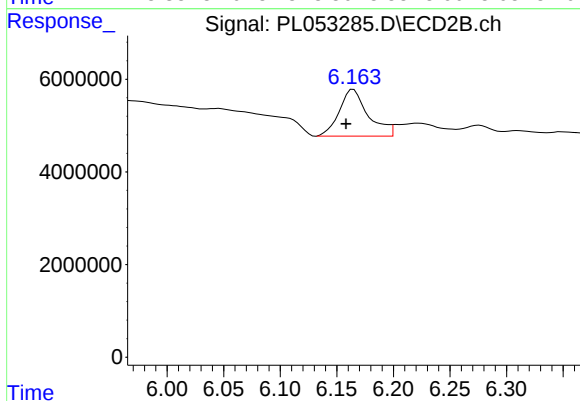

#10 gamma-Chlordane

R.T.: 6.165 min
Delta R.T.: 0.006 min
Response: 17928282
Conc: 5.30 ng/ml

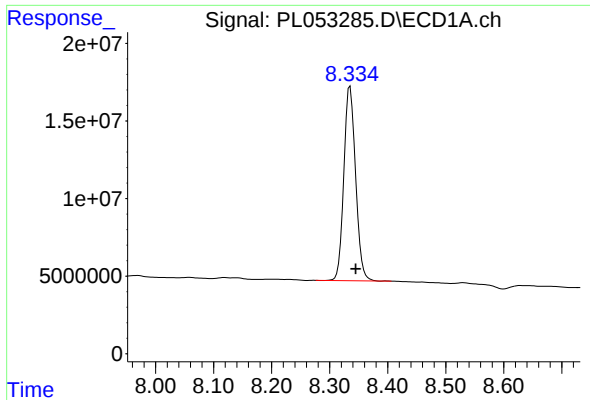


#28 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: -0.010 min
Response: 176052923
Conc: 17.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
AMENDED-COMPOSITE-A

Manual Integrations
APPROVED

Ankita
10/14/2019 3:00:13 PM

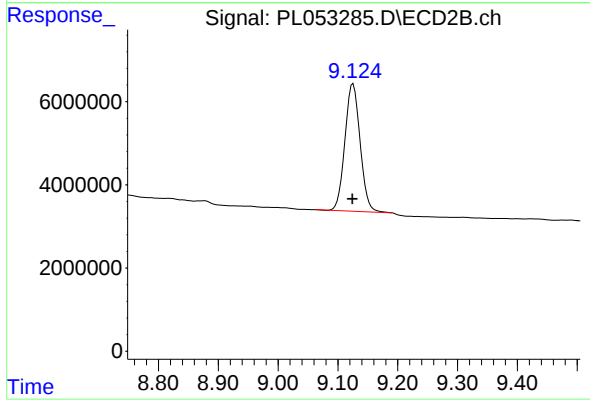

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.001 min
Response: 54080547
Conc: 18.43 ng/ml