

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101219\
 Data File : PL053286.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2019 07:17
 Operator : SG\AJ
 Sample : K5266-14
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AMENDED-COMPOSITE-C

Manual Integrations
 APPROVED

Ankita
 10/14/2019 3:00:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 00:40:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	4.046	176.0E6	44629694	17.690	16.621
28)	SA Decachlor...	8.335	9.125	176.6E6	53282042	17.634	18.162
Target Compounds							
10)	B gamma-Chl...	5.525	6.165	11327310	6071761	0.842m	1.795 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101219\
Data File : PL053286.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2019 07:17
Operator : SG\AJ
Sample : K5266-14
Misc :
ALS Vial : 45 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
AMENDED-COMPOSITE-C


Manual Integrations
APPROVED

Ankita
10/14/2019 3:00:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 00:40:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

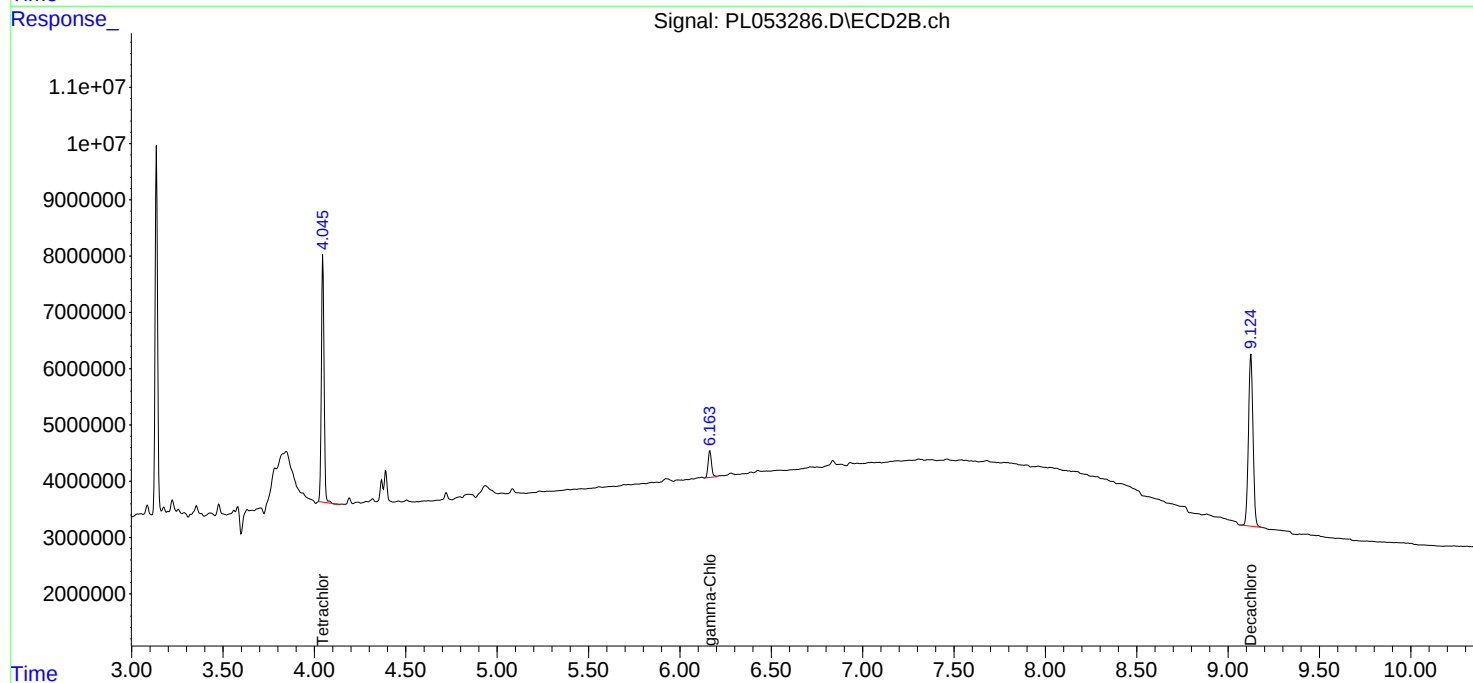

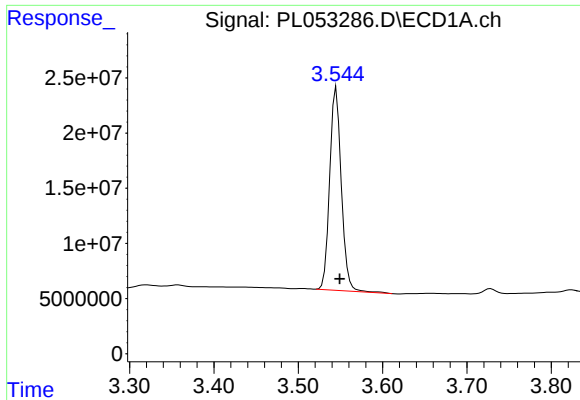


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: -0.004 min
Response: 175954131
Conc: 17.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
AMENDED-COMPOSITE-C


Manual Integrations
APPROVED

Ankita
10/14/2019 3:00:16 PM

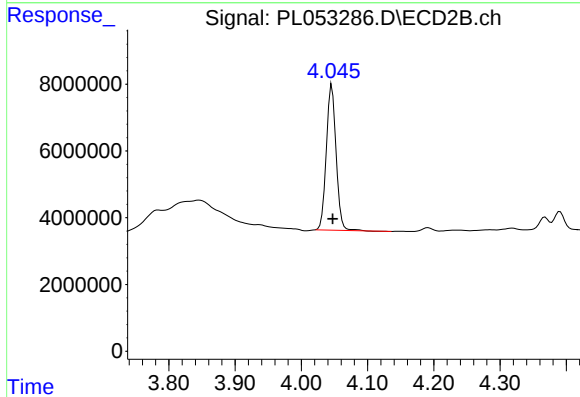


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: -0.001 min
Response: 44629694
Conc: 16.62 ng/ml

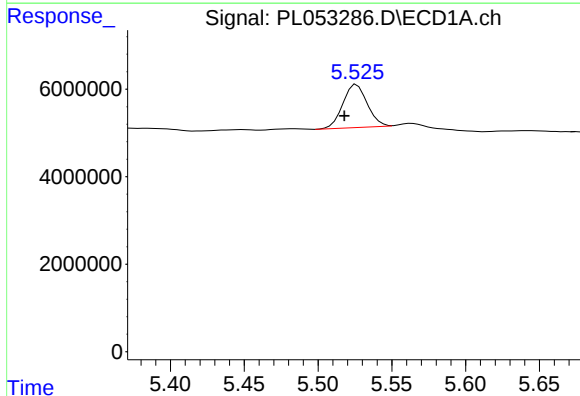


#10 gamma-Chlordane

R.T.: 5.525 min
Delta R.T.: 0.007 min
Response: 11327310
Conc: 0.84 ng/ml m

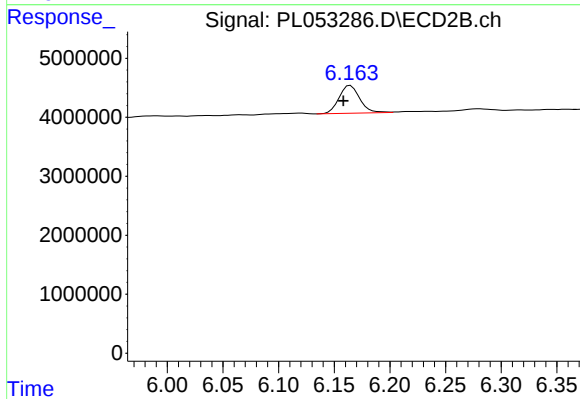

#10 gamma-Chlordane

R.T.: 6.165 min
Delta R.T.: 0.006 min
Response: 6071761
Conc: 1.79 ng/ml

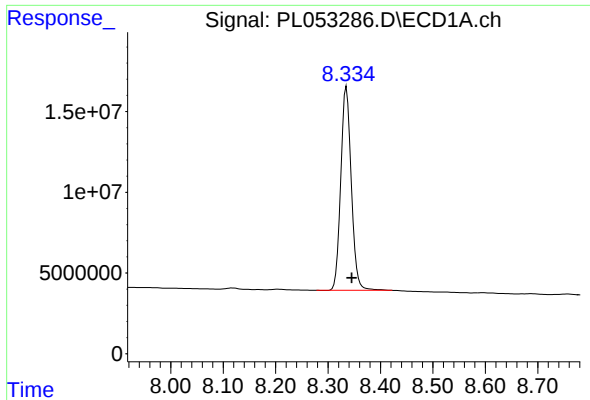

#28 Decachlorobiphenyl

R.T.: 8.335 min

Delta R.T.: -0.010 min


Response: 176622431

Conc: 17.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
AMENDED-COMPOSITE-C

Manual Integrations
APPROVED

Ankita
10/14/2019 3:00:16 PM

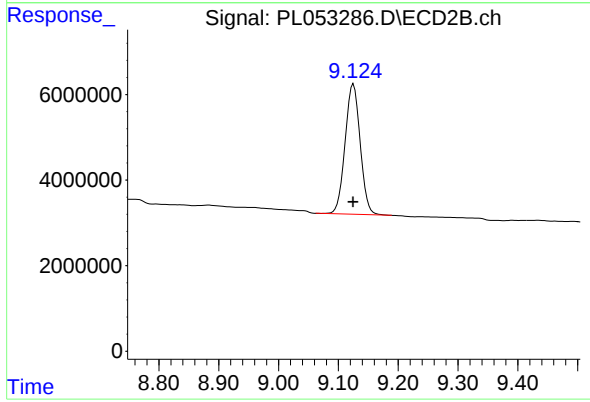

#28 Decachlorobiphenyl

R.T.: 9.125 min

Delta R.T.: 0.000 min

Response: 53282042

Conc: 18.16 ng/ml