

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101219\
 Data File : PL053287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2019 07:31
 Operator : SG\AJ
 Sample : K5292-06
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20190855-AMENDED-COMP-B

Manual Integrations
 APPROVED

Ankita
 10/14/2019 3:00:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 00:40:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.546	4.046	195.5E6	43526995	19.654	16.210
28) SA Decachlor...	8.336	9.125	180.5E6	55762699	18.021	19.007
Target Compounds						
10) B gamma-Chl...	5.525	6.163	14985508	12028934	1.114m	3.556m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101219\
Data File : PL053287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2019 07:31
Operator : SG\AJ
Sample : K5292-06
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20190855-AMENDED-COMP-B


Manual Integrations
APPROVED

Ankita
10/14/2019 3:00:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 00:40:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

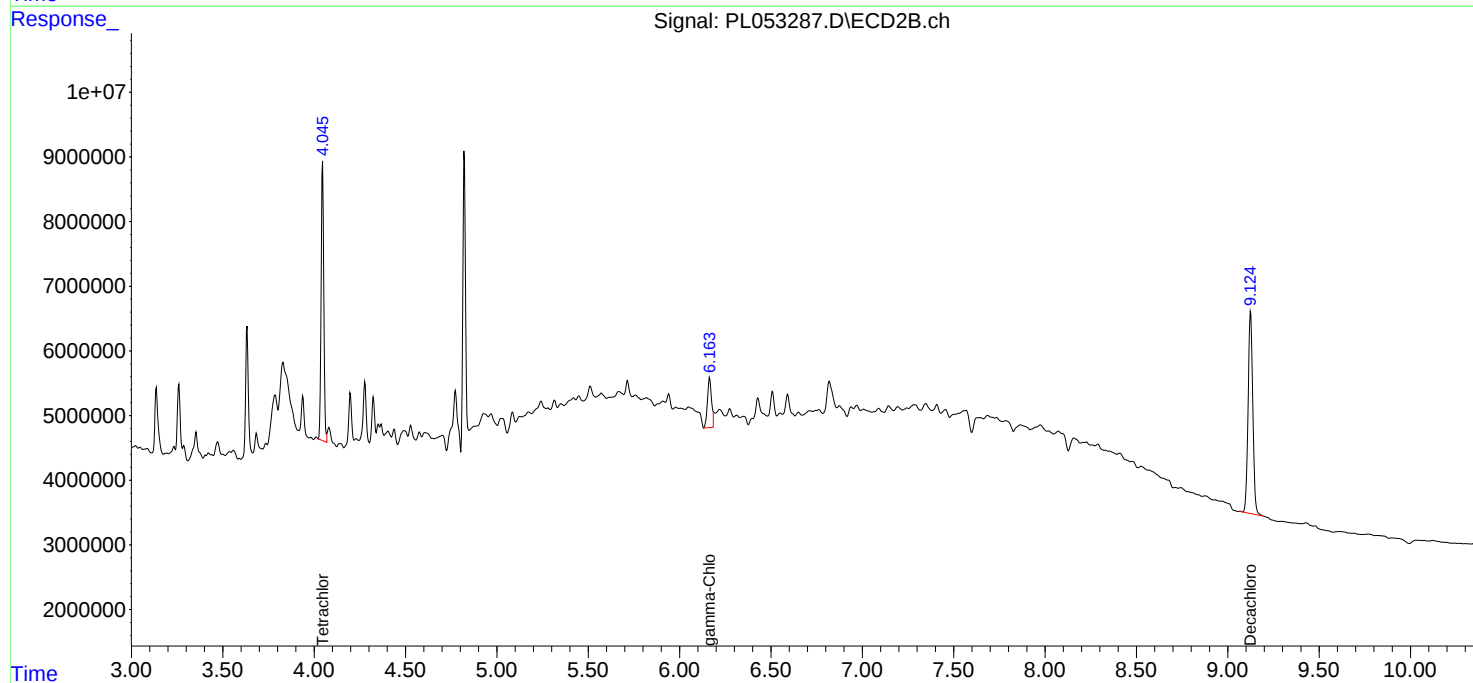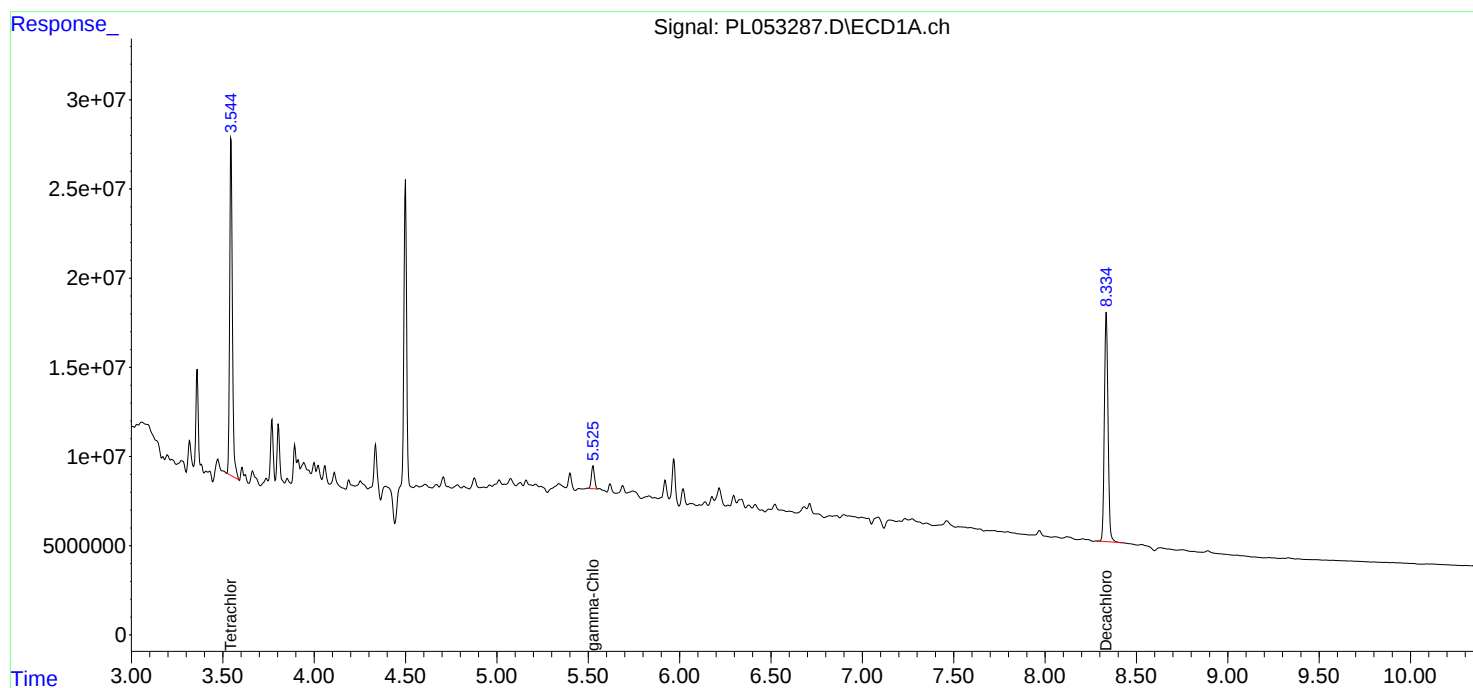

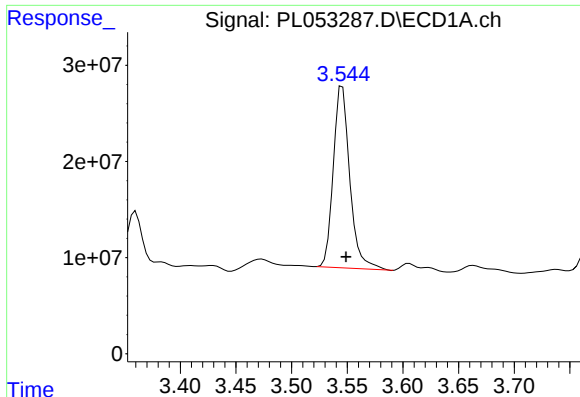


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.003 min
Response: 195488883
Conc: 19.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190855-AMENDED-COMP-B


Manual Integrations
APPROVED

Ankita
10/14/2019 3:00:17 PM

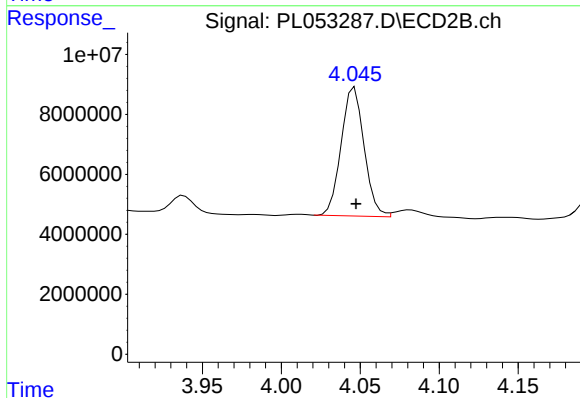


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 43526995
Conc: 16.21 ng/ml

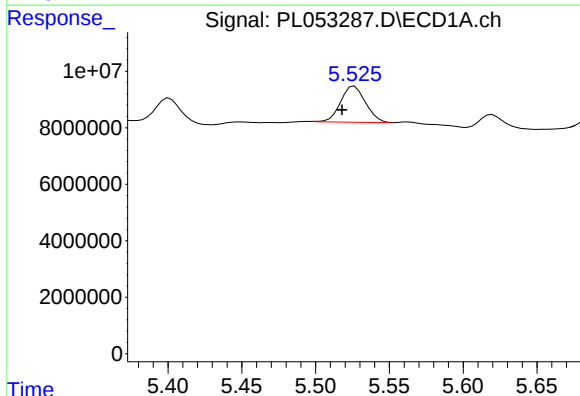


#10 gamma-Chlordane

R.T.: 5.525 min
Delta R.T.: 0.007 min
Response: 14985508
Conc: 1.11 ng/ml m

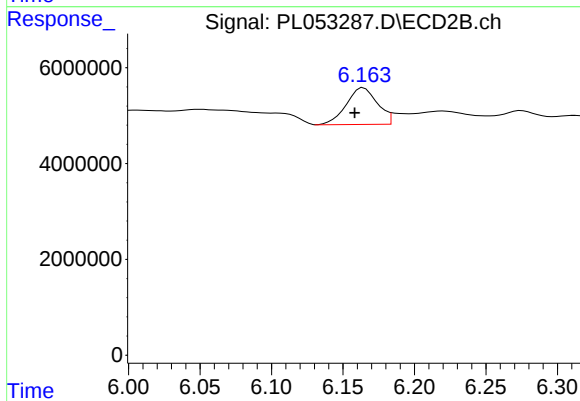

#10 gamma-Chlordane

R.T.: 6.163 min
Delta R.T.: 0.005 min
Response: 12028934
Conc: 3.56 ng/ml m

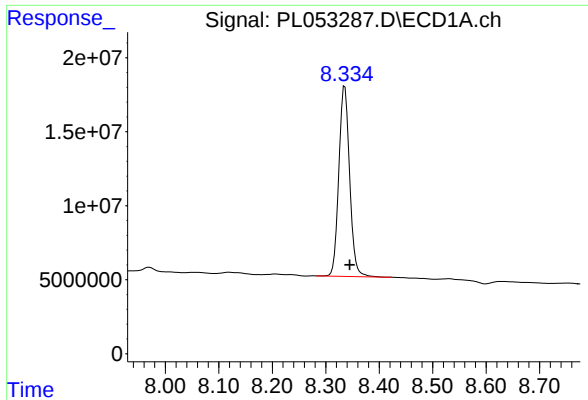


#28 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.010 min
Response: 180497248
Conc: 18.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190855-AMENDED-COMP-B

Manual Integrations
APPROVED

Ankita
10/14/2019 3:00:17 PM

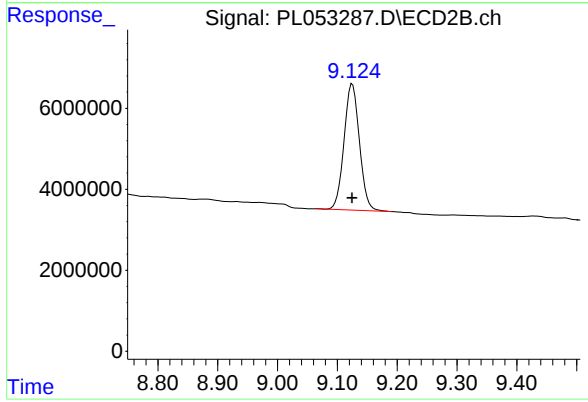

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.000 min
Response: 55762699
Conc: 19.01 ng/ml