

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101220\
 Data File : PL062211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2020 11:09
 Operator : DD\AJ
 Sample : L1955-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-07

Manual Integrations
 APPROVED

Ankita
 10/13/2020 12:27:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 12:16:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100920CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 10 05:27:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	25686971	41367273	14.406	14.515
27)	SA Decachlor...	8.125	8.991	56135215	82957036	29.530	29.850
Target Compounds							
2)	A alpha-BHC	3.842	4.337	1966031	2548822	0.805m	0.637
3)	MA gamma-BHC...	4.122	4.620	1420682	2547398	0.628	0.683
4)	MA Heptachlor	4.420	5.127	1409763	3872690	0.700	1.037 #
5)	MB Aldrin	4.664	5.429	1370278	2396556	0.749	0.710
6)	B beta-BHC	4.371	4.793	701322	1798604	0.736	1.001 #
7)	B delta-BHC	4.571	5.005	1302344	2388773	0.617	0.890 #
8)	B Heptachlo...	5.102	5.814	1252544	2275164	0.718	0.797
9)	A Endosulfan I	5.437	6.170	1160598	2182487	0.717	0.737
10)	B trans-Chl...	5.327	6.048	1255594	2150529	0.723	0.704
11)	B cis-Chlor...	5.385	6.121	1298666	2392891	0.746	0.774
12)	B 4,4'-DDE	5.549	6.279	1145631	2070398	0.698	0.697
13)	MA Dieldrin	5.678	6.427	1137010	2384066	0.637	0.777
14)	MA Endrin	5.930	6.643	1138805	1505737	0.714m	0.618
15)	B Endosulfa...	6.202	6.853	1251276	2705341	0.793m	1.028m#
16)	A 4,4'-DDD	6.060	6.767	1013434	1749027	0.726	0.746m
17)	MA 4,4'-DDT	6.299	7.068	499696	1948434	0.378	0.856 #
18)	B Endrin al...	6.371	6.977	1073952	1989824	0.791	0.890
19)	B Endosulfa...	6.582	7.200	1354186	2142929	0.811	0.803
20)	A Methoxychlor	6.843	7.526	541311	1041157	0.661	0.783
21)	B Endrin ke...	7.069	7.667	1104274	2045014	0.651	0.786m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101220\
Data File : PL062211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2020 11:09
Operator : DD\AJ
Sample : L1955-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 12:16:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100920CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 10 05:27:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

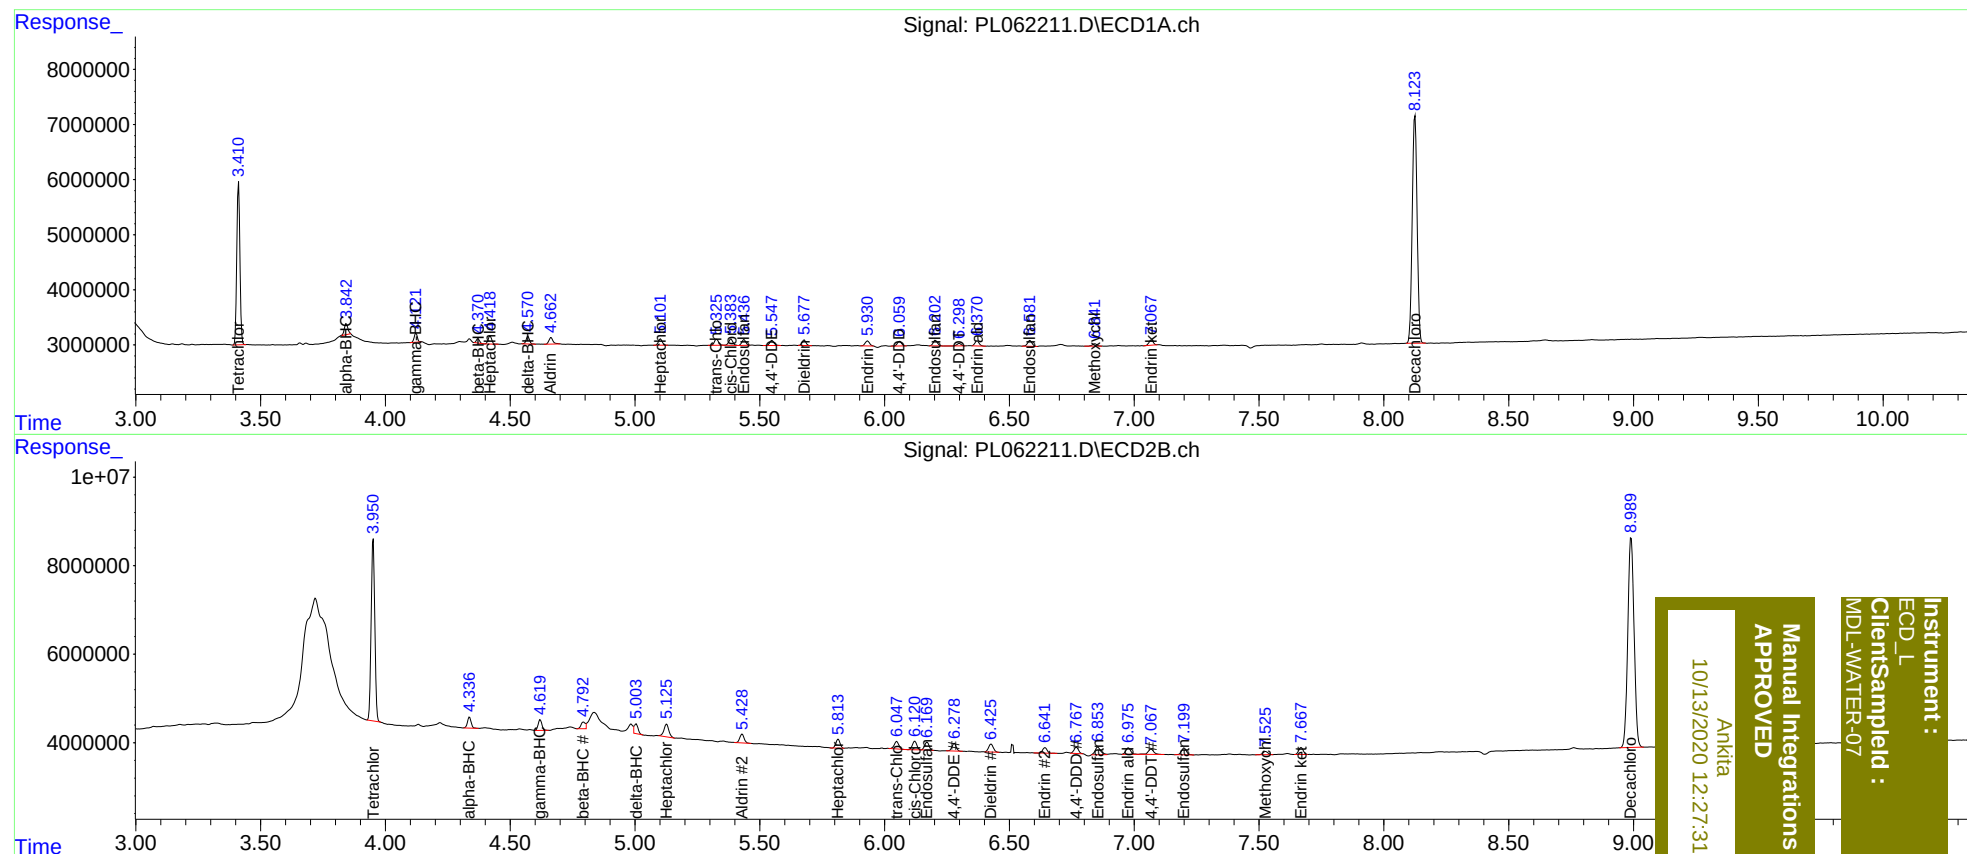

10/13/2020 12:27:31 PM
Ankitia

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sample :
MDL-WATER-07