

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101220\
 Data File : PL062210.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2020 10:55
 Operator : DD\AJ
 Sample : L1955-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-06

Manual Integrations
 APPROVED

Ankita
 10/13/2020 12:27:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 12:16:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100920CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 10 05:27:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	24606481	39512469	13.800	13.864
27)	SA Decachlor...	8.125	8.991	55644003	81195808	29.271	29.216
Target Compounds							
2)	A alpha-BHC	3.844	4.337	2521004	2463433	1.032	0.616 #
3)	MA gamma-BHC...	4.123	4.620	1465627	2551787	0.648	0.684
4)	MA Heptachlor	4.420	5.127	1360172	4336337	0.676	1.161 #
5)	MB Aldrin	4.665	5.429	1315863	2523556	0.719	0.748
6)	B beta-BHC	4.372	4.794	704926	1735235	0.740	0.966 #
7)	B delta-BHC	4.572	5.005	1302926	2420964	0.617	0.902 #
8)	B Heptachlo...	5.103	5.814	1238294	2579584	0.709	0.903 #
9)	A Endosulfan I	5.437	6.170	1140113	2254947	0.705	0.761
10)	B trans-Chl...	5.327	6.049	1285004	2135007	0.740	0.699
11)	B cis-Chlor...	5.385	6.121	1244430	2334098	0.715	0.755
12)	B 4,4'-DDE	5.549	6.279	1024556	2060470	0.625	0.693
13)	MA Dieldrin	5.677	6.427	1091866	2315013	0.612	0.755
14)	MA Endrin	5.932	6.644	1199342	1629585	0.751m	0.669
15)	B Endosulfa...	6.204	6.853	1259533	2871240	0.799	1.091m#
16)	A 4,4'-DDD	6.061	6.768	984911	1699200	0.705	0.725m
17)	MA 4,4'-DDT	6.300	7.068	526929	1861627	0.398	0.818 #
18)	B Endrin al...	6.371	6.978	1012054	2005874	0.745	0.898
19)	B Endosulfa...	6.583	7.200	1299113	2090230	0.778	0.784
20)	A Methoxychlor	6.842	7.528	520999	948069	0.636	0.713
21)	B Endrin ke...	7.069	7.668	1279246	2102802	0.755	0.808m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101220\
Data File : PL062210.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2020 10:55
Operator : DD\AJ
Sample : L1955-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 12:16:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100920CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 10 05:27:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

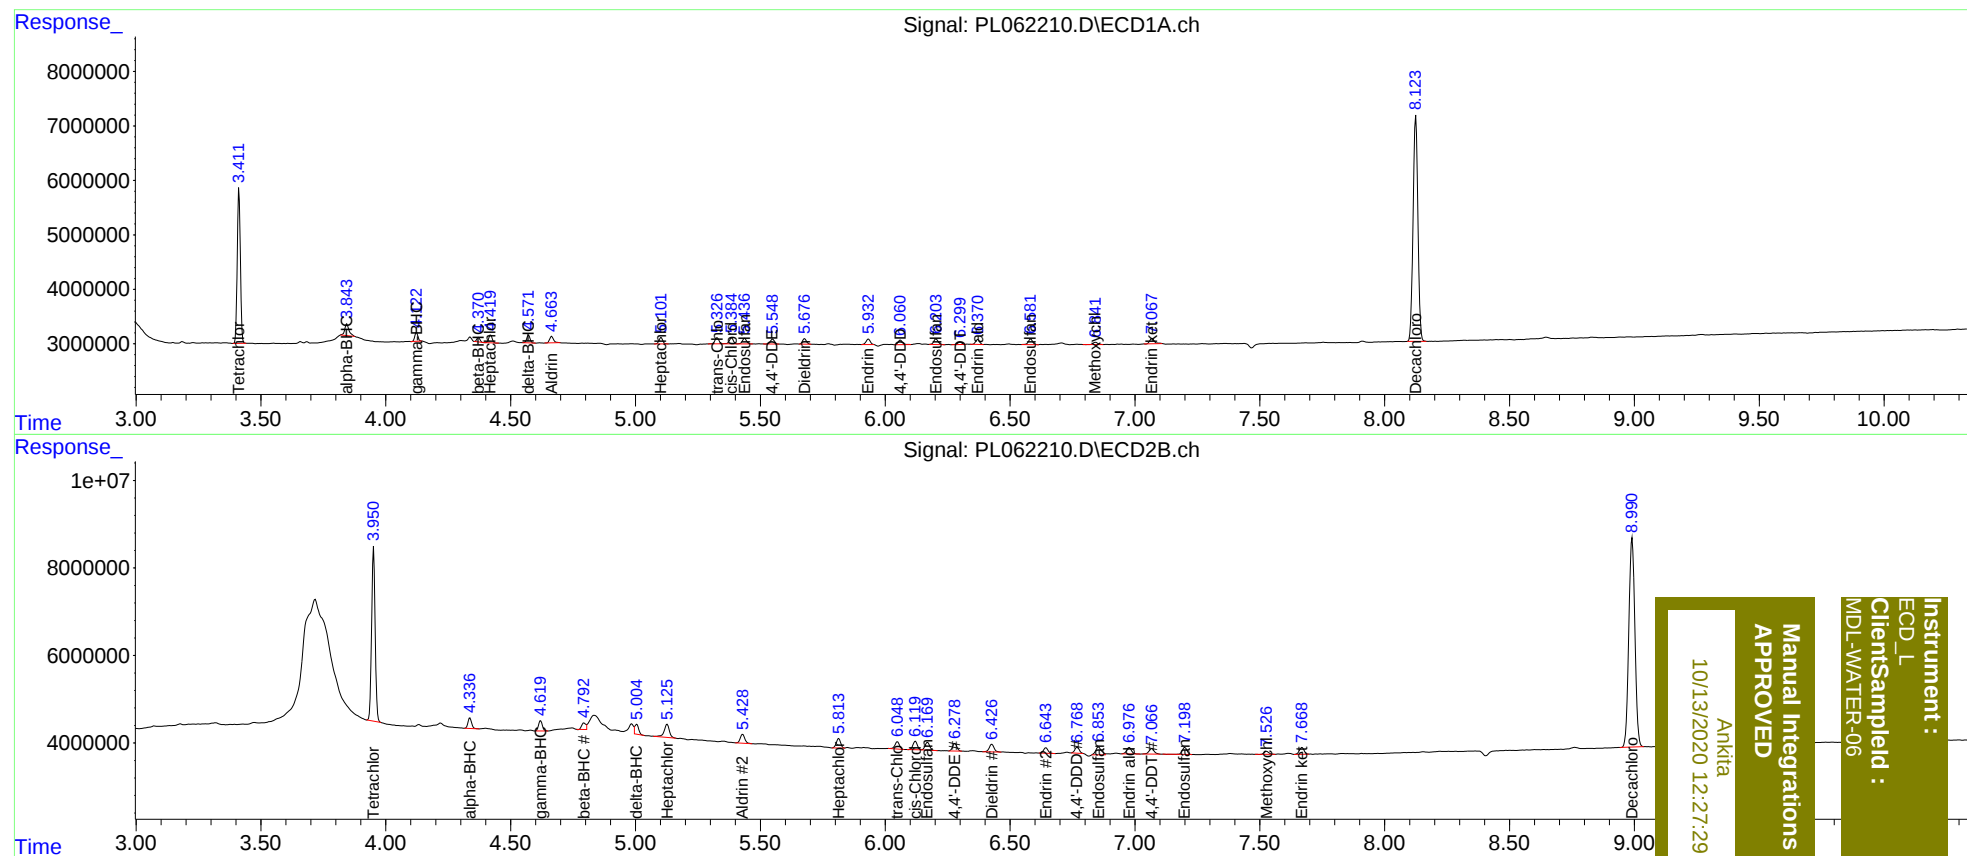

Manual Integrations
APPROVED

Ankita
10/13/2020 12:27:29 PM

Instrument :
ECD_L
Client/Sample :
MDL-WATER-06