

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101222\
 Data File : PL078294.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 12:14
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 13:55:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 13:54:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	2.620	171.1E6	314.1E6	99.605	96.539
28)	SA Decachlor...	8.901	7.716	144.2E6	207.7E6	92.873	91.738
Target Compounds							
23)	Chlordane-1	4.572	3.596	65214540	95384695	981.772	954.490
24)	Chlordane-2	5.106	4.166	68275463	98416545	951.777	936.441
25)	Chlordane-3	5.818	4.790	270.3E6	297.9E6	1008.530	957.720
26)	Chlordane-4	5.896	4.851	325.1E6	313.6E6	997.329	959.522
27)	Chlordane-5	6.755	5.514	52426996	76031717	982.750	944.617



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101222\
Data File : PL078294.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 12:14
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 13:55:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 13:54:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

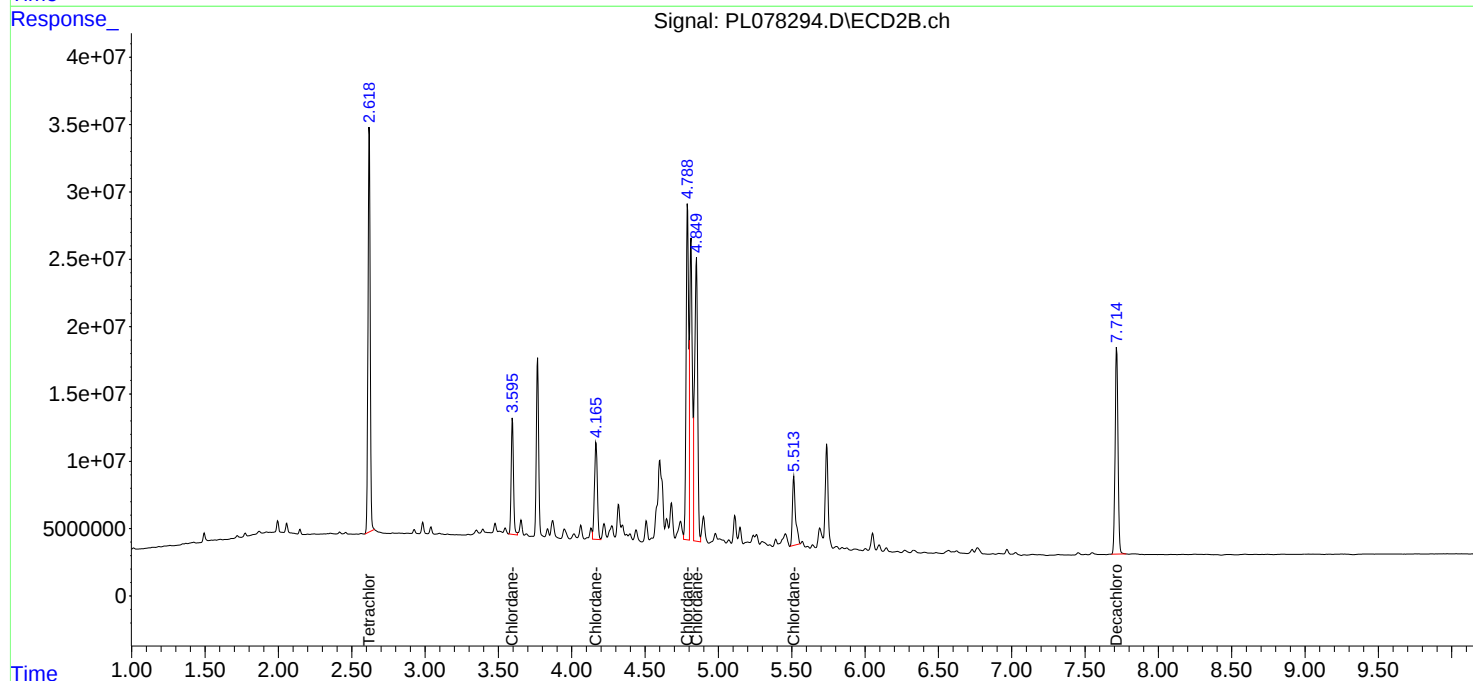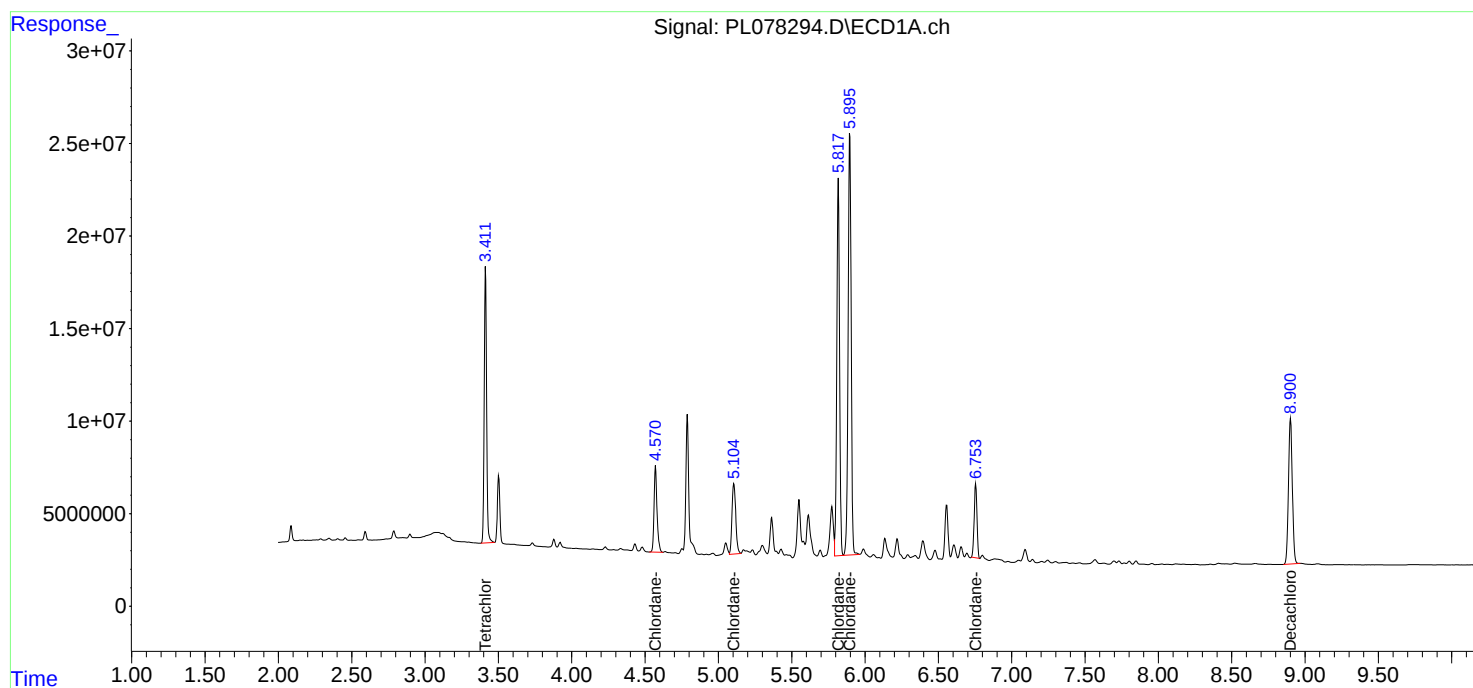


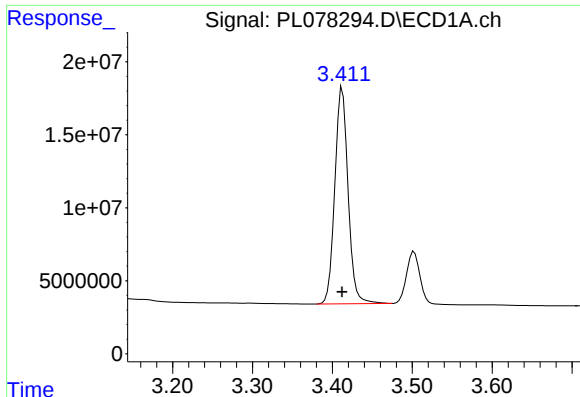

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 171060438
Conc: 99.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

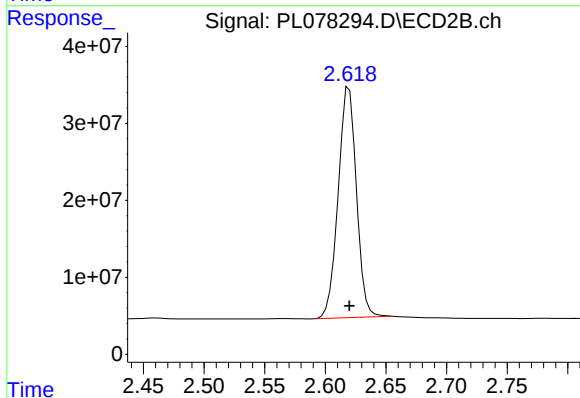


#1 Tetrachloro-m-xylene

R.T.: 2.620 min
Delta R.T.: 0.000 min
Response: 314083489
Conc: 96.54 ng/ml

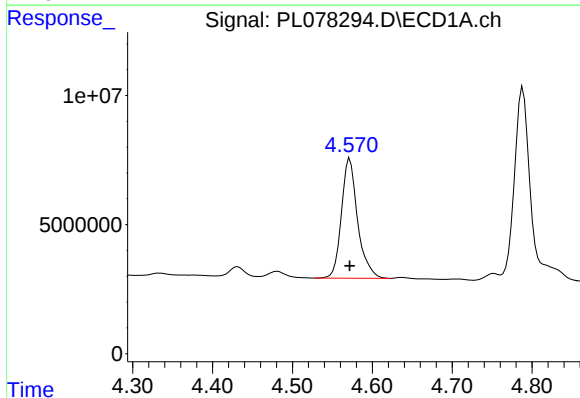


#23 Chlordane-1

R.T.: 4.572 min
Delta R.T.: 0.000 min
Response: 65214540
Conc: 981.77 ng/ml

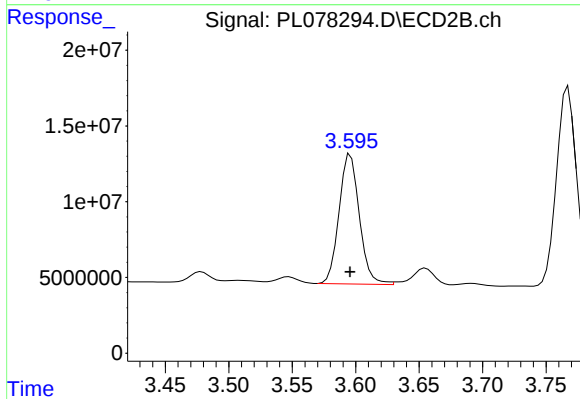

#23 Chlordane-1


R.T.: 3.596 min
Delta R.T.: 0.000 min
Response: 95384695
Conc: 954.49 ng/ml

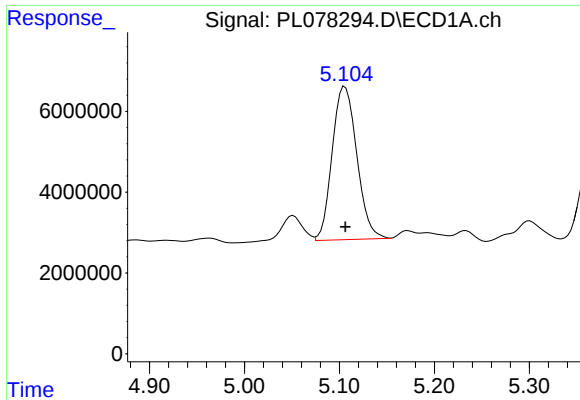

#24 Chlordane-2


R.T.: 5.106 min
Delta R.T.: 0.000 min
Response: 68275463
Conc: 951.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

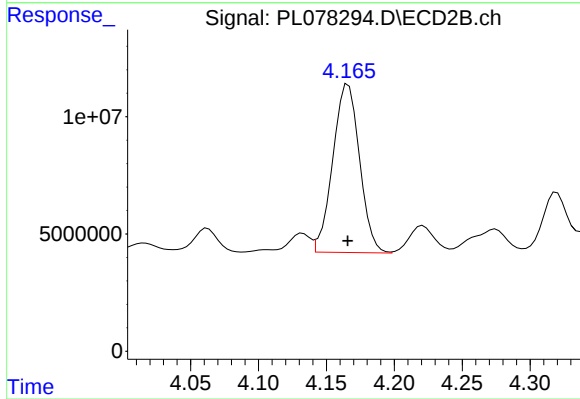


#24 Chlordane-2

R.T.: 4.166 min
Delta R.T.: 0.000 min
Response: 98416545
Conc: 936.44 ng/ml

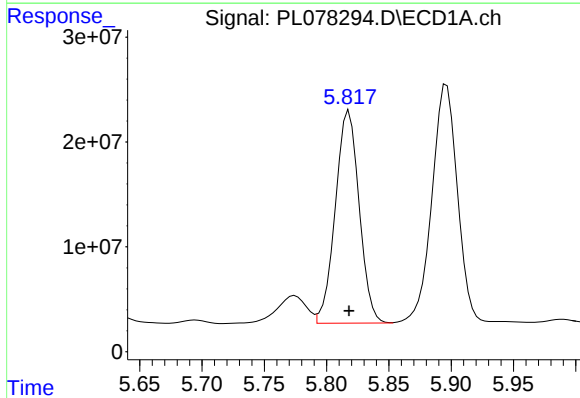


#25 Chlordane-3

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 270281279
Conc: 1008.53 ng/ml

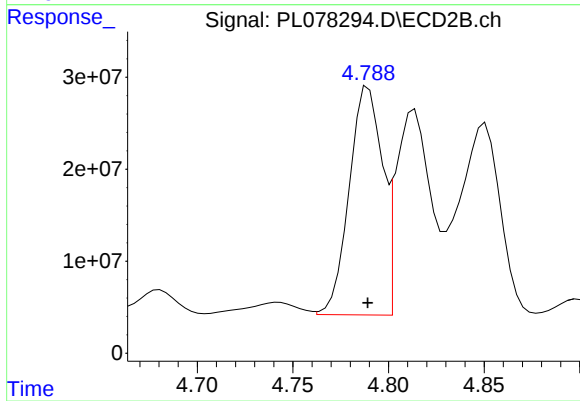

#25 Chlordane-3


R.T.: 4.790 min
Delta R.T.: 0.000 min
Response: 297943258
Conc: 957.72 ng/ml

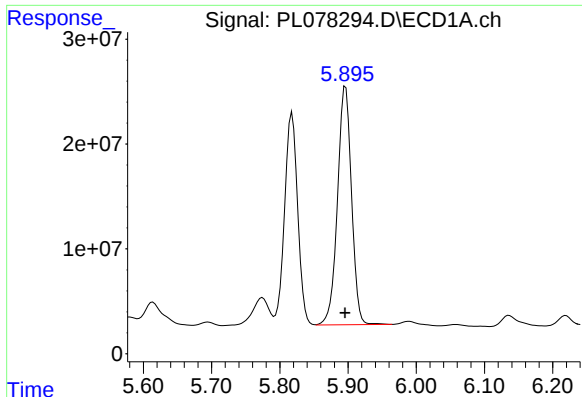

#26 Chlordane-4


R.T.: 5.896 min
Delta R.T.: 0.000 min
Response: 325096802
Conc: 997.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

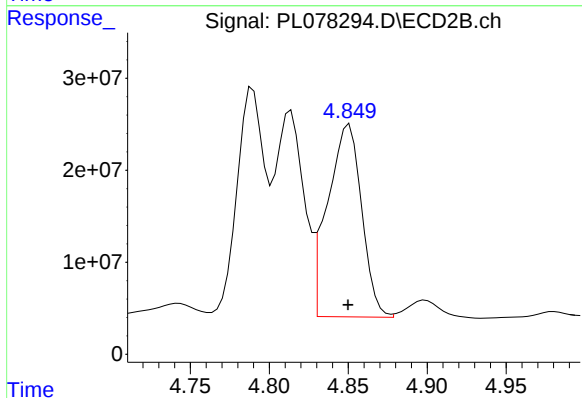


#26 Chlordane-4

R.T.: 4.851 min
Delta R.T.: 0.000 min
Response: 313555454
Conc: 959.52 ng/ml

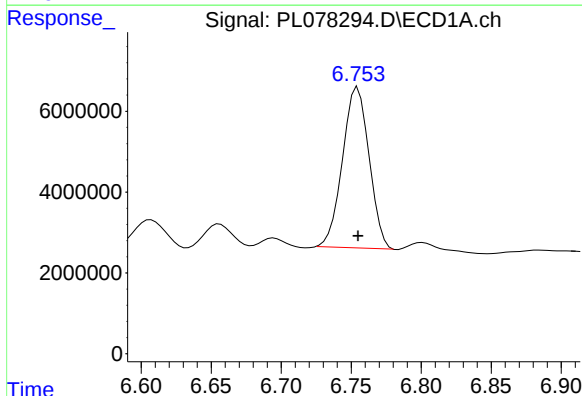


#27 Chlordane-5

R.T.: 6.755 min
Delta R.T.: 0.000 min
Response: 52426996
Conc: 982.75 ng/ml

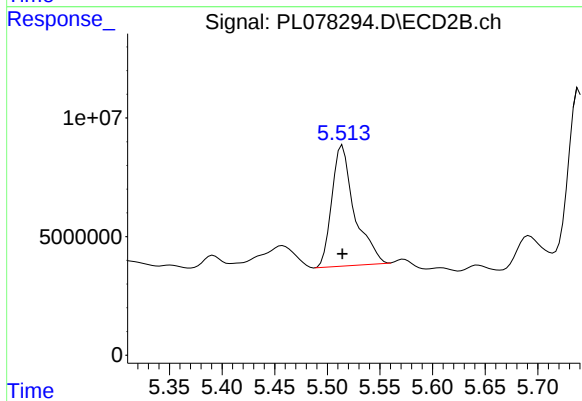

#27 Chlordane-5


R.T.: 5.514 min
Delta R.T.: 0.000 min
Response: 76031717
Conc: 944.62 ng/ml

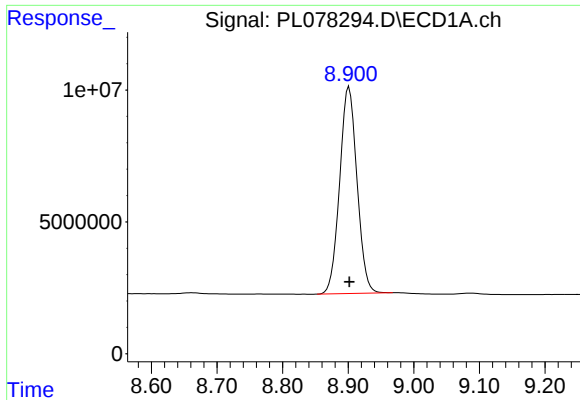

#28 Decachlorobiphenyl

R.T.: 8.901 min
Delta R.T.: 0.000 min
Response: 144159331
Conc: 92.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

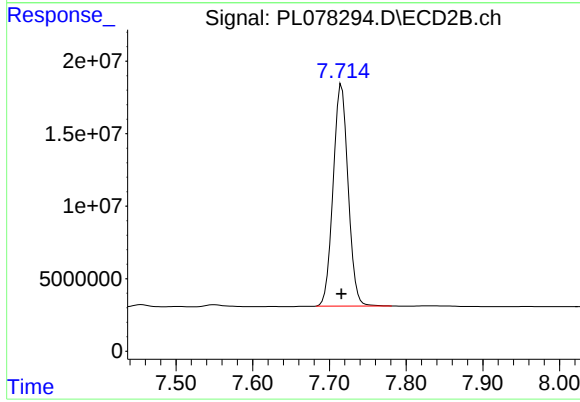

#28 Decachlorobiphenyl

R.T.: 7.716 min
Delta R.T.: 0.000 min
Response: 207697941
Conc: 91.74 ng/ml