

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101222\
 Data File : PL078295.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 12:28
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 13:55:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 13:54:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.413	2.620	129.1E6	241.4E6	75.161	74.209
28)	SA Decachlor...	8.902	7.716	110.6E6	159.3E6	71.259	70.369
Target Compounds							
23)	Chlordane-1	4.572	3.596	49558698	73277873	746.081	733.273
24)	Chlordane-2	5.106	4.166	52397459	76555835	730.434	728.435
25)	Chlordane-3	5.819	4.789	202.3E6	226.6E6	754.806	728.269
26)	Chlordane-4	5.896	4.850	244.0E6	238.6E6	748.603	730.096
27)	Chlordane-5	6.754	5.514	39395374	57996612	738.471	720.549



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101222\
Data File : PL078295.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 12:28
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 13:55:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 13:54:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

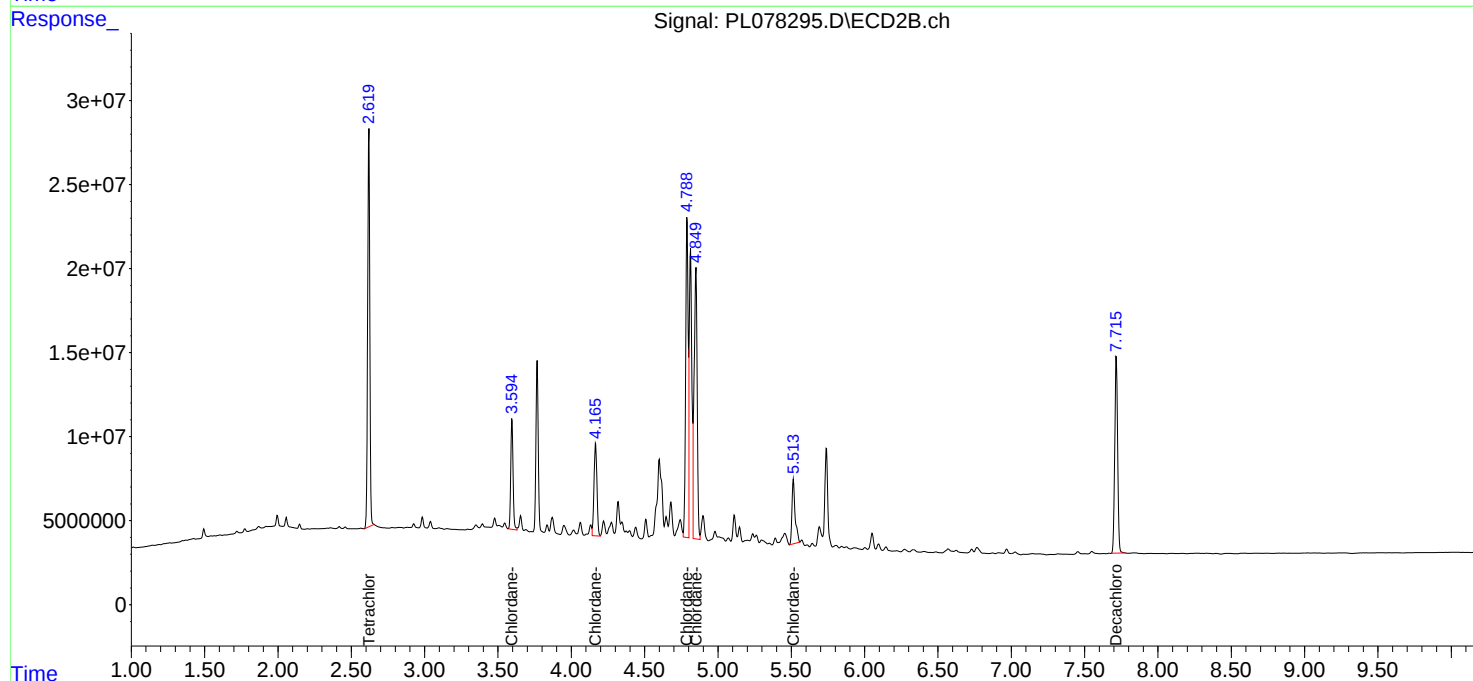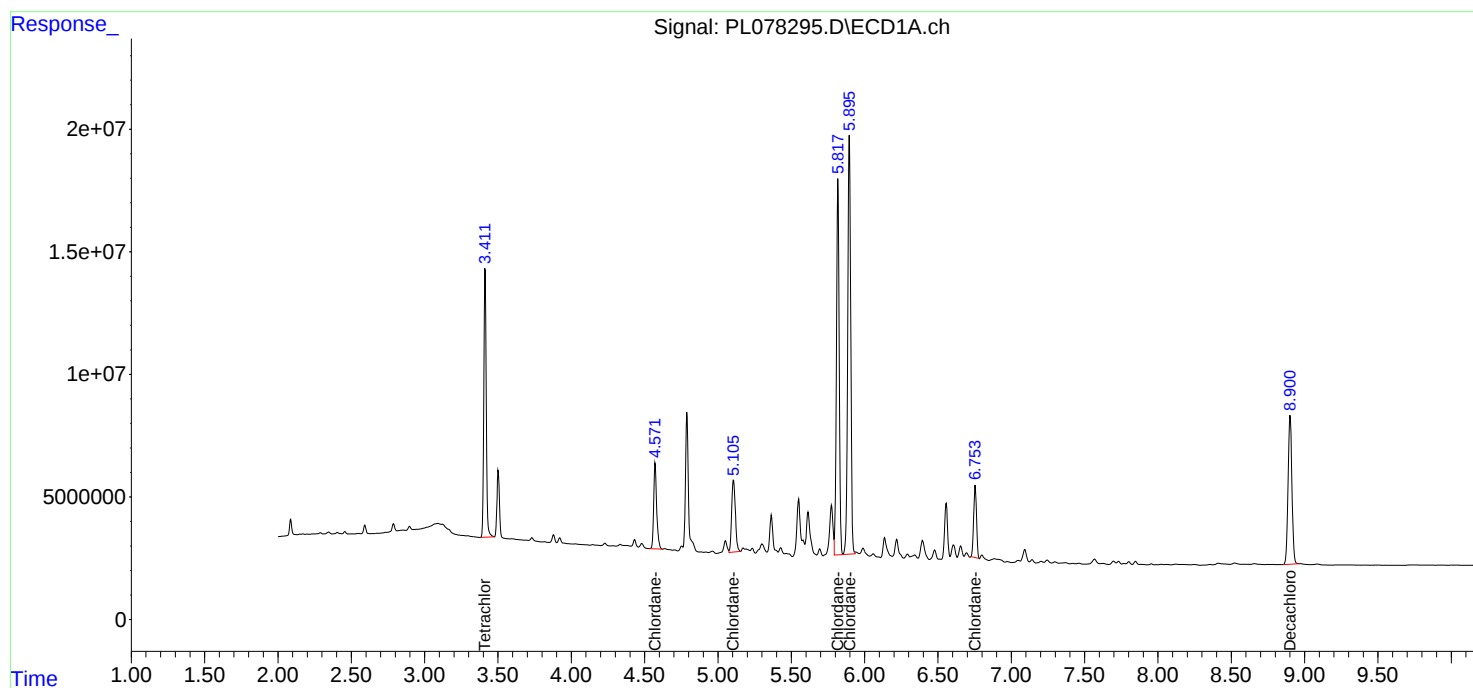


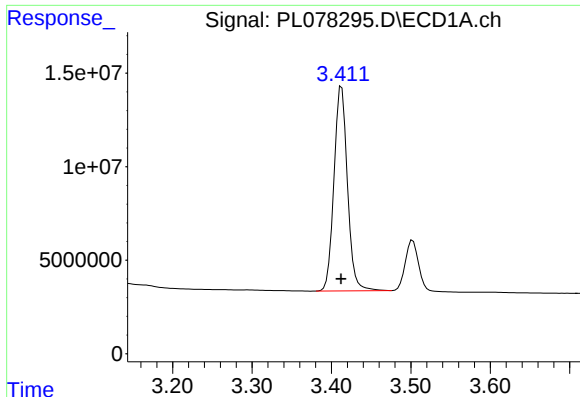

#1 Tetrachloro-m-xylene


R.T.: 3.413 min
Delta R.T.: 0.000 min
Response: 129081795
Conc: 75.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

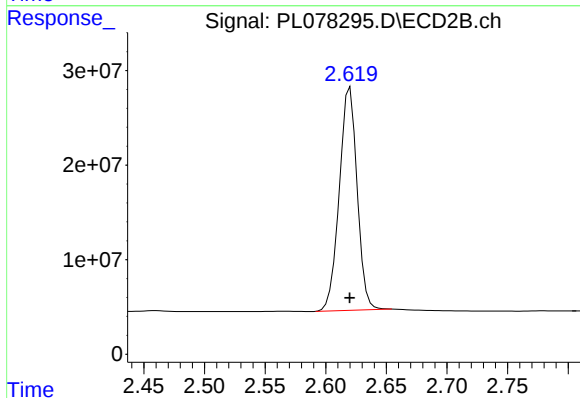


#1 Tetrachloro-m-xylene

R.T.: 2.620 min
Delta R.T.: 0.000 min
Response: 241432070
Conc: 74.21 ng/ml

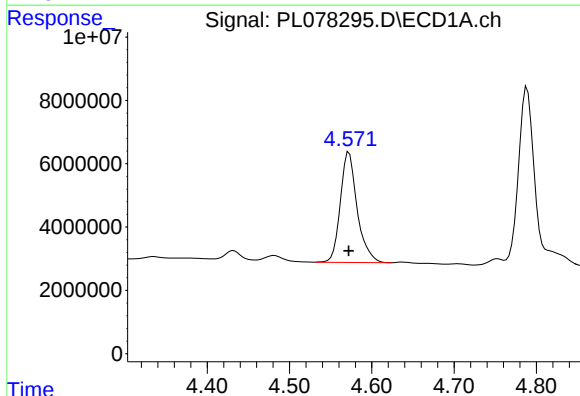


#23 Chlordane-1

R.T.: 4.572 min
Delta R.T.: 0.000 min
Response: 49558698
Conc: 746.08 ng/ml

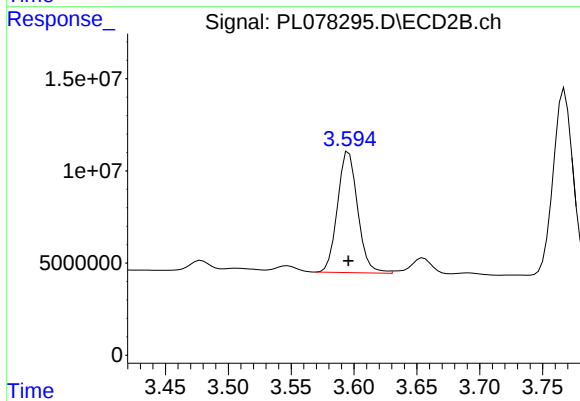

#23 Chlordane-1


R.T.: 3.596 min
Delta R.T.: 0.000 min
Response: 73277873
Conc: 733.27 ng/ml

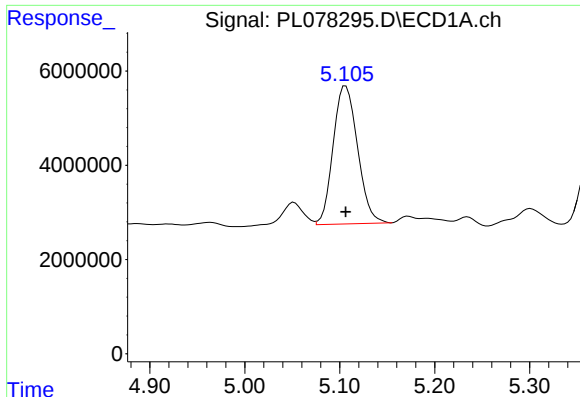

#24 Chlordane-2


R.T.: 5.106 min
Delta R.T.: 0.000 min
Response: 52397459
Conc: 730.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

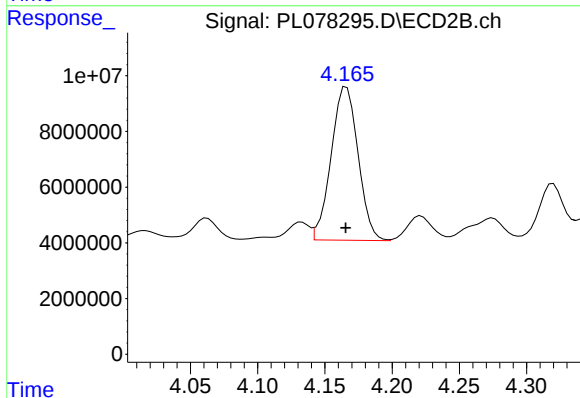


#24 Chlordane-2

R.T.: 4.166 min
Delta R.T.: 0.000 min
Response: 76555835
Conc: 728.44 ng/ml

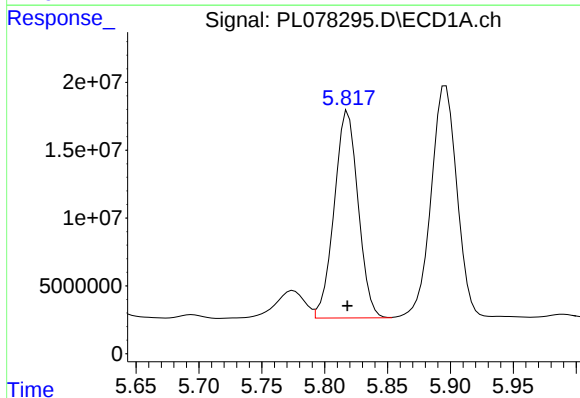


#25 Chlordane-3

R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 202284399
Conc: 754.81 ng/ml

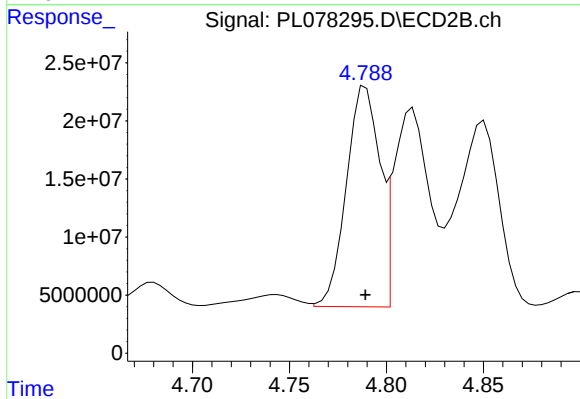

#25 Chlordane-3


R.T.: 4.789 min
Delta R.T.: 0.000 min
Response: 226561931
Conc: 728.27 ng/ml

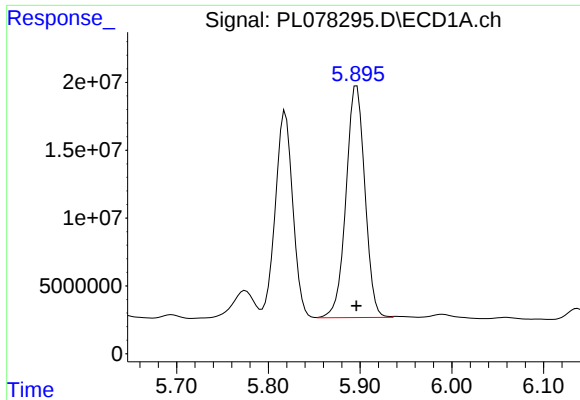

#26 Chlordane-4


R.T.: 5.896 min
Delta R.T.: 0.000 min
Response: 244020161
Conc: 748.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

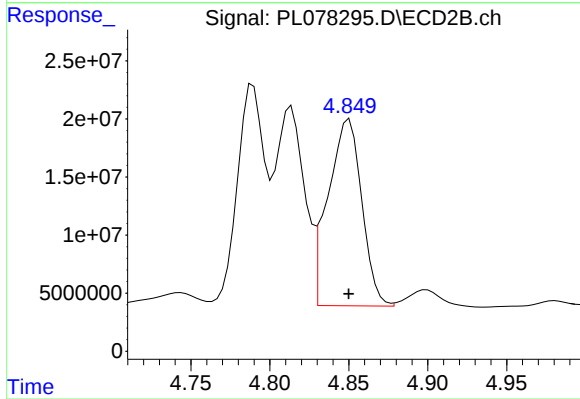


#26 Chlordane-4

R.T.: 4.850 min
Delta R.T.: 0.000 min
Response: 238582924
Conc: 730.10 ng/ml

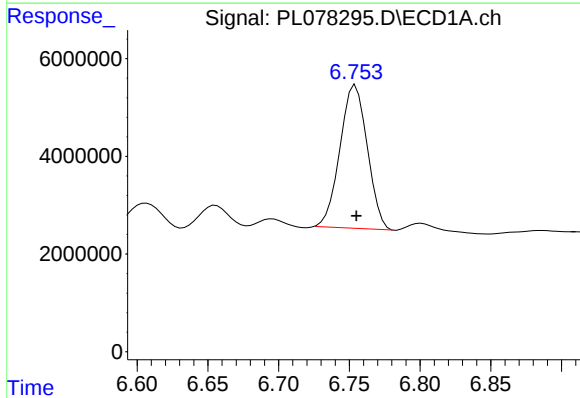


#27 Chlordane-5

R.T.: 6.754 min
Delta R.T.: 0.000 min
Response: 39395374
Conc: 738.47 ng/ml

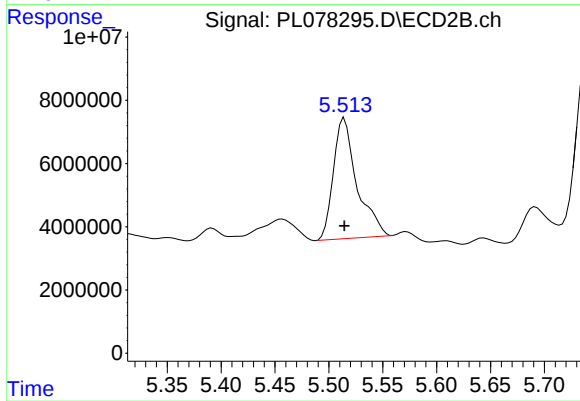

#27 Chlordane-5


R.T.: 5.514 min
Delta R.T.: 0.000 min
Response: 57996612
Conc: 720.55 ng/ml

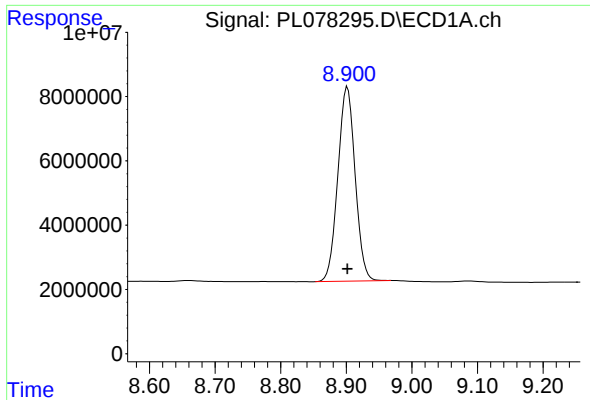

#28 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.000 min
Response: 110610538
Conc: 71.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

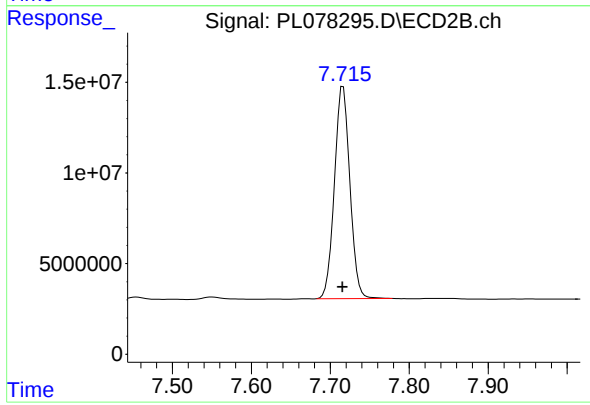

#28 Decachlorobiphenyl

R.T.: 7.716 min
Delta R.T.: 0.000 min
Response: 159316053
Conc: 70.37 ng/ml