

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101222\
 Data File : PL078305.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 18:29
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL101222CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 00:59:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 15:30:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.418	2.617	77874680	147.5E6	47.122	55.795
28)	SA Decachlor...	8.906	7.717	70619027	103.9E6	45.744	47.805
Target Compounds							
23)	Chlordane-1	4.578	3.594	30156181	44375207	476.703	462.993
24)	Chlordane-2	5.112	4.164	32168904	45488994	456.727	451.320
25)	Chlordane-3	5.823	4.788	122.7E6	142.4E6	471.926	465.312
26)	Chlordane-4	5.901	4.849	149.2E6	150.0E6	467.268	464.415
27)	Chlordane-5	6.760	5.514	23033031	37536209	453.585	439.889



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101222\
Data File : PL078305.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 18:29
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL101222CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 00:59:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 15:30:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

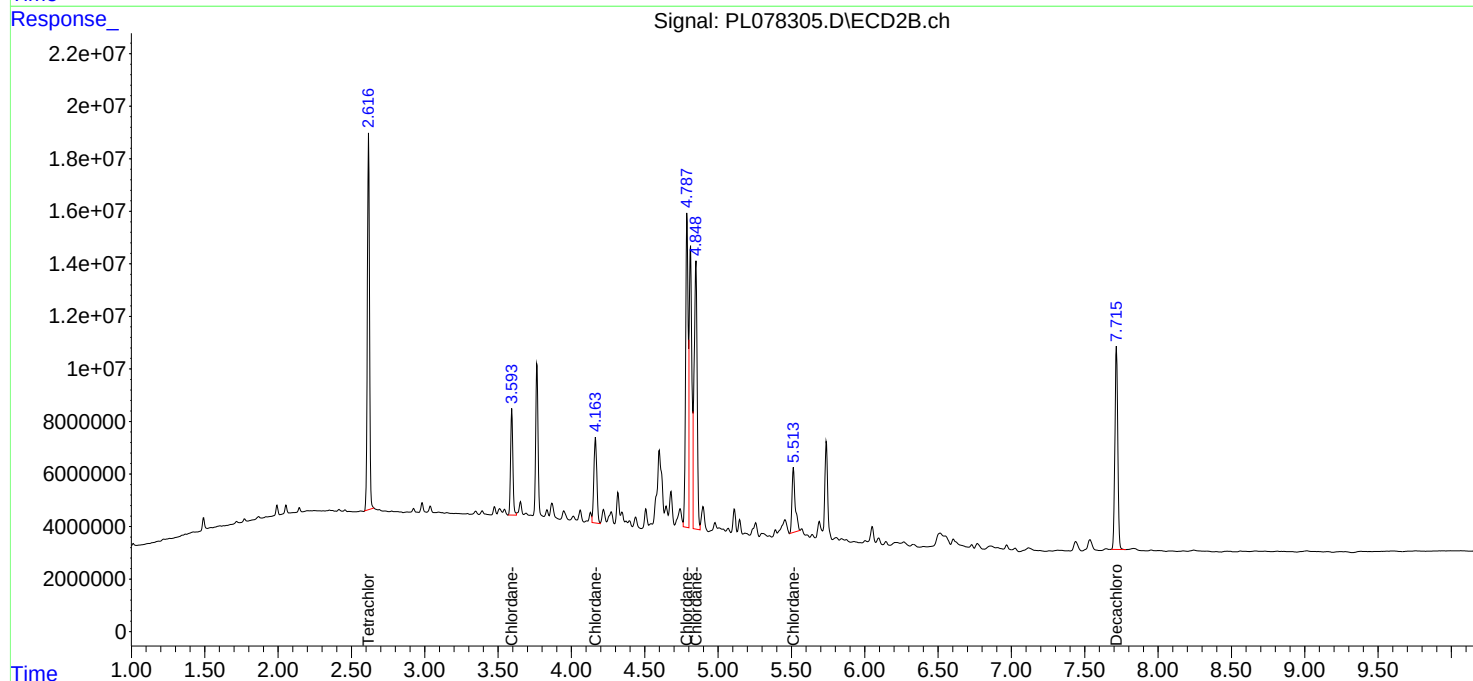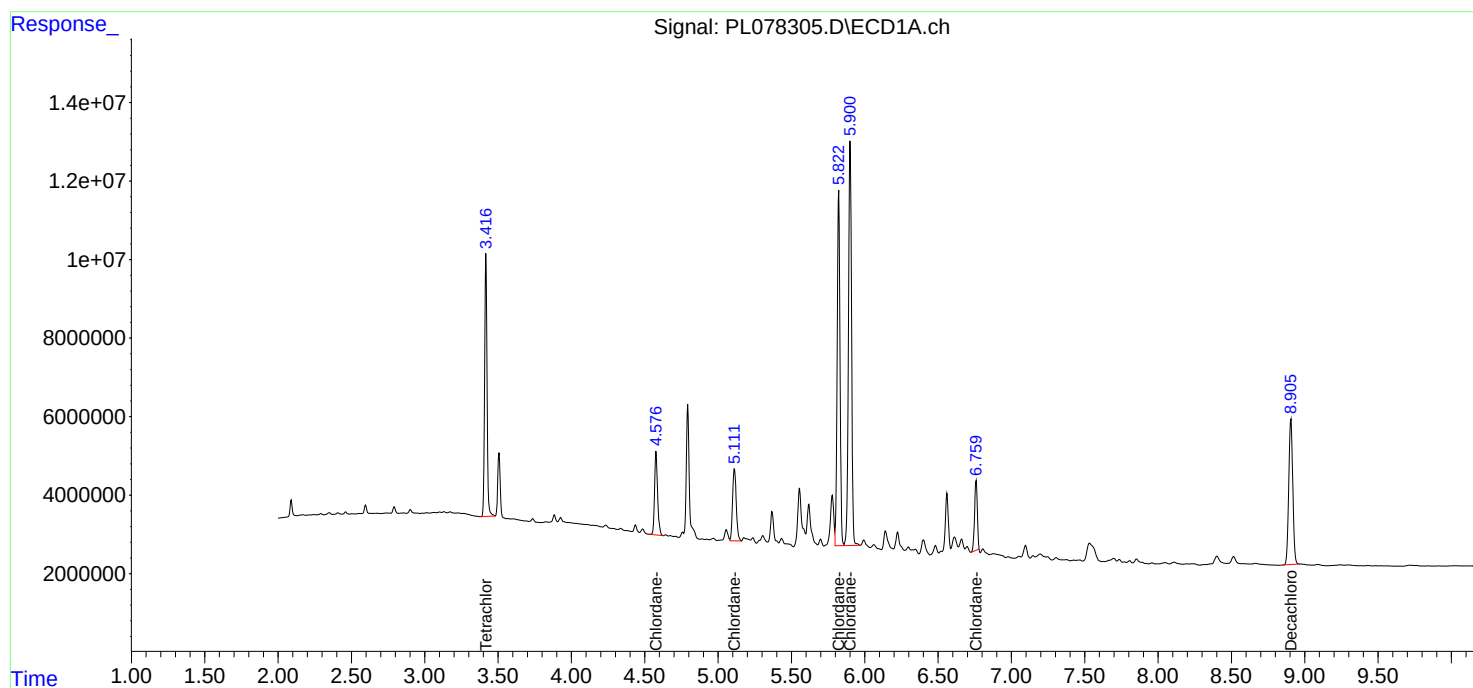


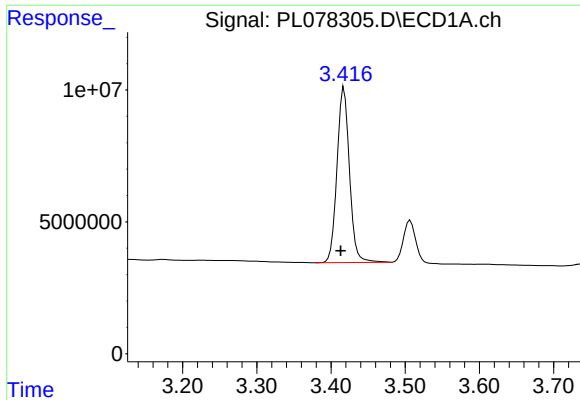

#1 Tetrachloro-m-xylene


R.T.: 3.418 min
Delta R.T.: 0.005 min
Response: 77874680
Conc: 47.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL101222CHLOR

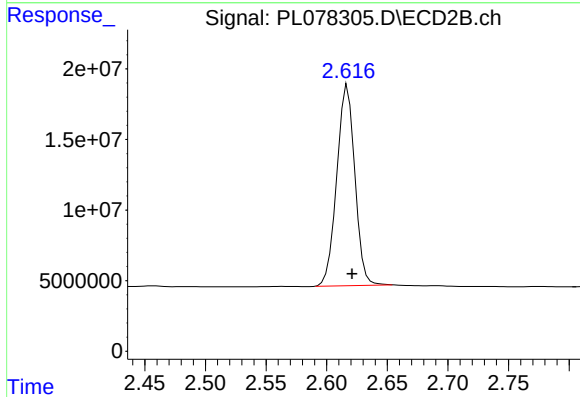


#1 Tetrachloro-m-xylene

R.T.: 2.617 min
Delta R.T.: -0.004 min
Response: 147480941
Conc: 55.79 ng/ml

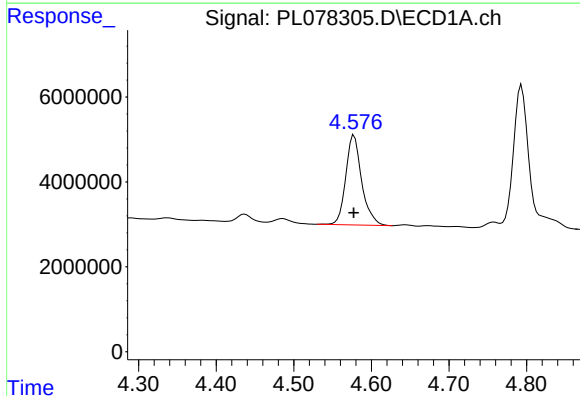


#23 Chlordane-1

R.T.: 4.578 min
Delta R.T.: 0.000 min
Response: 30156181
Conc: 476.70 ng/ml

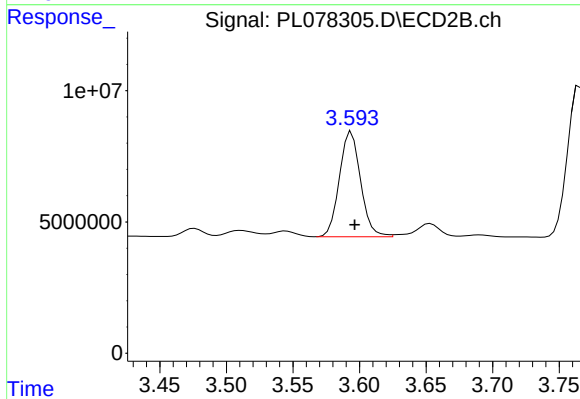

#23 Chlordane-1


R.T.: 3.594 min
Delta R.T.: -0.003 min
Response: 44375207
Conc: 462.99 ng/ml

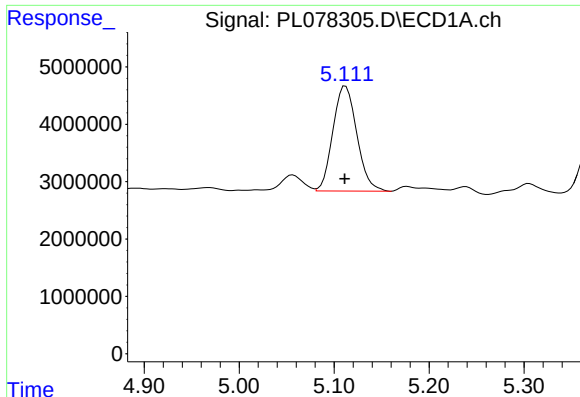

#24 Chlordane-2


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 32168904
Conc: 456.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL101222CHLOR

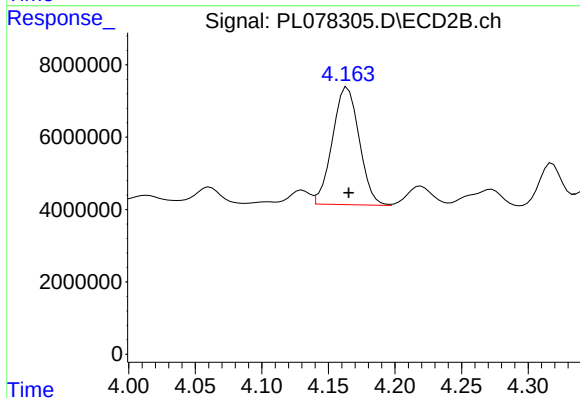


#24 Chlordane-2

R.T.: 4.164 min
Delta R.T.: 0.000 min
Response: 45488994
Conc: 451.32 ng/ml

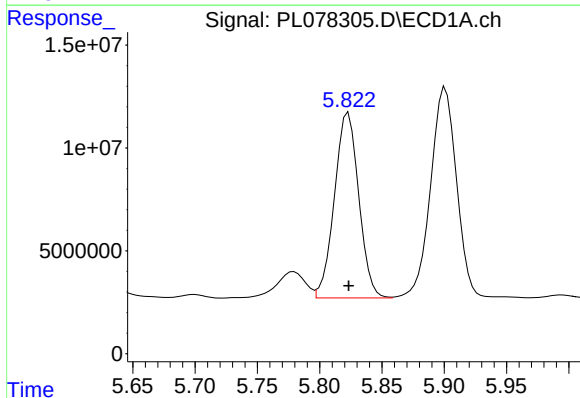


#25 Chlordane-3

R.T.: 5.823 min
Delta R.T.: 0.000 min
Response: 122691164
Conc: 471.93 ng/ml

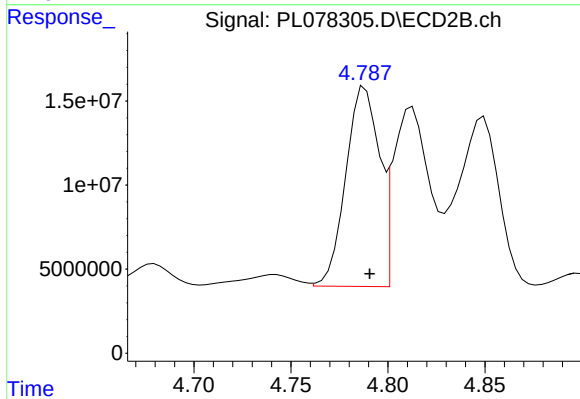

#25 Chlordane-3


R.T.: 4.788 min
Delta R.T.: -0.002 min
Response: 142366278
Conc: 465.31 ng/ml

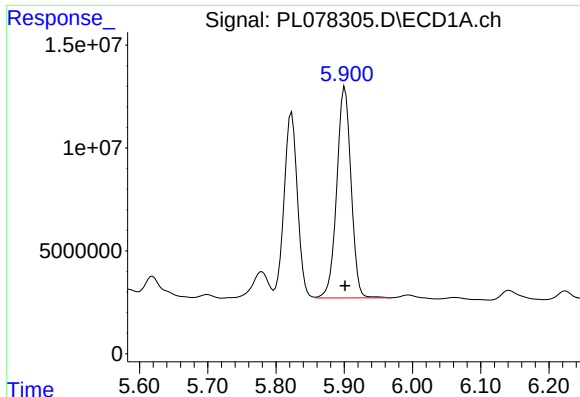

#26 Chlordane-4


R.T.: 5.901 min
Delta R.T.: 0.000 min
Response: 149232973
Conc: 467.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL101222CHLOR

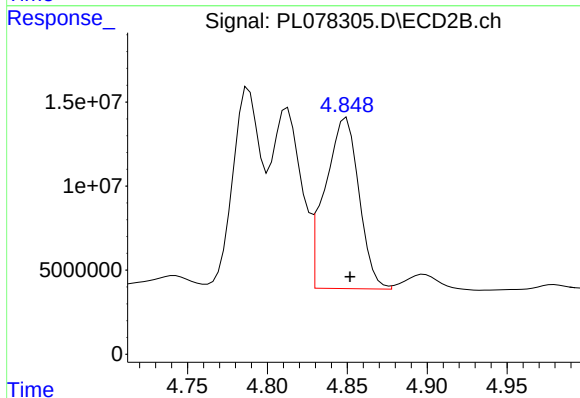


#26 Chlordane-4

R.T.: 4.849 min
Delta R.T.: -0.002 min
Response: 149966916
Conc: 464.41 ng/ml

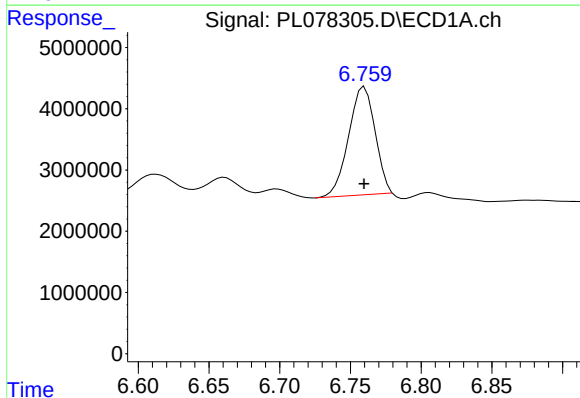


#27 Chlordane-5

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 23033031
Conc: 453.59 ng/ml

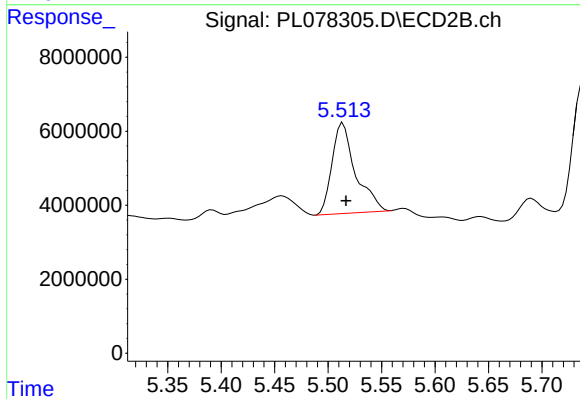

#27 Chlordane-5


R.T.: 5.514 min
Delta R.T.: -0.003 min
Response: 37536209
Conc: 439.89 ng/ml

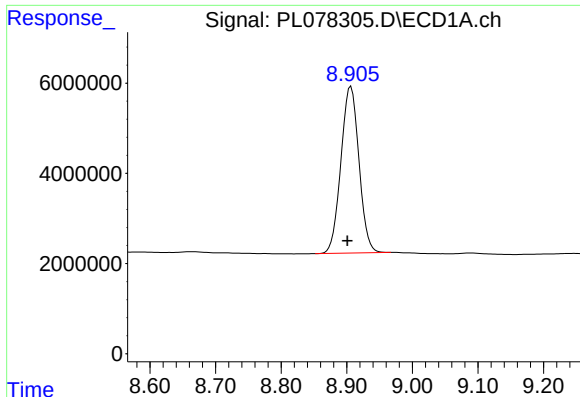

#28 Decachlorobiphenyl

R.T.: 8.906 min
Delta R.T.: 0.005 min
Response: 70619027
Conc: 45.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL101222CHLOR

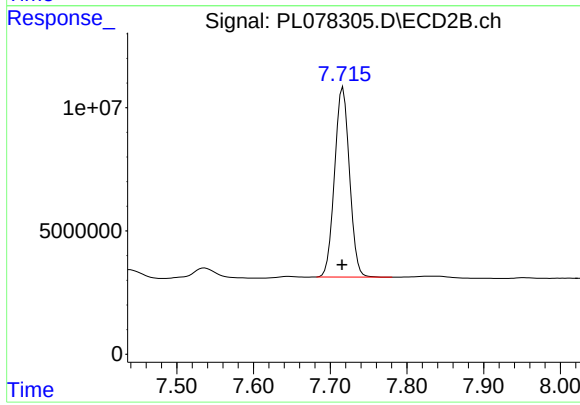

#28 Decachlorobiphenyl

R.T.: 7.717 min
Delta R.T.: 0.001 min
Response: 103919916
Conc: 47.81 ng/ml