

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101223\
 Data File : PL085880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2023 15:22
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 21:14:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.365	2.621	131.2E6	51295378	44.119	54.913
28) SA Decachlor...	8.867	7.777	114.6E6	50701202	52.607	54.932
Target Compounds						
23) Chlordane-1	4.523	3.612	59298355	15051086	493.272	461.706
24) Chlordane-2	5.055	4.190	61595043	19555211	473.648	502.526
25) Chlordane-3	5.766	4.819	249.5E6	53995416	489.033	534.356
26) Chlordane-4	5.848	4.881	307.7E6	57191617	485.058	493.950
27) Chlordane-5	6.696	5.552	47067758	14323270	458.801	513.906



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101223\
Data File : PL085880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2023 15:22
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 21:14:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

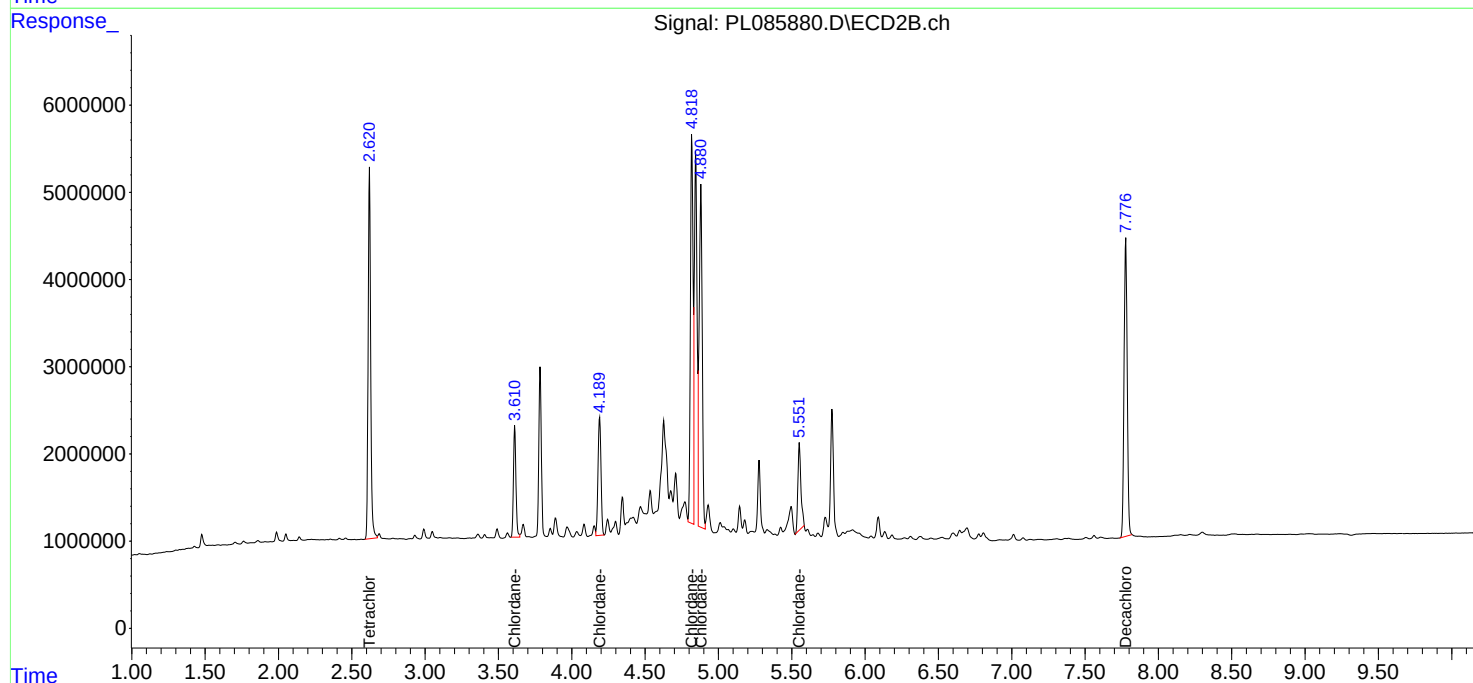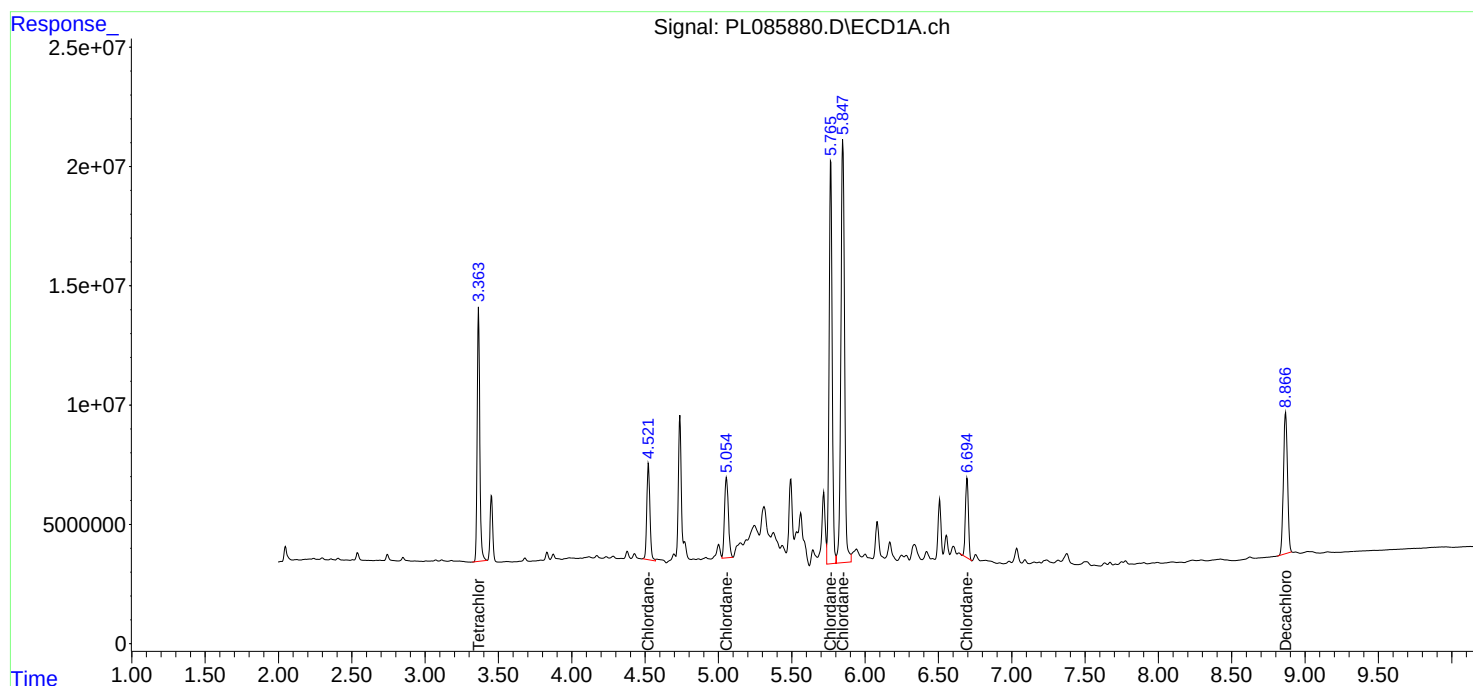


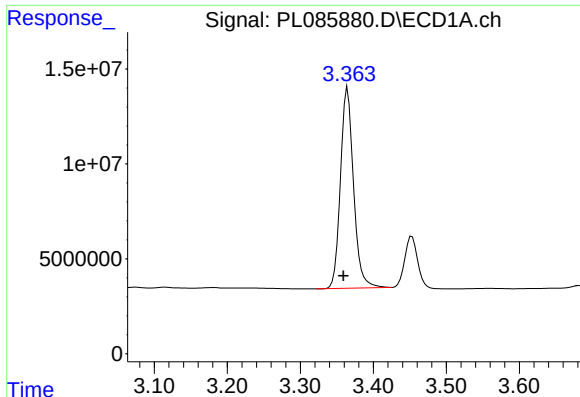

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: 0.006 min
Response: 131217381
Conc: 44.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

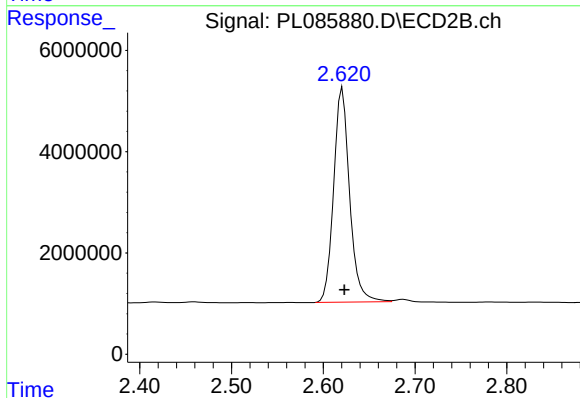


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: -0.002 min
Response: 51295378
Conc: 54.91 ng/ml

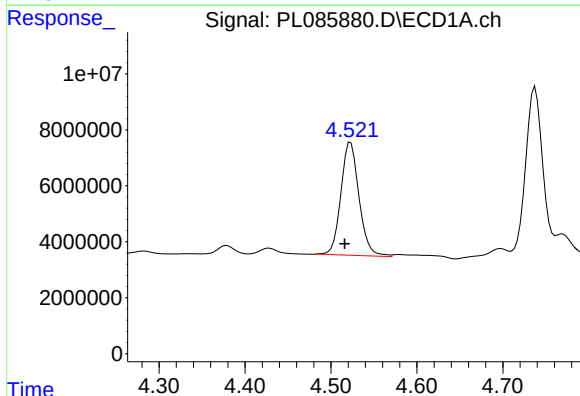


#23 Chlordane-1

R.T.: 4.523 min
Delta R.T.: 0.007 min
Response: 59298355
Conc: 493.27 ng/ml

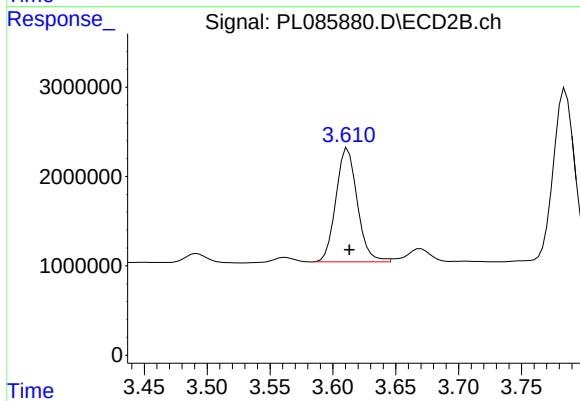

#23 Chlordane-1


R.T.: 3.612 min
Delta R.T.: -0.001 min
Response: 15051086
Conc: 461.71 ng/ml

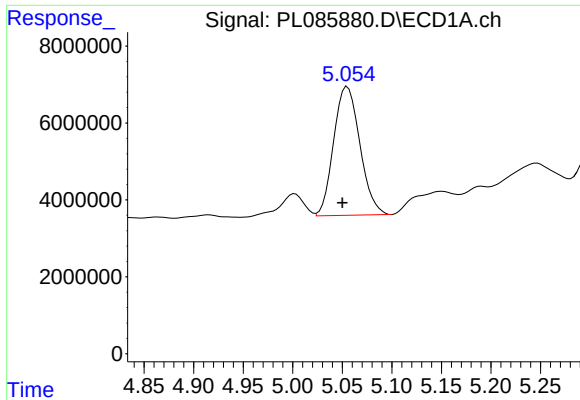

#24 Chlordane-2


R.T.: 5.055 min
Delta R.T.: 0.005 min
Response: 61595043
Conc: 473.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

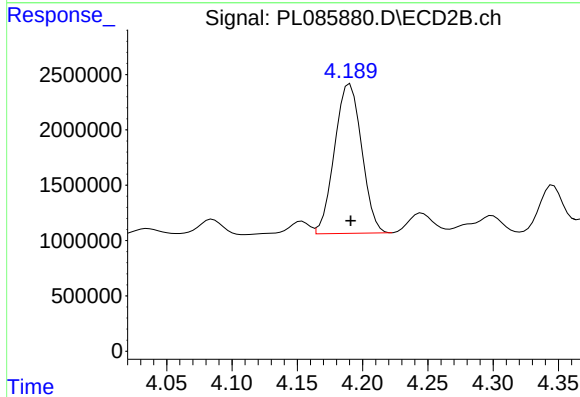


#24 Chlordane-2

R.T.: 4.190 min
Delta R.T.: 0.000 min
Response: 19555211
Conc: 502.53 ng/ml

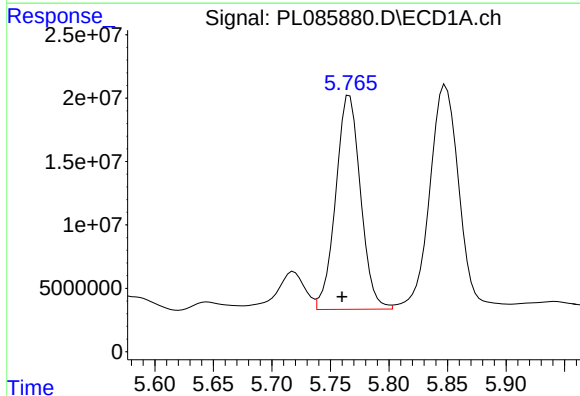


#25 Chlordane-3

R.T.: 5.766 min
Delta R.T.: 0.006 min
Response: 249505145
Conc: 489.03 ng/ml

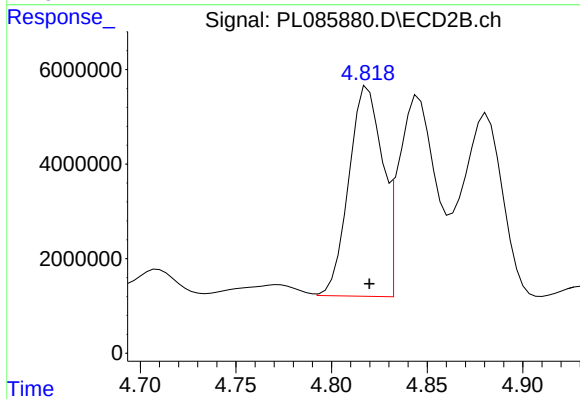

#25 Chlordane-3


R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 53995416
Conc: 534.36 ng/ml

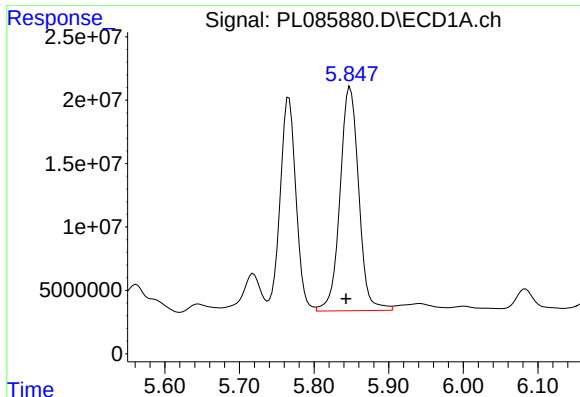

#26 Chlordane-4


R.T.: 5.848 min
Delta R.T.: 0.005 min
Response: 307740309
Conc: 485.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

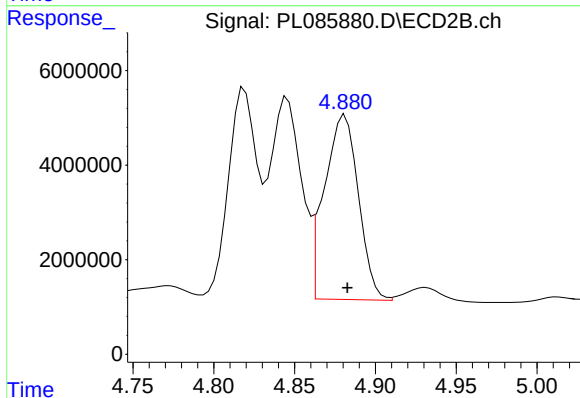


#26 Chlordane-4

R.T.: 4.881 min
Delta R.T.: -0.001 min
Response: 57191617
Conc: 493.95 ng/ml

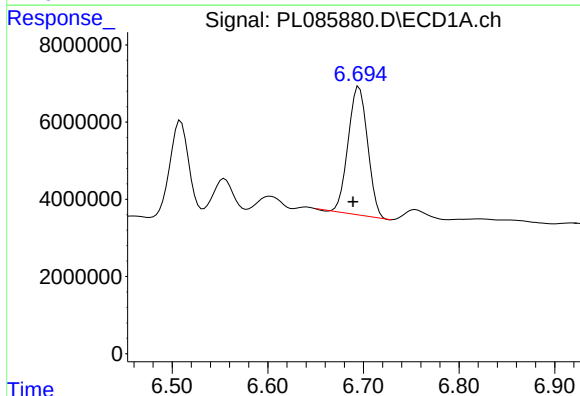


#27 Chlordane-5

R.T.: 6.696 min
Delta R.T.: 0.007 min
Response: 47067758
Conc: 458.80 ng/ml

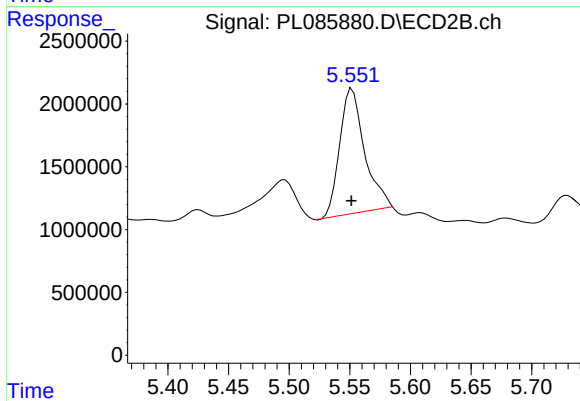

#27 Chlordane-5


R.T.: 5.552 min
Delta R.T.: 0.000 min
Response: 14323270
Conc: 513.91 ng/ml

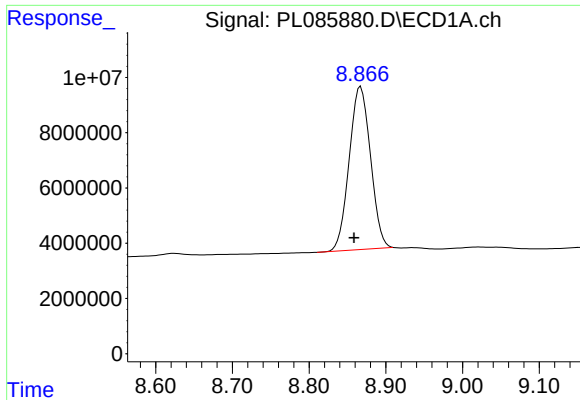

#28 Decachlorobiphenyl

R.T.: 8.867 min
Delta R.T.: 0.009 min
Response: 114579770
Conc: 52.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

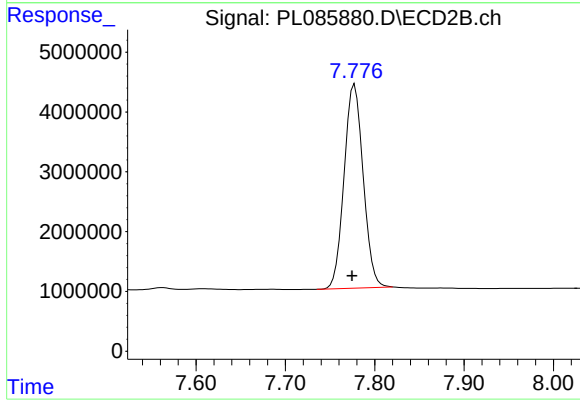

#28 Decachlorobiphenyl

R.T.: 7.777 min
Delta R.T.: 0.003 min
Response: 50701202
Conc: 54.93 ng/ml