

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101320\
 Data File : PL062237.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2020 19:53
 Operator : DD\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 04:20:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 13 04:19:56 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.952	197.5E6	280.0E6	99.712	99.946
28)	SA Decachlor...	8.125	8.992	169.9E6	254.9E6	94.266	94.225
Target Compounds							
23)	Chlordane-1	4.270	4.940	51009744	102.5E6	969.906	1002.339
24)	Chlordane-2	4.766	5.405	57273661	103.7E6	949.180	976.358
25)	Chlordane-3	5.328	6.050	162.0E6	423.7E6	994.552	1008.303
26)	Chlordane-4	5.385	6.124	134.2E6	503.4E6	986.221	994.034
27)	Chlordane-5	6.213	6.926	54804001	82955155	1004.443	1001.904



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101320\
Data File : PL062237.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2020 19:53
Operator : DD\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 04:20:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
Quant Title : GC Extractables
QLast Update : Tue Oct 13 04:19:56 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

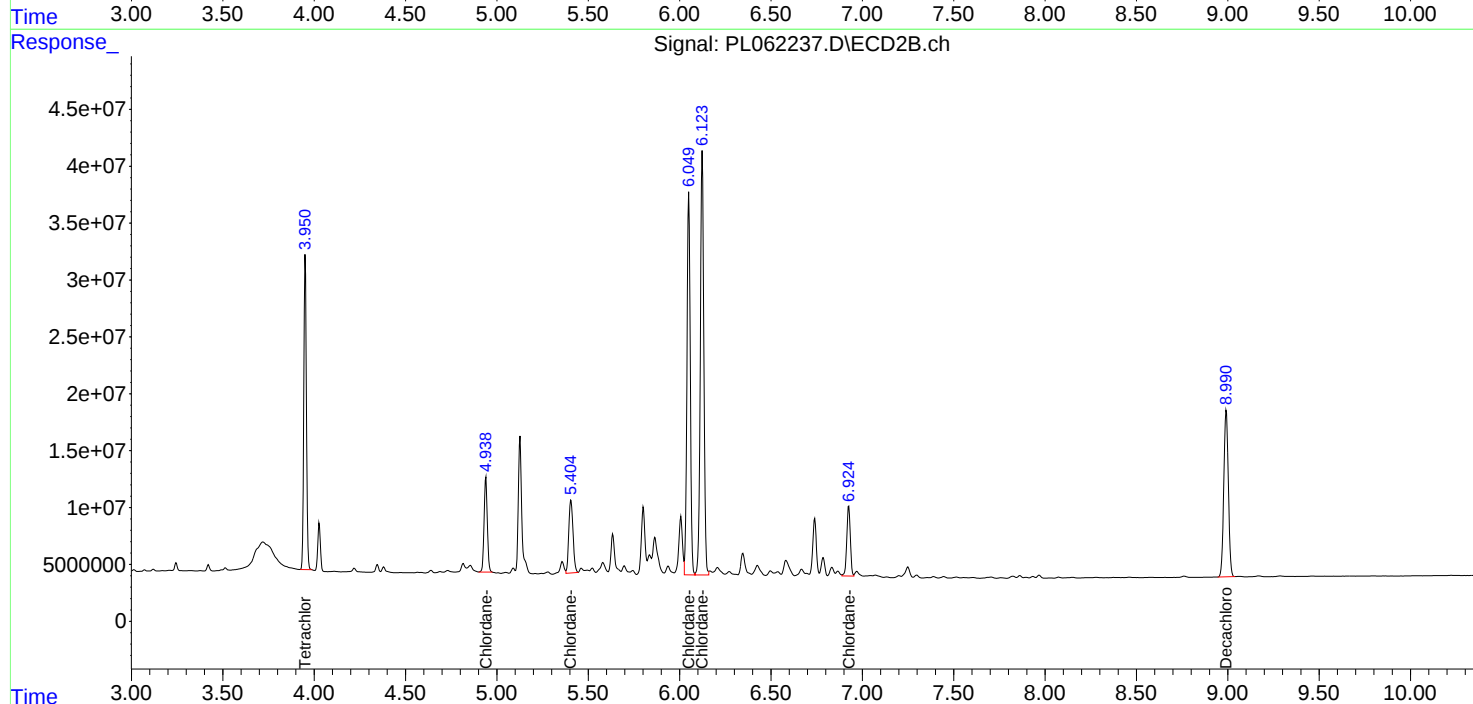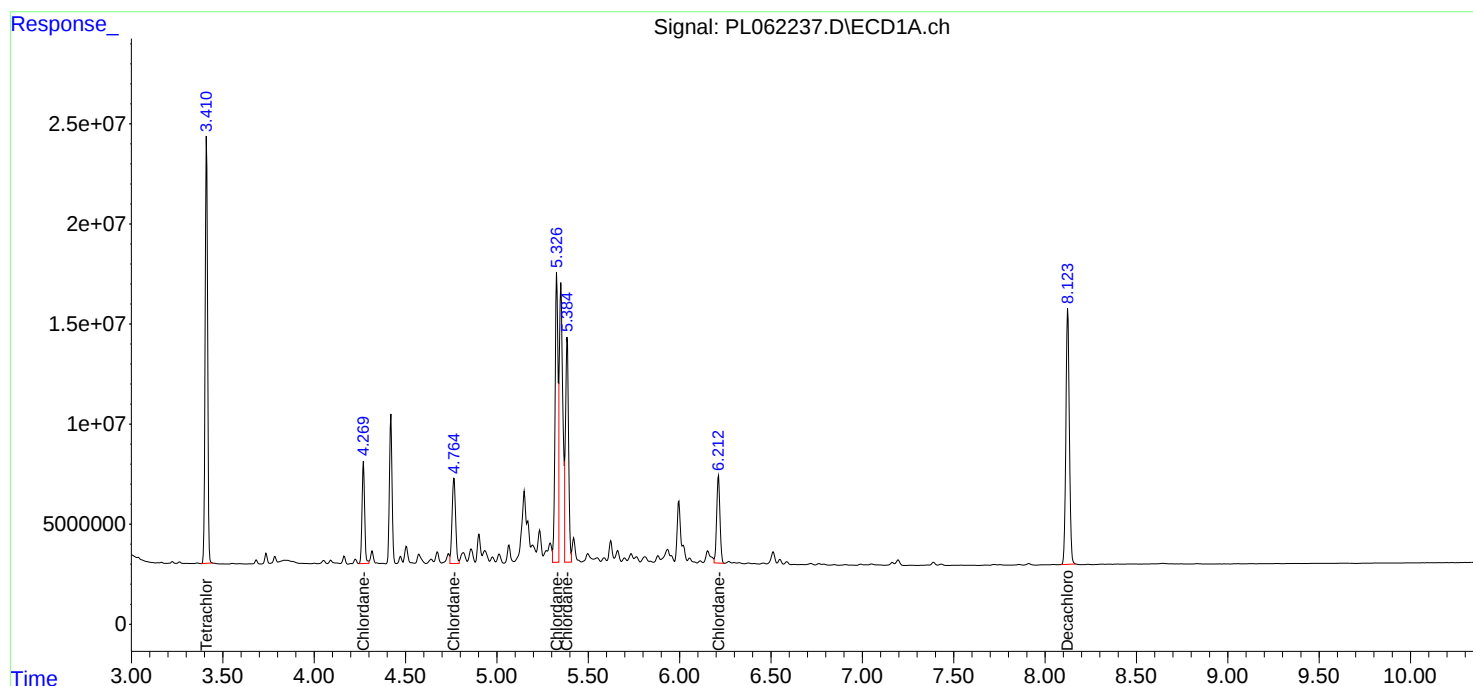


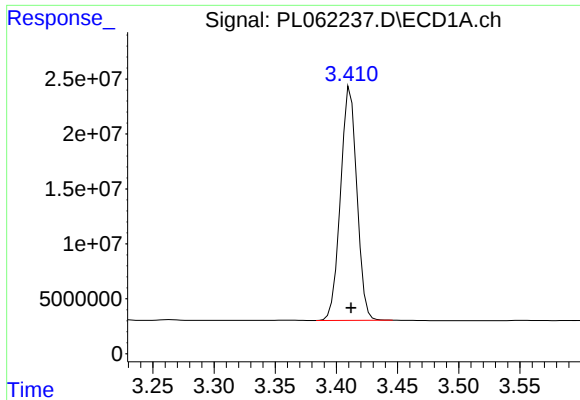

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 197533281
Conc: 99.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

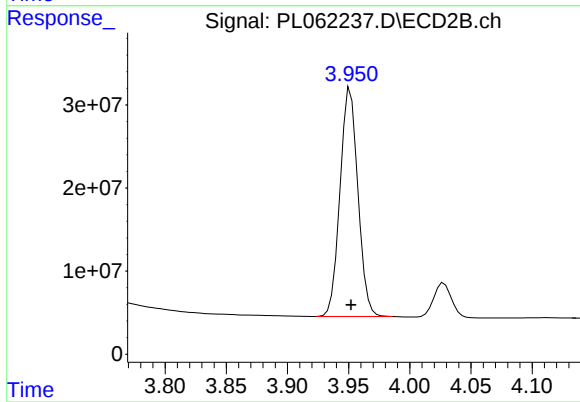


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 279974512
Conc: 99.95 ng/ml

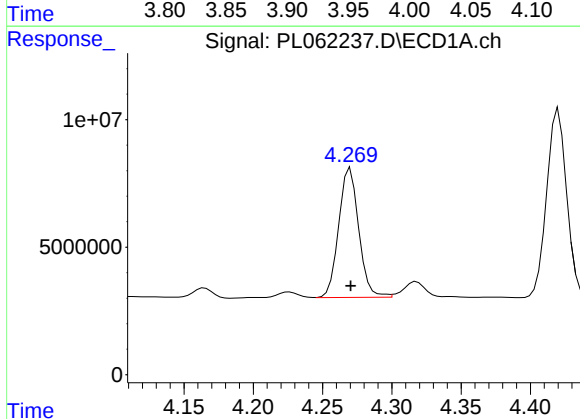


#23 Chlordane-1

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 51009744
Conc: 969.91 ng/ml

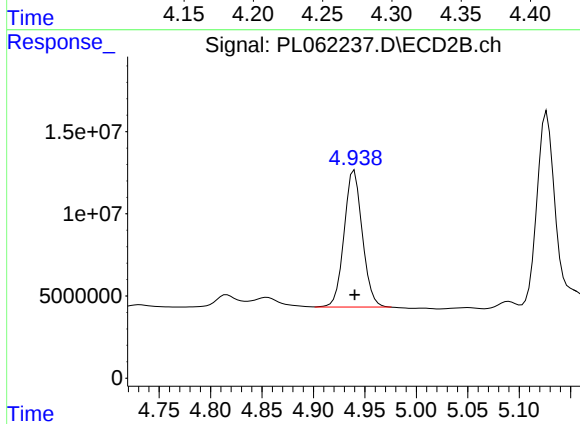

#23 Chlordane-1


R.T.: 4.940 min
Delta R.T.: 0.000 min
Response: 102482505
Conc: 1002.34 ng/ml

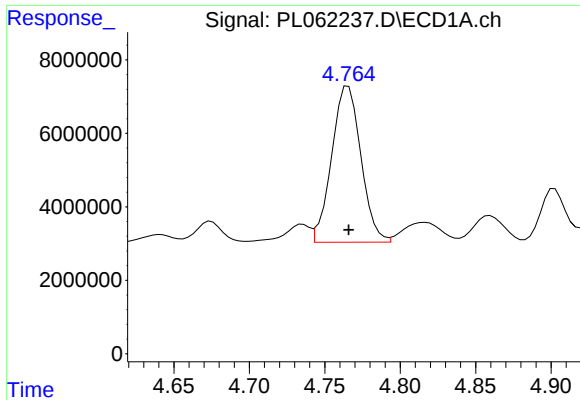

#24 Chlordane-2


R.T.: 4.766 min
Delta R.T.: 0.000 min
Response: 57273661
Conc: 949.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

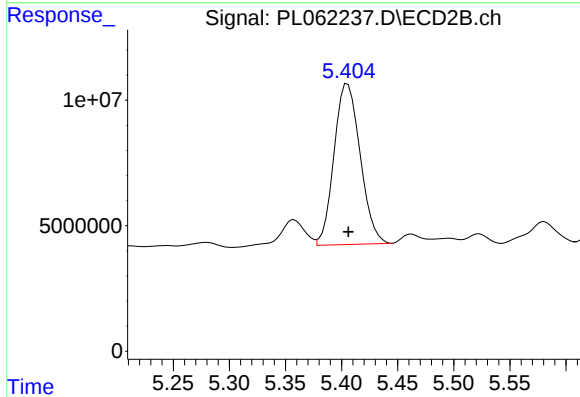


#24 Chlordane-2

R.T.: 5.405 min
Delta R.T.: 0.000 min
Response: 103716463
Conc: 976.36 ng/ml

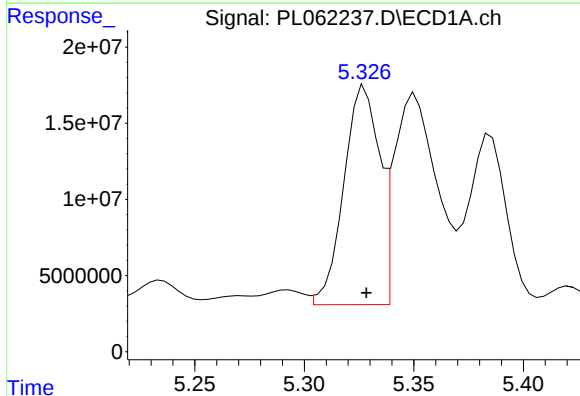


#25 Chlordane-3

R.T.: 5.328 min
Delta R.T.: 0.000 min
Response: 161984505
Conc: 994.55 ng/ml

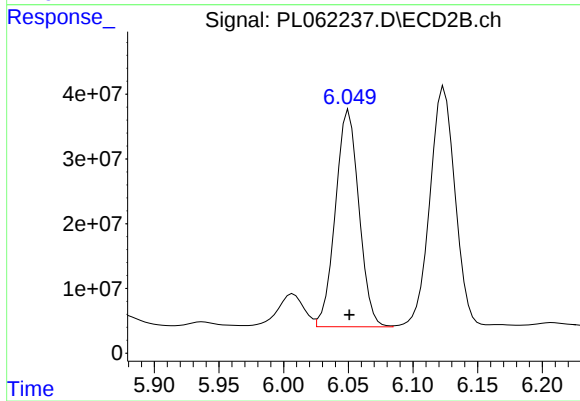

#25 Chlordane-3


R.T.: 6.050 min
Delta R.T.: 0.000 min
Response: 423727790
Conc: 1008.30 ng/ml

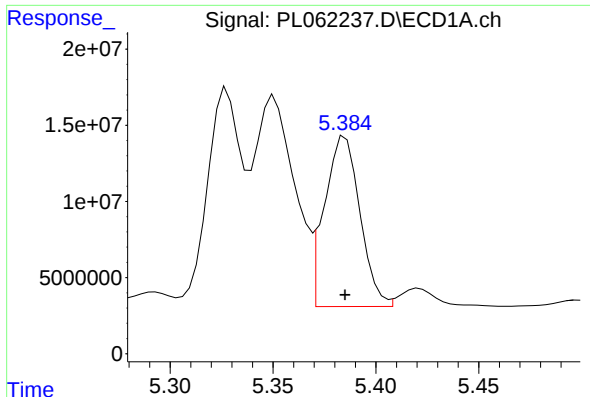

#26 Chlordane-4


R.T.: 5.385 min
Delta R.T.: 0.000 min
Response: 134159924
Conc: 986.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

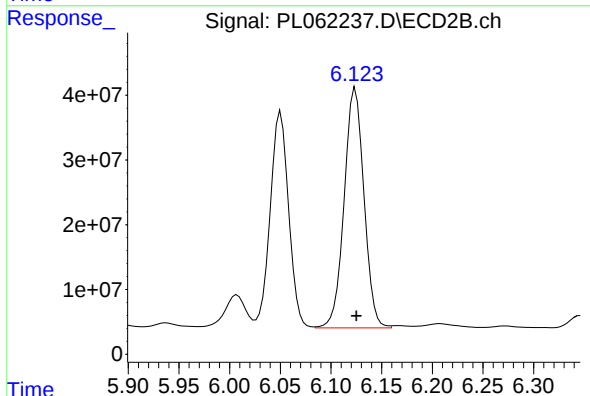


#26 Chlordane-4

R.T.: 6.124 min
Delta R.T.: 0.000 min
Response: 503402703
Conc: 994.03 ng/ml

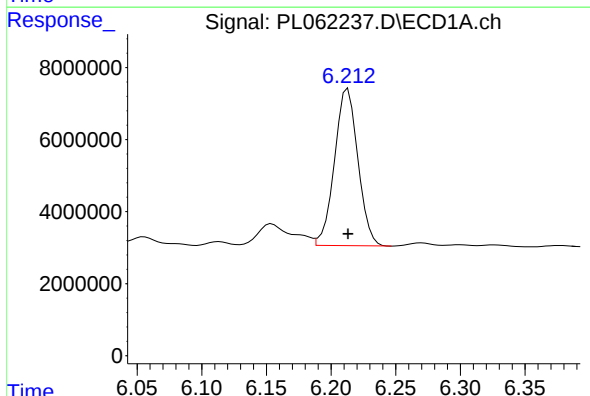


#27 Chlordane-5

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 54804001
Conc: 1004.44 ng/ml

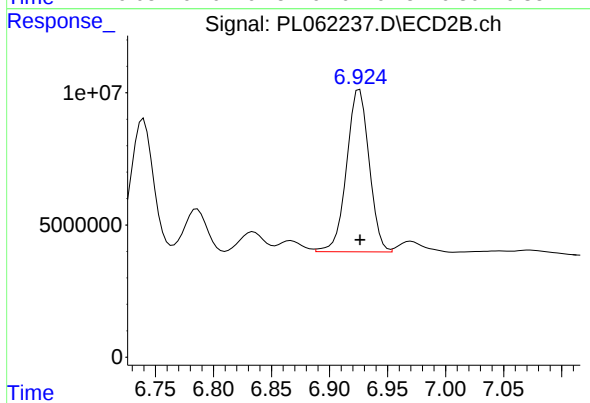

#27 Chlordane-5

R.T.: 6.926 min
Delta R.T.: 0.000 min
Response: 82955155
Conc: 1001.90 ng/ml

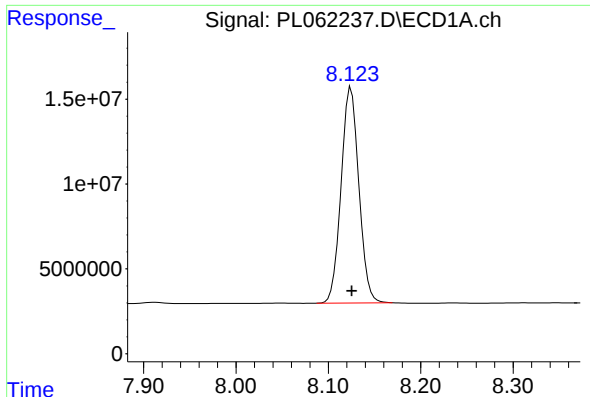

#28 Decachlorobiphenyl


R.T.: 8.125 min

Delta R.T.: 0.000 min

Response: 169935257

Conc: 94.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

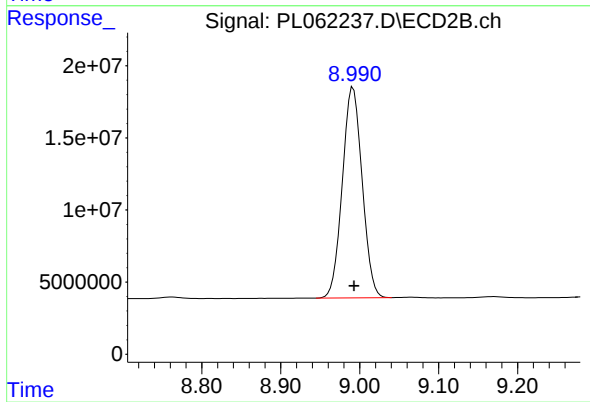

#28 Decachlorobiphenyl

R.T.: 8.992 min

Delta R.T.: -0.001 min

Response: 254858865

Conc: 94.23 ng/ml