

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101320\
 Data File : PL062240.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2020 20:36
 Operator : DD\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 04:20:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 13 04:19:56 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.952	47493267	68374097	23.974	24.408
28)	SA Decachlor...	8.124	8.993	45639929	68312759	25.317	25.256
Target Compounds							
23)	Chlordane-1	4.270	4.939	12571578	24993098	239.038	244.447
24)	Chlordane-2	4.766	5.405	16313097	26583647	270.352	250.251
25)	Chlordane-3	5.328	6.050	37562270	100.5E6	230.625	239.042
26)	Chlordane-4	5.385	6.125	31282882	122.4E6	229.963	241.754
27)	Chlordane-5	6.213	6.926	12947210	18938365	237.295	228.731



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101320\
Data File : PL062240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2020 20:36
Operator : DD\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 04:20:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
Quant Title : GC Extractables
QLast Update : Tue Oct 13 04:19:56 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

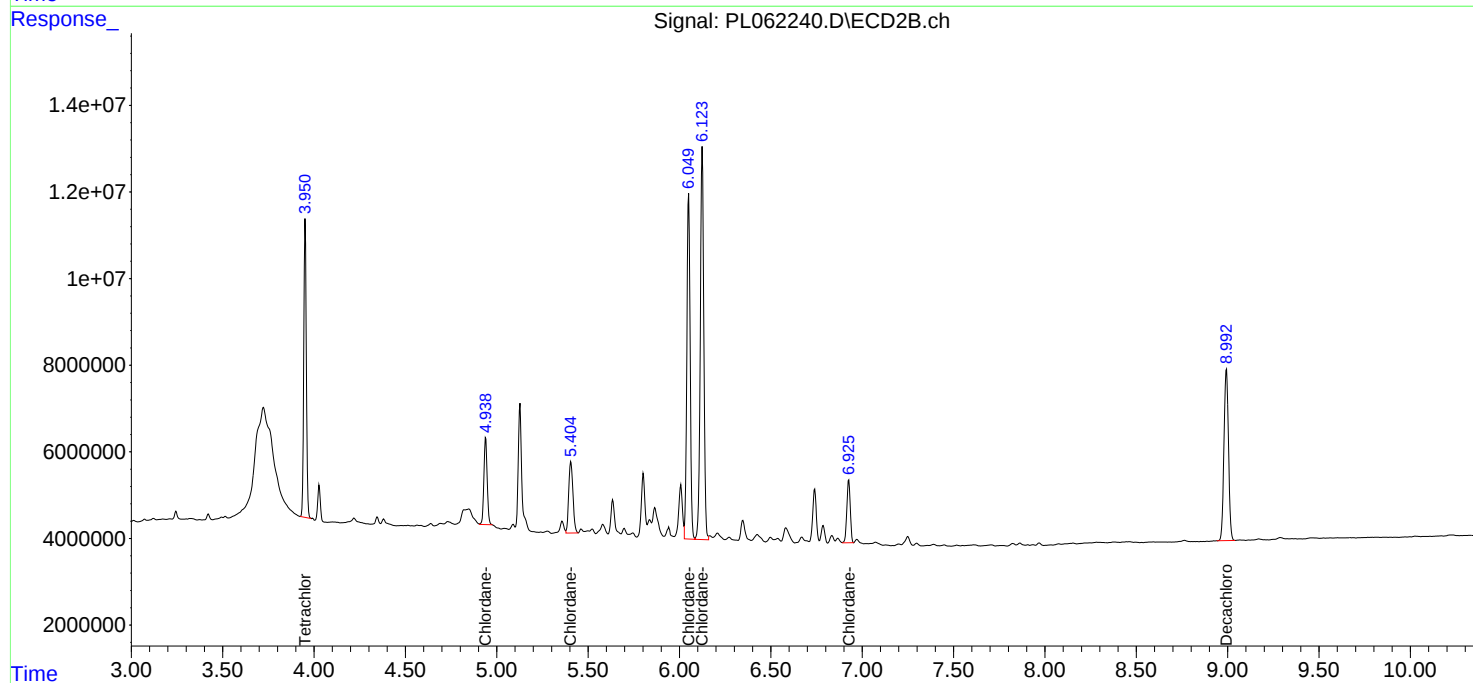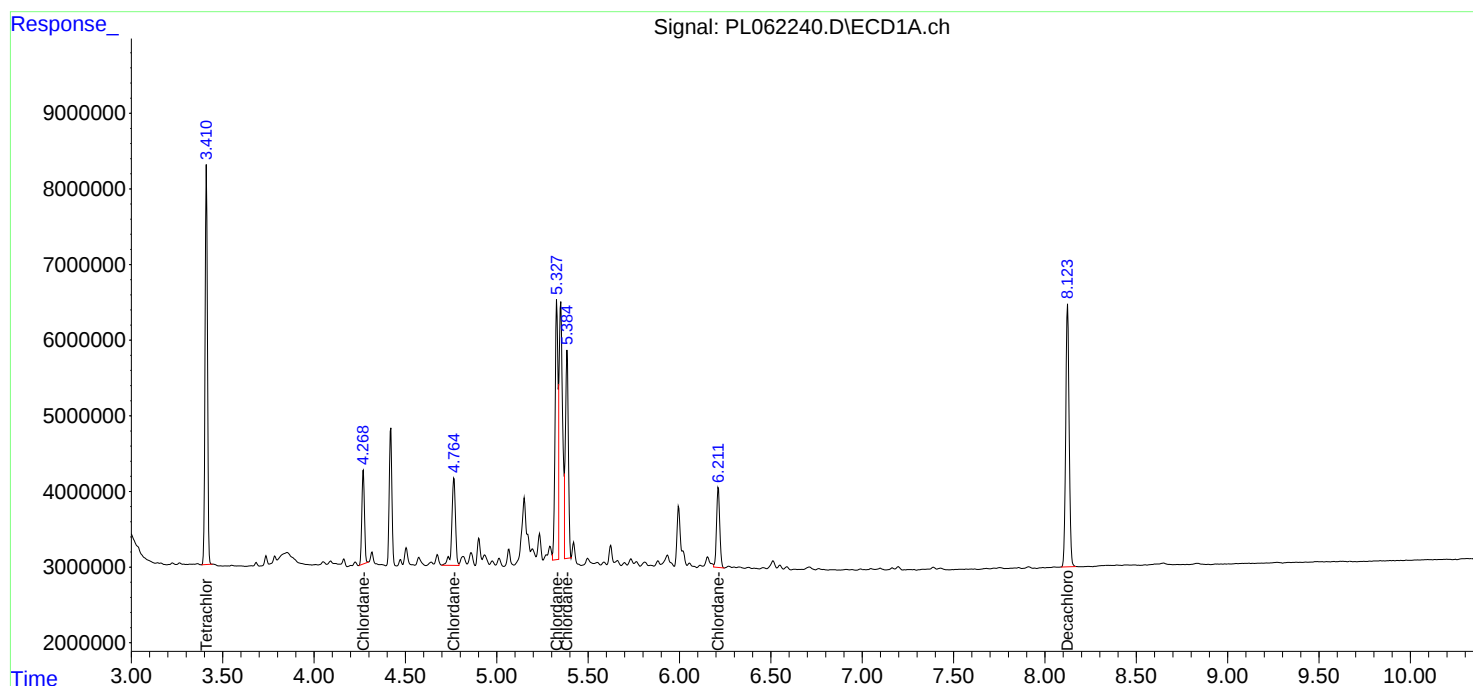


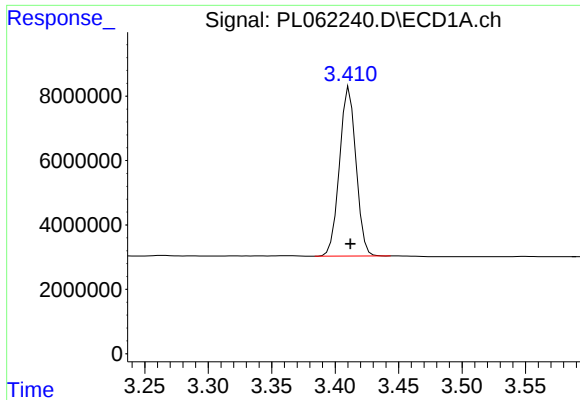

#1 Tetrachloro-m-xylene


R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 47493267
Conc: 23.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

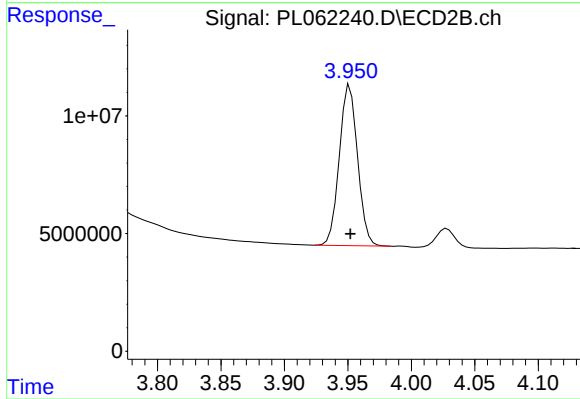


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 68374097
Conc: 24.41 ng/ml

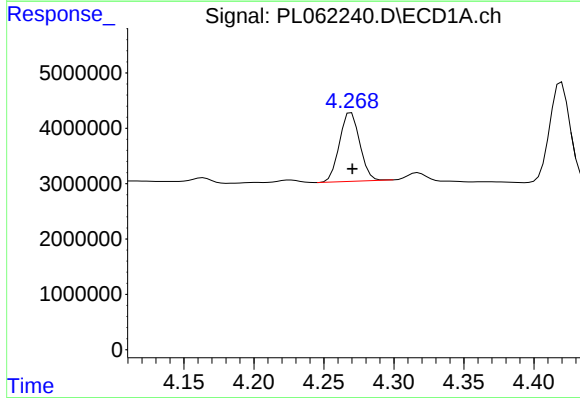


#23 Chlordane-1

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 12571578
Conc: 239.04 ng/ml

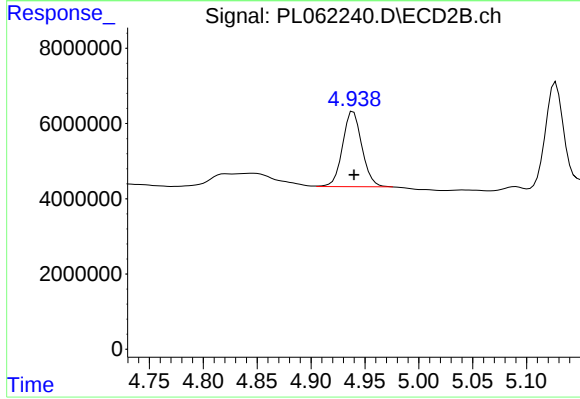

#23 Chlordane-1


R.T.: 4.939 min
Delta R.T.: 0.000 min
Response: 24993098
Conc: 244.45 ng/ml

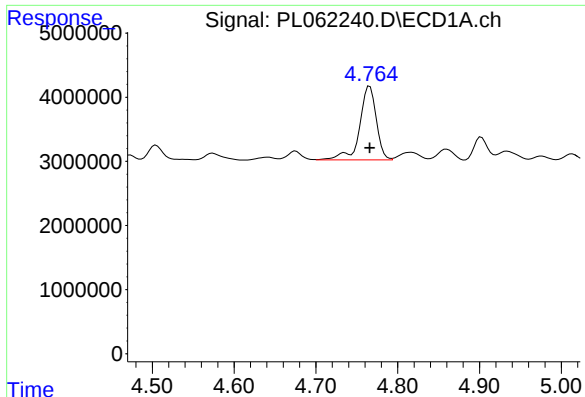

#24 Chlordane-2


R.T.: 4.766 min
Delta R.T.: 0.000 min
Response: 16313097
Conc: 270.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

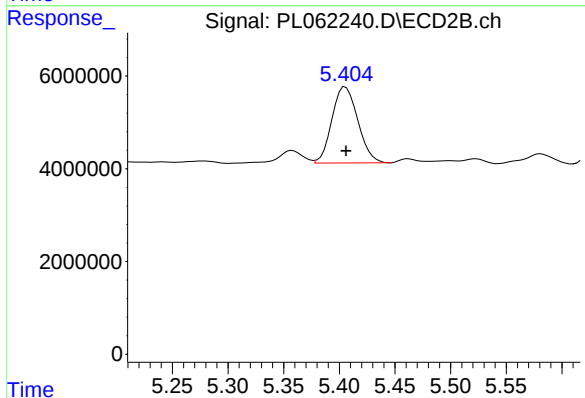


#24 Chlordane-2

R.T.: 5.405 min
Delta R.T.: 0.000 min
Response: 26583647
Conc: 250.25 ng/ml

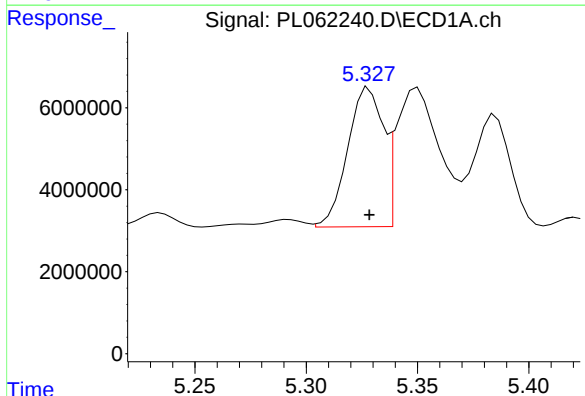


#25 Chlordane-3

R.T.: 5.328 min
Delta R.T.: 0.000 min
Response: 37562270
Conc: 230.62 ng/ml

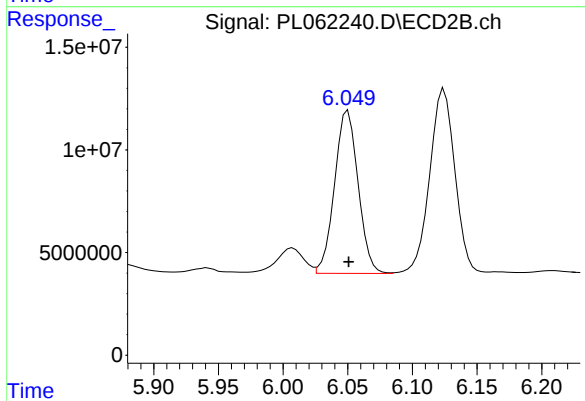

#25 Chlordane-3


R.T.: 6.050 min
Delta R.T.: 0.000 min
Response: 100454732
Conc: 239.04 ng/ml

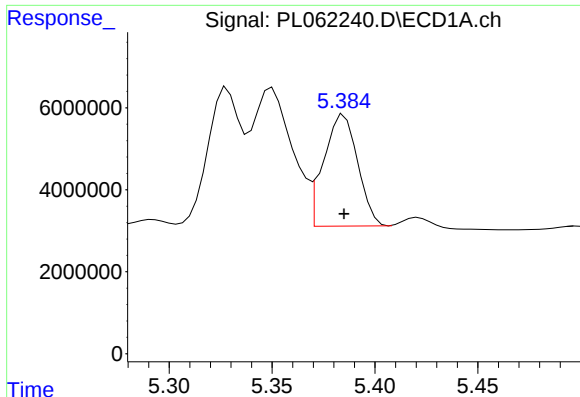

#26 Chlordane-4


R.T.: 5.385 min
Delta R.T.: 0.000 min
Response: 31282882
Conc: 229.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

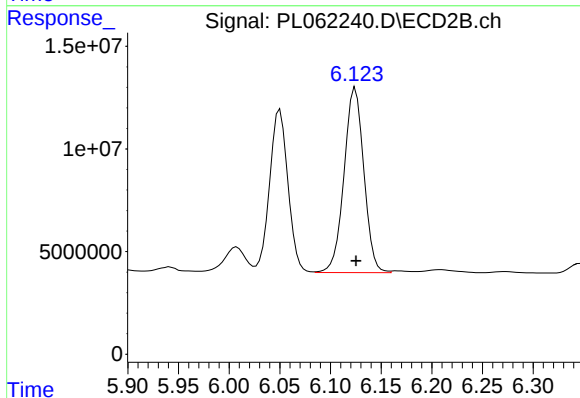


#26 Chlordane-4

R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 122430032
Conc: 241.75 ng/ml

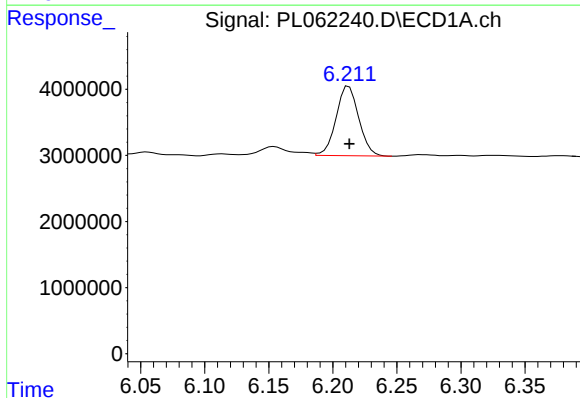


#27 Chlordane-5

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 12947210
Conc: 237.30 ng/ml

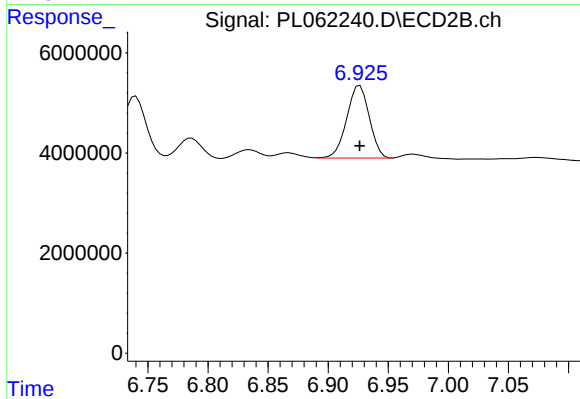

#27 Chlordane-5


R.T.: 6.926 min
Delta R.T.: 0.000 min
Response: 18938365
Conc: 228.73 ng/ml

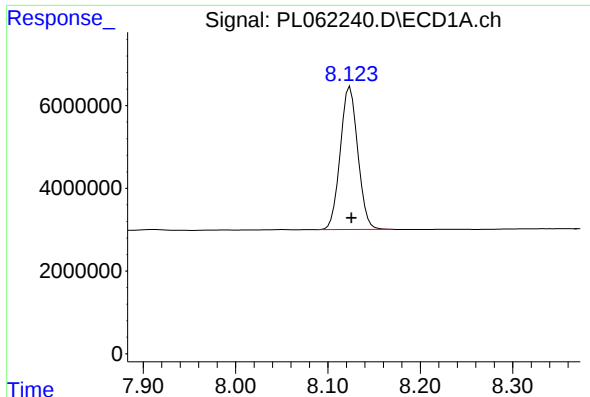

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.001 min
Response: 45639929
Conc: 25.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

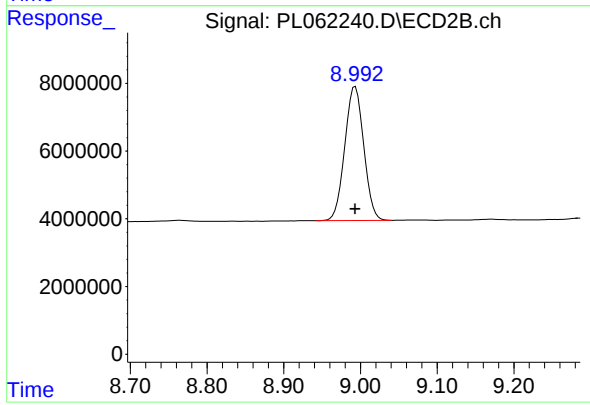

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 68312759
Conc: 25.26 ng/ml