

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101320\
 Data File : PL062241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2020 20:50
 Operator : DD\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 04:21:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 13 04:19:56 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.952	9540341	12937707	4.816	4.619
28)	SA Decachlor...	8.124	8.992	9637117	14153254	5.346	5.233
Target Compounds							
23)	Chlordane-1	4.270	4.939	2287730	4428433	43.499	43.313
24)	Chlordane-2	0.000	5.405	0	5335678	N.D.	50.229 #
25)	Chlordane-3	5.328	6.050	7578972	19028186	46.533	45.279
26)	Chlordane-4	5.385	6.124	6270828	23170332	46.097	45.753
27)	Chlordane-5	0.000	6.926	0	3645591	N.D.	44.030 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101320\
Data File : PL062241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2020 20:50
Operator : DD\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleID :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 04:21:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
Quant Title : GC Extractables
QLast Update : Tue Oct 13 04:19:56 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

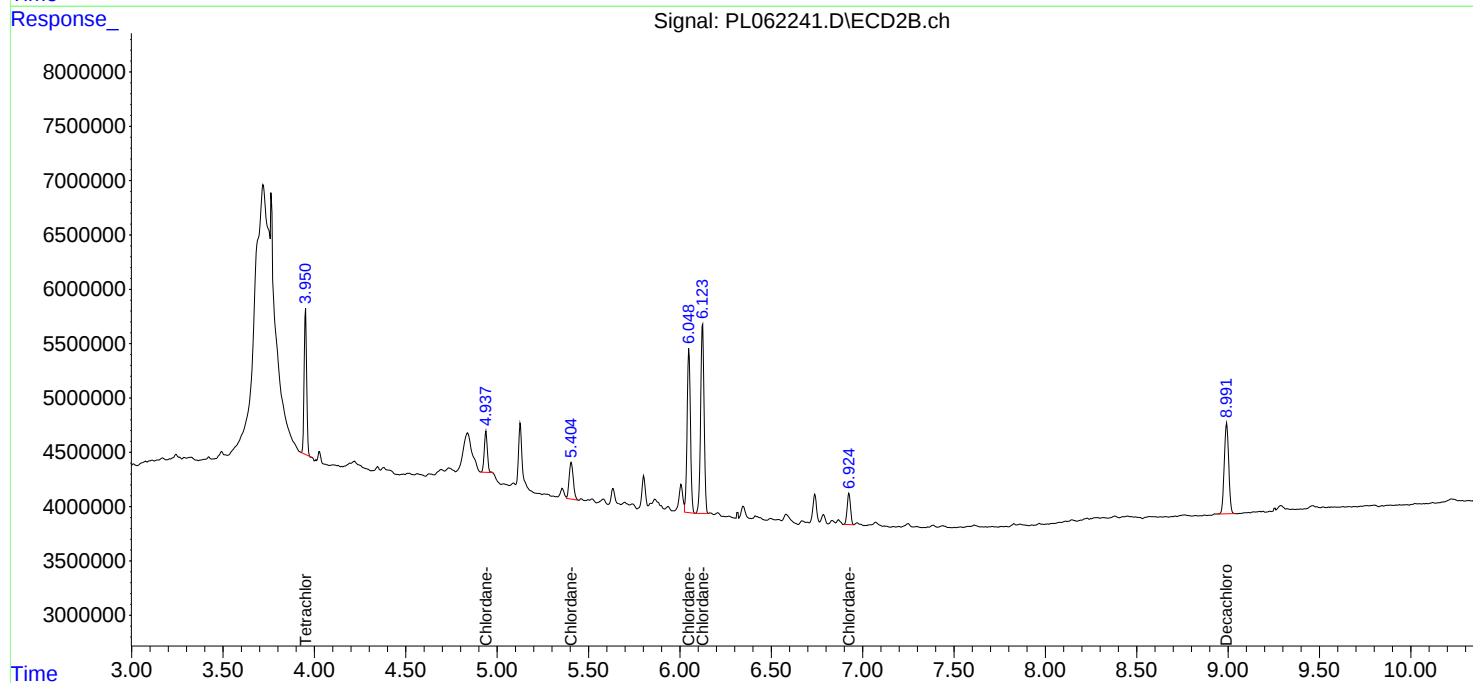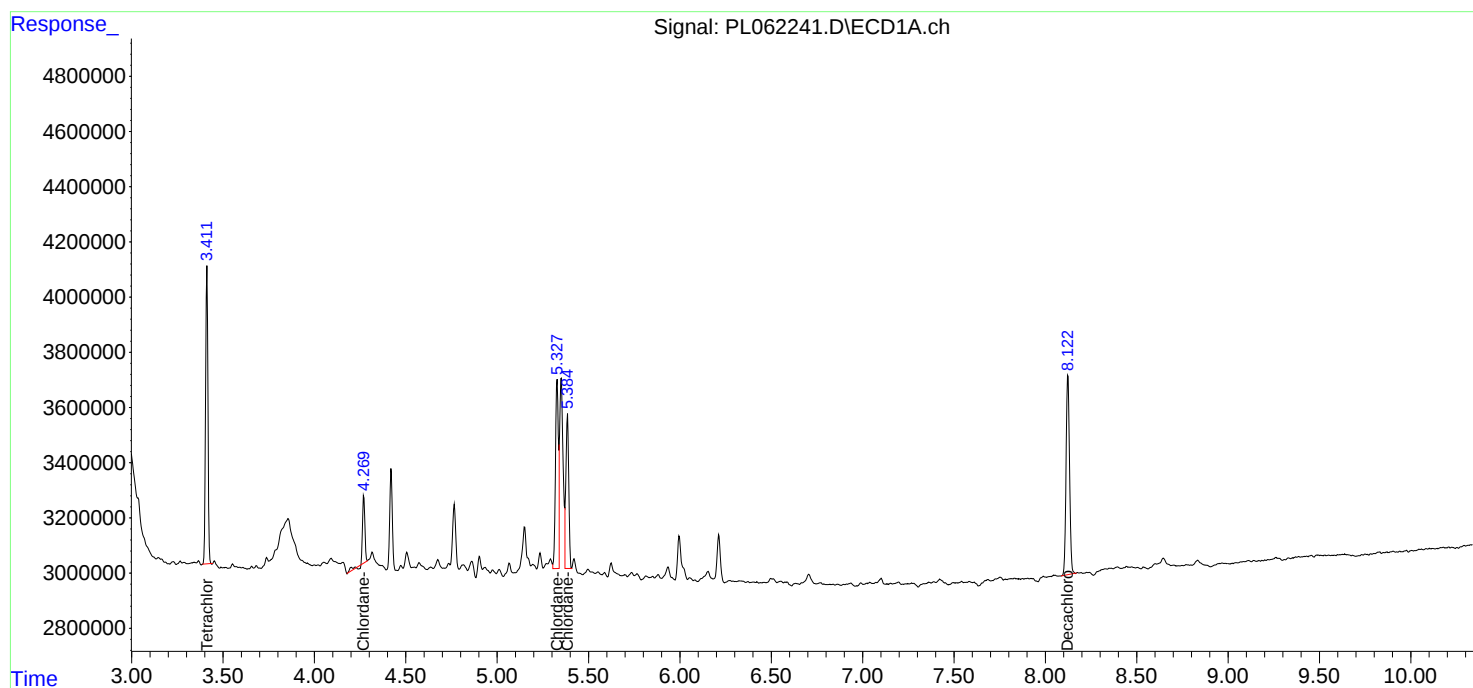


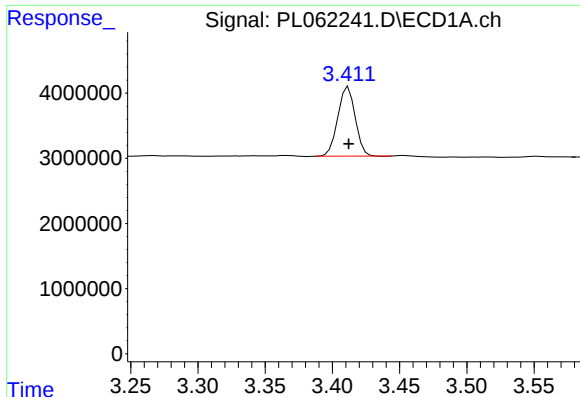

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 9540341
Conc: 4.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

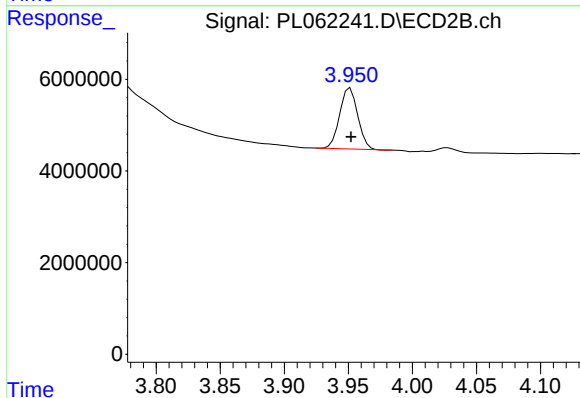


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 12937707
Conc: 4.62 ng/ml

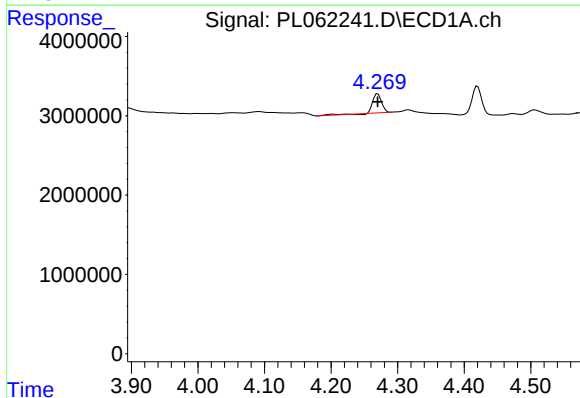


#23 Chlordane-1

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 2287730
Conc: 43.50 ng/ml

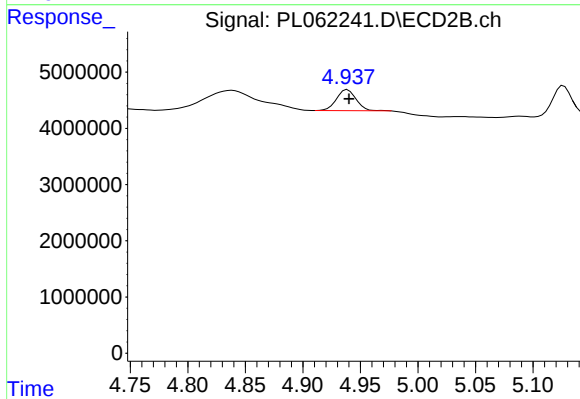

#23 Chlordane-1


R.T.: 4.939 min
Delta R.T.: -0.001 min
Response: 4428433
Conc: 43.31 ng/ml

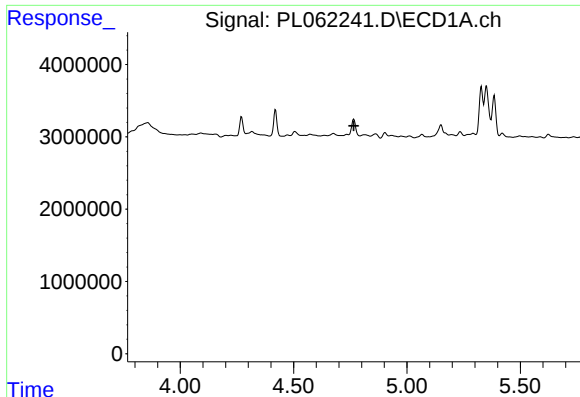

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.766 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

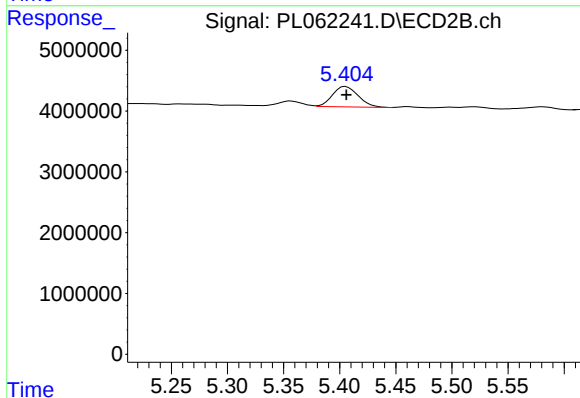


#24 Chlordane-2

R.T.: 5.405 min
Delta R.T.: 0.000 min
Response: 5335678
Conc: 50.23 ng/ml

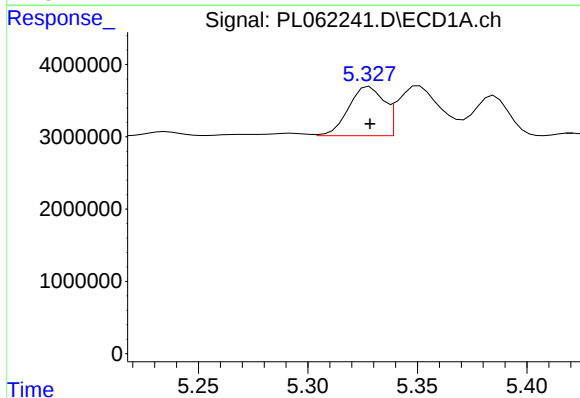


#25 Chlordane-3

R.T.: 5.328 min
Delta R.T.: 0.000 min
Response: 7578972
Conc: 46.53 ng/ml

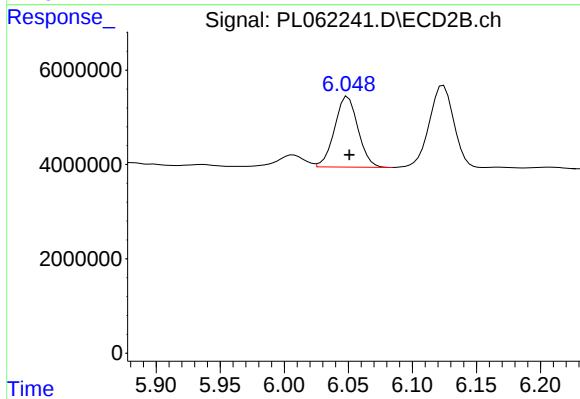

#25 Chlordane-3


R.T.: 6.050 min
Delta R.T.: -0.001 min
Response: 19028186
Conc: 45.28 ng/ml

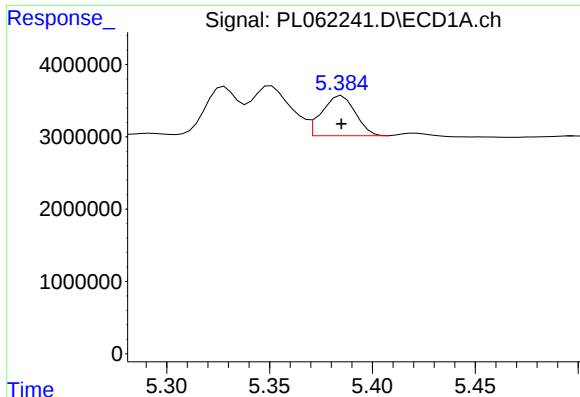

#26 Chlordane-4


R.T.: 5.385 min
Delta R.T.: 0.000 min
Response: 6270828
Conc: 46.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

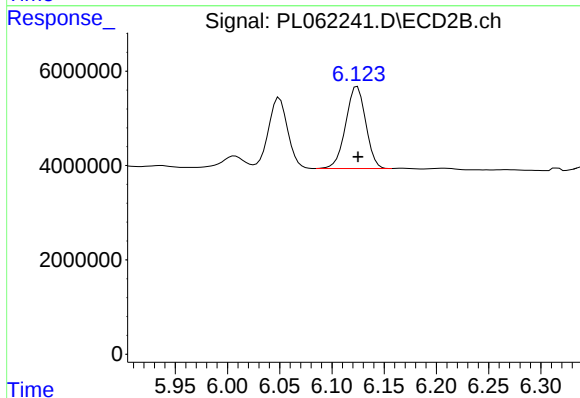


#26 Chlordane-4

R.T.: 6.124 min
Delta R.T.: 0.000 min
Response: 23170332
Conc: 45.75 ng/ml

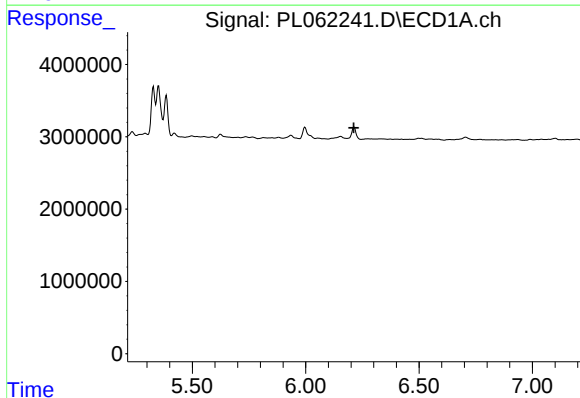


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.213 min
Response: 0
Conc: N.D.

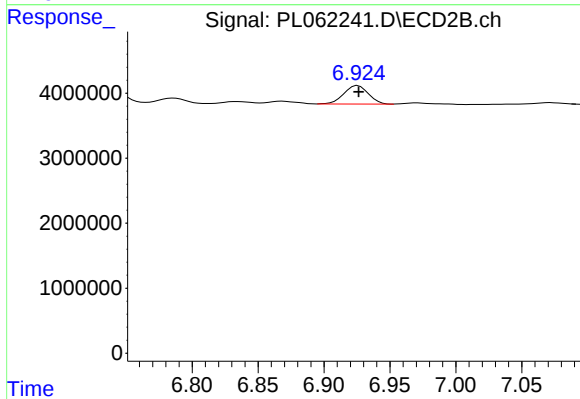

#27 Chlordane-5


R.T.: 6.926 min
Delta R.T.: 0.000 min
Response: 3645591
Conc: 44.03 ng/ml

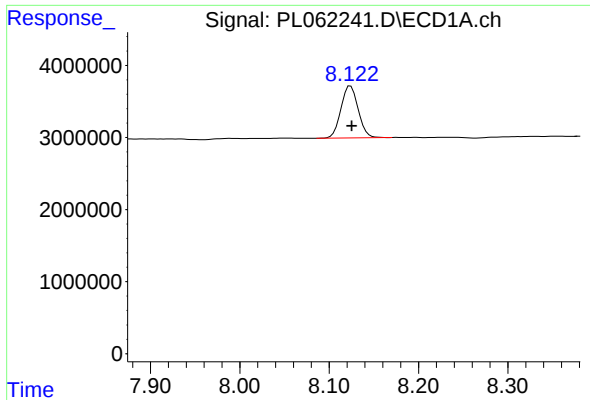

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.001 min
Response: 9637117
Conc: 5.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

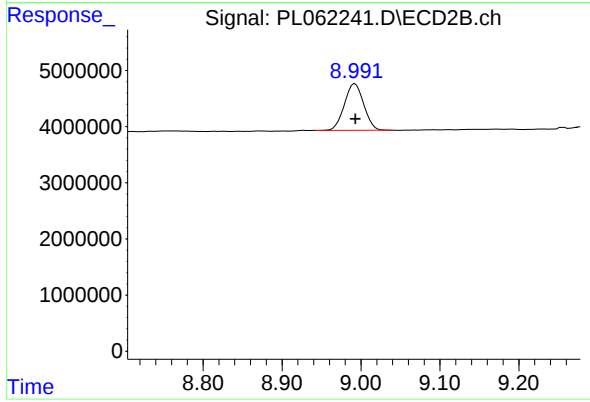

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 14153254
Conc: 5.23 ng/ml