

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101323\
 Data File : PL085921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2023 19:12
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 01:25:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.356	2.622	136.9E6	50727785	46.030	54.306
28)	SA Decachlor...	8.859	7.776	117.5E6	49559932	53.960	53.695
Target Compounds							
23)	Chlordane-1	4.514	3.612	61629016	15442247	512.660	473.705
24)	Chlordane-2	5.045	4.190	65297101	20913398	502.116	537.429
25)	Chlordane-3	5.757	4.818	250.0E6	54939826	489.989	543.702
26)	Chlordane-4	5.840	4.880	307.0E6	58519911	483.889	505.423
27)	Chlordane-5	6.688	5.550	49829087	14555368	485.717	522.233



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101323\
Data File : PL085921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2023 19:12
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 01:25:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

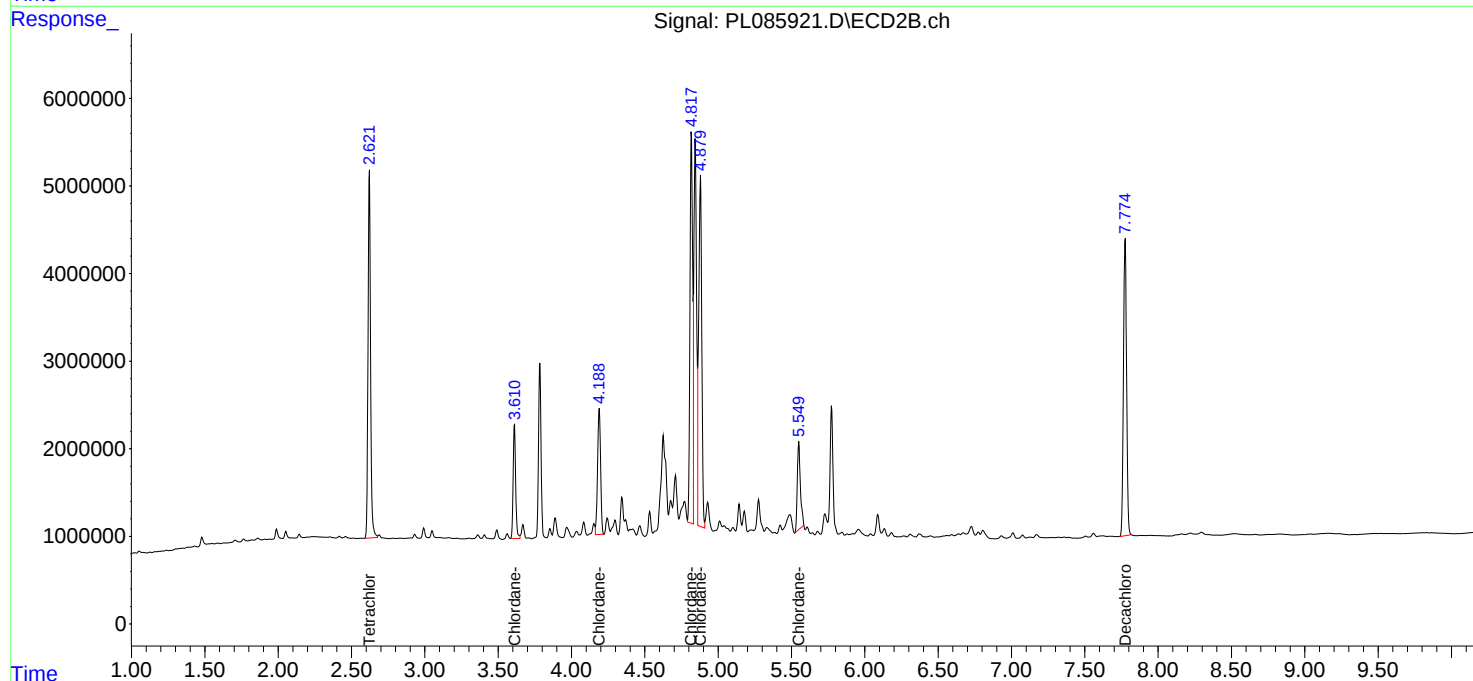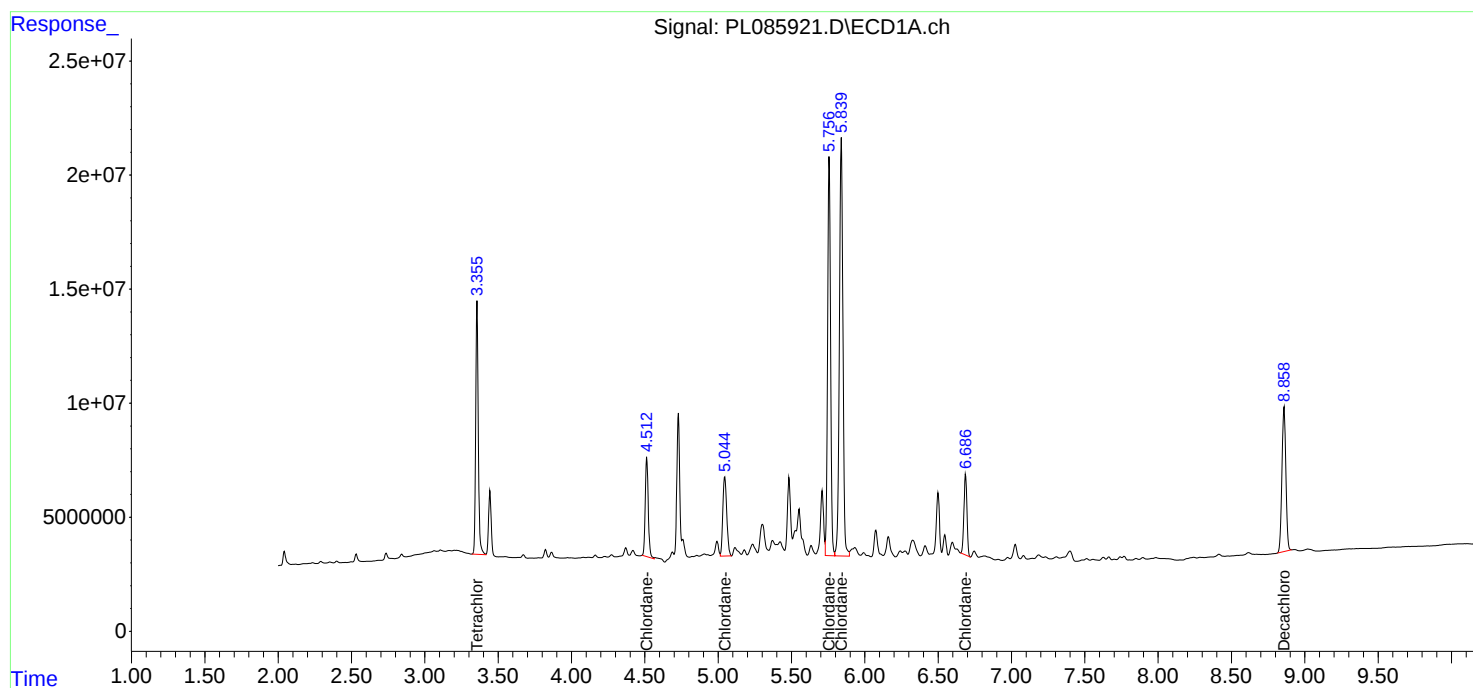


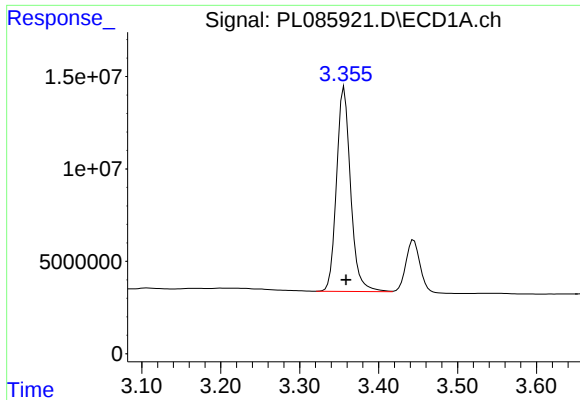

#1 Tetrachloro-m-xylene


R.T.: 3.356 min
Delta R.T.: -0.003 min
Response: 136899840
Conc: 46.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

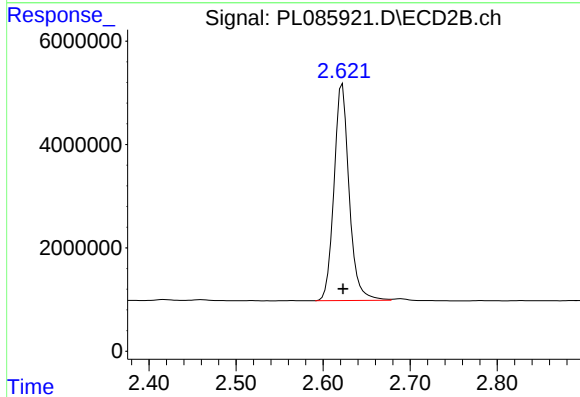


#1 Tetrachloro-m-xylene

R.T.: 2.622 min
Delta R.T.: 0.000 min
Response: 50727785
Conc: 54.31 ng/ml

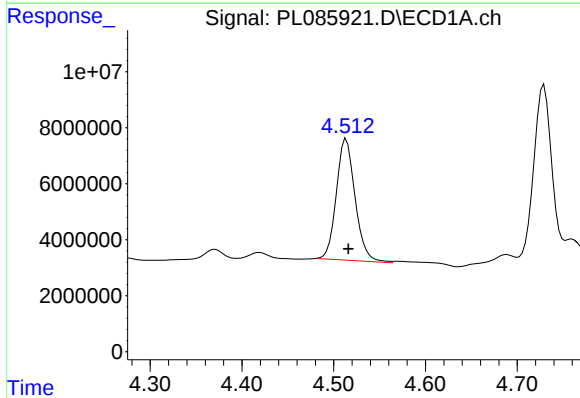


#23 Chlordane-1

R.T.: 4.514 min
Delta R.T.: -0.002 min
Response: 61629016
Conc: 512.66 ng/ml

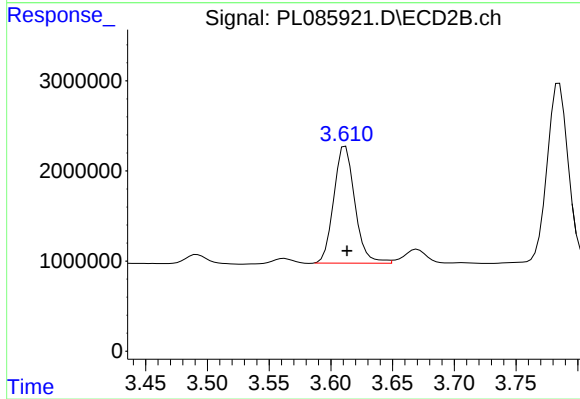

#23 Chlordane-1


R.T.: 3.612 min
Delta R.T.: -0.001 min
Response: 15442247
Conc: 473.70 ng/ml

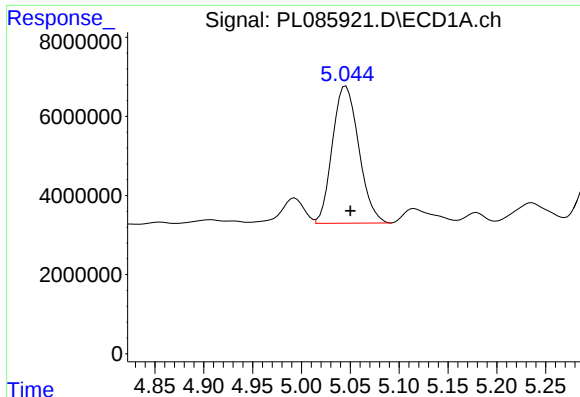

#24 Chlordane-2


R.T.: 5.045 min
Delta R.T.: -0.005 min
Response: 65297101
Conc: 502.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

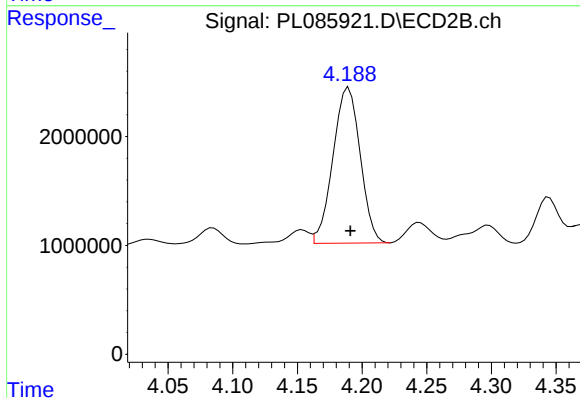


#24 Chlordane-2

R.T.: 4.190 min
Delta R.T.: -0.001 min
Response: 20913398
Conc: 537.43 ng/ml

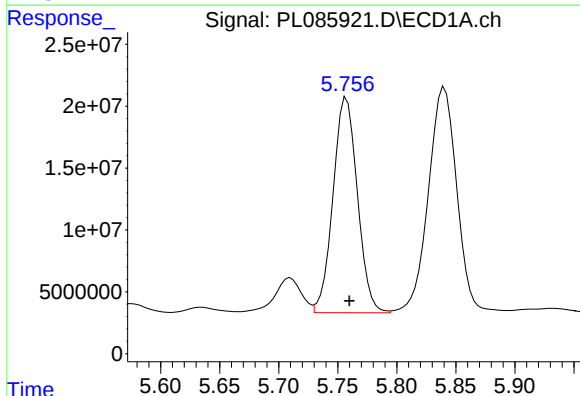


#25 Chlordane-3

R.T.: 5.757 min
Delta R.T.: -0.003 min
Response: 249993015
Conc: 489.99 ng/ml

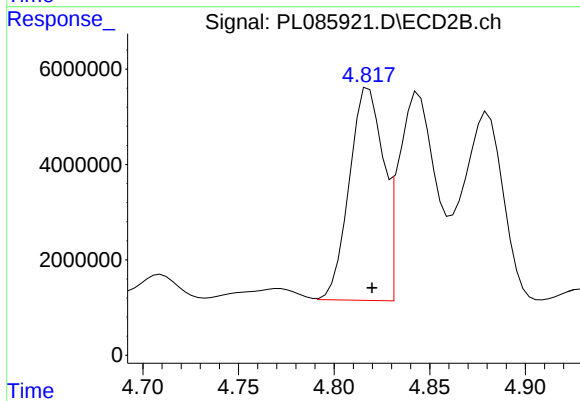

#25 Chlordane-3


R.T.: 4.818 min
Delta R.T.: -0.002 min
Response: 54939826
Conc: 543.70 ng/ml

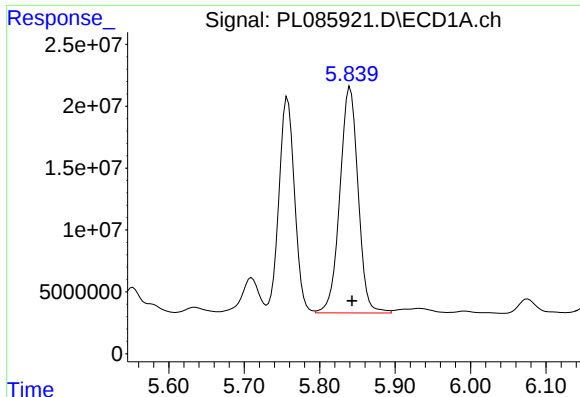

#26 Chlordane-4


R.T.: 5.840 min
Delta R.T.: -0.003 min
Response: 306998965
Conc: 483.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

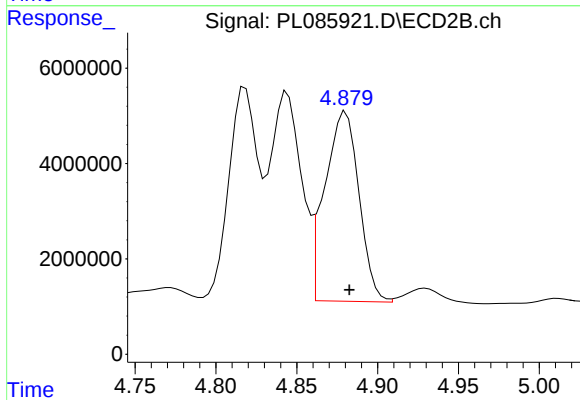


#26 Chlordane-4

R.T.: 4.880 min
Delta R.T.: -0.002 min
Response: 58519911
Conc: 505.42 ng/ml

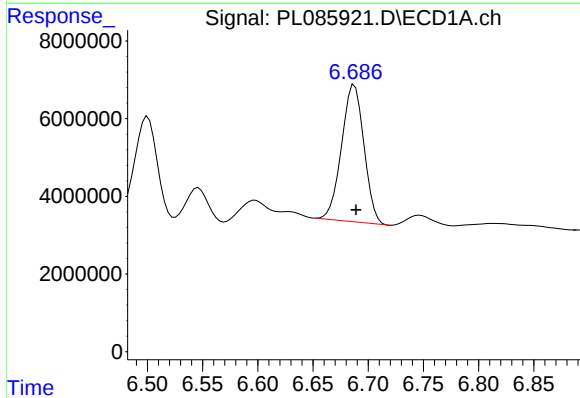


#27 Chlordane-5

R.T.: 6.688 min
Delta R.T.: -0.001 min
Response: 49829087
Conc: 485.72 ng/ml

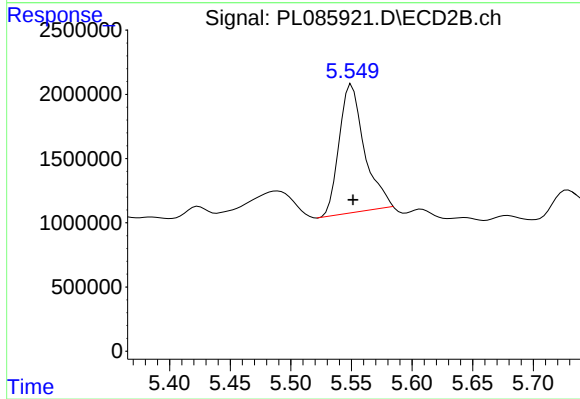

#27 Chlordane-5


R.T.: 5.550 min
Delta R.T.: -0.001 min
Response: 14555368
Conc: 522.23 ng/ml

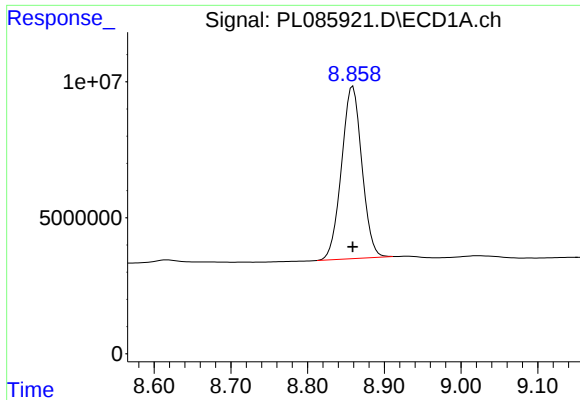

#28 Decachlorobiphenyl

R.T.: 8.859 min
Delta R.T.: 0.000 min
Response: 117528685
Conc: 53.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

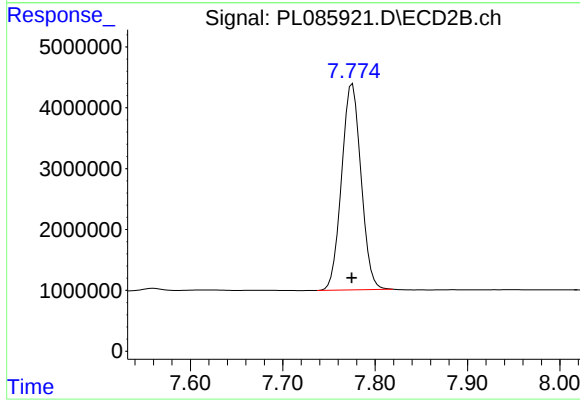

#28 Decachlorobiphenyl

R.T.: 7.776 min
Delta R.T.: 0.000 min
Response: 49559932
Conc: 53.70 ng/ml