

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101325\
 Data File : PL097629.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2025 16:40
 Operator : AR\AJ
 Sample : Q3323-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SED-05-0-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 03:13:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 07 16:47:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.525	2.823	41812889	58759644	10.256	9.654
28)	SA Decachlor...	8.997	7.981	30880749	43090889	10.385	8.304
Target Compounds							
5)	MB Aldrin	5.251f	0.000	19842829	0	3.300	N.D. #
8)	B Heptachlo...	5.642	0.000	8283805	0	1.423	N.D. #
9)	A Endosulfan I	0.000	5.174	0	8617366	N.D.	1.169 #
11)	B alpha-Chl...	5.955f	0.000	2617618	0	0.482	N.D. #
12)	B 4,4'-DDE	6.164	0.000	8519645	0	1.829	N.D. #
23)	Chlordane-1	0.000	3.825	0	13918529	N.D.	54.786 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101325\
Data File : PL097629.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2025 16:40
Operator : AR\AJ
Sample : Q3323-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SED-05-0-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 03:13:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
Quant Title : GC Extractables
QLast Update : Tue Oct 07 16:47:00 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

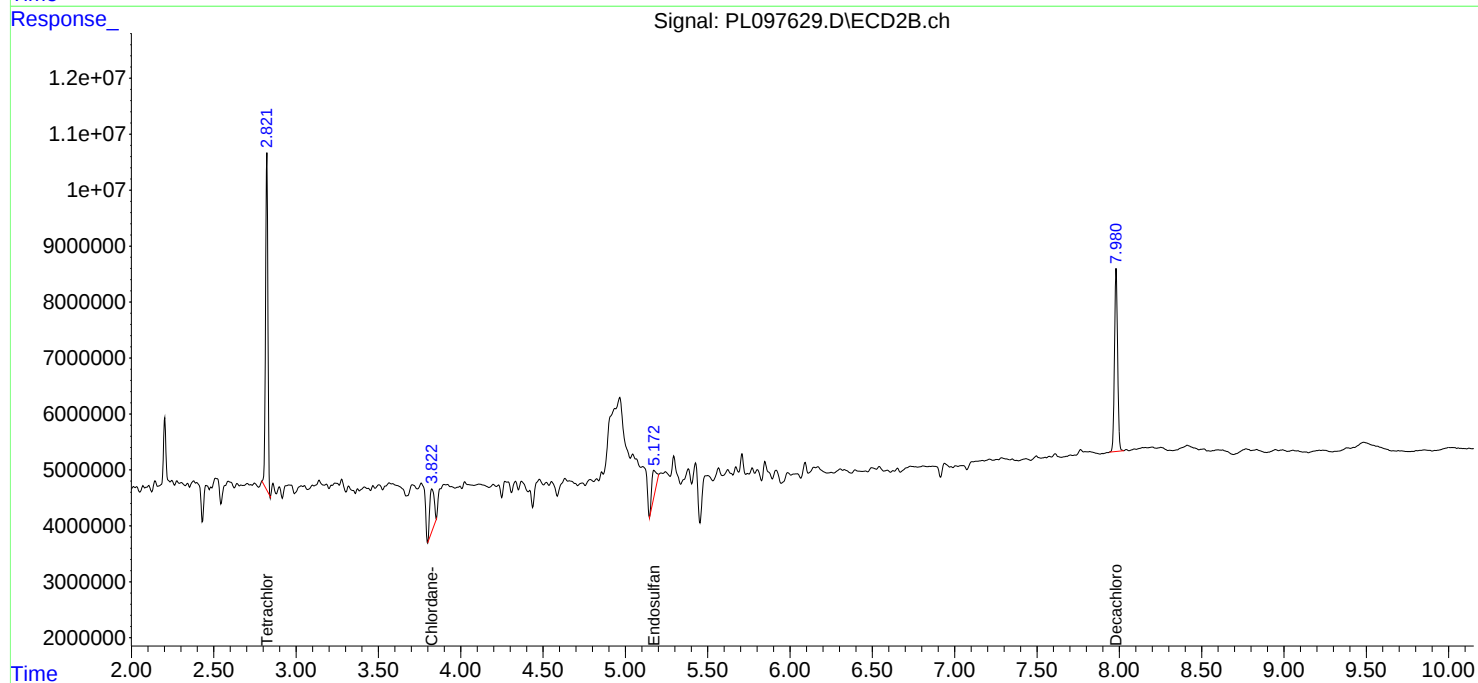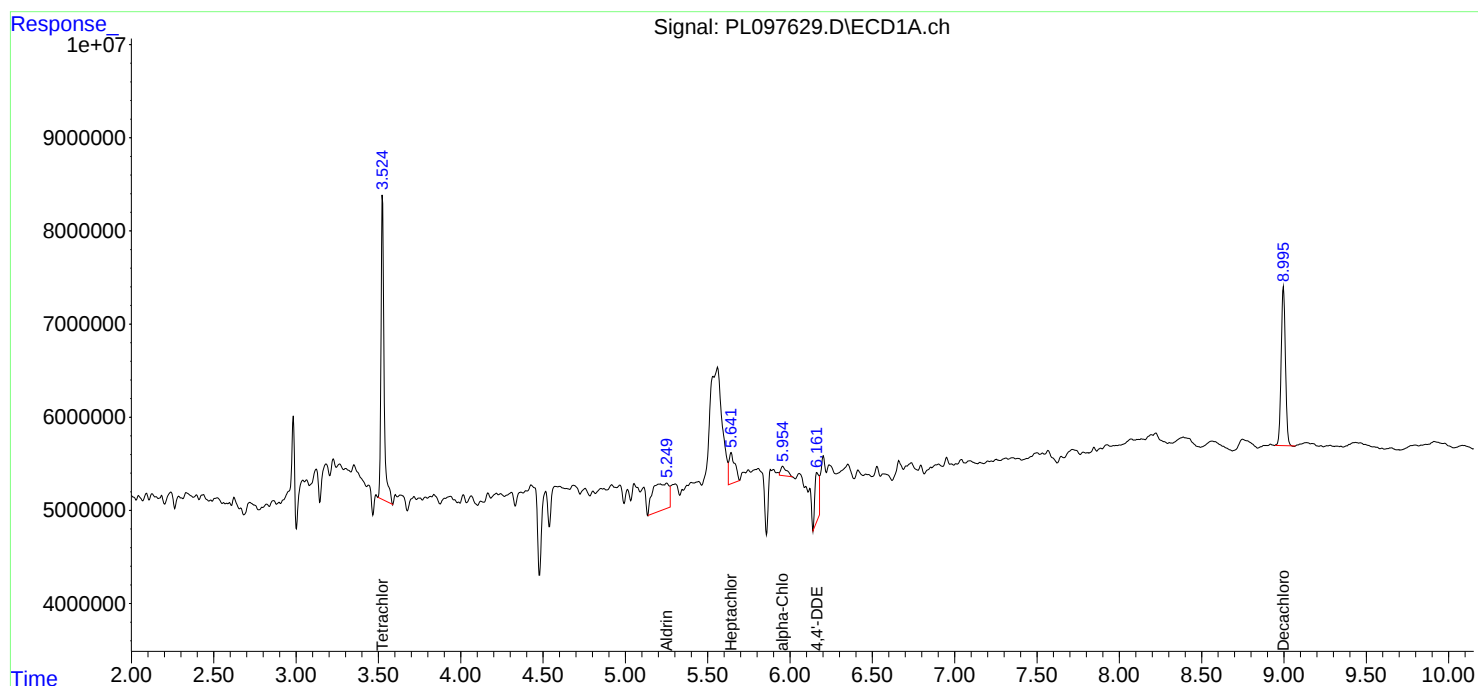


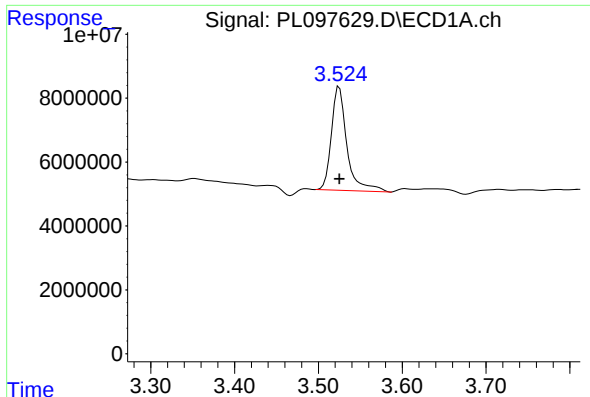

#1 Tetrachloro-m-xylene


R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 41812889
Conc: 10.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
SED-05-0-2

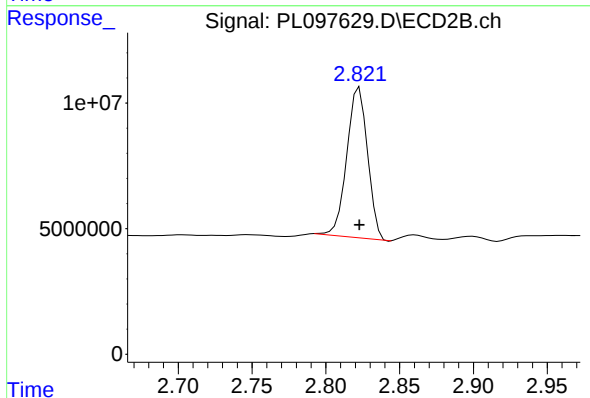


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 58759644
Conc: 9.65 ng/ml

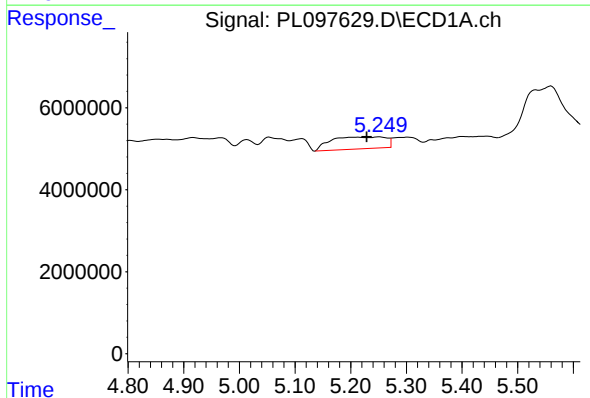


#5 Aldrin

R.T.: 5.251 min
Delta R.T.: 0.023 min
Response: 19842829
Conc: 3.30 ng/ml

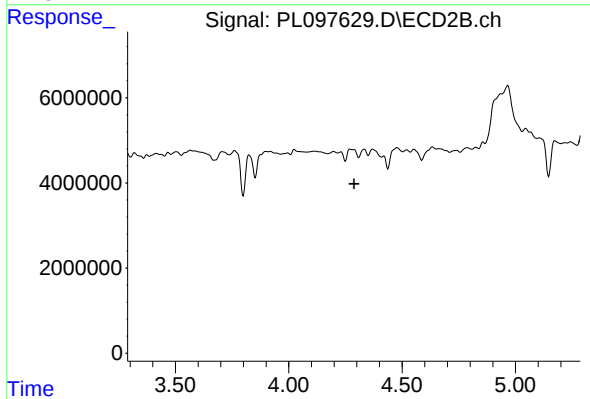

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.288 min
Response: 0
Conc: N.D.

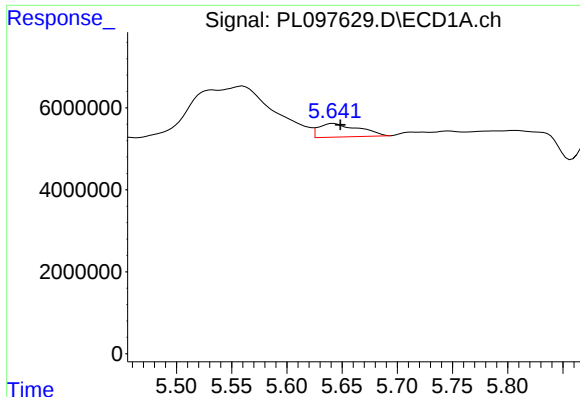

#8 Heptachlor epoxide


R.T.: 5.642 min
Delta R.T.: -0.006 min
Response: 8283805
Conc: 1.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
SED-05-0-2

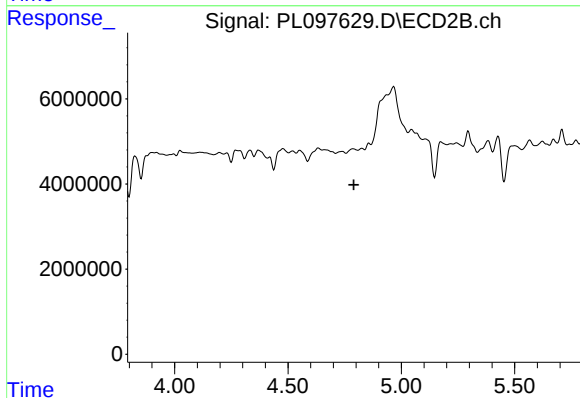


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.790 min
Response: 0
Conc: N.D.

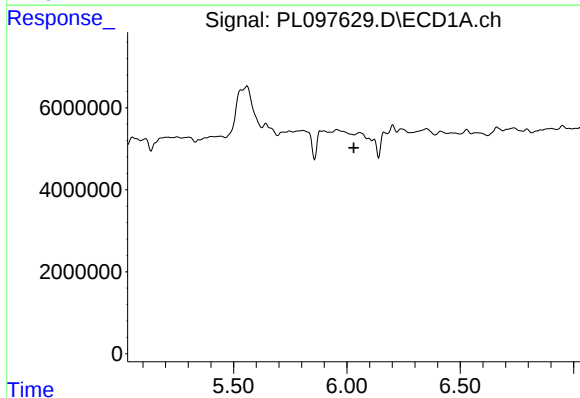


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.030 min
Response: 0
Conc: N.D.

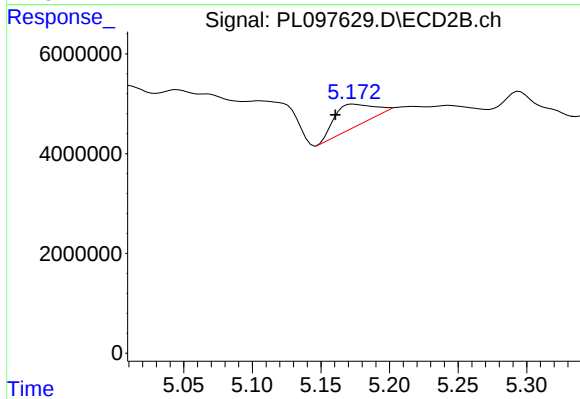

#9 Endosulfan I


R.T.: 5.174 min
Delta R.T.: 0.013 min
Response: 8617366
Conc: 1.17 ng/ml

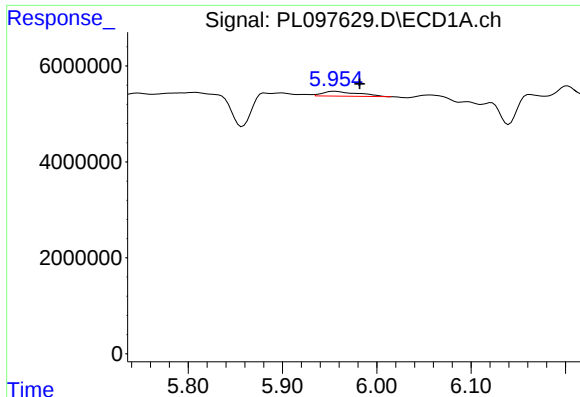

#11 alpha-Chlordane


R.T.: 5.955 min
Delta R.T.: -0.027 min
Response: 2617618
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
SED-05-0-2

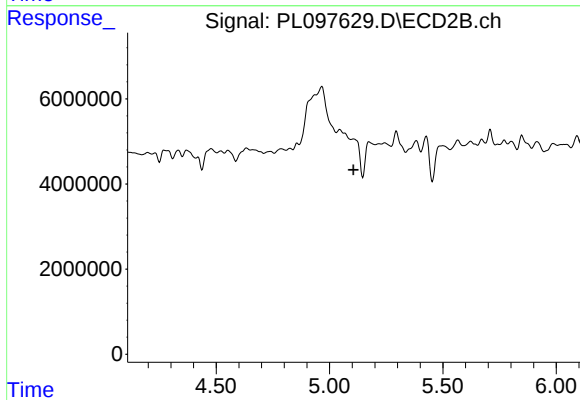


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.106 min
Response: 0
Conc: N.D.

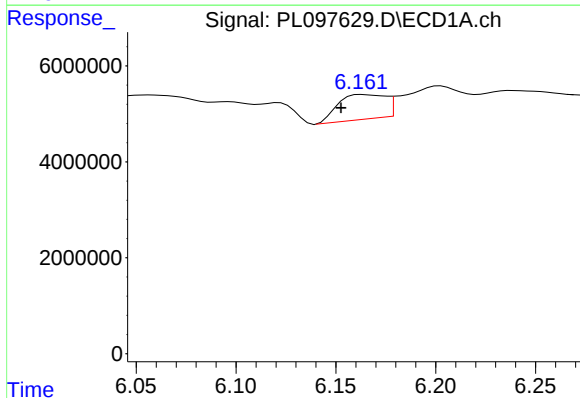


#12 4,4'-DDE

R.T.: 6.164 min
Delta R.T.: 0.011 min
Response: 8519645
Conc: 1.83 ng/ml

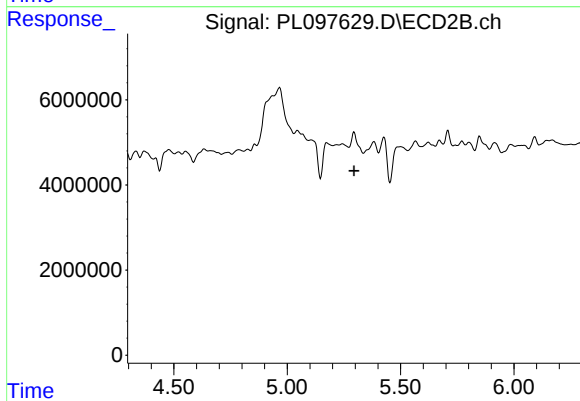

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 5.295 min
Response: 0
Conc: N.D.

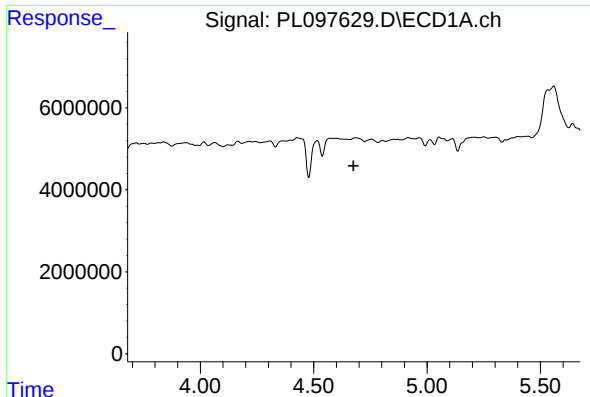

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.676 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SED-05-0-2

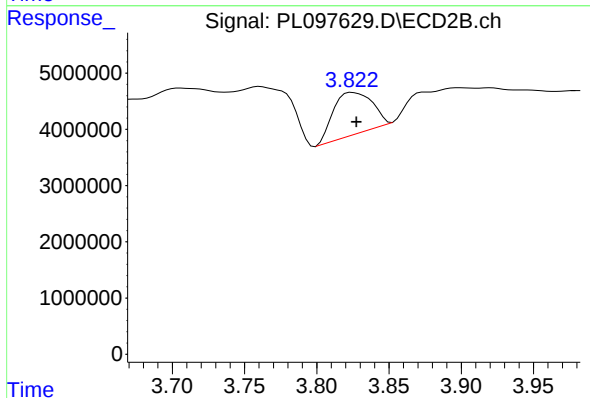


#23 Chlordane-1

R.T.: 3.825 min
Delta R.T.: -0.002 min
Response: 13918529
Conc: 54.79 ng/ml

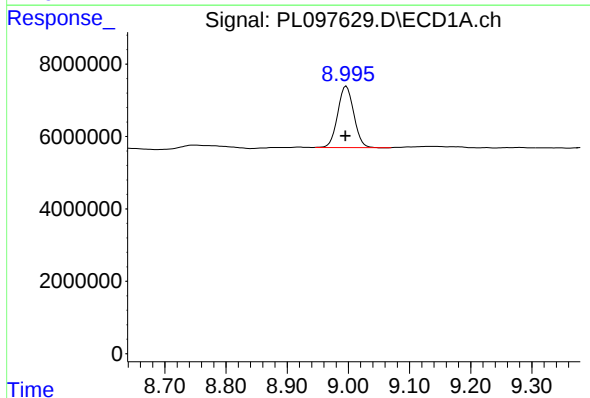

#28 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.001 min
Response: 30880749
Conc: 10.38 ng/ml

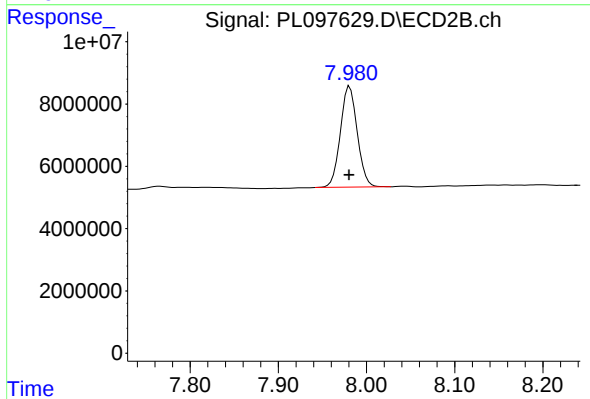

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: 0.000 min
Response: 43090889
Conc: 8.30 ng/ml