

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101325\
 Data File : PL097630.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2025 16:53
 Operator : AR\AJ
 Sample : Q3323-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SED-06-0-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 03:13:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 07 16:47:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.525	2.822	102.0E6	96025206	25.012	15.777 #
28)	SA Decachlor...	8.996	7.981	26893816	41907936	9.044	8.076
Target Compounds							
3)	MA gamma-BHC...	0.000	3.663	0	6651345	N.D.	0.724 #
9)	A Endosulfan I	0.000	5.182f	0	19447931	N.D.	2.637 #
13)	MA Dieldrin	0.000	5.427	0	14249108	N.D.	1.723 #
20)	A Methoxychlor	0.000	6.698f	0	9241787	N.D.	2.535 #
23)	Chlordane-1	0.000	3.832	0	6290150	N.D.	24.759 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101325\
Data File : PL097630.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2025 16:53
Operator : AR\AJ
Sample : Q3323-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SED-06-0-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 03:13:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
Quant Title : GC Extractables
QLast Update : Tue Oct 07 16:47:00 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

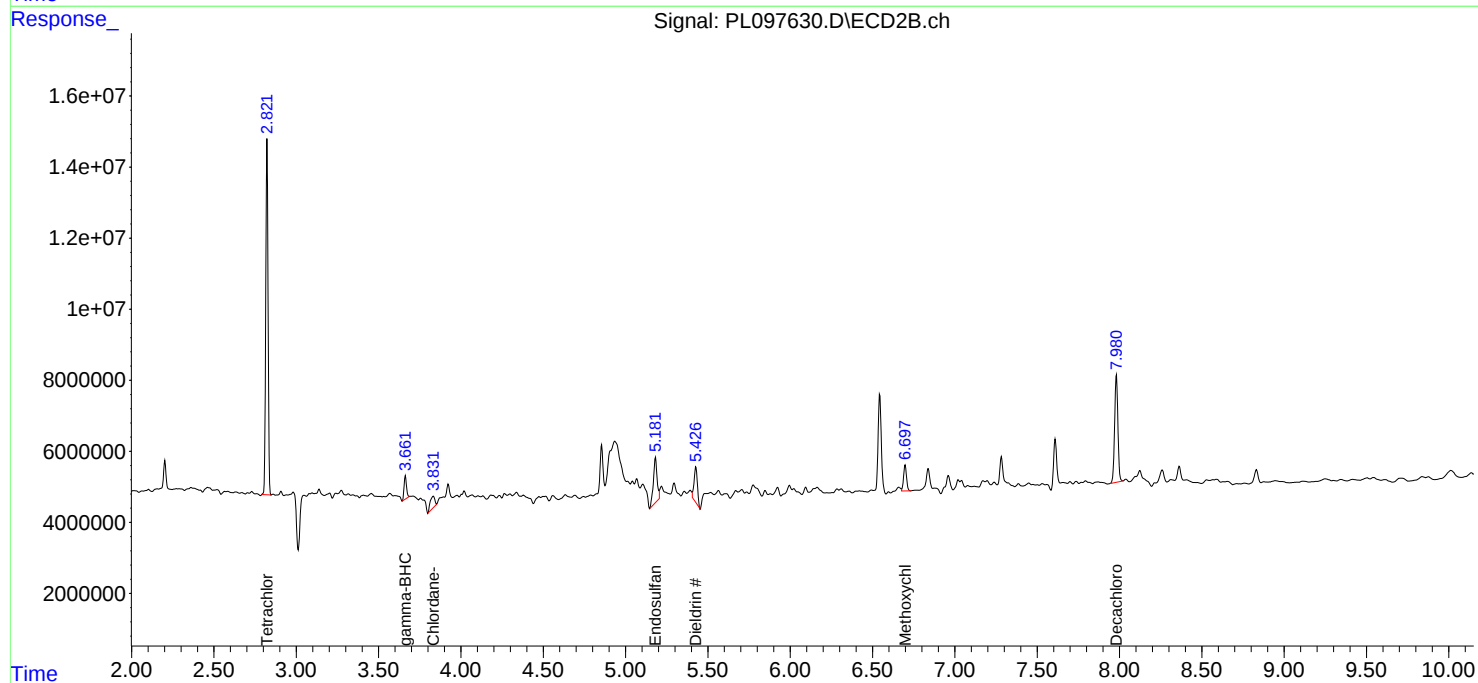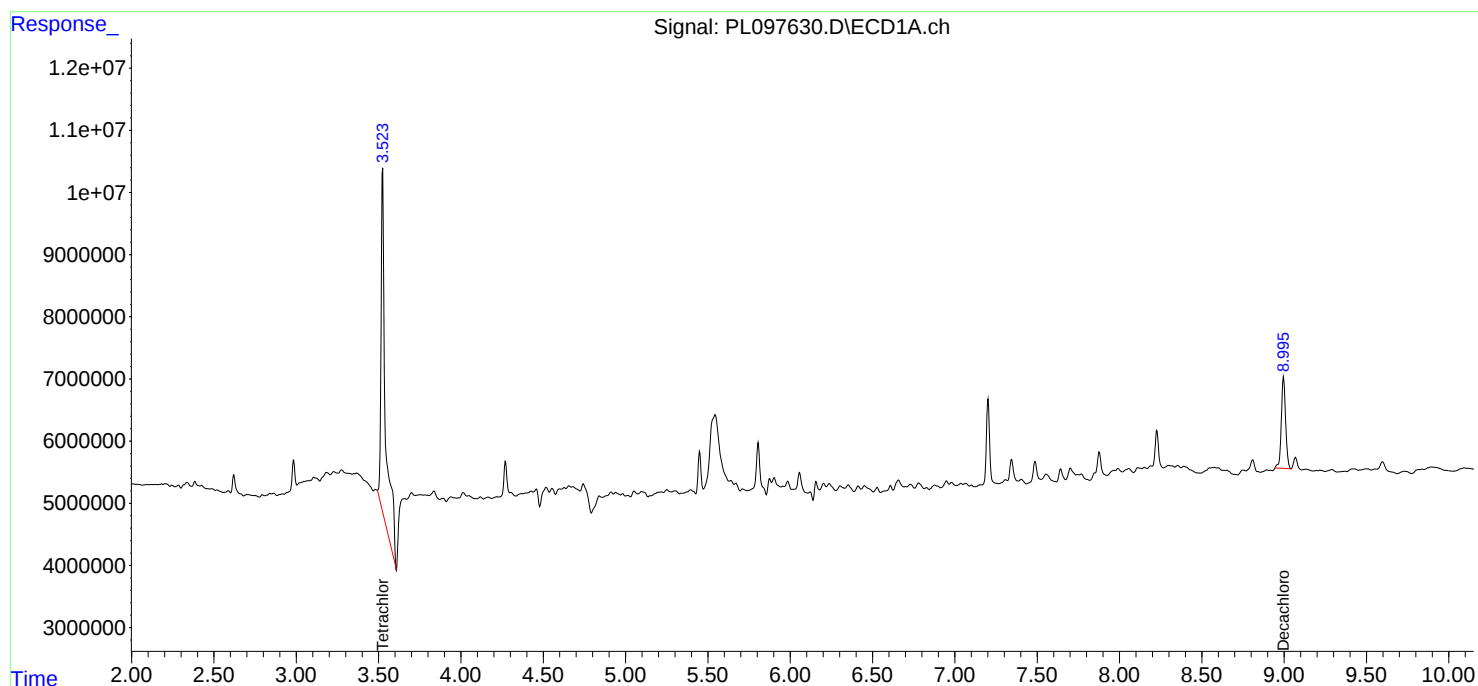


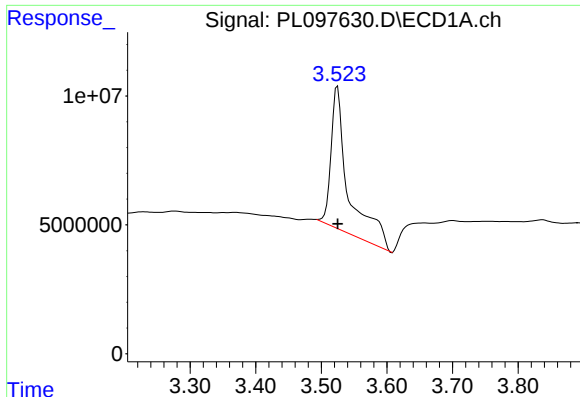

#1 Tetrachloro-m-xylene


R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 101965315
Conc: 25.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
SED-06-0-2

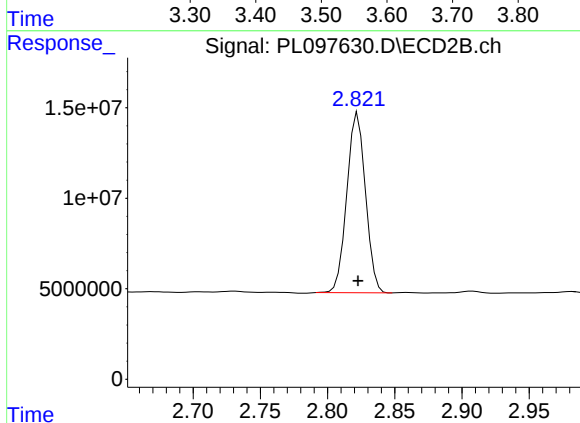


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: 0.000 min
Response: 96025206
Conc: 15.78 ng/ml

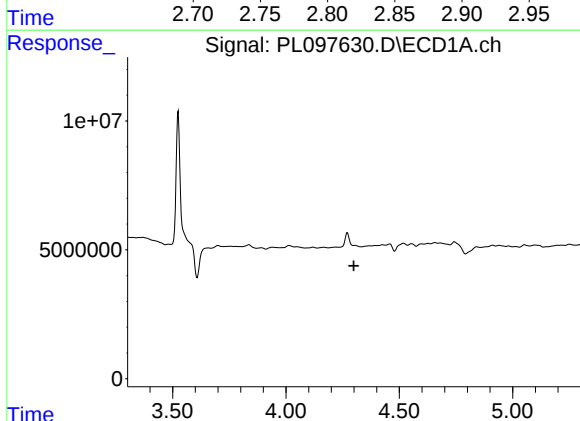


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.300 min
Response: 0
Conc: N.D.

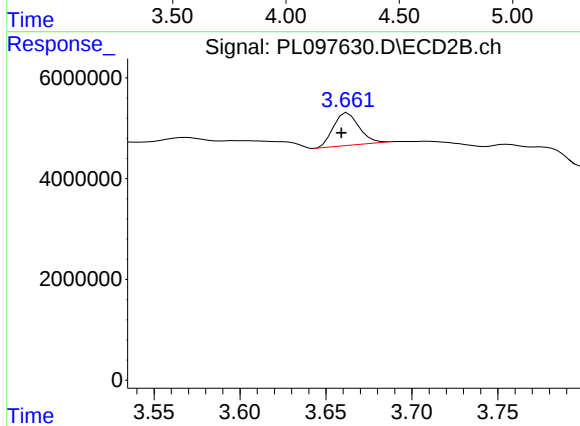

#3 gamma-BHC (Lindane)


R.T.: 3.663 min
Delta R.T.: 0.004 min
Response: 6651345
Conc: 0.72 ng/ml

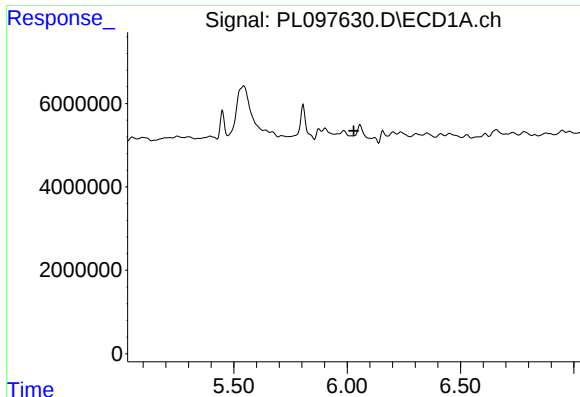

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.030 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SED-06-0-2

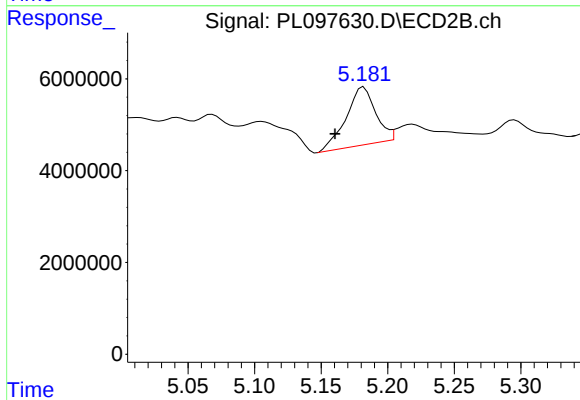


#9 Endosulfan I

R.T.: 5.182 min
Delta R.T.: 0.021 min
Response: 19447931
Conc: 2.64 ng/ml

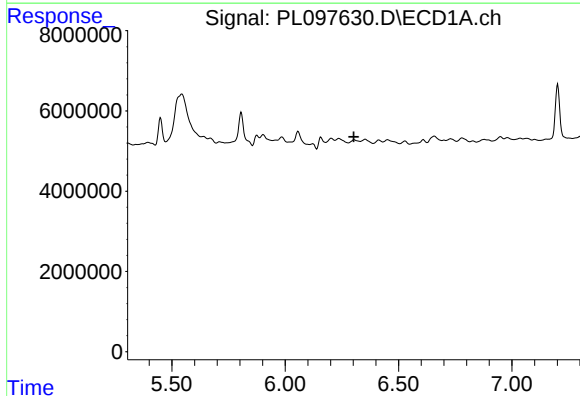


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.302 min
Response: 0
Conc: N.D.

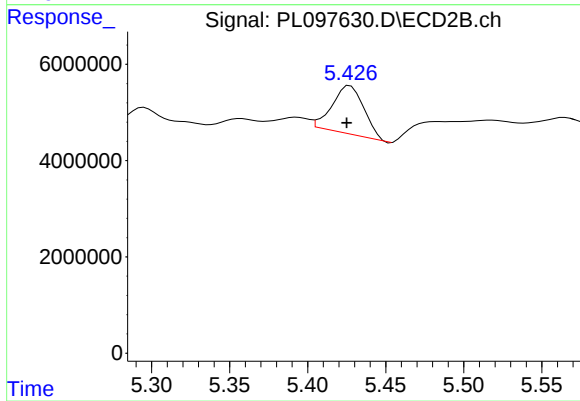

#13 Dieldrin


R.T.: 5.427 min
Delta R.T.: 0.002 min
Response: 14249108
Conc: 1.72 ng/ml

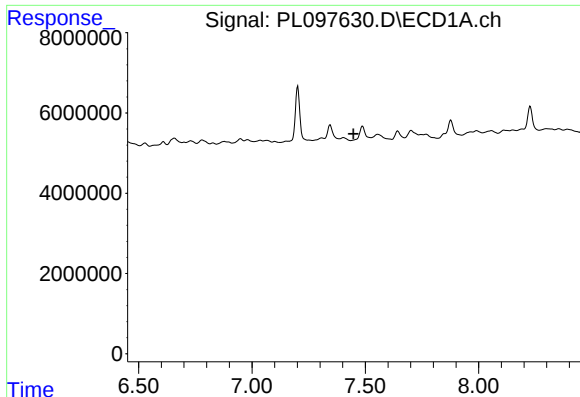

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.448 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SED-06-0-2

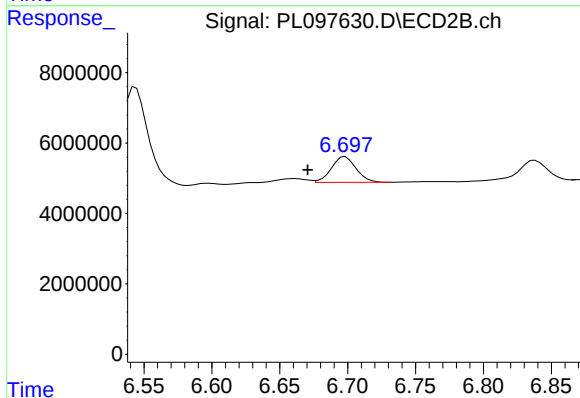


#20 Methoxychlor

R.T.: 6.698 min
Delta R.T.: 0.028 min
Response: 9241787
Conc: 2.54 ng/ml

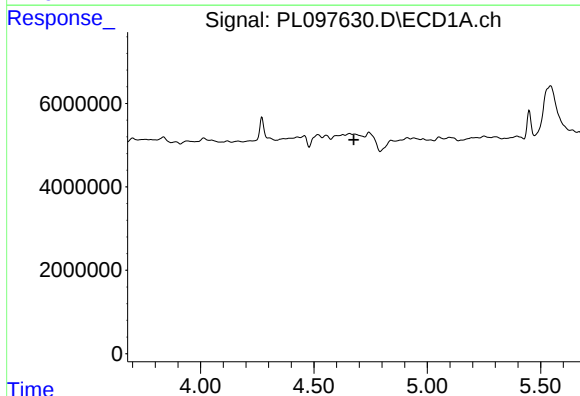


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.676 min
Response: 0
Conc: N.D.

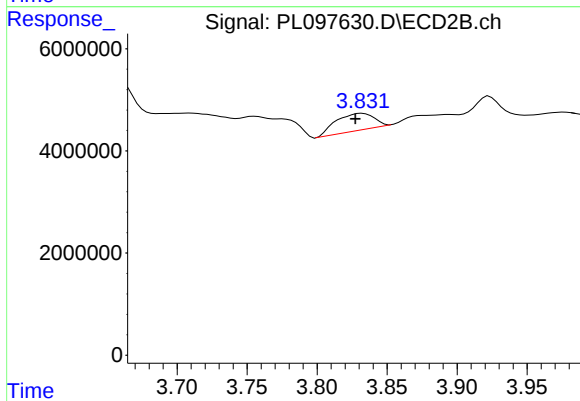

#23 Chlordane-1


R.T.: 3.832 min
Delta R.T.: 0.005 min
Response: 6290150
Conc: 24.76 ng/ml

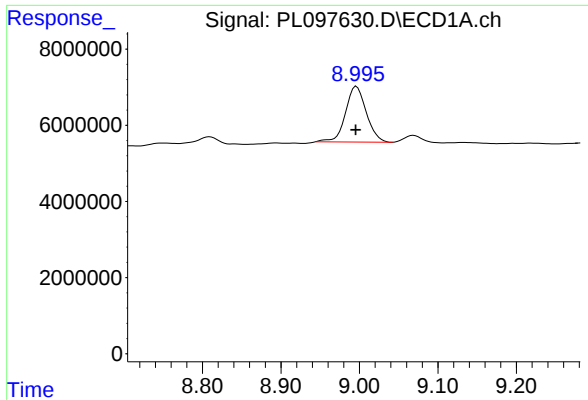

#28 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 26893816
Conc: 9.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
SED-06-0-2

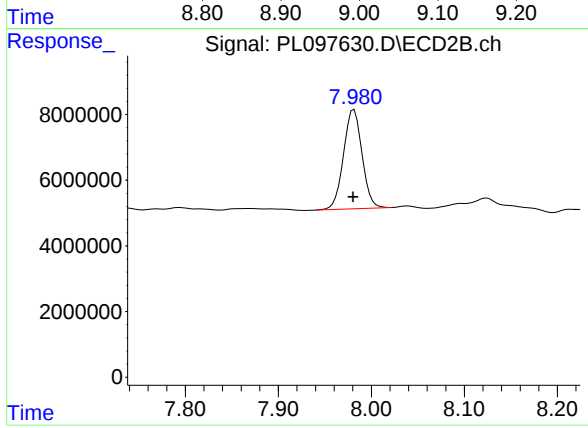

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: 0.001 min
Response: 41907936
Conc: 8.08 ng/ml