

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101325\
 Data File : PL097631.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2025 17:07
 Operator : AR\AJ
 Sample : Q3323-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SED-07-0-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 03:14:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 07 16:47:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.525	2.823	95774827	86982495	23.493	14.291 #
28)	SA Decachlor...	8.997	7.981	34205670	50018227	11.503	9.639
Target Compounds							
3)	MA gamma-BHC...	0.000	3.663	0	5889012	N.D.	0.641 #
4)	MA Heptachlor	4.912f	0.000	13709907	0	2.125	N.D. #
7)	B delta-BHC	4.742	0.000	18813908	0	3.098	N.D. #
9)	A Endosulfan I	0.000	5.181f	0	9911091	N.D.	1.344 #
12)	B 4,4'-DDE	6.156	5.295	3957417	4997720	0.850	0.658
13)	MA Dieldrin	0.000	5.427	0	11385767	N.D.	1.377 #
17)	MA 4,4'-DDT	0.000	6.098	0	2314481	N.D.	0.347 #
20)	A Methoxychlor	0.000	6.699f	0	6392803	N.D.	1.754 #
23)	Chlordane-1	0.000	3.834	0	7029279	N.D.	27.669 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101325\
Data File : PL097631.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2025 17:07
Operator : AR\AJ
Sample : Q3323-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SED-07-0-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 03:14:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
Quant Title : GC Extractables
QLast Update : Tue Oct 07 16:47:00 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

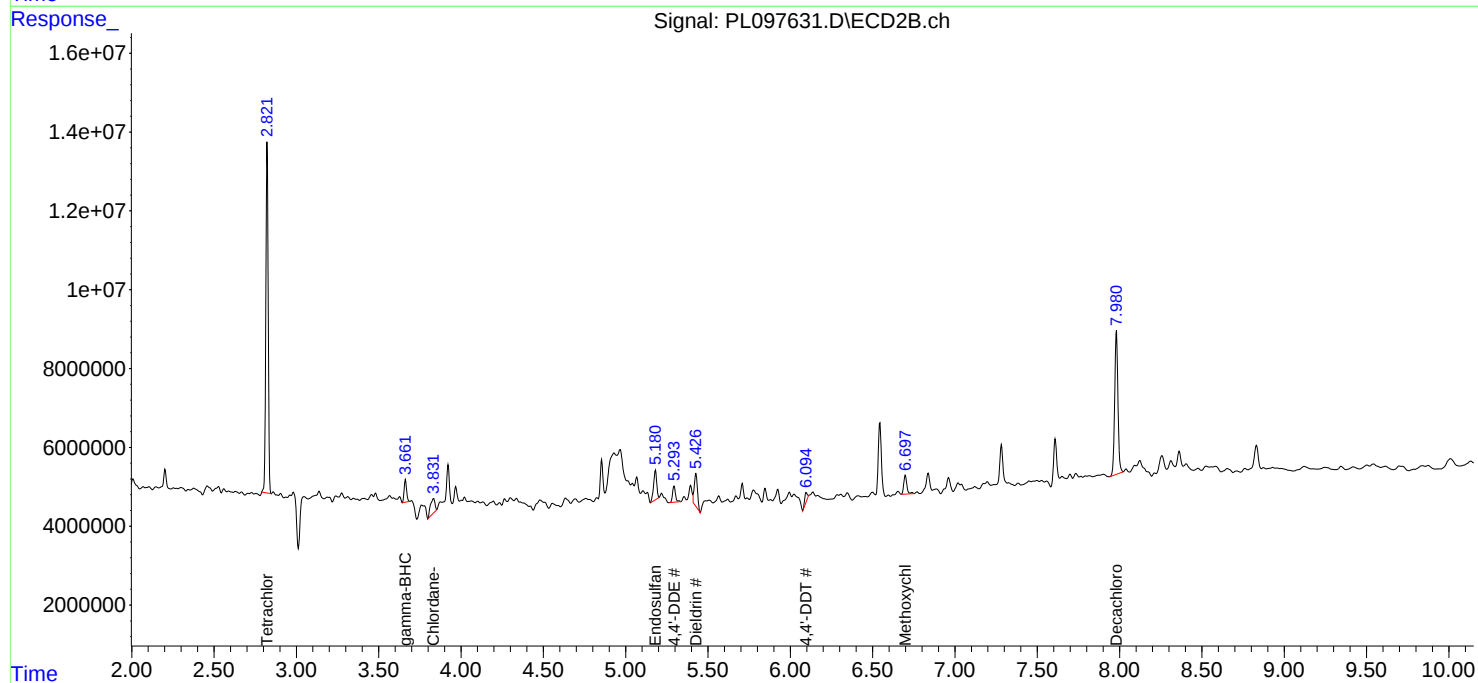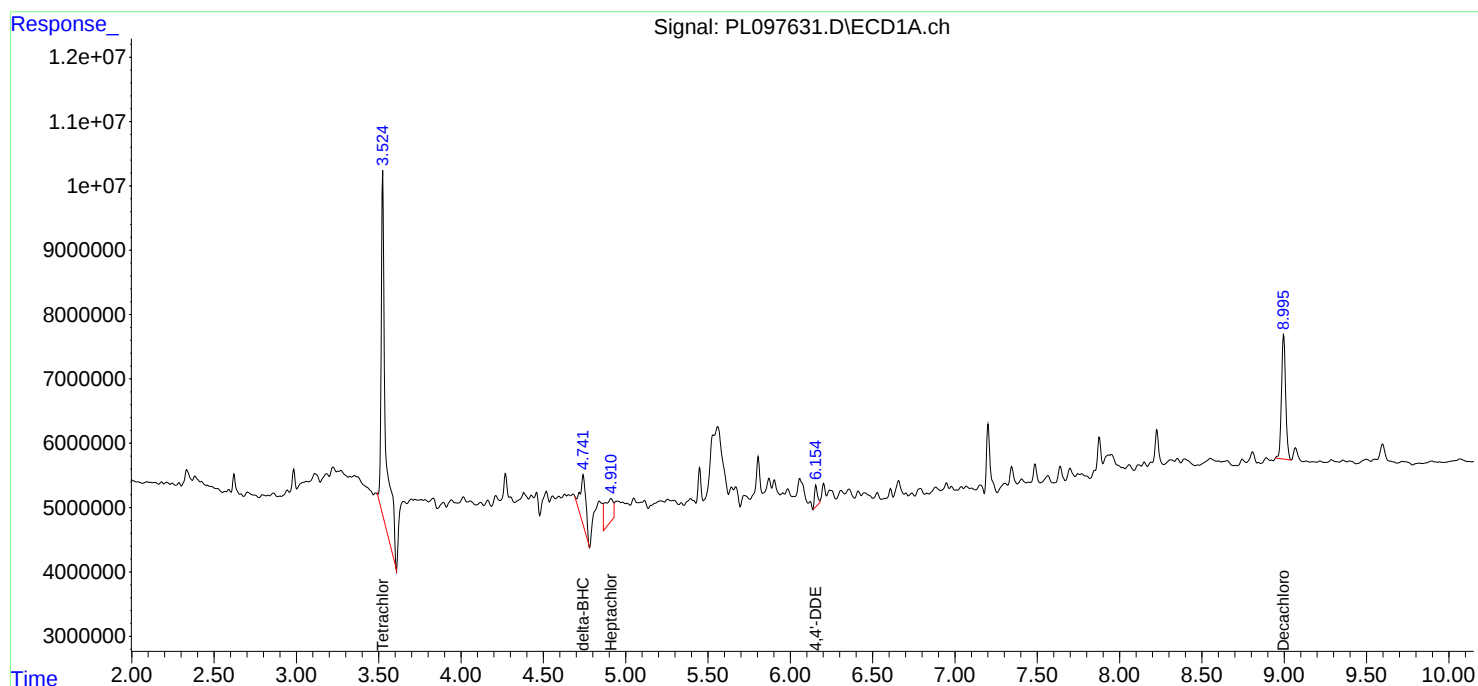


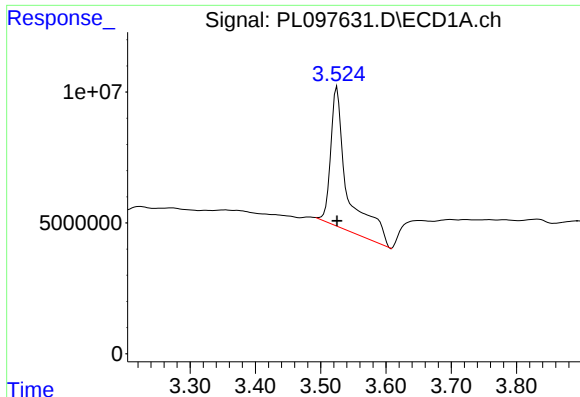

#1 Tetrachloro-m-xylene


R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 95774827
Conc: 23.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
SED-07-0-2

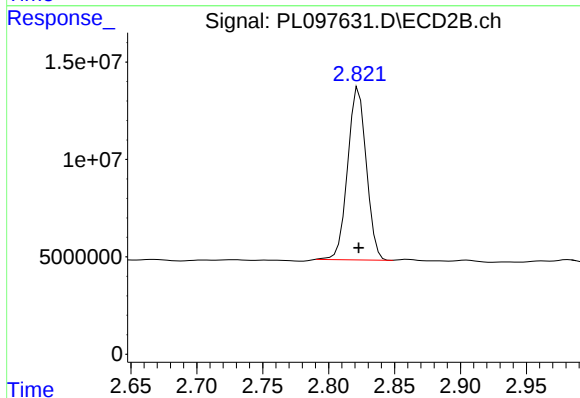


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 86982495
Conc: 14.29 ng/ml

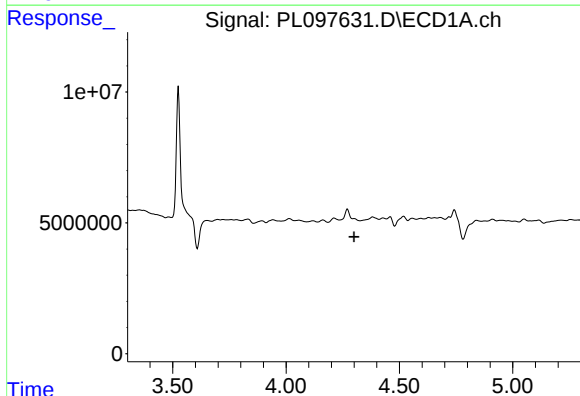


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.300 min
Response: 0
Conc: N.D.

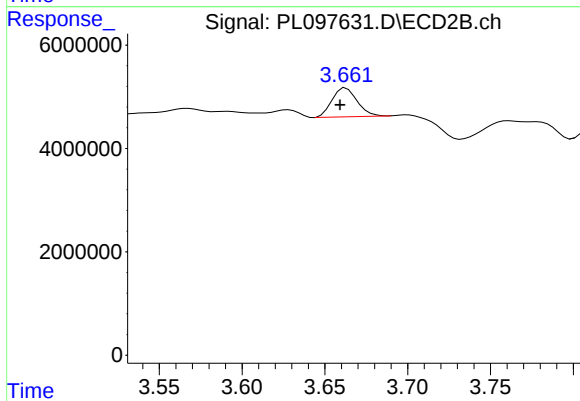

#3 gamma-BHC (Lindane)


R.T.: 3.663 min
Delta R.T.: 0.004 min
Response: 5889012
Conc: 0.64 ng/ml

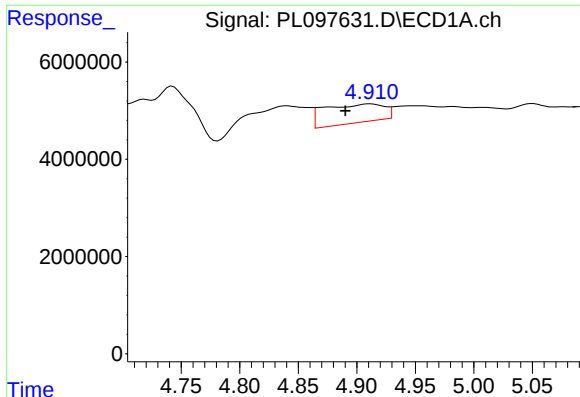

#4 Heptachlor


R.T.: 4.912 min
Delta R.T.: 0.022 min
Response: 13709907
Conc: 2.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
SED-07-0-2

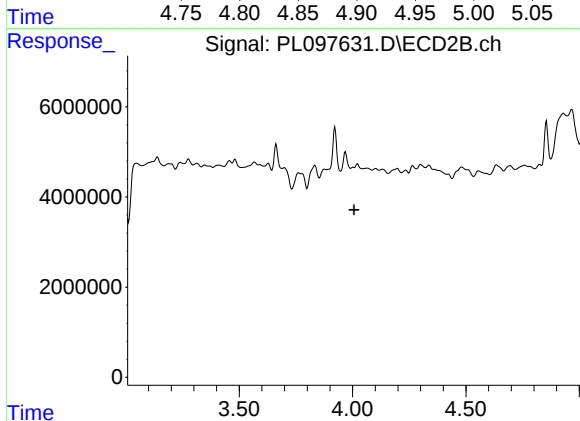


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.007 min
Response: 0
Conc: N.D.

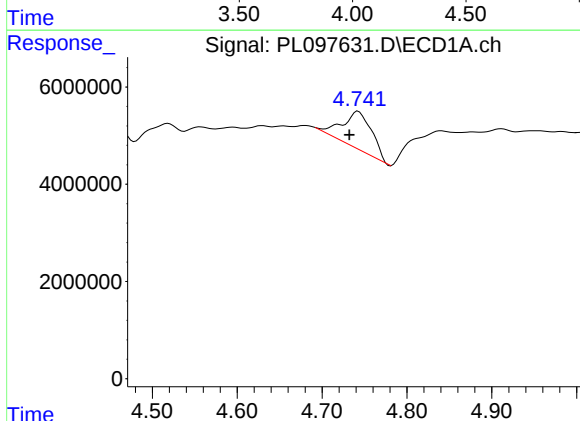


#7 delta-BHC

R.T.: 4.742 min
Delta R.T.: 0.010 min
Response: 18813908
Conc: 3.10 ng/ml

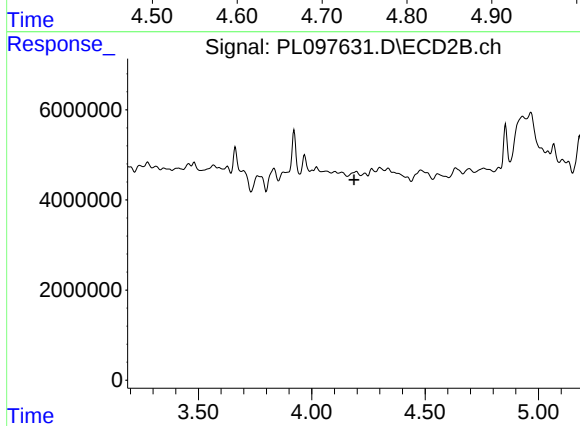

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.187 min
Response: 0
Conc: N.D.

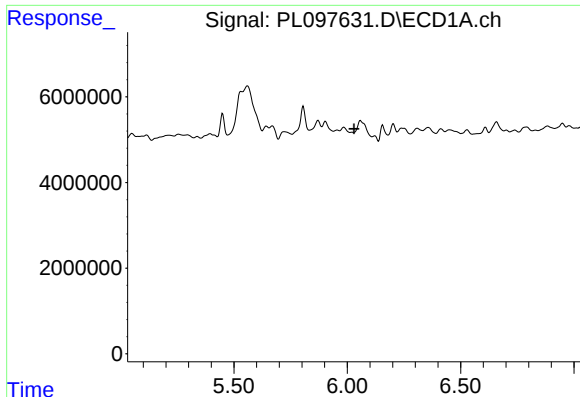

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.030 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SED-07-0-2

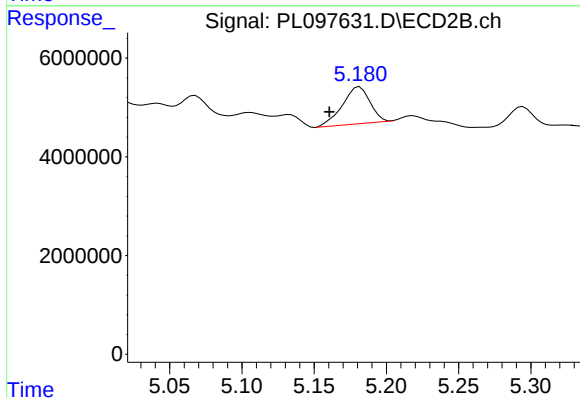


#9 Endosulfan I

R.T.: 5.181 min
Delta R.T.: 0.021 min
Response: 9911091
Conc: 1.34 ng/ml

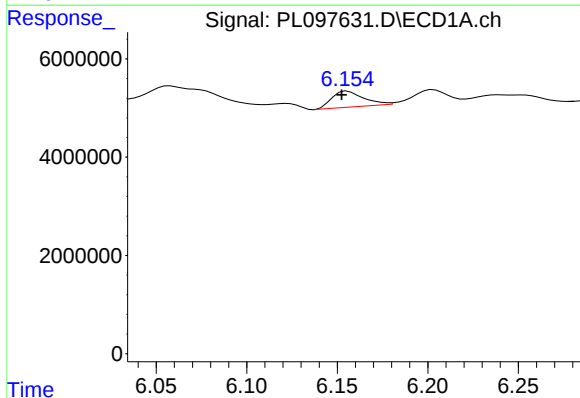


#12 4,4'-DDE

R.T.: 6.156 min
Delta R.T.: 0.003 min
Response: 3957417
Conc: 0.85 ng/ml

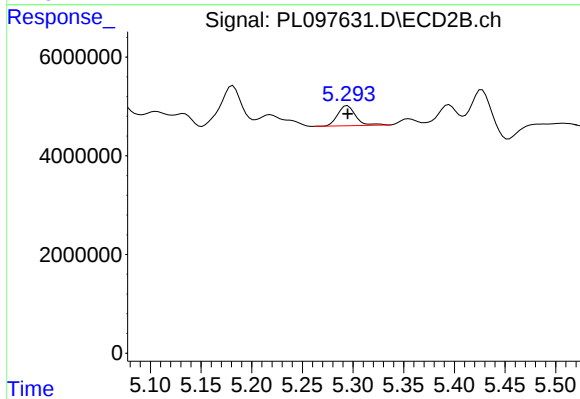

#12 4,4'-DDE


R.T.: 5.295 min
Delta R.T.: 0.000 min
Response: 4997720
Conc: 0.66 ng/ml

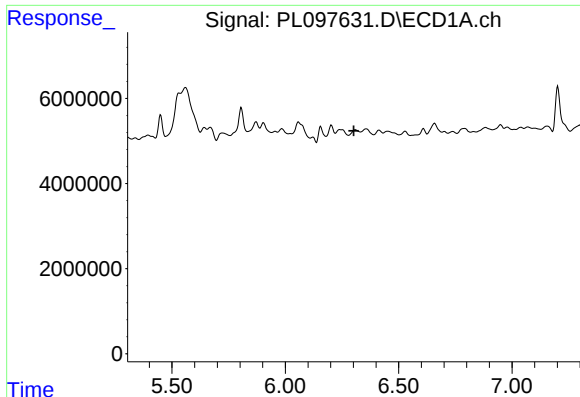

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.302 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SED-07-0-2

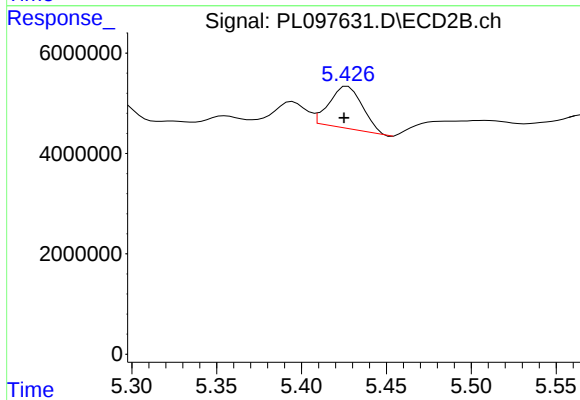


#13 Dieldrin

R.T.: 5.427 min
Delta R.T.: 0.002 min
Response: 11385767
Conc: 1.38 ng/ml

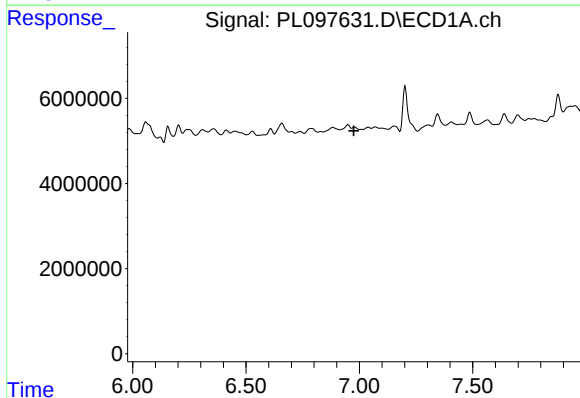


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.975 min
Response: 0
Conc: N.D.

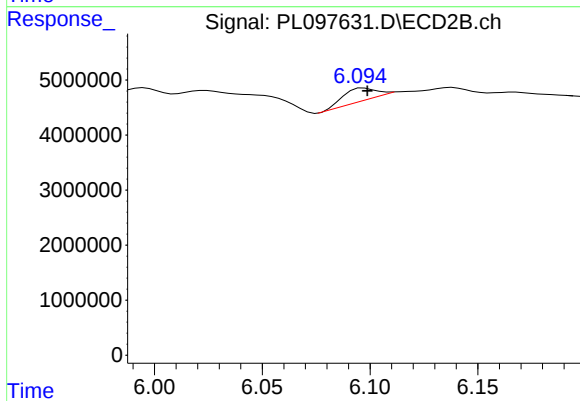

#17 4,4'-DDT


R.T.: 6.098 min
Delta R.T.: 0.000 min
Response: 2314481
Conc: 0.35 ng/ml

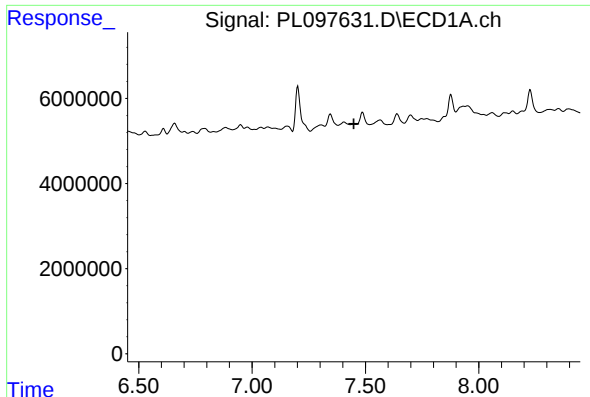

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.448 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SED-07-0-2

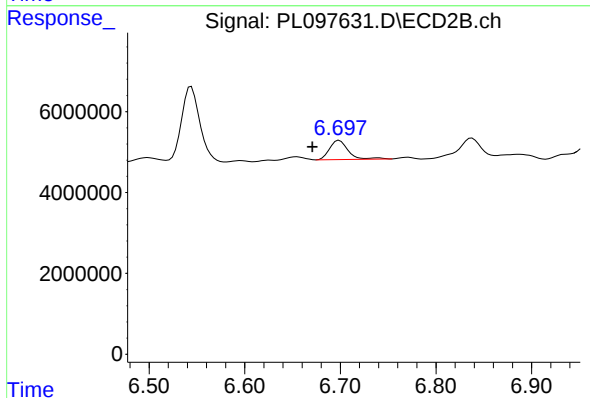


#20 Methoxychlor

R.T.: 6.699 min
Delta R.T.: 0.028 min
Response: 6392803
Conc: 1.75 ng/ml

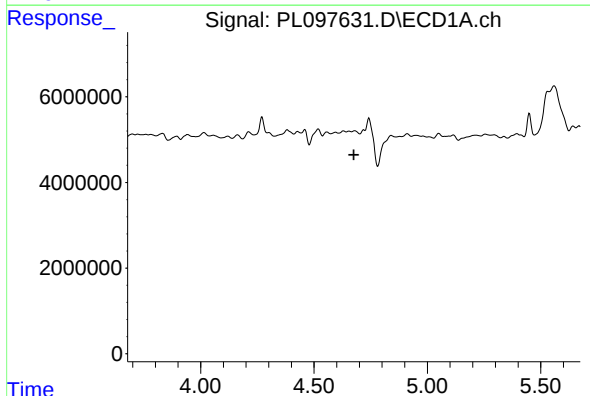


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.676 min
Response: 0
Conc: N.D.

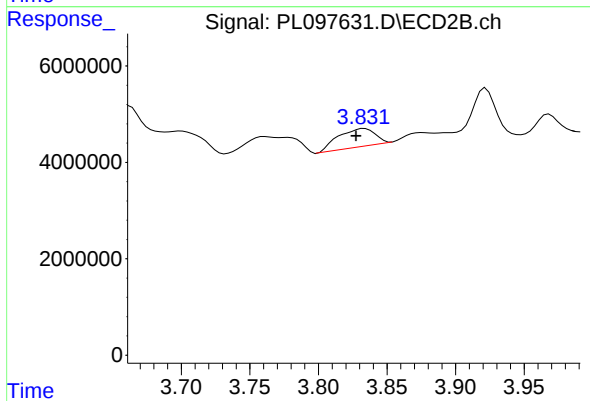

#23 Chlordane-1


R.T.: 3.834 min
Delta R.T.: 0.006 min
Response: 7029279
Conc: 27.67 ng/ml

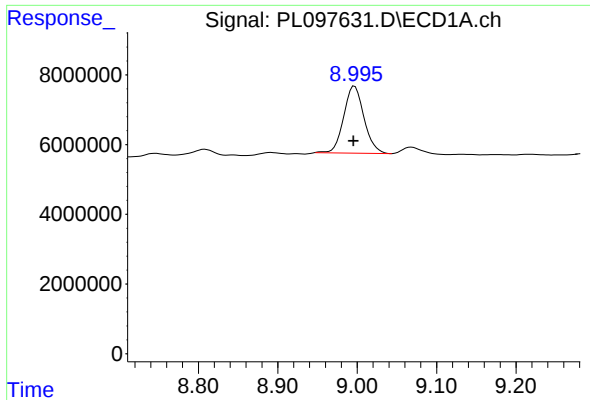

#28 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.001 min
Response: 34205670
Conc: 11.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
SED-07-0-2

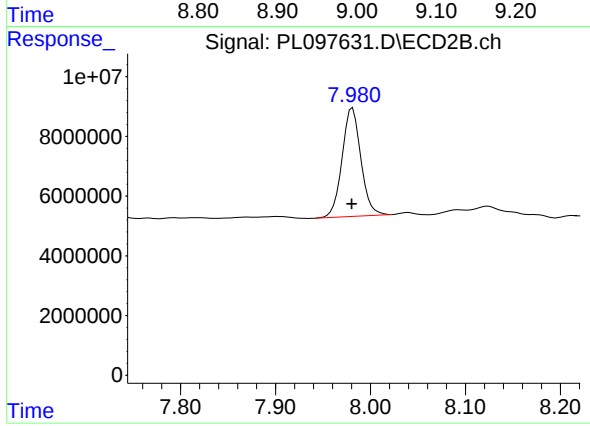

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: 0.000 min
Response: 50018227
Conc: 9.64 ng/ml