

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101325\
 Data File : PL097624.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2025 15:32
 Operator : AR\AJ
 Sample : Q3323-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SED-01-0-2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/14/2025
 Supervised By : mohammad ahmed 10/15/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 02:24:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 07 16:47:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.523	2.822	62545228	86415271	15.342m	14.198
28) SA Decachlor...	8.999	7.982	36929168	50468487	12.419	9.726

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101325\
Data File : PL097624.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2025 15:32
Operator : AR\AJ
Sample : Q3323-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SED-01-0-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/14/2025
Supervised By :mohammad ahmed 10/15/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 02:24:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100725.M
Quant Title : GC Extractables
QLast Update : Tue Oct 07 16:47:00 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

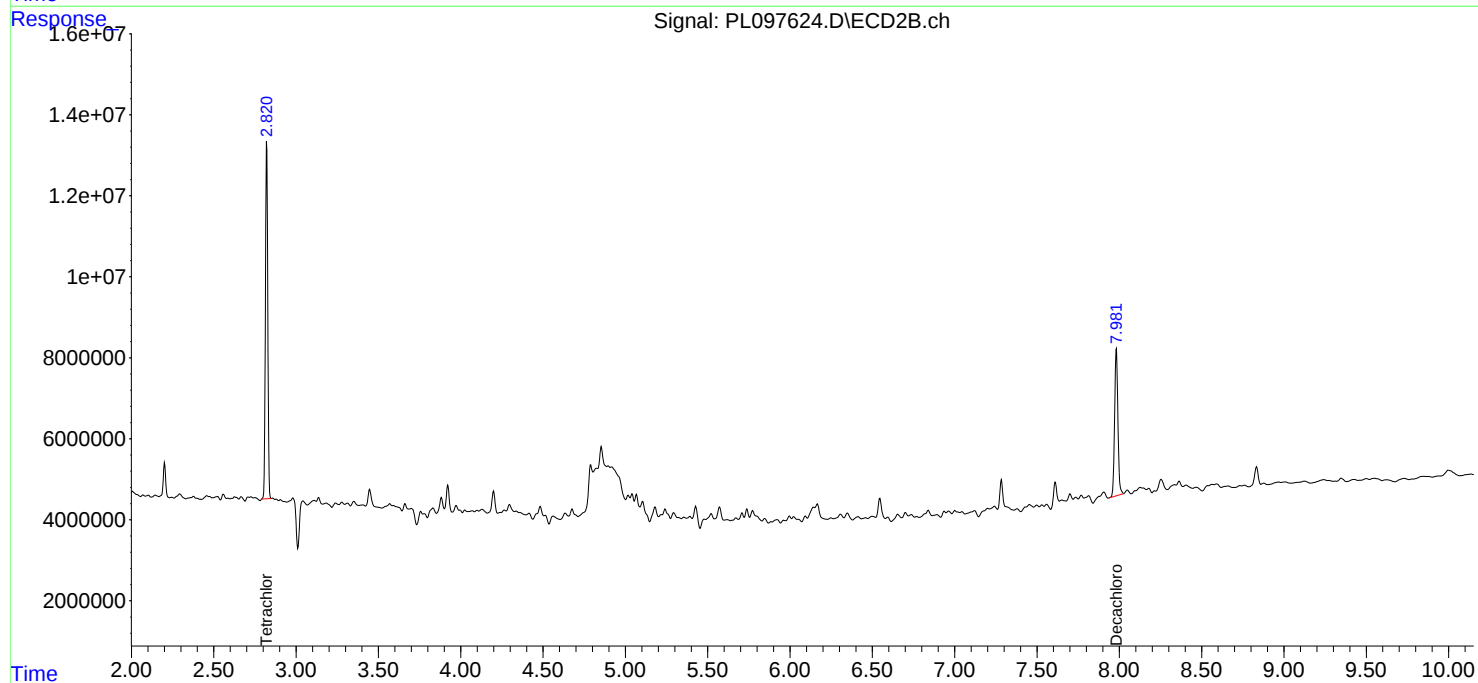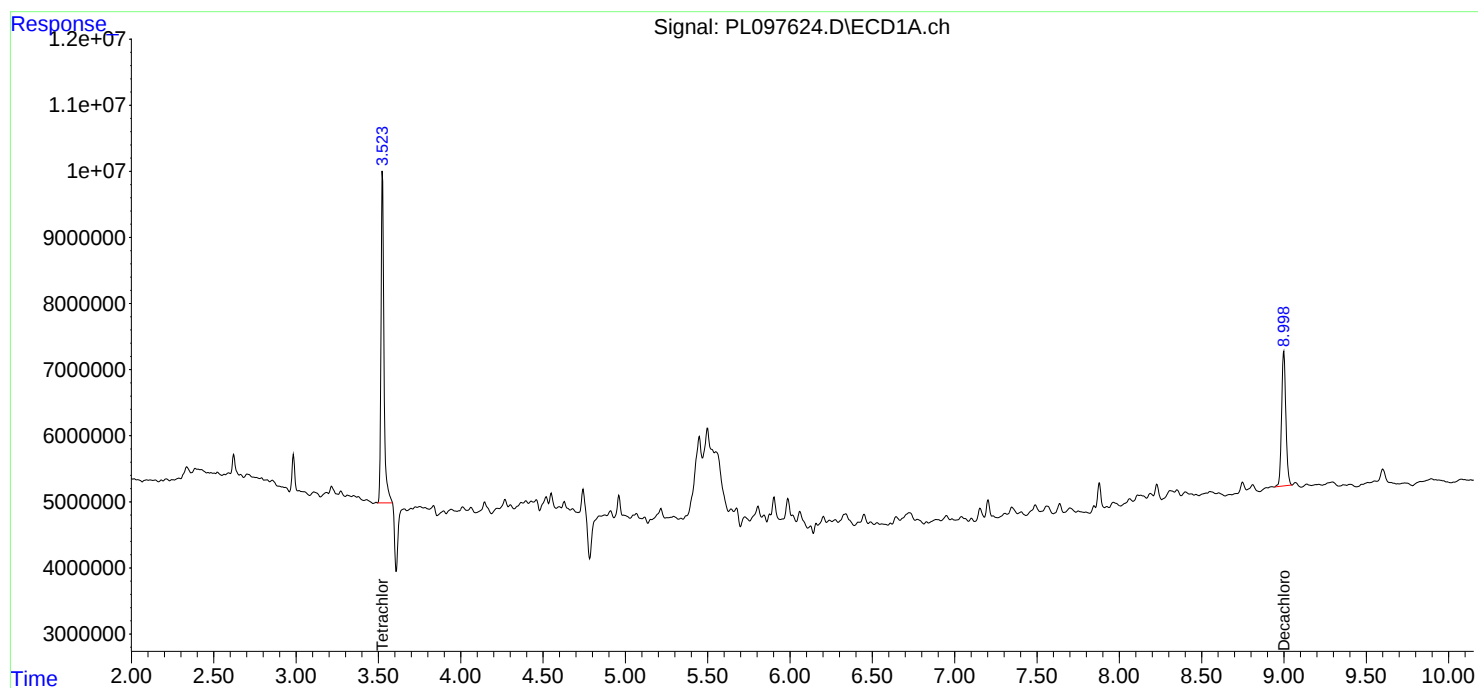

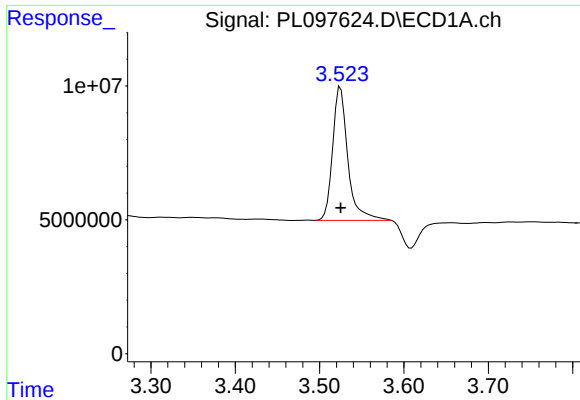


#1 Tetrachloro-m-xylene

R.T.: 3.523 min
Delta R.T.: -0.002 min
Response: 62545228
Conc: 15.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
SED-01-0-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/14/2025
Supervised By :mohammad ahmed 10/15/2025

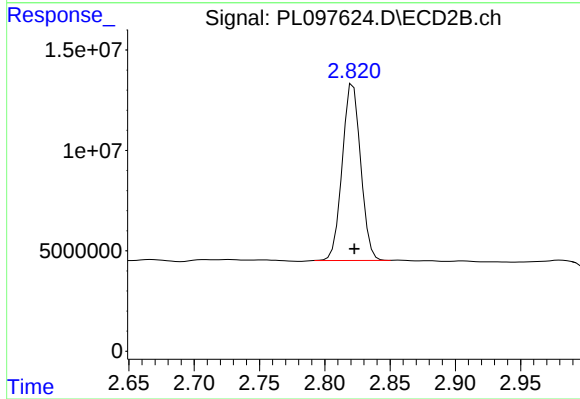


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: -0.001 min
Response: 86415271
Conc: 14.20 ng/ml

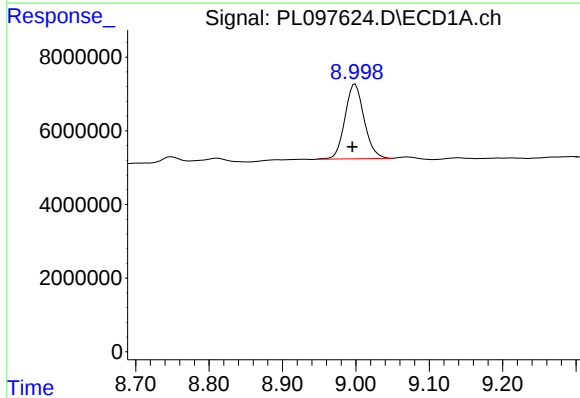

#28 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: 0.004 min
Response: 36929168
Conc: 12.42 ng/ml

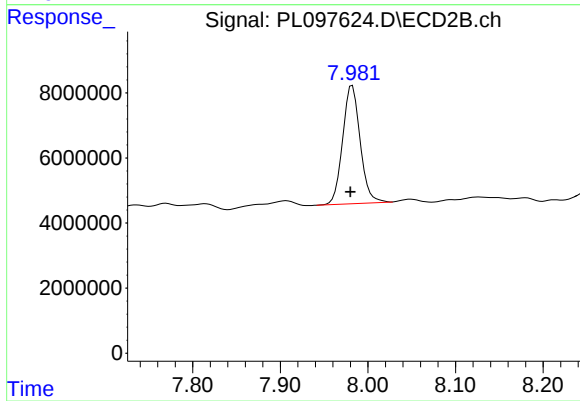

#28 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: 0.002 min
Response: 50468487
Conc: 9.73 ng/ml