

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101419\
 Data File : PL053295.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2019 11:15
 Operator : SG\AJ
 Sample : TOXAPH353
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 11:31:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 28 05:45:16 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.552	4.046	206.4E6	49368912	22.177	19.659
27)	SA Decachlor...	8.343	9.128	367.6E6	102.6E6	40.545	38.418
Target Compounds							
22)	Toxaphene-1	5.836	6.439	154.6E6	22490768	2069.125	1573.409
23)	Toxaphene-2	5.999	6.729	157.5E6	30510859	2110.288	1788.315
24)	Toxaphene-3	6.322	7.135	179.4E6	50321492	2158.939	1999.444m
25)	Toxaphene-4	6.440	7.213	397.5E6	131.5E6	2066.748m	1910.488
26)	Toxaphene-5	7.178	7.711	383.9E6	60932166	2002.297	2001.989m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101419\
Data File : PL053295.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2019 11:15
Operator : SG\AJ
Sample : TOXAPH353
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 11:31:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 28 05:45:16 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

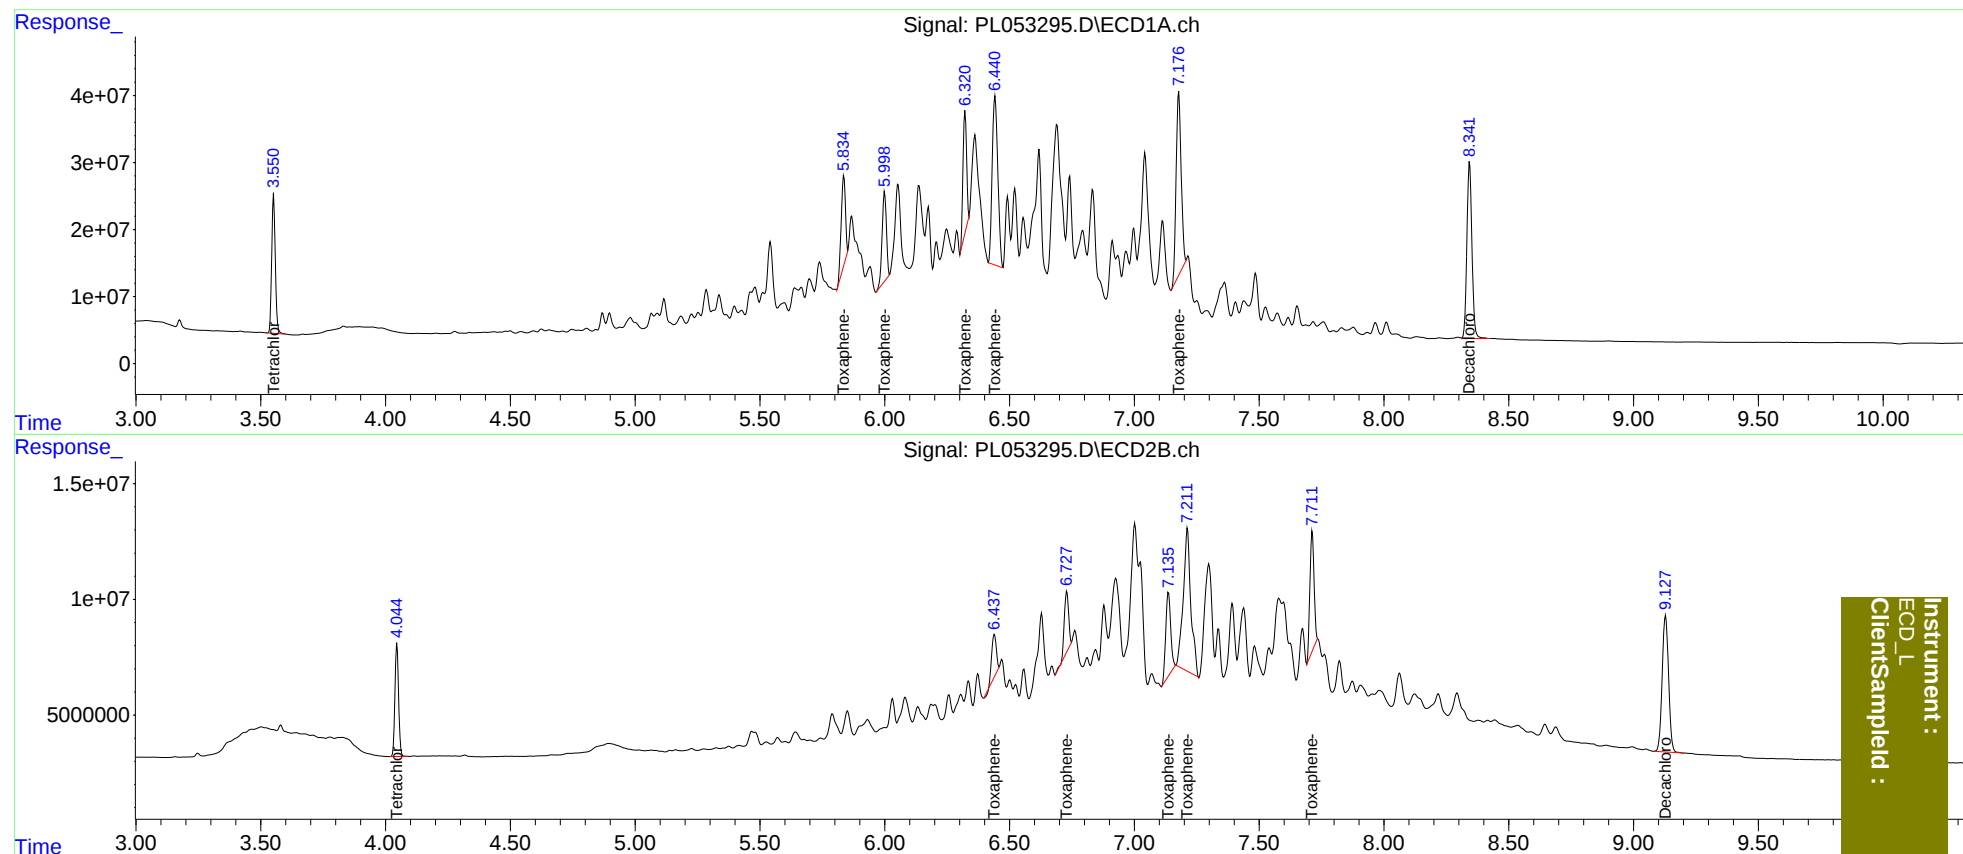

Instrument :
ECD_L
ClientSampleId :