

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101419\
 Data File : PL053305.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2019 14:34
 Operator : SG\AJ
 Sample : TOXAPH354
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TOXAPH354

Manual Integrations
 APPROVED

Ankita
 10/15/2019 8:44:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 14:44:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 28 05:45:16 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	4.046	198.6E6	49838961	21.338	19.846
27)	SA Decachlor...	8.335	9.124	373.0E6	106.0E6	41.150	39.667
Target Compounds							
22)	Toxaphene-1	5.829	6.437	141.4E6	30067652	1892.365	2103.472
23)	Toxaphene-2	5.992	6.728	158.2E6	31695868	2119.285	1857.771
24)	Toxaphene-3	6.314	7.135	171.5E6	51020180	2064.011	2027.205
25)	Toxaphene-4	6.435	7.210	381.2E6	133.0E6	1982.065	1932.804
26)	Toxaphene-5	7.169	7.709	379.0E6	61543248	1976.430	2022.067m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101419\
Data File : PL053305.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2019 14:34
Operator : SG\AJ
Sample : TOXAPH354
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 14:44:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 28 05:45:16 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

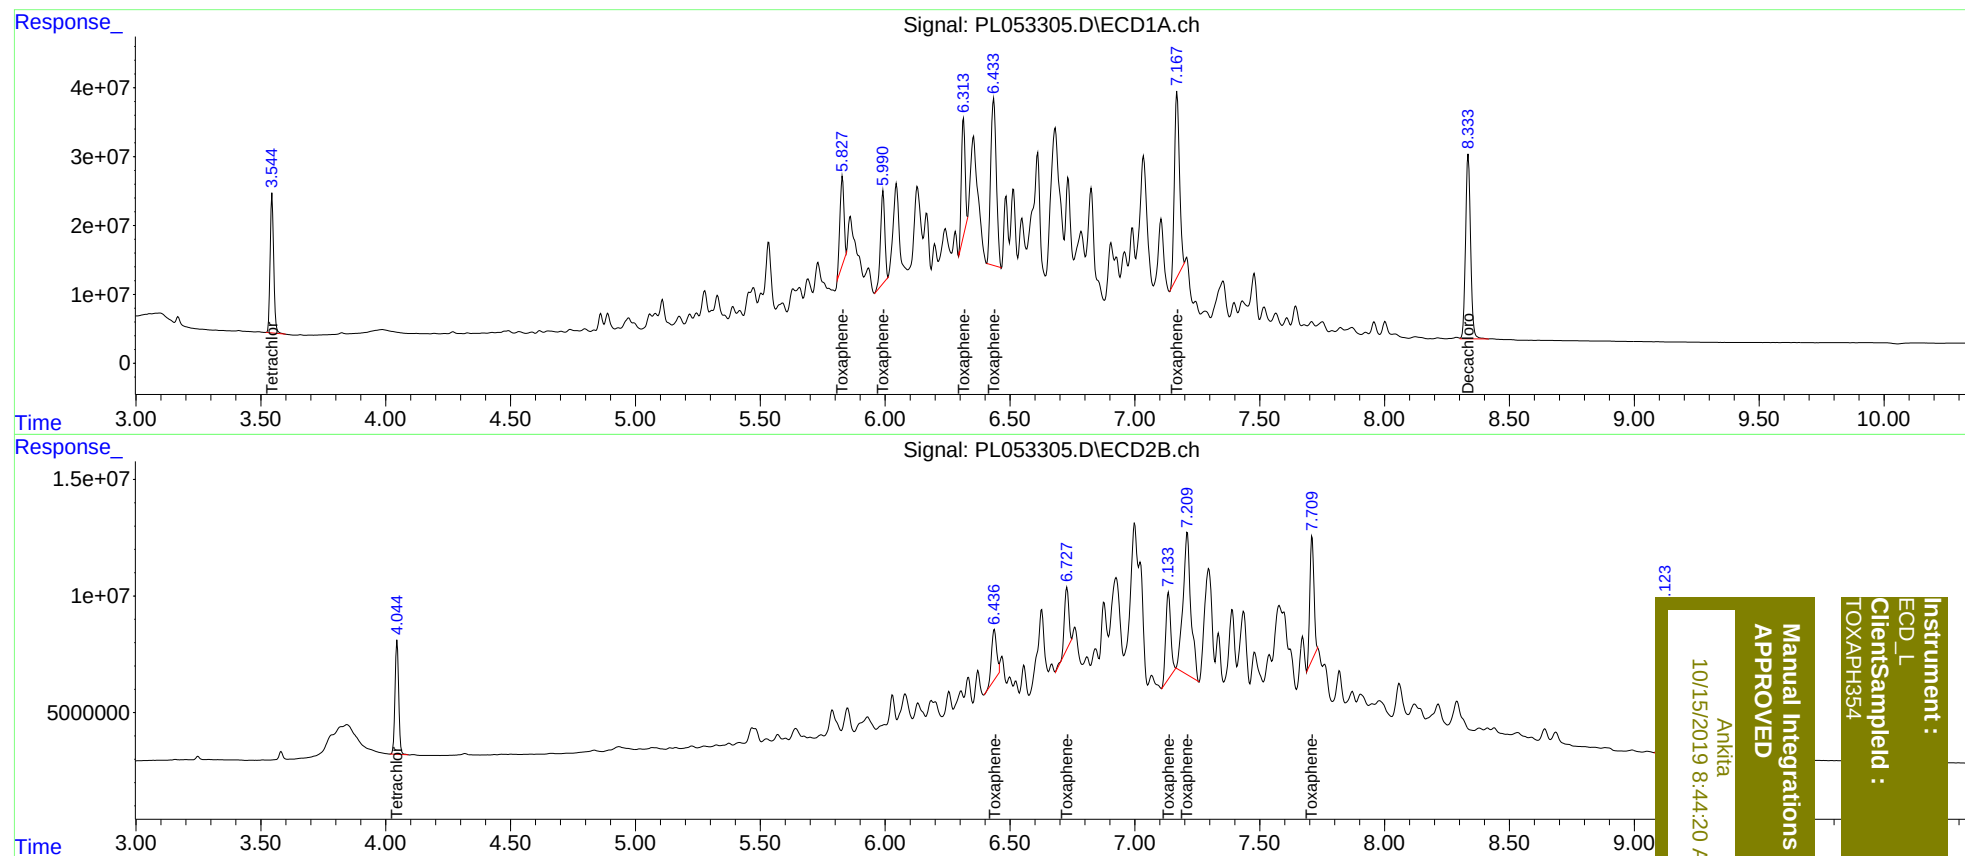

10/15/2019 8:44:20 AM
Ankita

Manual Integrations
APPROVED

Instrument :
ECD_L
ClientSampled :
TOXAPH354