

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101422\
 Data File : PL078362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2022 14:19
 Operator : AR\AJ
 Sample : PB148340BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 00:17:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 15:30:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.622	32543335	48305618	19.692	18.275
28)	SA Decachlor...	8.916	7.722	30082943	42023586	19.486	19.332
Target Compounds							
2)	A alpha-BHC	0.000	3.117	0	85094	N.D.	0.020 #
7)	B delta-BHC	4.649f	0.000	311198	0	0.169	N.D. #
10)	B gamma-Chl...	0.000	4.797	0	501910	N.D.	0.168 #
14)	MA Endrin	0.000	5.467f	0	469608	N.D.	0.204 #
16)	A 4,4'-DDD	0.000	5.625f	0	1223349	N.D.	0.549 #
18)	B Endrin al...	6.826	0.000	734300	0	0.642	N.D. #
19)	B Endosulfa...	0.000	6.135	0	447579	N.D.	0.186 #
21)	B Endrin ke...	0.000	6.610f	0	452930	N.D.	0.171 #
25)	Chlordane-3	0.000	4.797	0	501910	N.D.	1.640 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101422\
Data File : PL078362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2022 14:19
Operator : AR\AJ
Sample : PB148340BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 00:17:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 15:30:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

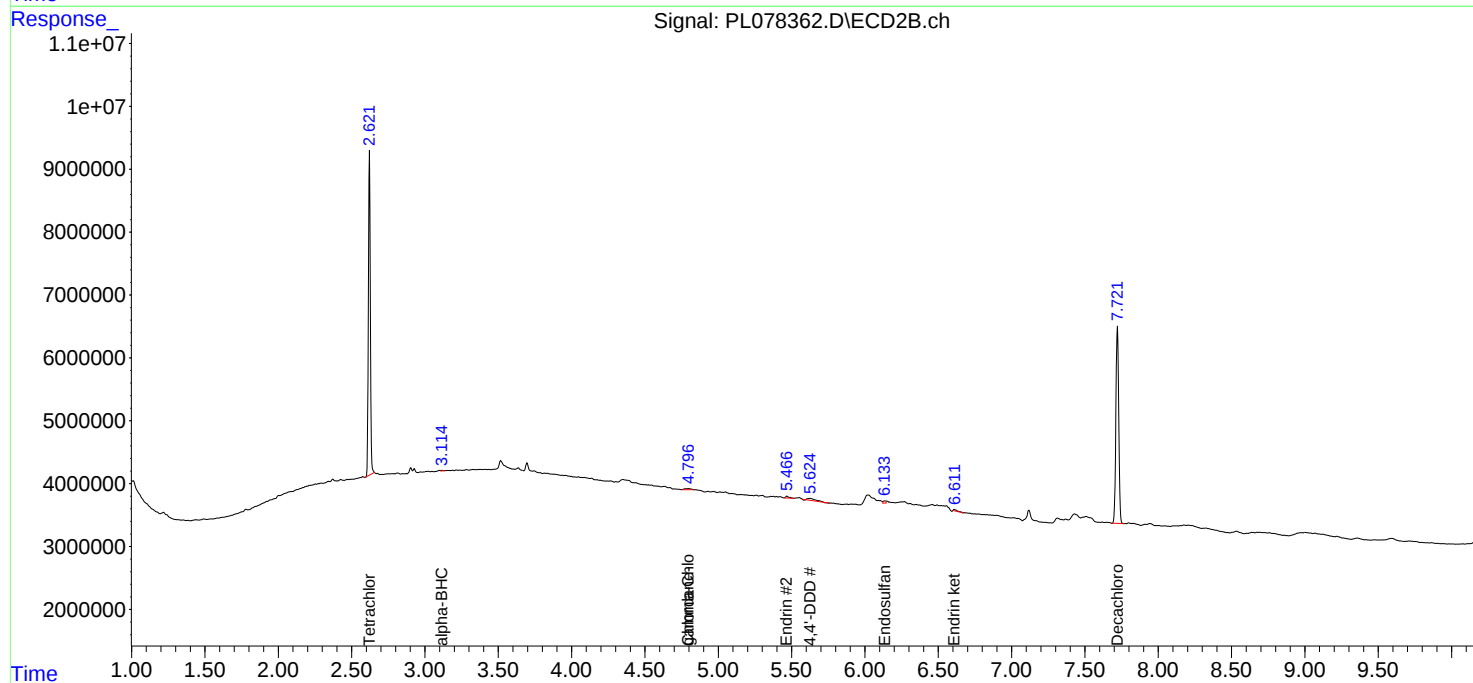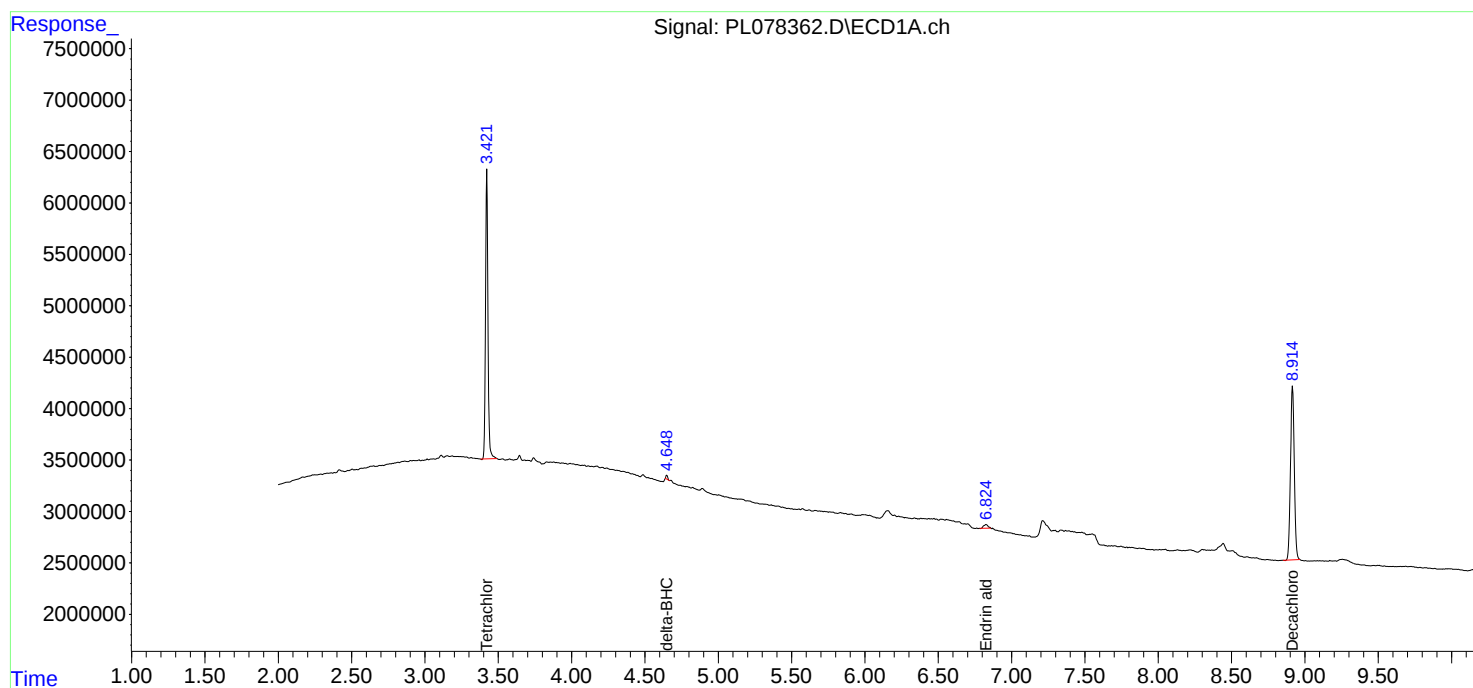


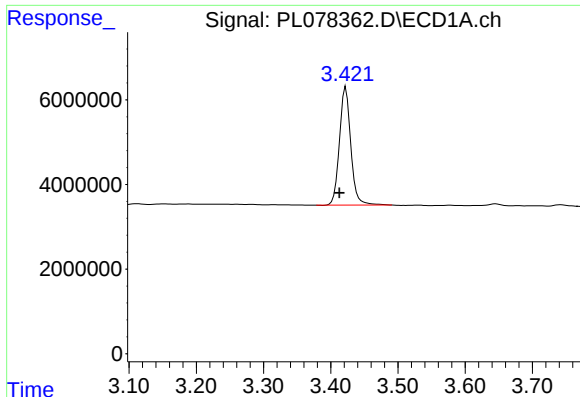

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.009 min
Response: 32543335
Conc: 19.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

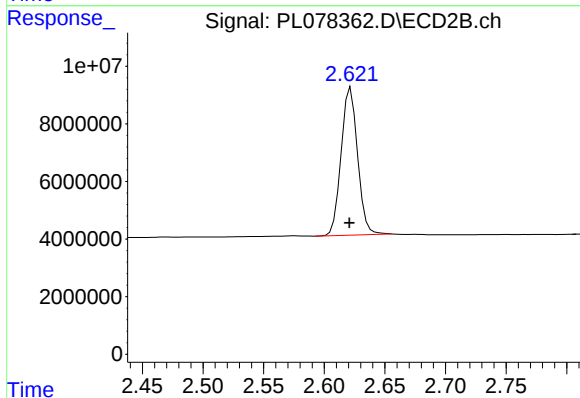


#1 Tetrachloro-m-xylene

R.T.: 2.622 min
Delta R.T.: 0.001 min
Response: 48305618
Conc: 18.27 ng/ml

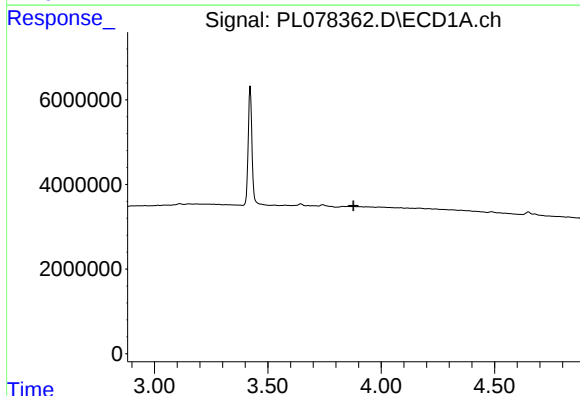


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.878 min
Response: 0
Conc: N.D.

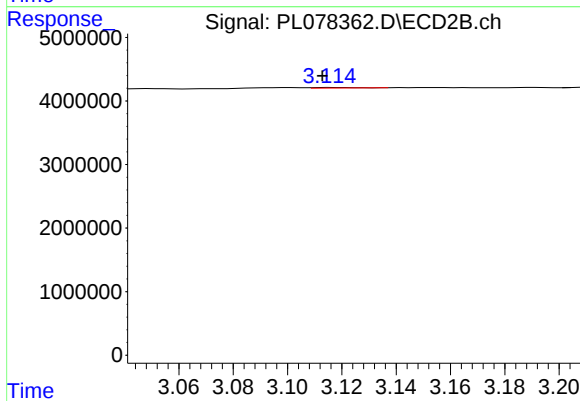

#2 alpha-BHC


R.T.: 3.117 min
Delta R.T.: 0.004 min
Response: 85094
Conc: 0.02 ng/ml

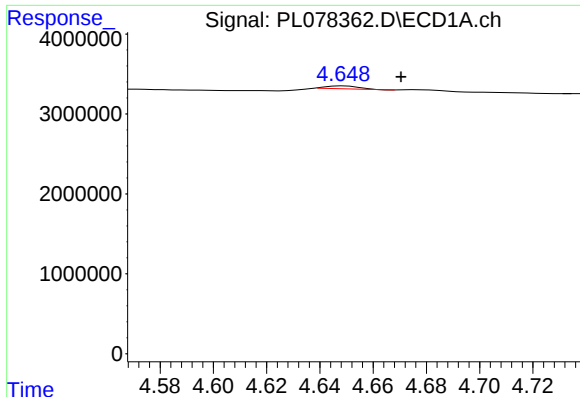

#7 delta-BHC


R.T.: 4.649 min
Delta R.T.: -0.022 min
Response: 311198
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

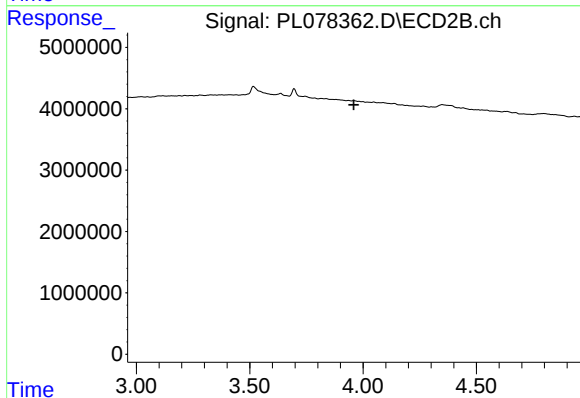


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 3.960 min
Response: 0
Conc: N.D.

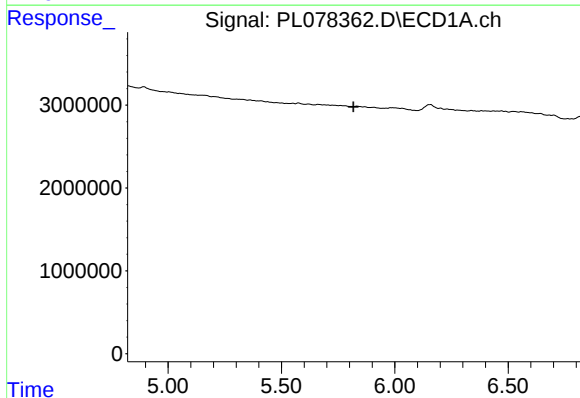


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.818 min
Response: 0
Conc: N.D.

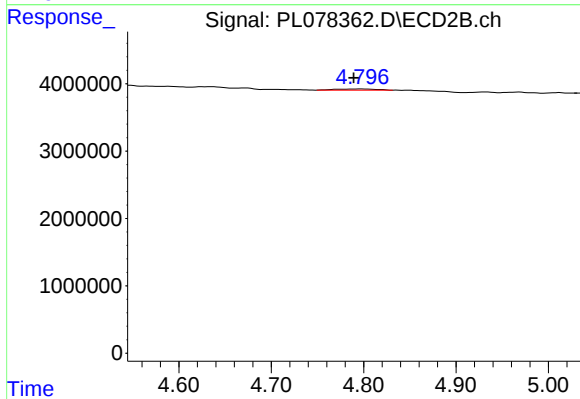

#10 gamma-Chlordane


R.T.: 4.797 min
Delta R.T.: 0.008 min
Response: 501910
Conc: 0.17 ng/ml

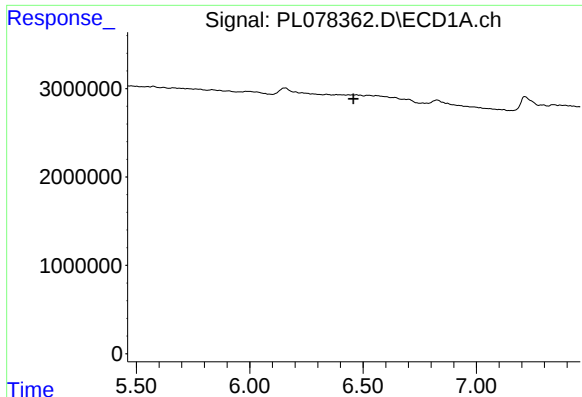

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

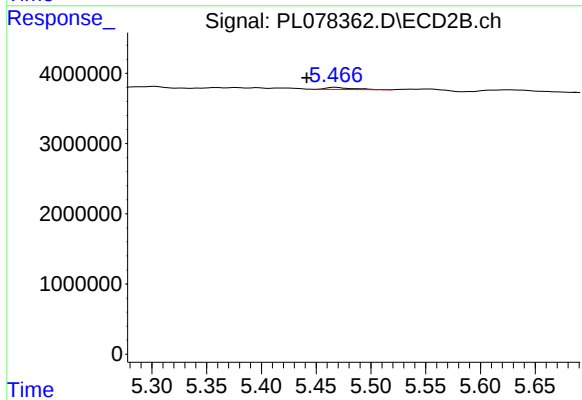


#14 Endrin

R.T.: 5.467 min
Delta R.T.: 0.026 min
Response: 469608
Conc: 0.20 ng/ml

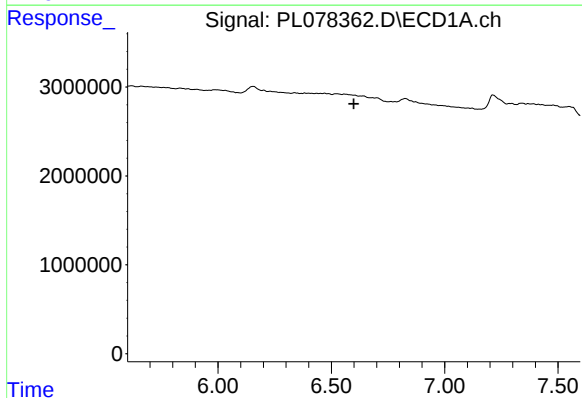


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.599 min
Response: 0
Conc: N.D.

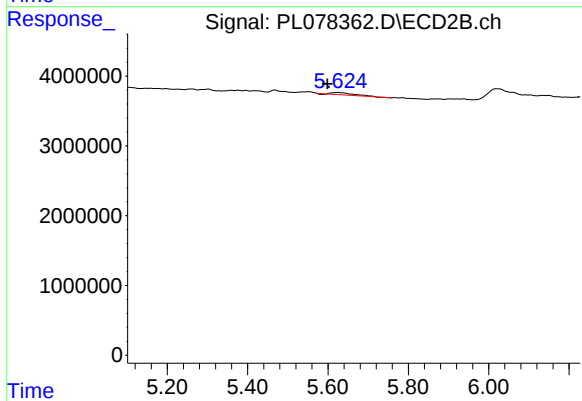

#16 4,4'-DDD


R.T.: 5.625 min
Delta R.T.: 0.027 min
Response: 1223349
Conc: 0.55 ng/ml

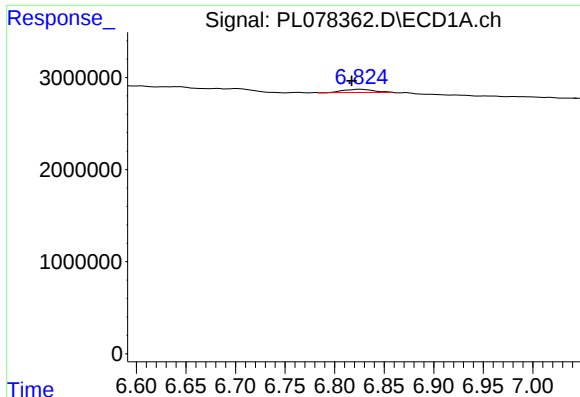

#18 Endrin aldehyde


R.T.: 6.826 min
Delta R.T.: 0.009 min
Response: 734300
Conc: 0.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

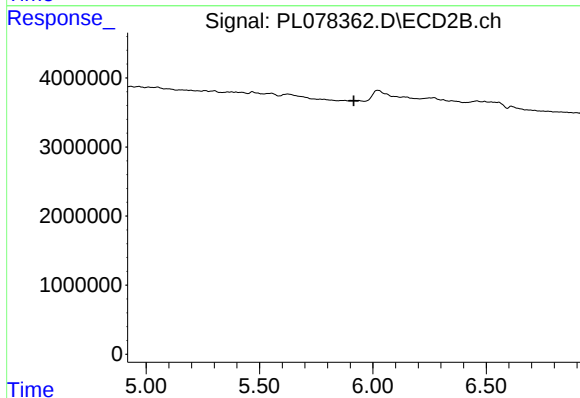


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 5.916 min
Response: 0
Conc: N.D.

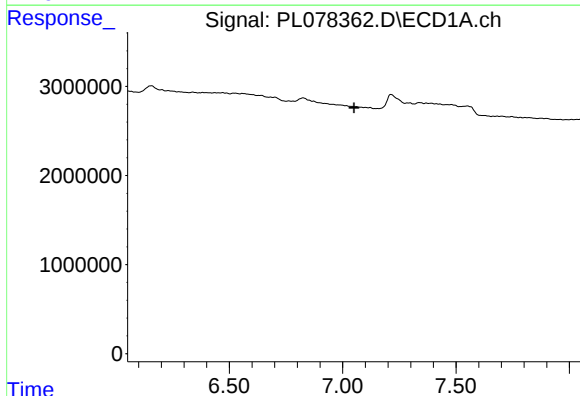


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.050 min
Response: 0
Conc: N.D.

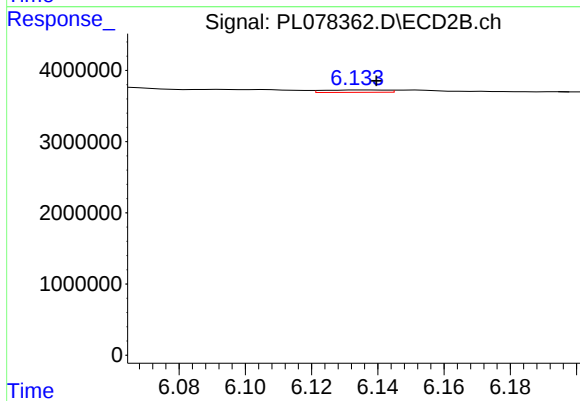

#19 Endosulfan Sulfate


R.T.: 6.135 min
Delta R.T.: -0.004 min
Response: 447579
Conc: 0.19 ng/ml

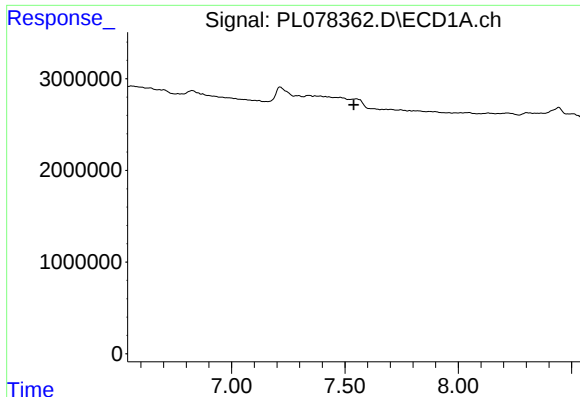

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.539 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

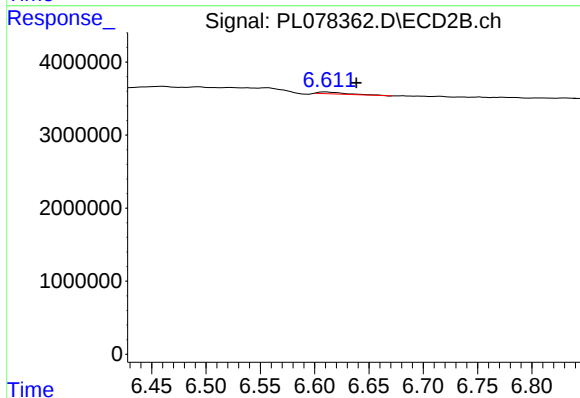


#21 Endrin ketone

R.T.: 6.610 min
Delta R.T.: -0.028 min
Response: 452930
Conc: 0.17 ng/ml

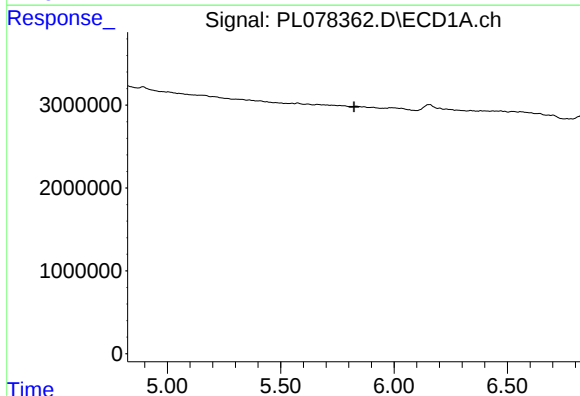


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.823 min
Response: 0
Conc: N.D.

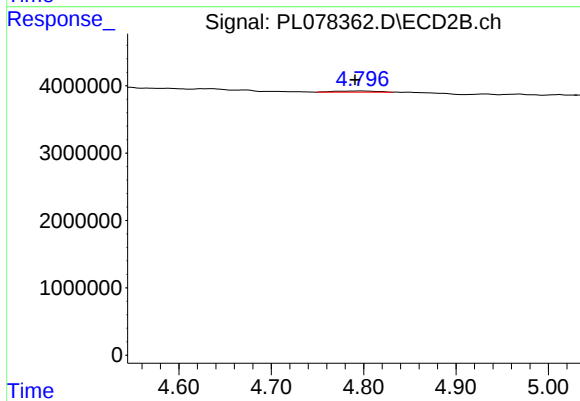

#25 Chlordane-3


R.T.: 4.797 min
Delta R.T.: 0.007 min
Response: 501910
Conc: 1.64 ng/ml

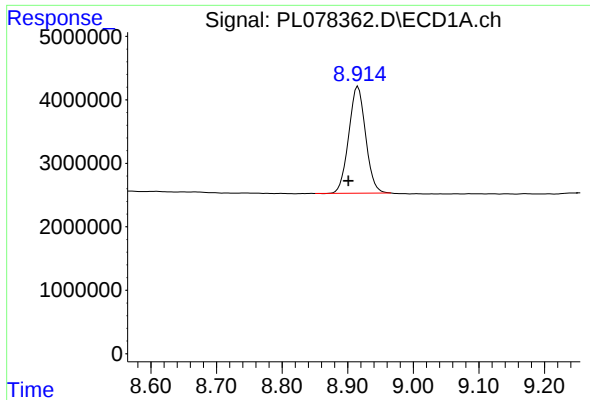

#28 Decachlorobiphenyl

R.T.: 8.916 min
Delta R.T.: 0.015 min
Response: 30082943
Conc: 19.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

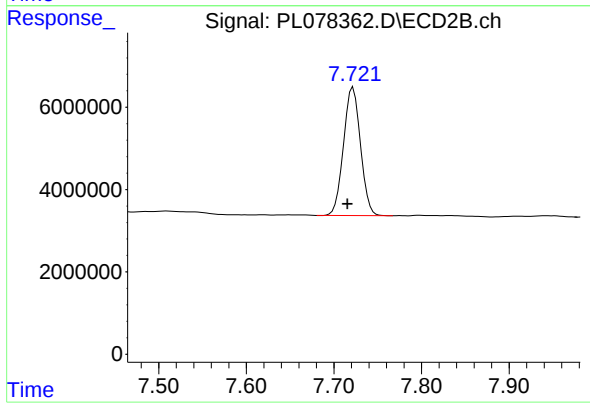

#28 Decachlorobiphenyl

R.T.: 7.722 min
Delta R.T.: 0.006 min
Response: 42023586
Conc: 19.33 ng/ml