

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101422\
 Data File : PL078367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2022 15:35
 Operator : AR\AJ
 Sample : N5142-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 00:21:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 15:30:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.413	2.622	27558343	42894359	16.676	16.228
28)	SA Decachlor...	8.906	7.718	25083680	32023111	16.248	14.731
Target Compounds							
8)	B Heptachlo...	5.592f	0.000	1598730	0	1.050	N.D. #
11)	B alpha-Chl...	5.897	0.000	311532	0	0.174	N.D. #
12)	B 4,4'-DDE	6.074	5.047	960456	2521755	0.570	0.882 #
14)	MA Endrin	0.000	5.465f	0	386244	N.D.	0.168 #
15)	B Endosulfa...	6.706f	0.000	527010	0	0.393	N.D. #
17)	MA 4,4'-DDT	0.000	5.840	0	800938	N.D.	0.353 #
22)	Mirex	8.022f	0.000	231488	0	0.196	N.D. #
24)	Chlordane-2	0.000	4.141f	0	267556	N.D.	2.655 #
26)	Chlordane-4	5.897	0.000	311532	0	0.975	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101422\
Data File : PL078367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2022 15:35
Operator : AR\AJ
Sample : N5142-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 00:21:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 15:30:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

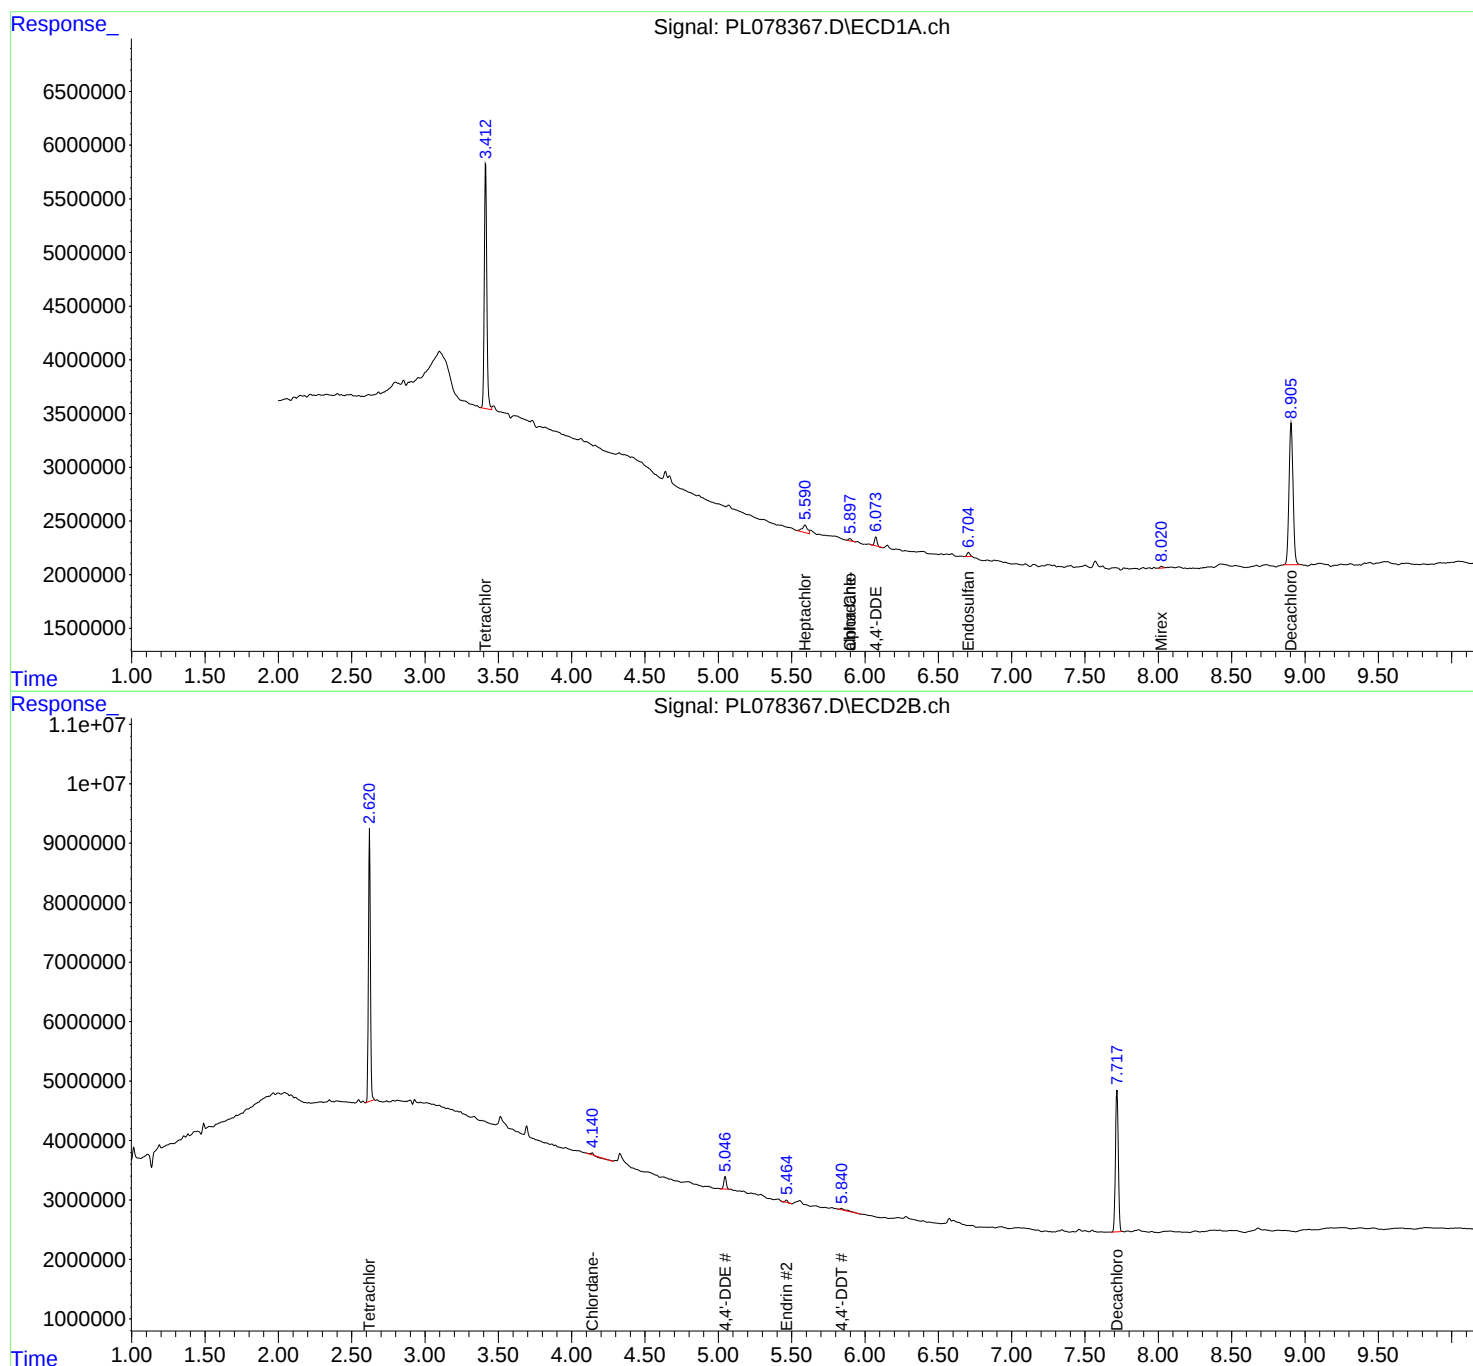


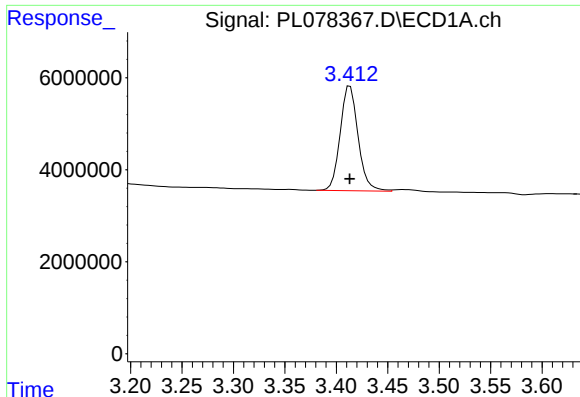

#1 Tetrachloro-m-xylene


R.T.: 3.413 min
Delta R.T.: 0.000 min
Response: 27558343
Conc: 16.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

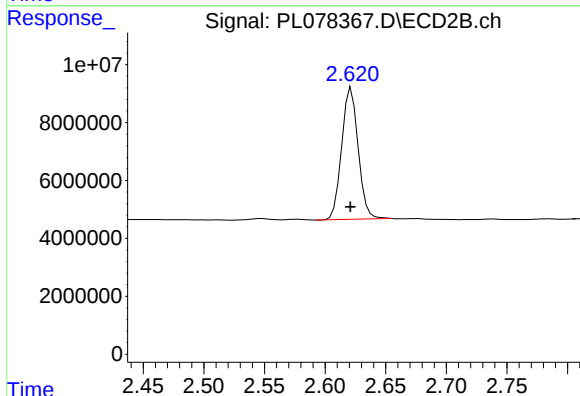


#1 Tetrachloro-m-xylene

R.T.: 2.622 min
Delta R.T.: 0.000 min
Response: 42894359
Conc: 16.23 ng/ml

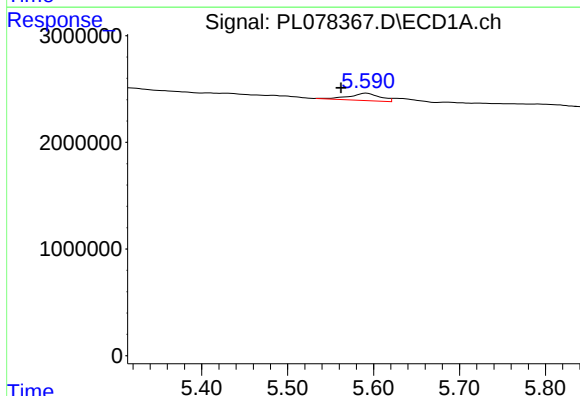


#8 Heptachlor epoxide

R.T.: 5.592 min
Delta R.T.: 0.030 min
Response: 1598730
Conc: 1.05 ng/ml

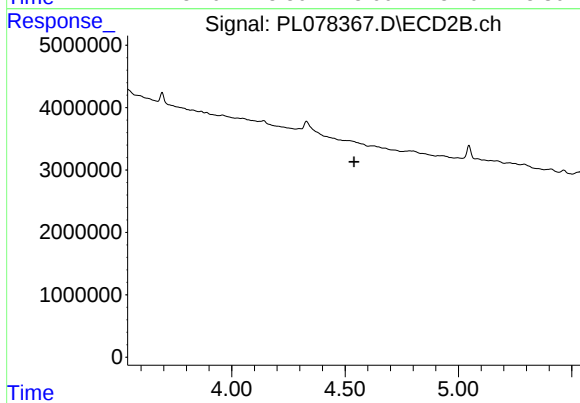

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.540 min
Response: 0
Conc: N.D.

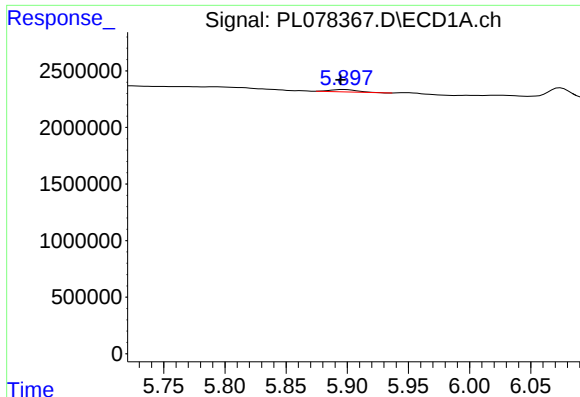

#11 alpha-Chlordane


R.T.: 5.897 min
Delta R.T.: 0.003 min
Response: 311532
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

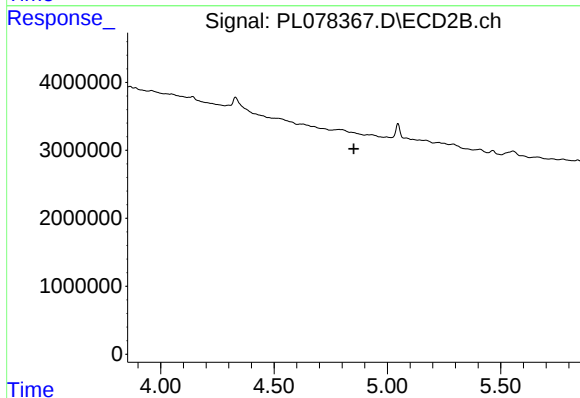


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.852 min
Response: 0
Conc: N.D.

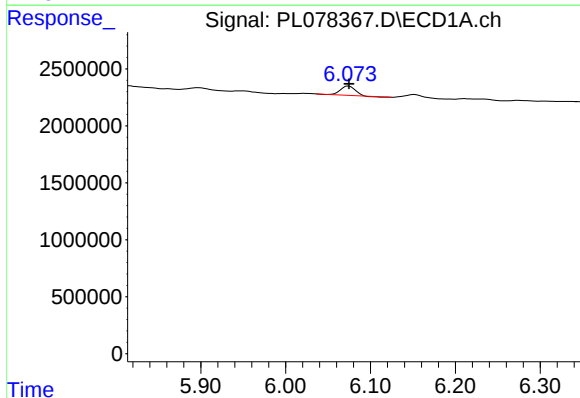


#12 4,4'-DDE

R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 960456
Conc: 0.57 ng/ml

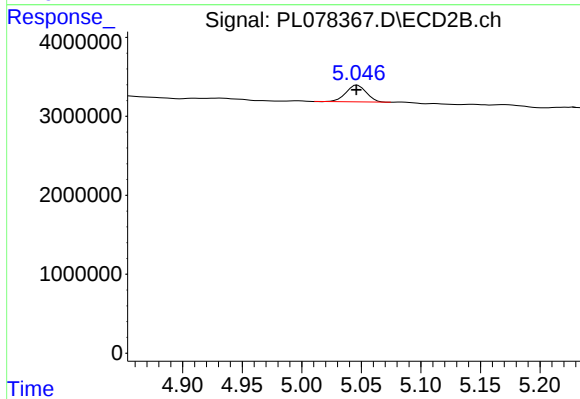

#12 4,4'-DDE


R.T.: 5.047 min
Delta R.T.: 0.001 min
Response: 2521755
Conc: 0.88 ng/ml

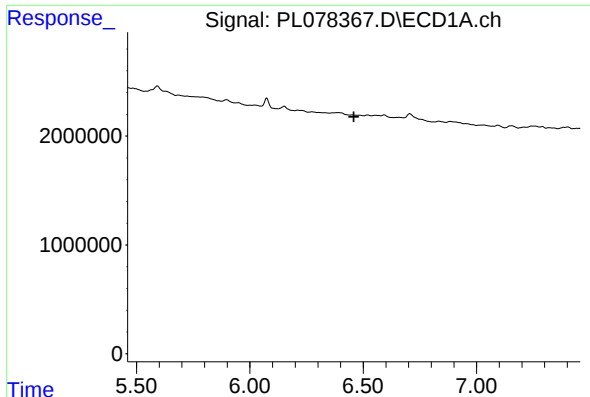

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

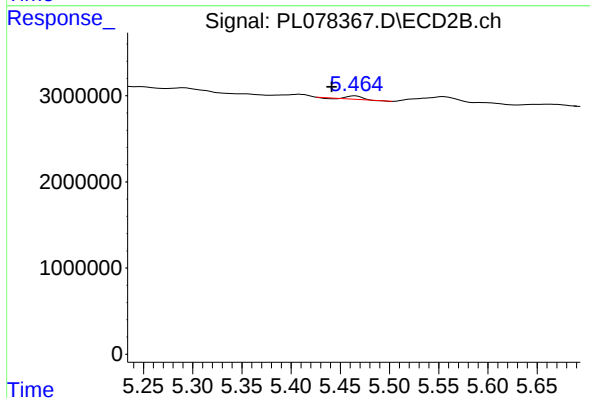


#14 Endrin

R.T.: 5.465 min
Delta R.T.: 0.024 min
Response: 386244
Conc: 0.17 ng/ml

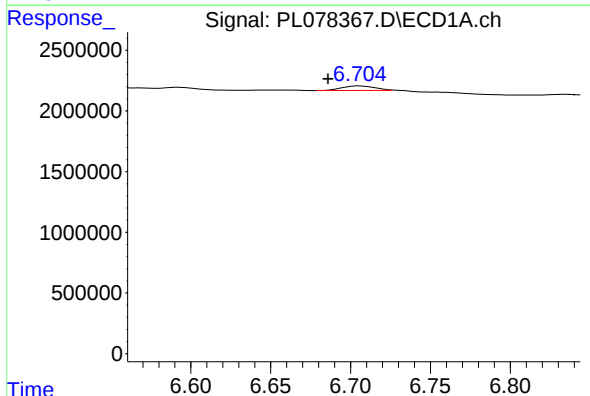


#15 Endosulfan II

R.T.: 6.706 min
Delta R.T.: 0.020 min
Response: 527010
Conc: 0.39 ng/ml

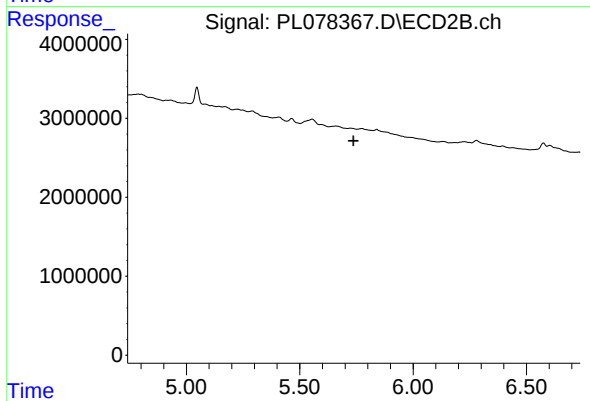

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.737 min
Response: 0
Conc: N.D.

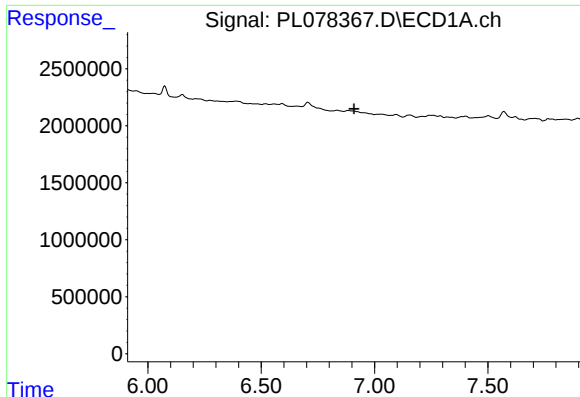

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

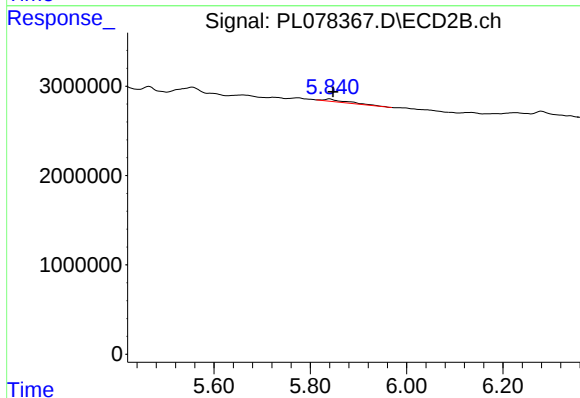


#17 4,4'-DDT

R.T.: 5.840 min
Delta R.T.: -0.007 min
Response: 800938
Conc: 0.35 ng/ml

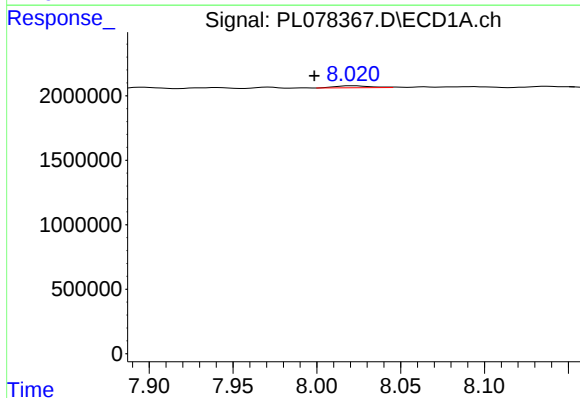


#22 Mirex

R.T.: 8.022 min
Delta R.T.: 0.023 min
Response: 231488
Conc: 0.20 ng/ml

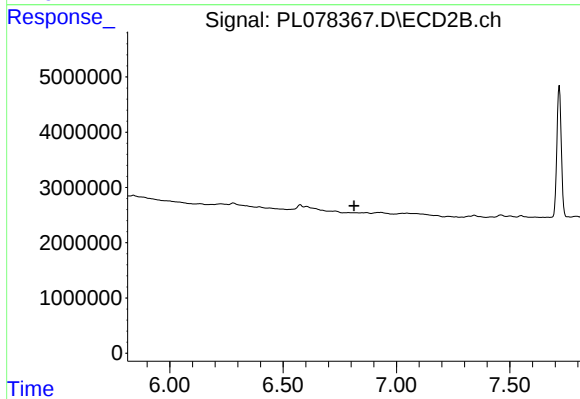

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 6.813 min
Response: 0
Conc: N.D.

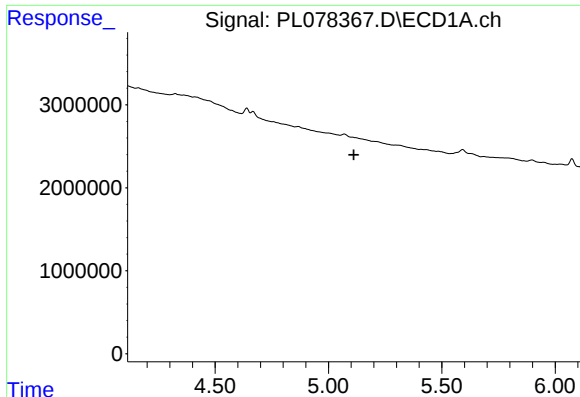

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.111 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

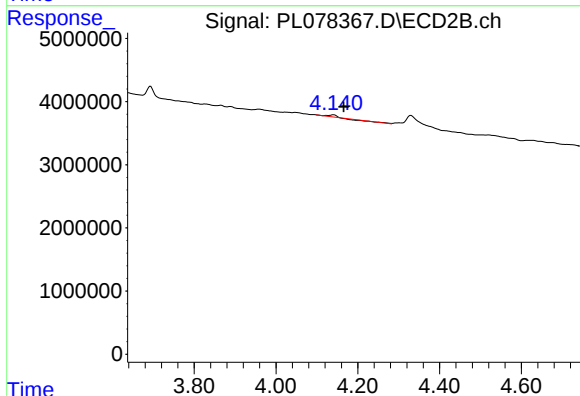


#24 Chlordane-2

R.T.: 4.141 min
Delta R.T.: -0.024 min
Response: 267556
Conc: 2.65 ng/ml

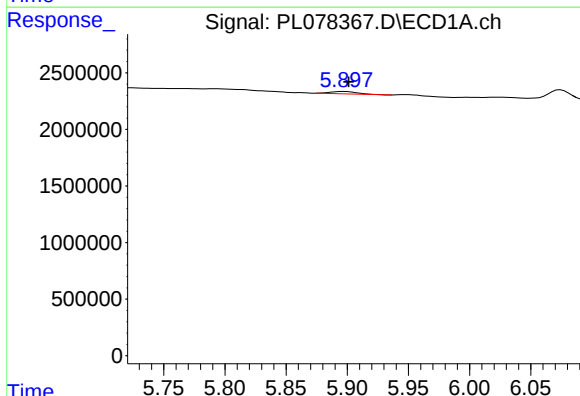


#26 Chlordane-4

R.T.: 5.897 min
Delta R.T.: -0.004 min
Response: 311532
Conc: 0.98 ng/ml

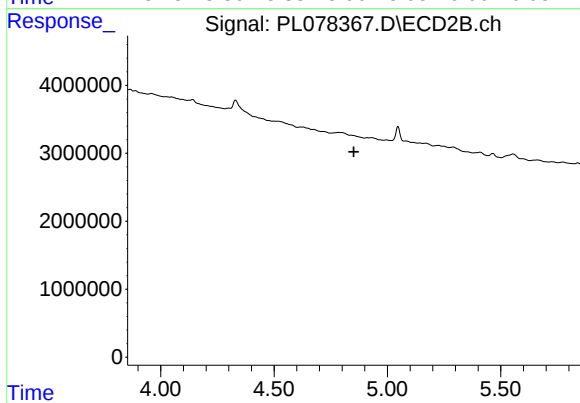

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 4.852 min
Response: 0
Conc: N.D.

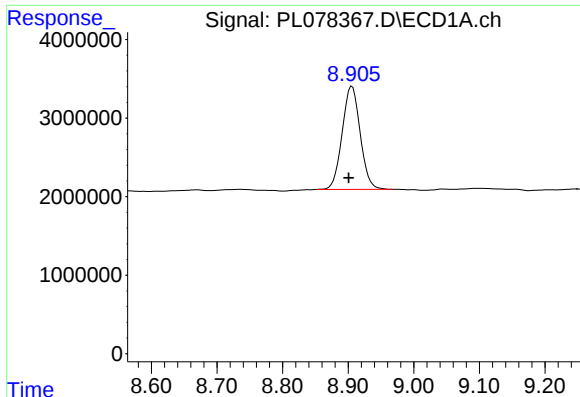

#28 Decachlorobiphenyl

R.T.: 8.906 min
Delta R.T.: 0.005 min
Response: 25083680
Conc: 16.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

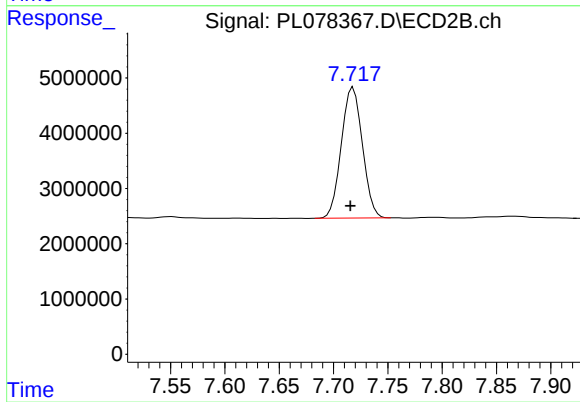

#28 Decachlorobiphenyl

R.T.: 7.718 min
Delta R.T.: 0.003 min
Response: 32023111
Conc: 14.73 ng/ml