

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101422\
 Data File : PL078370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2022 16:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 00:23:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 15:30:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.414	2.622	28040929	42786063	16.968	16.187
28)	SA Decachlor...	8.904	7.718	24473896	32941664	15.853	15.154
Target Compounds							
4)	MA Heptachlor	0.000	3.740f	0	52807	N.D.	0.015 #
5)	MB Aldrin	0.000	4.056	0	452261	N.D.	0.133 #
6)	B beta-BHC	0.000	3.740	0	52807	N.D.	0.036 #
8)	B Heptachlo...	5.569	0.000	89096	0	0.059	N.D. #
13)	MA Dieldrin	0.000	5.149f	0	435923	N.D.	0.149 #
14)	MA Endrin	0.000	5.464f	0	1325189	N.D.	0.575 #
15)	B Endosulfa...	6.707f	0.000	608171	0	0.454	N.D. #
19)	B Endosulfa...	0.000	6.146	0	34145	N.D.	0.014 #
22)	Mirex	8.013	0.000	54793	0	0.046	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101422\
Data File : PL078370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2022 16:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 00:23:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 15:30:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

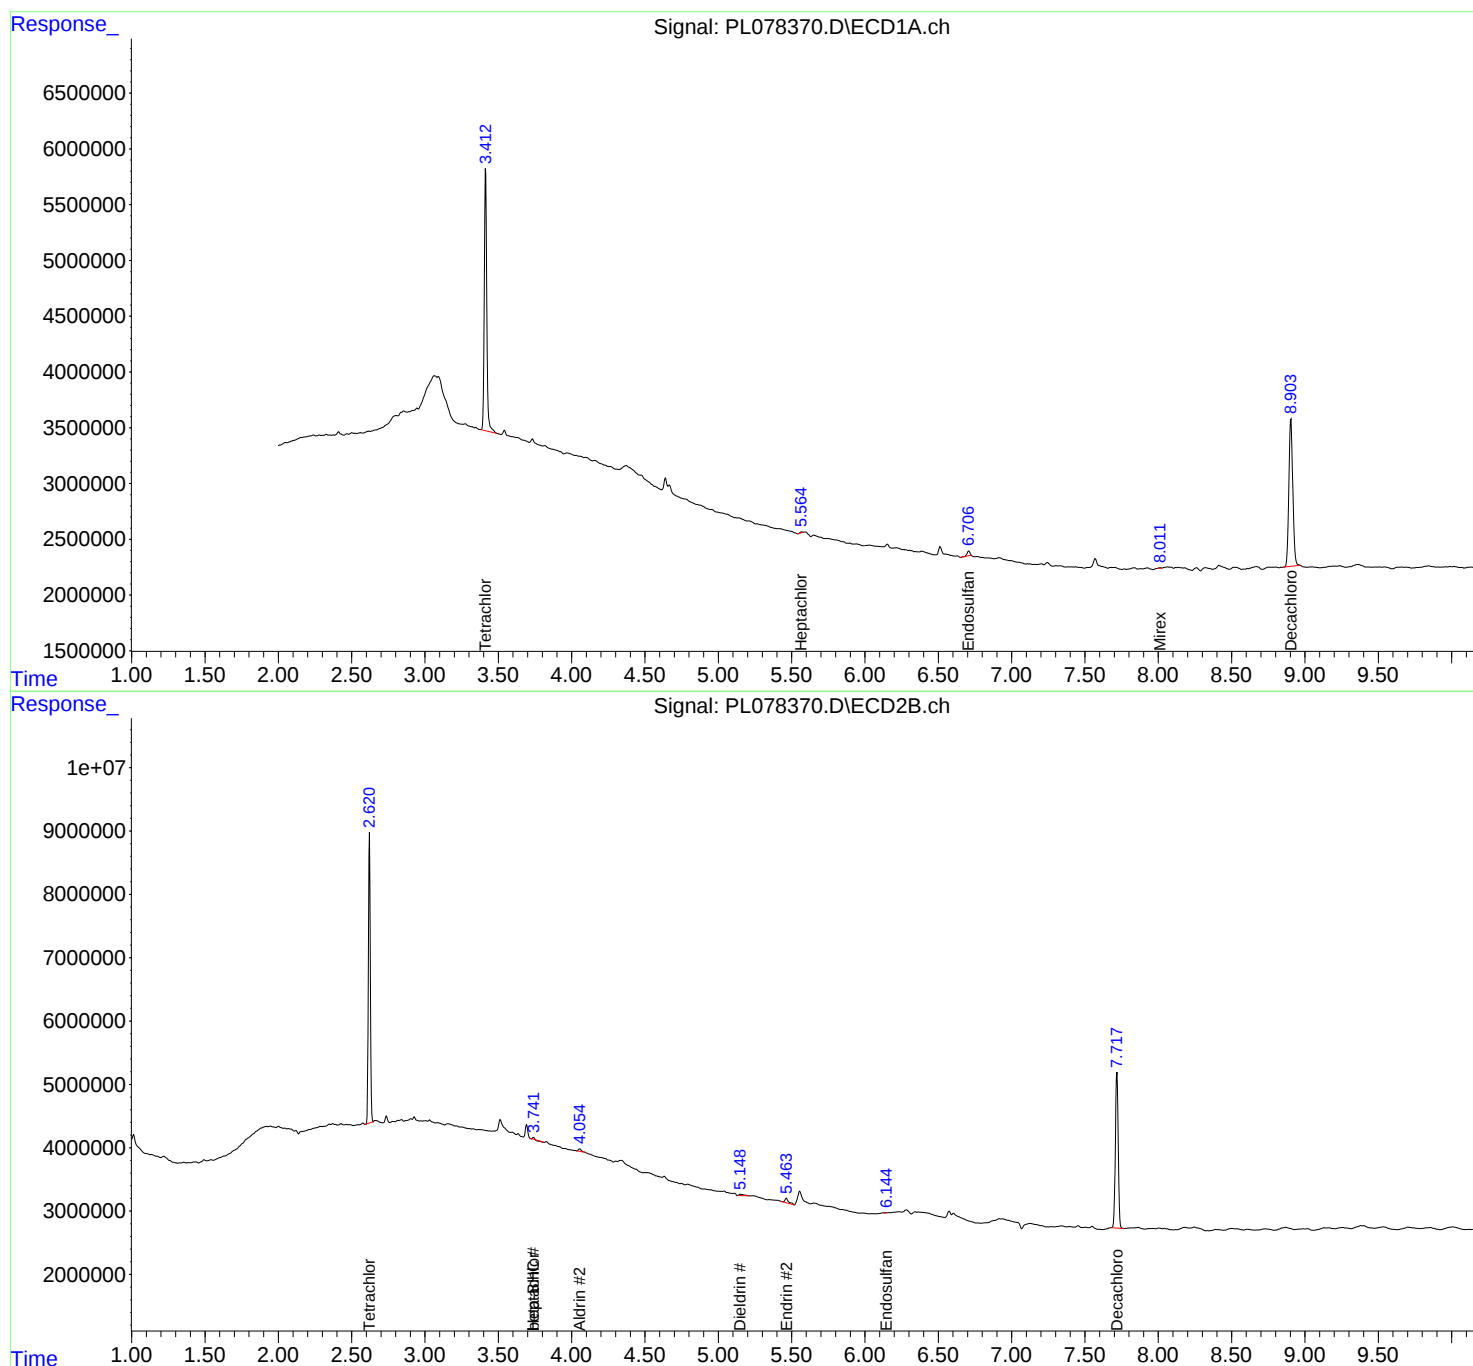


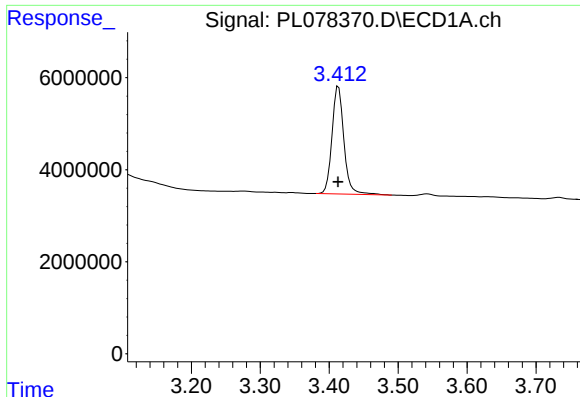

#1 Tetrachloro-m-xylene


R.T.: 3.414 min
Delta R.T.: 0.000 min
Response: 28040929
Conc: 16.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

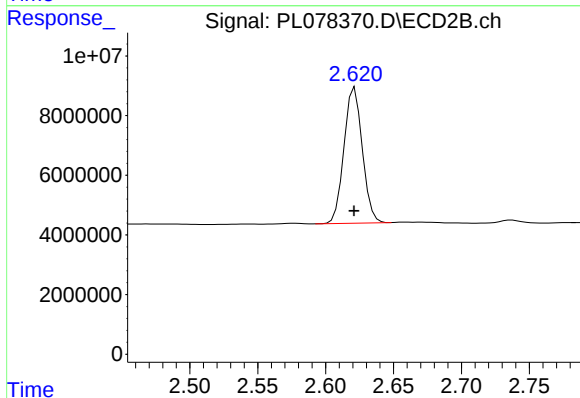


#1 Tetrachloro-m-xylene

R.T.: 2.622 min
Delta R.T.: 0.000 min
Response: 42786063
Conc: 16.19 ng/ml

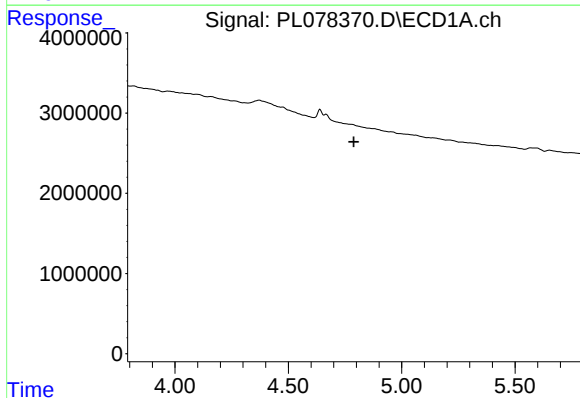


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.789 min
Response: 0
Conc: N.D.

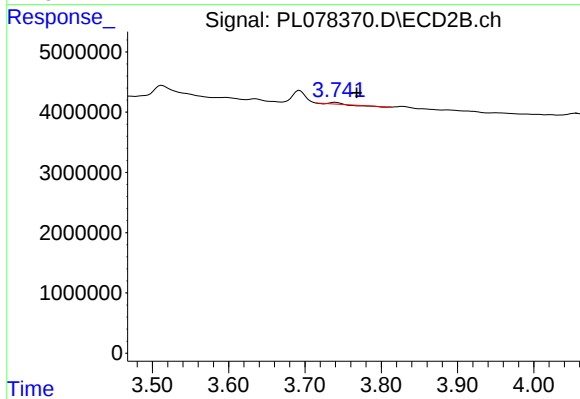

#4 Heptachlor


R.T.: 3.740 min
Delta R.T.: -0.028 min
Response: 52807
Conc: 0.01 ng/ml

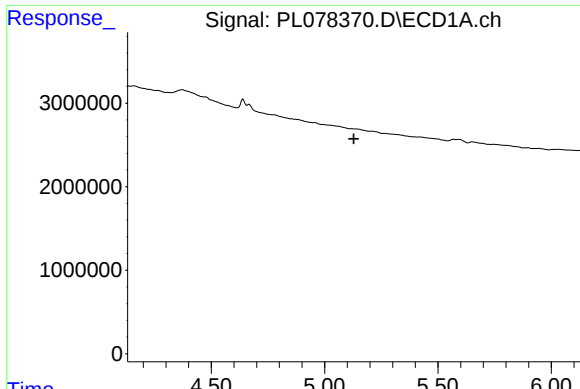

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

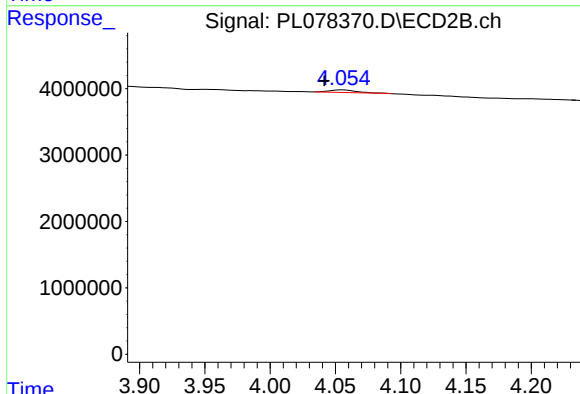


#5 Aldrin

R.T.: 4.056 min
Delta R.T.: 0.014 min
Response: 452261
Conc: 0.13 ng/ml

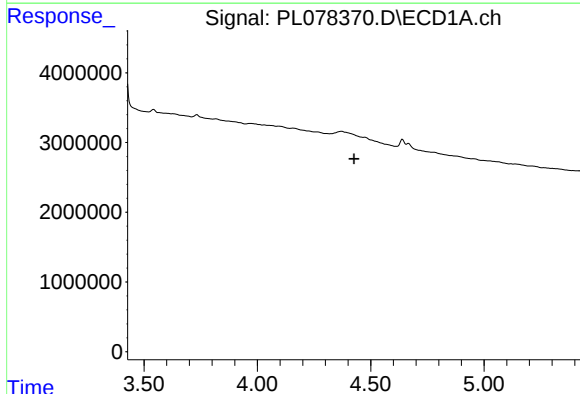


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.427 min
Response: 0
Conc: N.D.

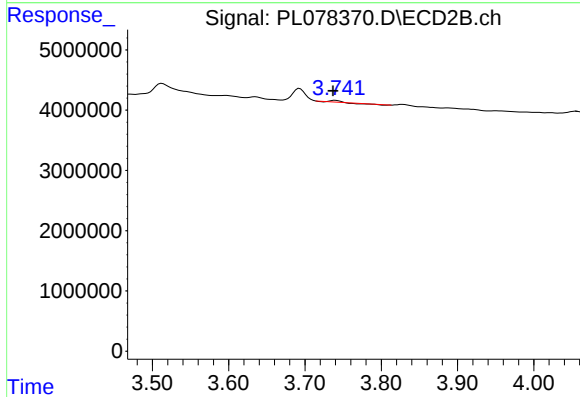

#6 beta-BHC


R.T.: 3.740 min
Delta R.T.: 0.003 min
Response: 52807
Conc: 0.04 ng/ml

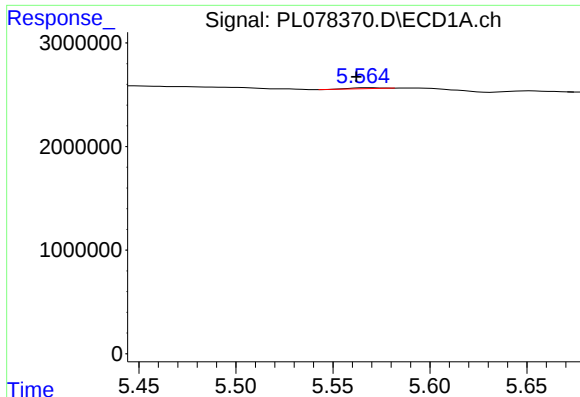

#8 Heptachlor epoxide


R.T.: 5.569 min
Delta R.T.: 0.007 min
Response: 89096
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

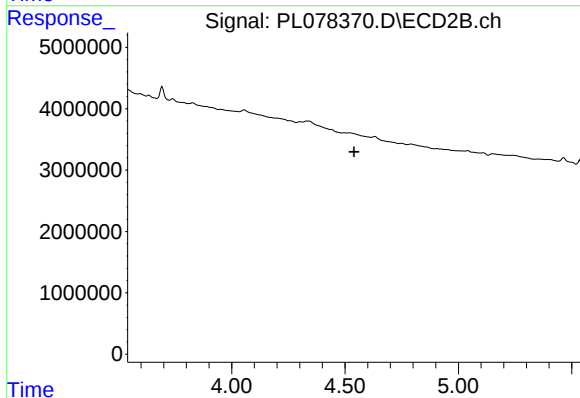


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.540 min
Response: 0
Conc: N.D.

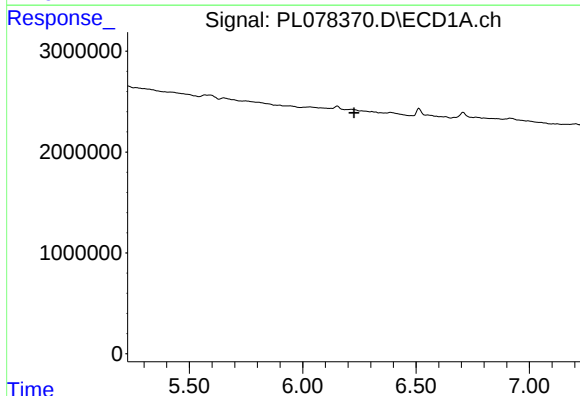


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.226 min
Response: 0
Conc: N.D.

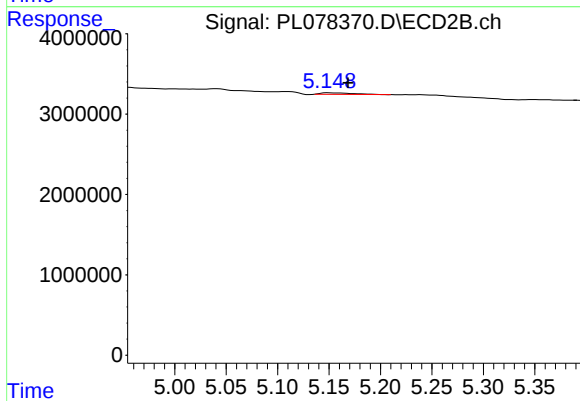

#13 Dieldrin


R.T.: 5.149 min
Delta R.T.: -0.019 min
Response: 435923
Conc: 0.15 ng/ml

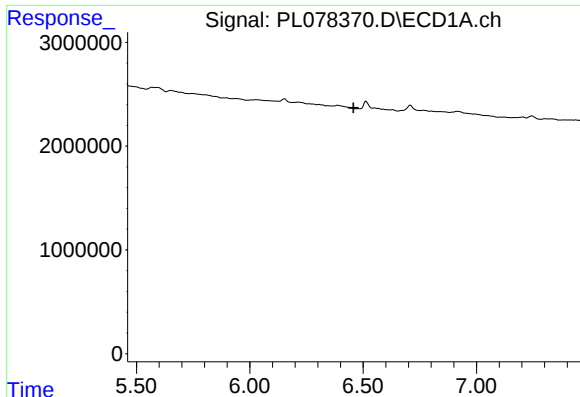

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

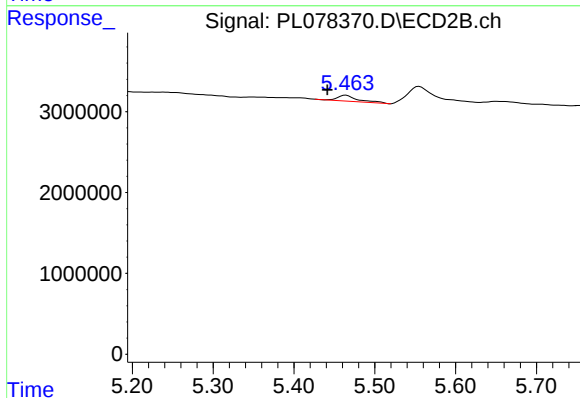


#14 Endrin

R.T.: 5.464 min
Delta R.T.: 0.023 min
Response: 1325189
Conc: 0.58 ng/ml

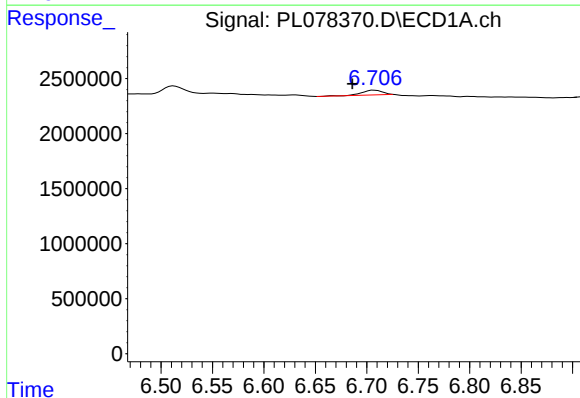


#15 Endosulfan II

R.T.: 6.707 min
Delta R.T.: 0.022 min
Response: 608171
Conc: 0.45 ng/ml

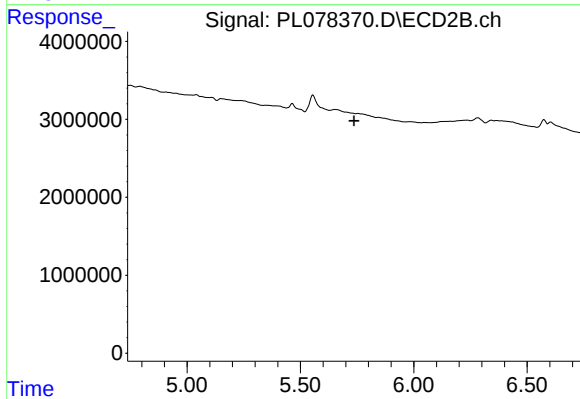

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.737 min
Response: 0
Conc: N.D.

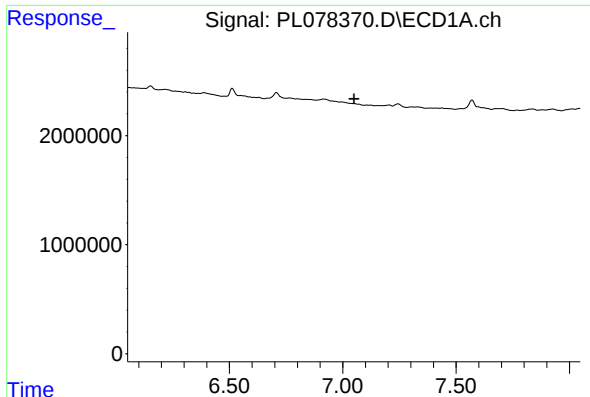

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

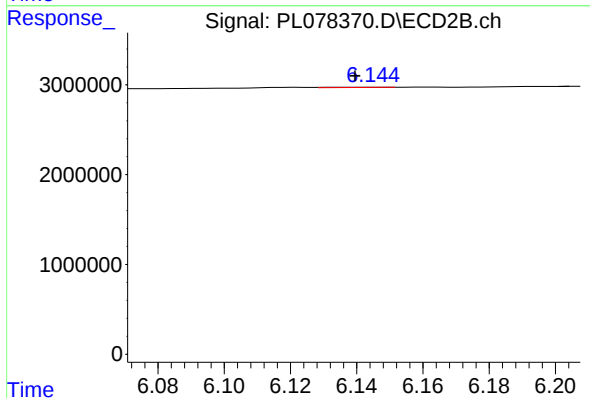


#19 Endosulfan Sulfate

R.T.: 6.146 min
Delta R.T.: 0.007 min
Response: 34145
Conc: 0.01 ng/ml

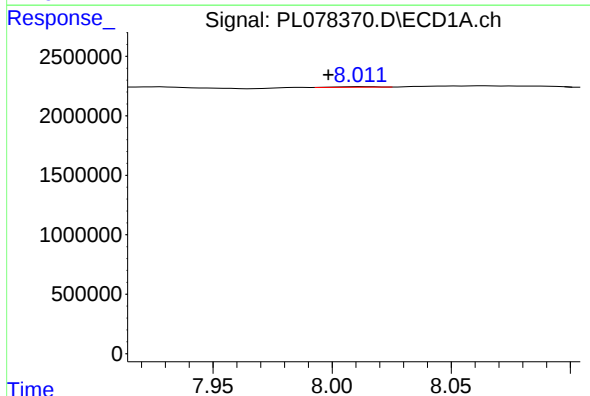


#22 Mirex

R.T.: 8.013 min
Delta R.T.: 0.014 min
Response: 54793
Conc: 0.05 ng/ml

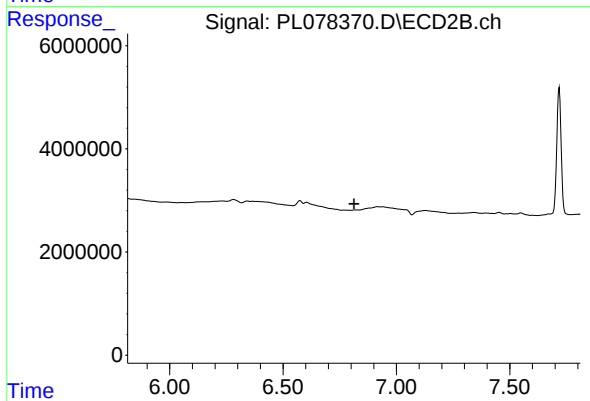

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 6.813 min
Response: 0
Conc: N.D.

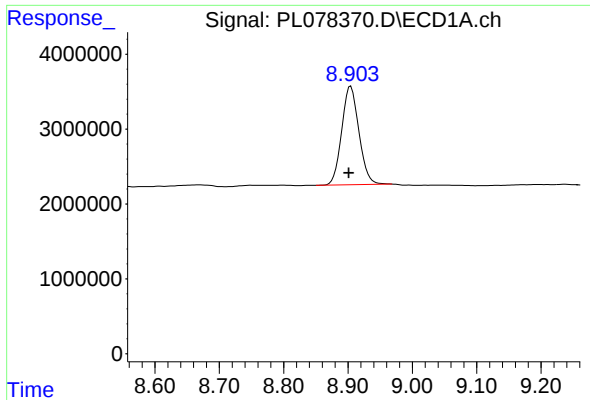

#28 Decachlorobiphenyl

R.T.: 8.904 min
Delta R.T.: 0.003 min
Response: 24473896
Conc: 15.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

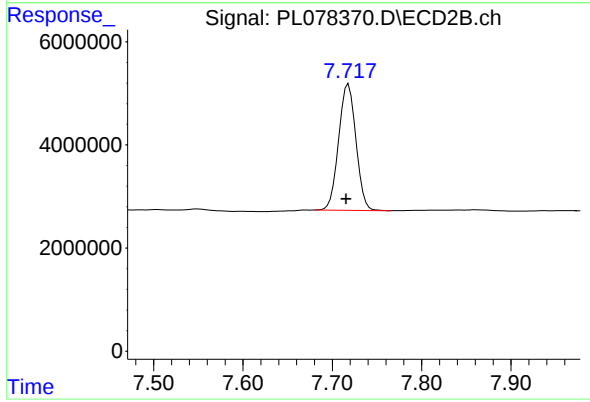

#28 Decachlorobiphenyl

R.T.: 7.718 min
Delta R.T.: 0.003 min
Response: 32941664
Conc: 15.15 ng/ml