

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101424\
 Data File : PL092352.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2024 11:57
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 01:56:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 16:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.781	104.3E6	143.6E6	46.901	57.258
28)	SA Decachlor...	9.069	7.924	77091400	112.4E6	47.058	44.942
Target Compounds							
23)	Chlordane-1	4.711	3.779	46475474	47373299	453.444	473.824
24)	Chlordane-2	5.240	4.357	50081133	51541165	466.972	459.262
25)	Chlordane-3	5.951	4.988	172.7E6	159.1E6	461.114	480.420
26)	Chlordane-4	6.033	5.050	208.5E6	151.5E6	460.472	477.421
27)	Chlordane-5	6.883	5.947	40212600	52987666	461.074	488.593



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101424\
Data File : PL092352.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2024 11:57
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 01:56:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 16:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

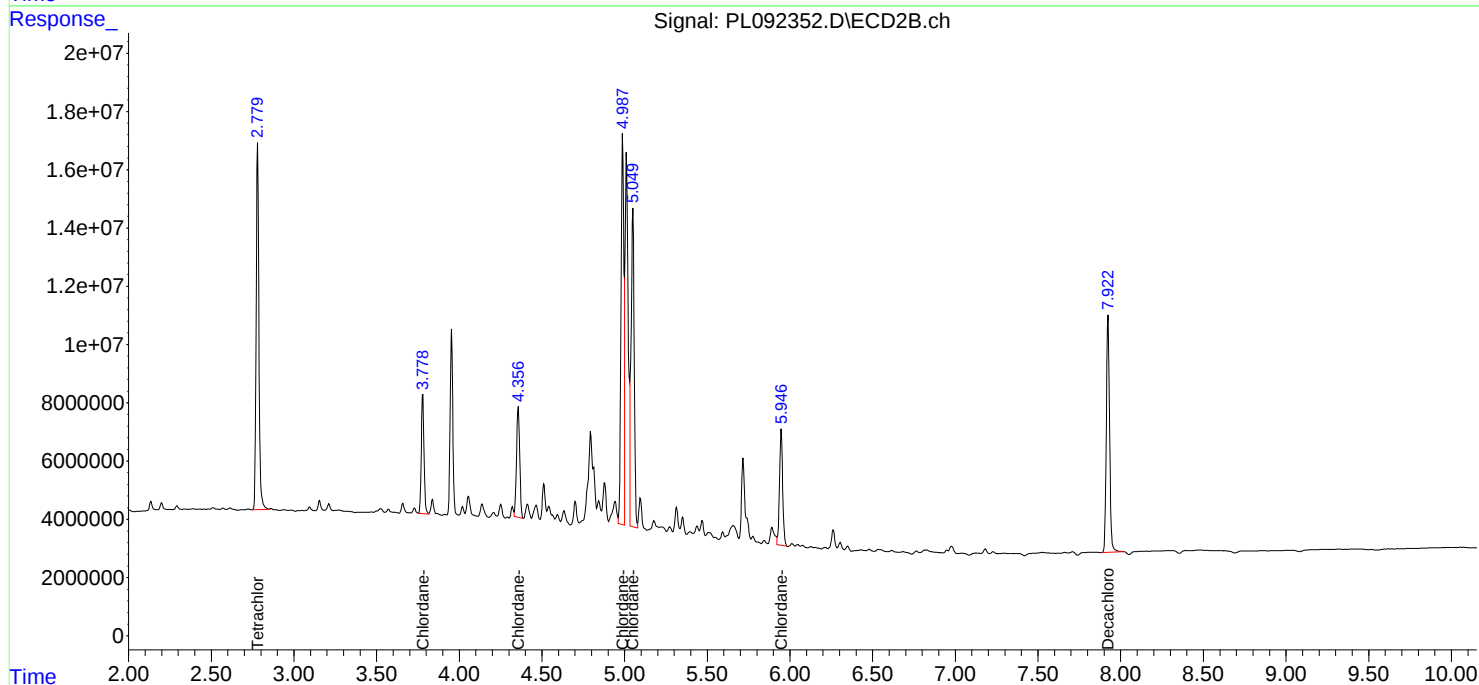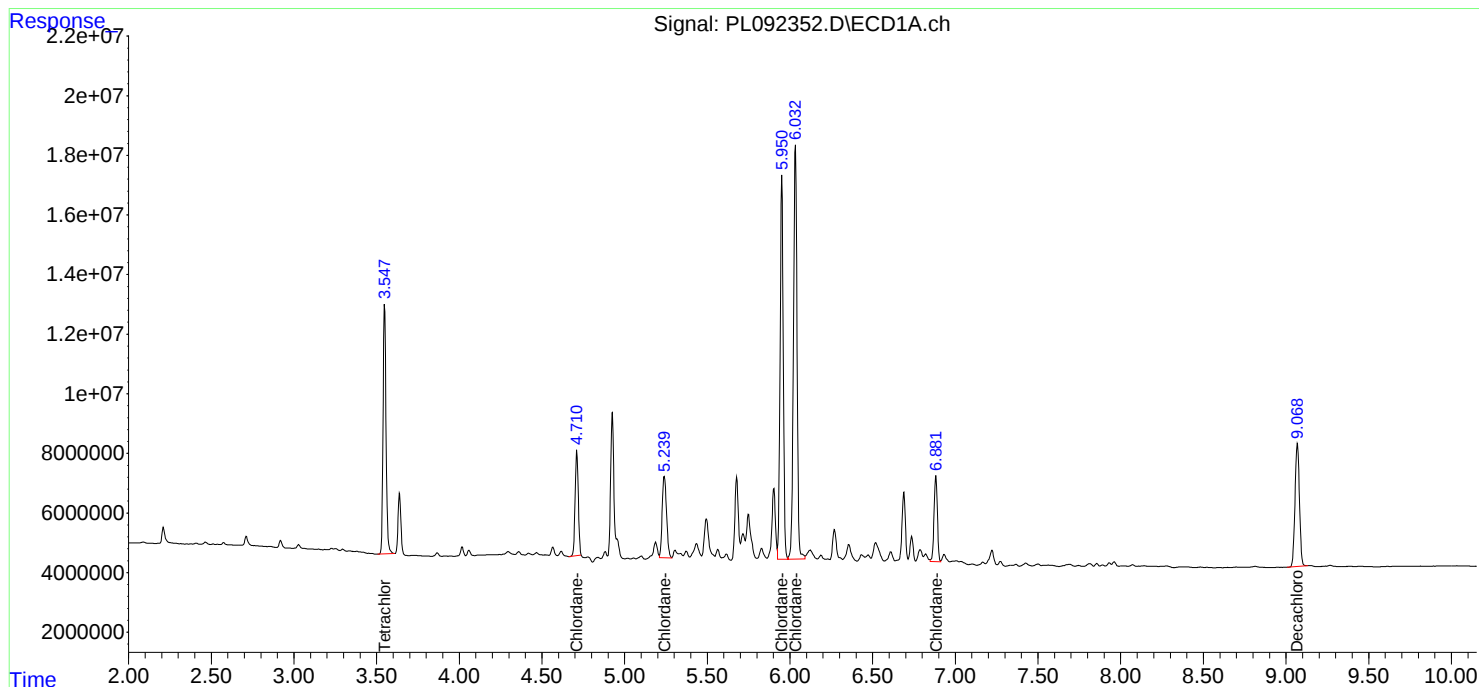


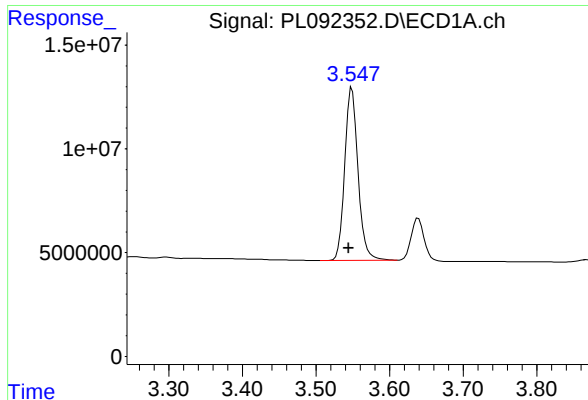

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.005 min
Response: 104338262
Conc: 46.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

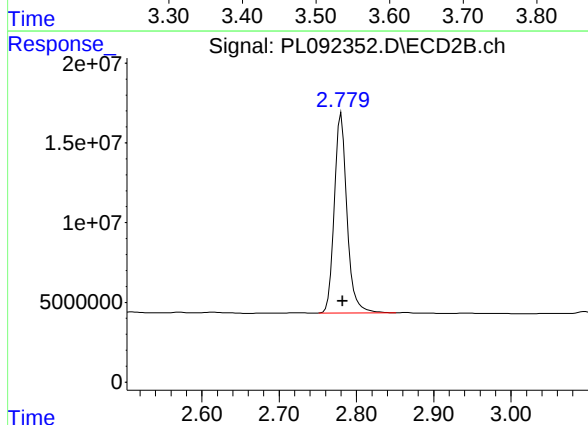


#1 Tetrachloro-m-xylene

R.T.: 2.781 min
Delta R.T.: -0.002 min
Response: 143608584
Conc: 57.26 ng/ml

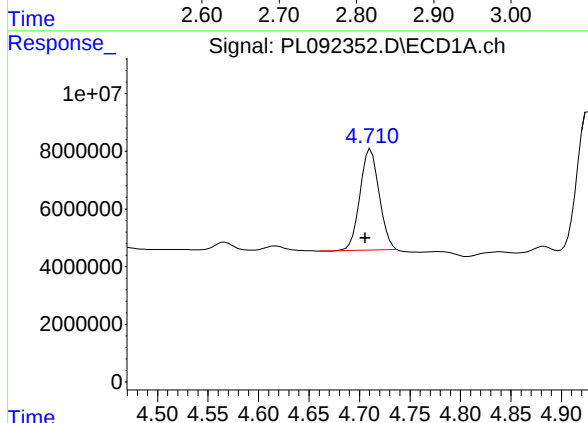


#23 Chlordane-1

R.T.: 4.711 min
Delta R.T.: 0.005 min
Response: 46475474
Conc: 453.44 ng/ml

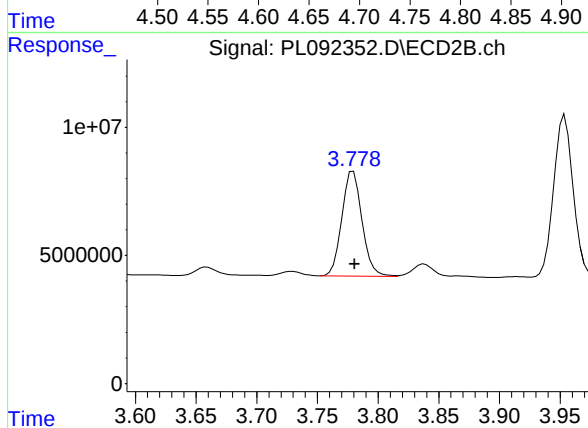

#23 Chlordane-1


R.T.: 3.779 min
Delta R.T.: -0.001 min
Response: 47373299
Conc: 473.82 ng/ml

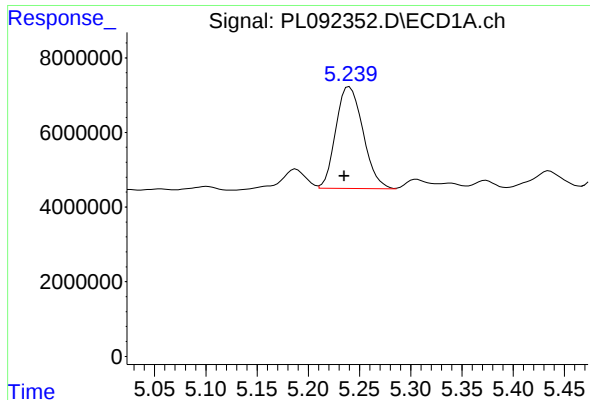

#24 Chlordane-2


R.T.: 5.240 min
Delta R.T.: 0.005 min
Response: 50081133
Conc: 466.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

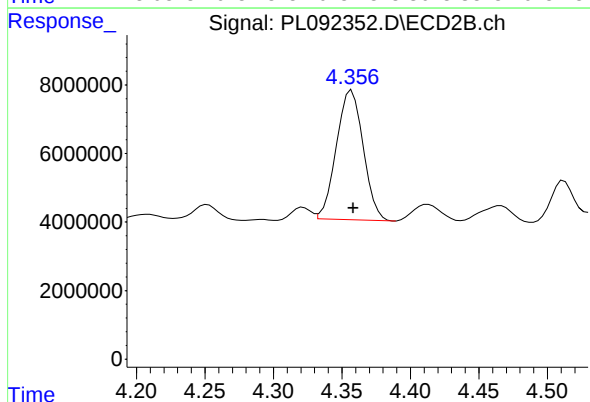


#24 Chlordane-2

R.T.: 4.357 min
Delta R.T.: -0.001 min
Response: 51541165
Conc: 459.26 ng/ml

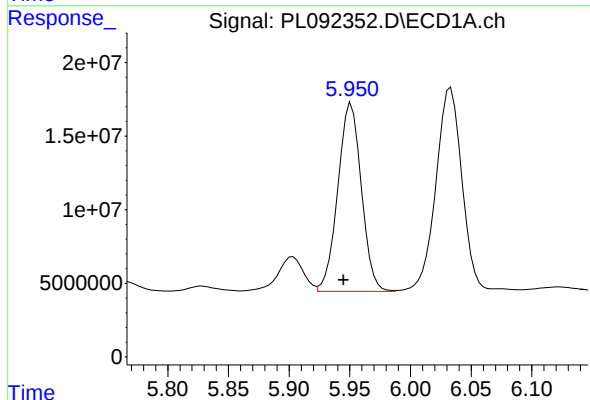


#25 Chlordane-3

R.T.: 5.951 min
Delta R.T.: 0.006 min
Response: 172722629
Conc: 461.11 ng/ml

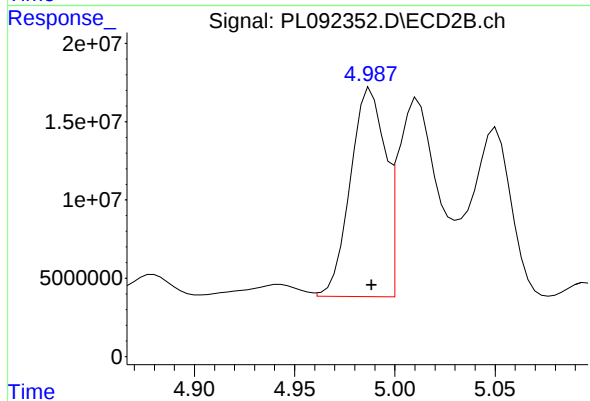

#25 Chlordane-3


R.T.: 4.988 min
Delta R.T.: 0.000 min
Response: 159128656
Conc: 480.42 ng/ml

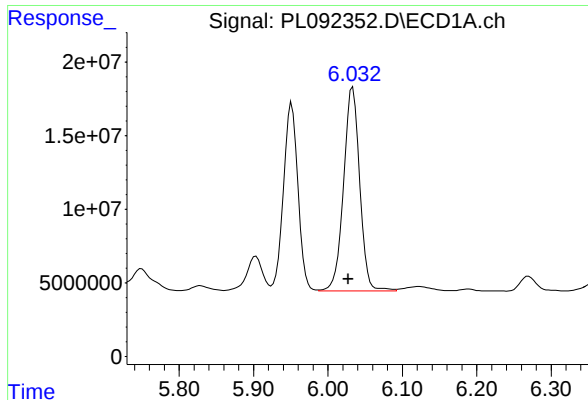

#26 Chlordane-4


R.T.: 6.033 min
Delta R.T.: 0.006 min
Response: 208523114
Conc: 460.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

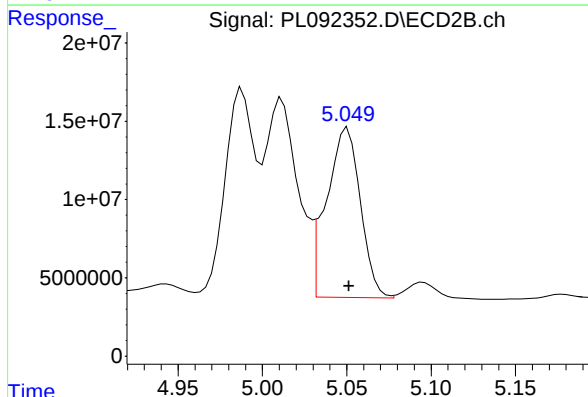


#26 Chlordane-4

R.T.: 5.050 min
Delta R.T.: 0.000 min
Response: 151476948
Conc: 477.42 ng/ml

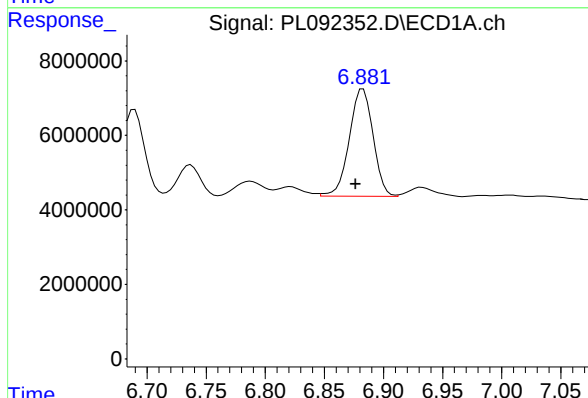


#27 Chlordane-5

R.T.: 6.883 min
Delta R.T.: 0.006 min
Response: 40212600
Conc: 461.07 ng/ml

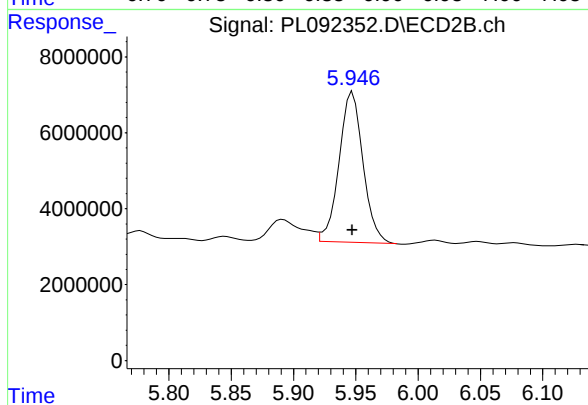

#27 Chlordane-5


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 52987666
Conc: 488.59 ng/ml

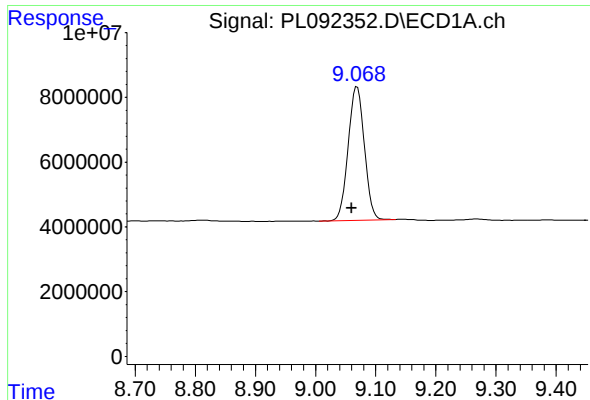

#28 Decachlorobiphenyl

R.T.: 9.069 min
Delta R.T.: 0.009 min
Response: 77091400
Conc: 47.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

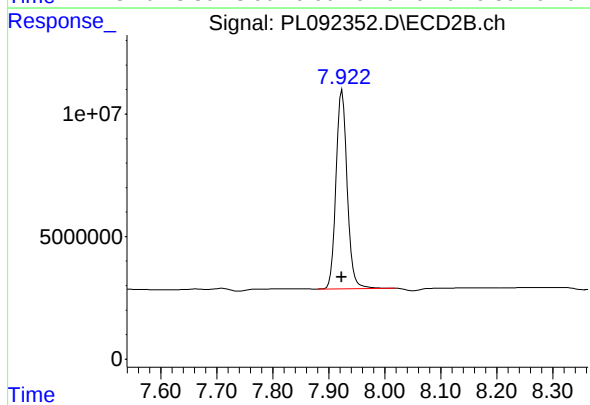

#28 Decachlorobiphenyl

R.T.: 7.924 min
Delta R.T.: 0.001 min
Response: 112441375
Conc: 44.94 ng/ml