

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101519\
 Data File : PL053322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2019 19:09
 Operator : SG\AJ
 Sample : K5352-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-20A-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 00:56:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	4.046	126.8E6	33538582	12.752	12.490
28)	SA Decachlor...	8.335	9.125	122.2E6	37396099	12.205	12.747
Target Compounds							
7)	B delta-BHC	0.000	5.084f	0	2322958	N.D.	0.642 #
8)	B Heptachlo...	0.000	5.930	0	508883	N.D.	0.152 #
11)	B alpha-Chl...	0.000	6.233	0	825985	N.D.	0.245 #
12)	B 4,4'-DDE	0.000	6.387	0	427045	N.D.	0.131 #
15)	B Endosulfa...	0.000	6.970	0	3037625	N.D.	1.024 #
26)	B Chlordane-4	0.000	6.233	0	825985	N.D.	1.556 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101519\
Data File : PL053322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2019 19:09
Operator : SG\AJ
Sample : K5352-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-20A-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 00:56:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

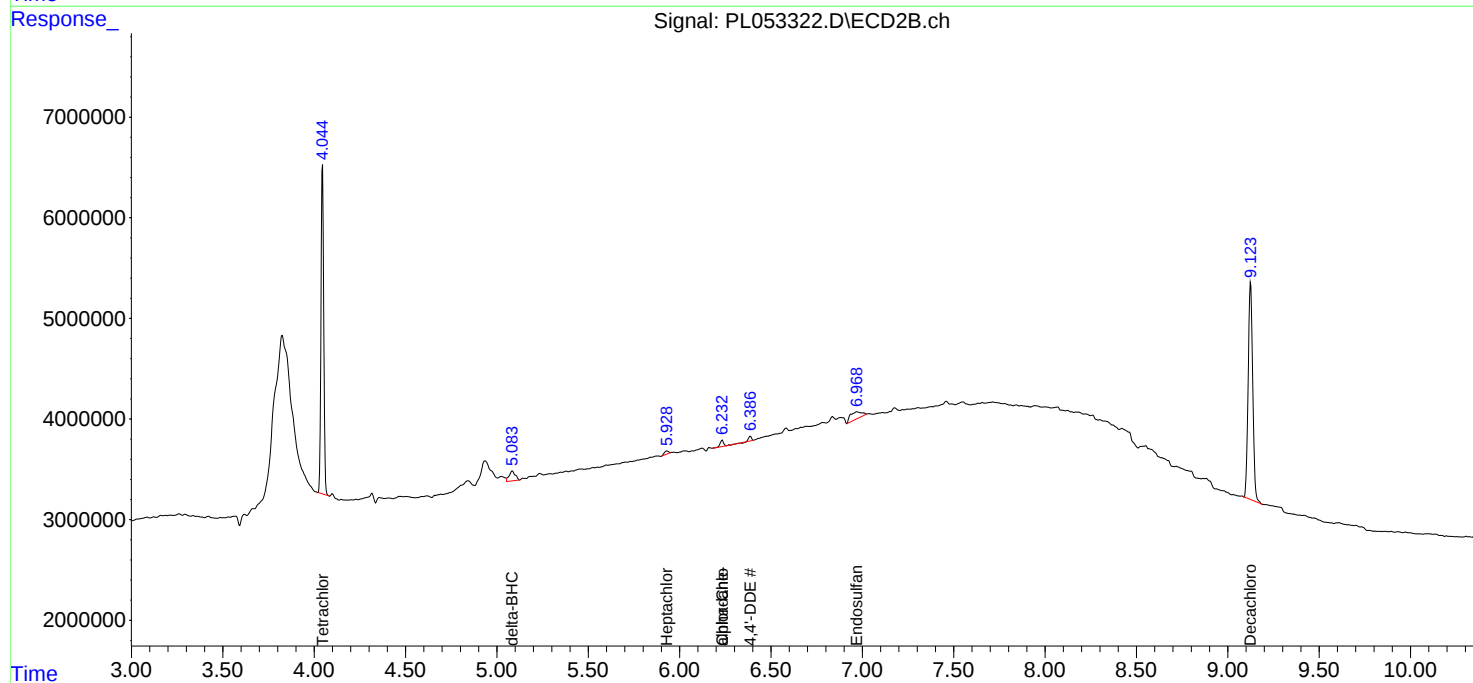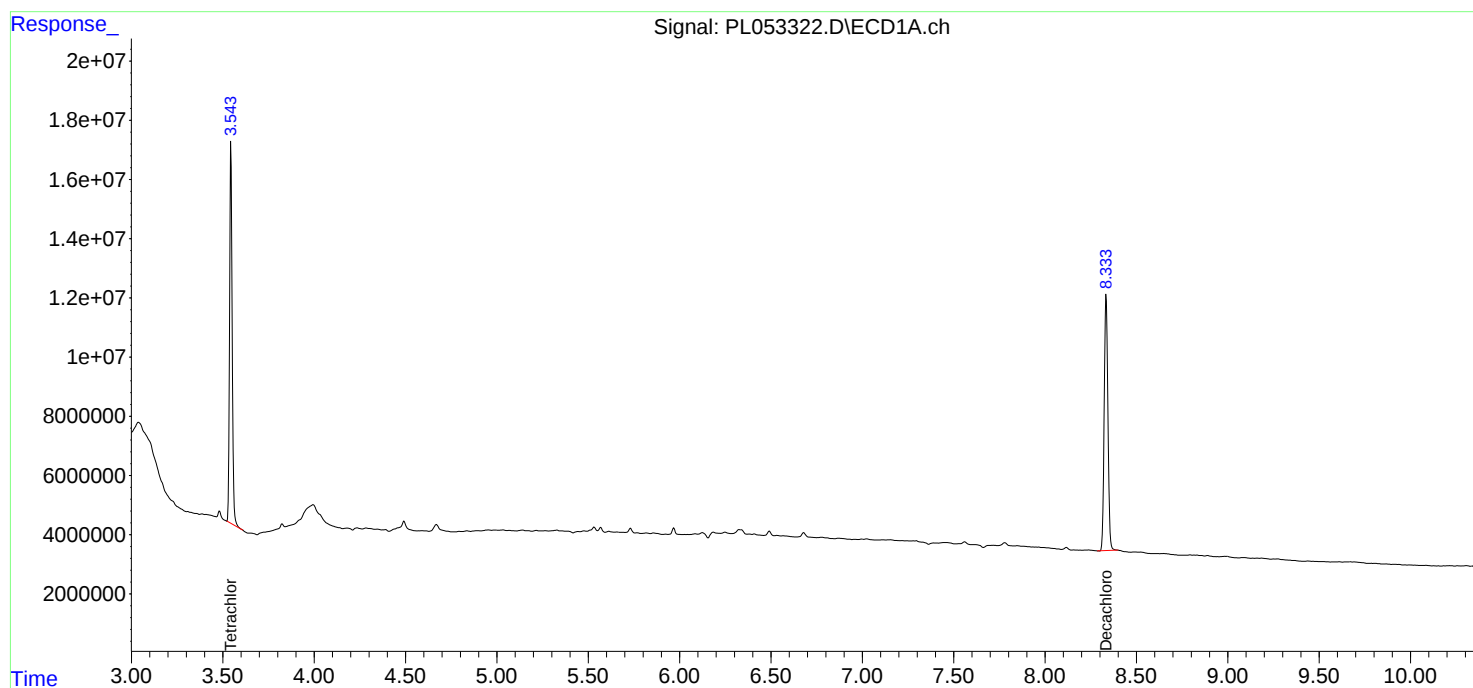


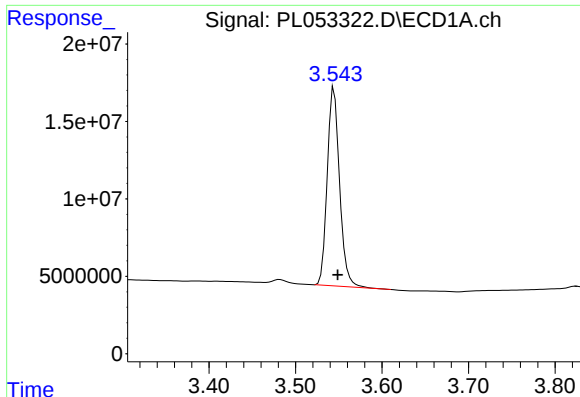

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: -0.004 min
Response: 126835902
Conc: 12.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-20A-S

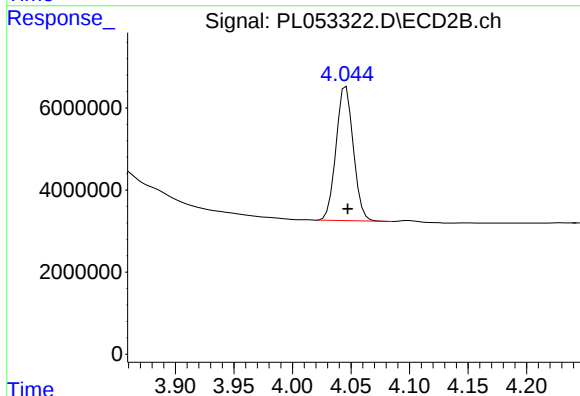


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: -0.001 min
Response: 33538582
Conc: 12.49 ng/ml

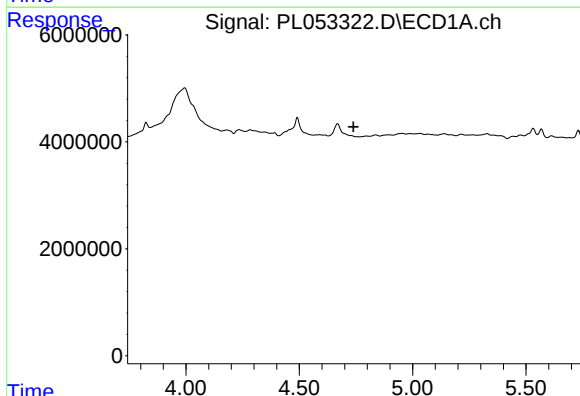


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.740 min
Response: 0
Conc: N.D.

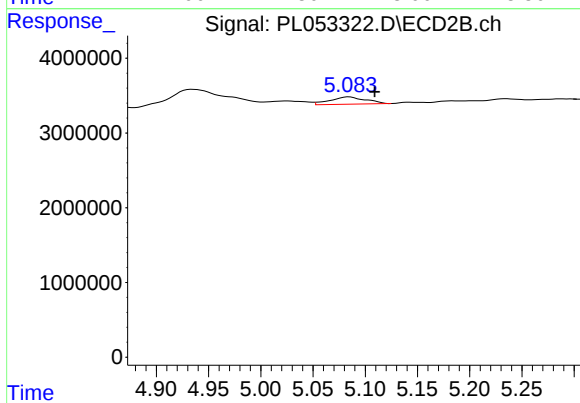

#7 delta-BHC


R.T.: 5.084 min
Delta R.T.: -0.025 min
Response: 2322958
Conc: 0.64 ng/ml

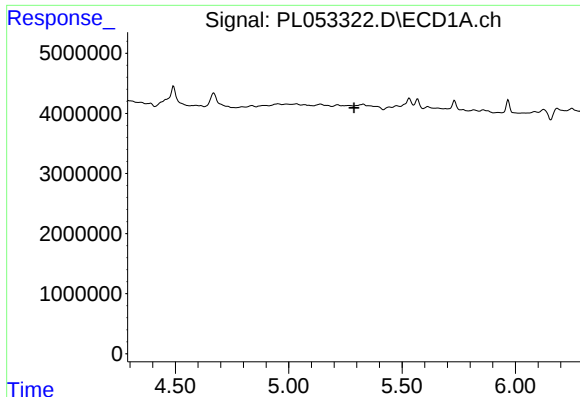

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-20A-S

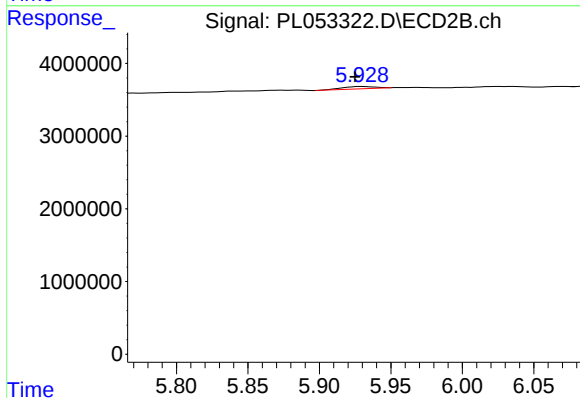


#8 Heptachlor epoxide

R.T.: 5.930 min
Delta R.T.: 0.005 min
Response: 508883
Conc: 0.15 ng/ml

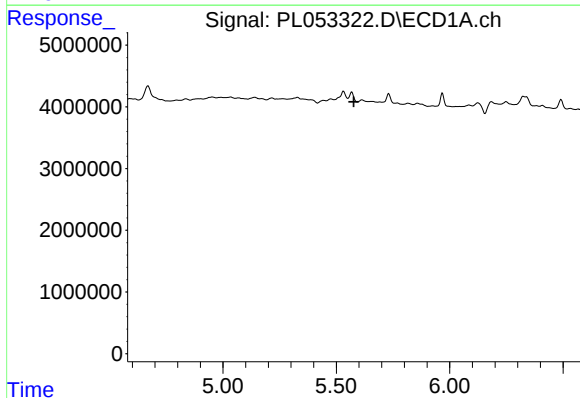


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

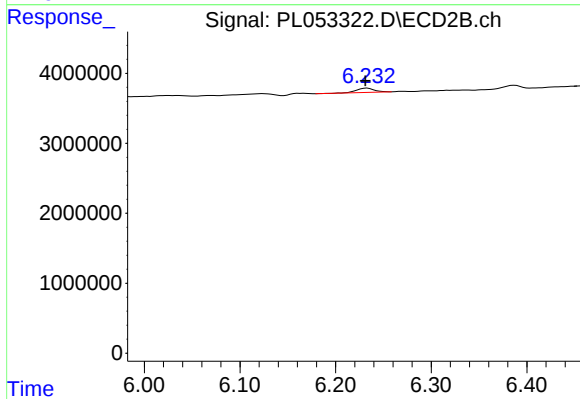

#11 alpha-Chlordane


R.T.: 6.233 min
Delta R.T.: 0.002 min
Response: 825985
Conc: 0.25 ng/ml

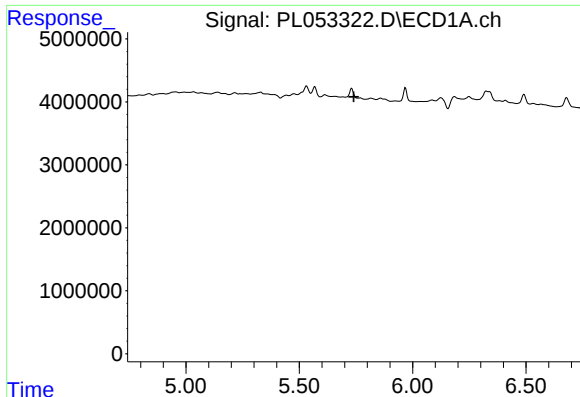

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.740 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-20A-S

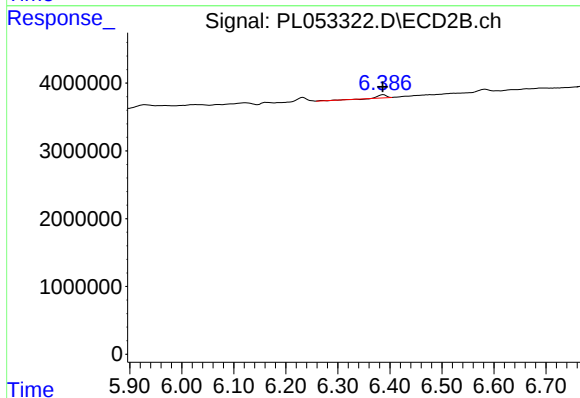


#12 4,4'-DDE

R.T.: 6.387 min
Delta R.T.: 0.000 min
Response: 427045
Conc: 0.13 ng/ml

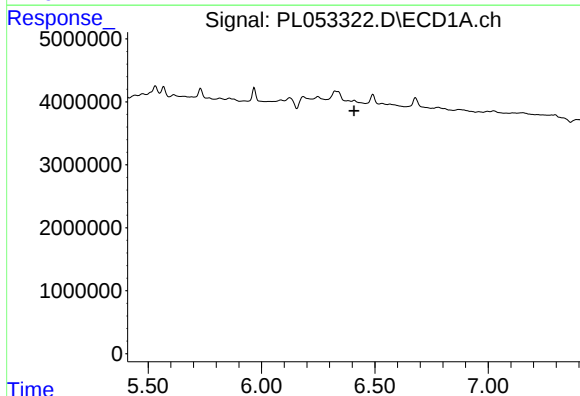


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

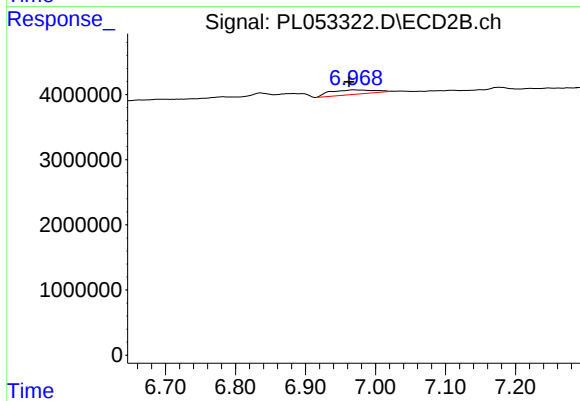

#15 Endosulfan II


R.T.: 6.970 min
Delta R.T.: 0.007 min
Response: 3037625
Conc: 1.02 ng/ml

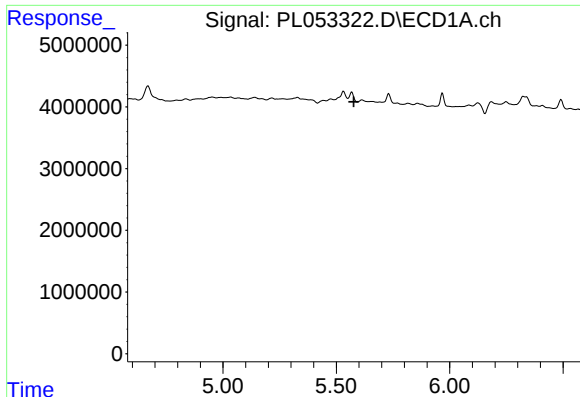

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-20A-S

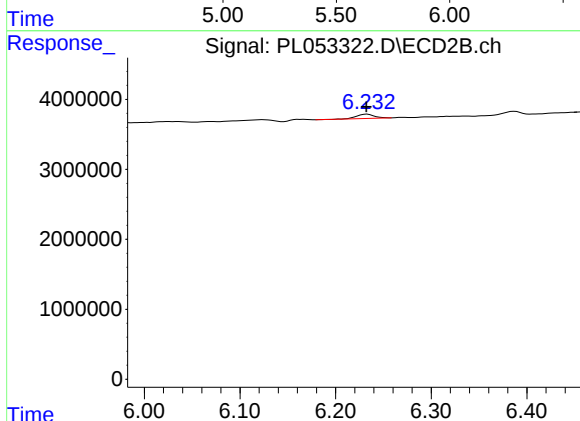


#26 Chlordane-4

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 825985
Conc: 1.56 ng/ml

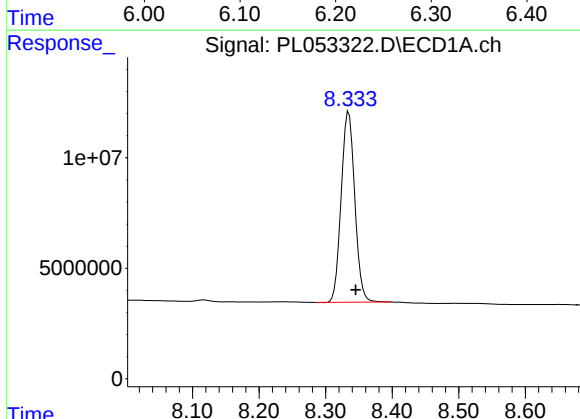

#28 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: -0.010 min
Response: 122244794
Conc: 12.20 ng/ml

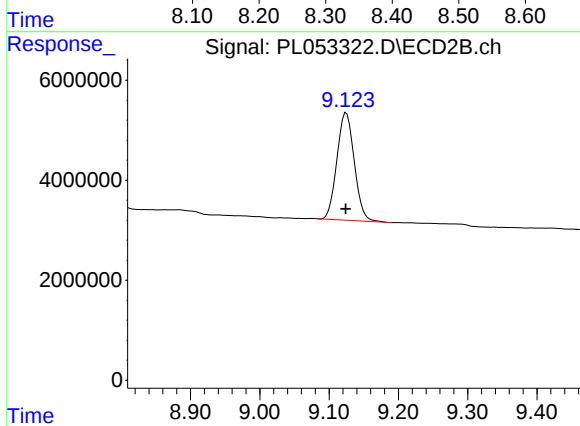

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.000 min
Response: 37396099
Conc: 12.75 ng/ml