

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101519\
 Data File : PL053323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2019 19:23
 Operator : SG\AJ
 Sample : K5352-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-20A-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 00:56:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.545	4.046	131.7E6	34580171	13.244	12.878
28) SA Decachlor...	8.335	9.125	127.2E6	38675442	12.696	13.183
Target Compounds						
7) B delta-BHC	0.000	5.085f	0	2508131	N.D.	0.693 #
15) B Endosulfa...	0.000	6.977	0	1583250	N.D.	0.534 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101519\
Data File : PL053323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2019 19:23
Operator : SG\AJ
Sample : K5352-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-20A-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 00:56:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

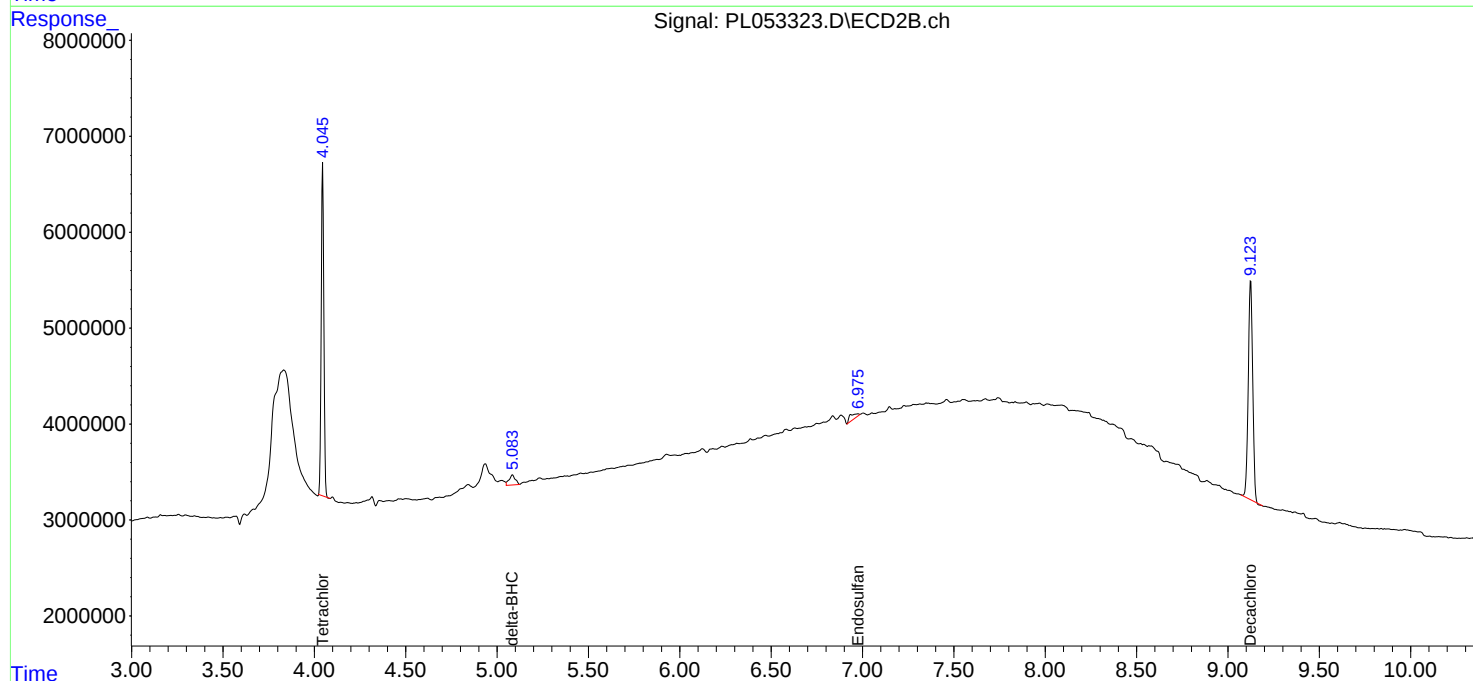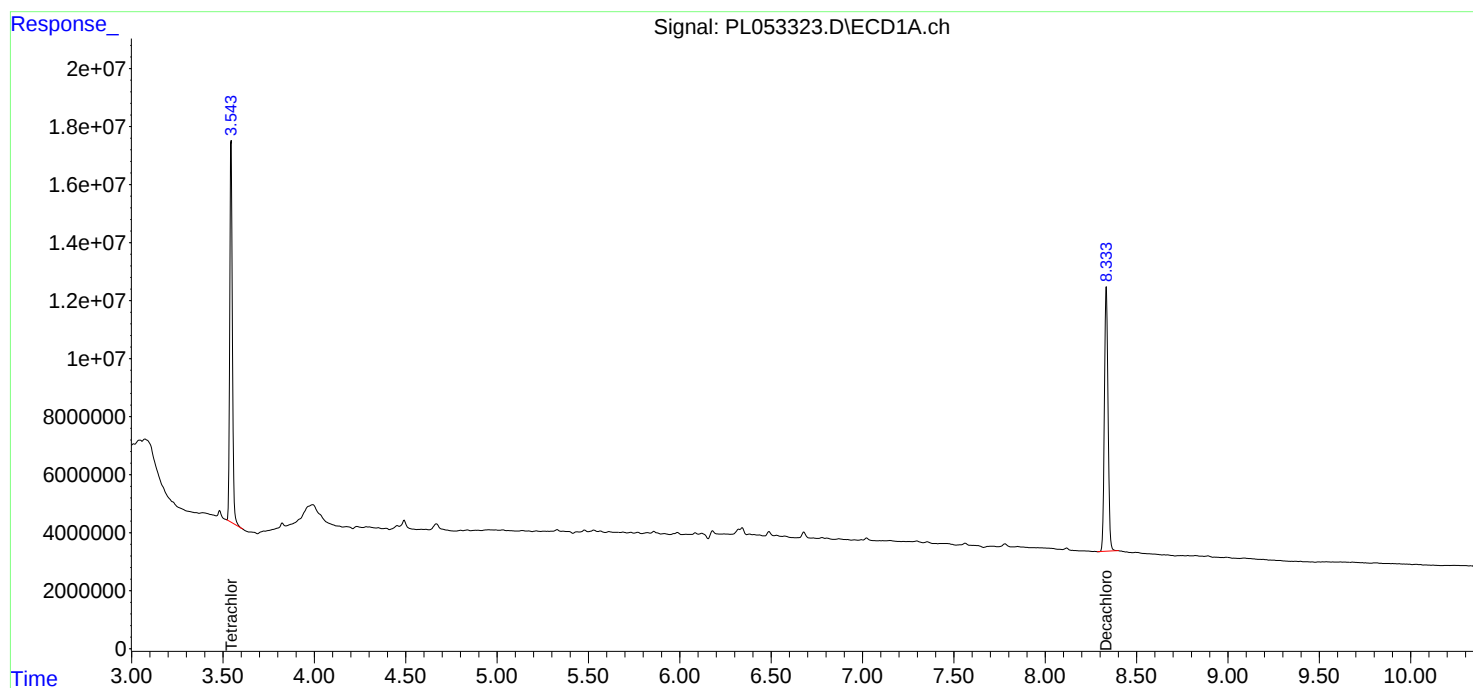


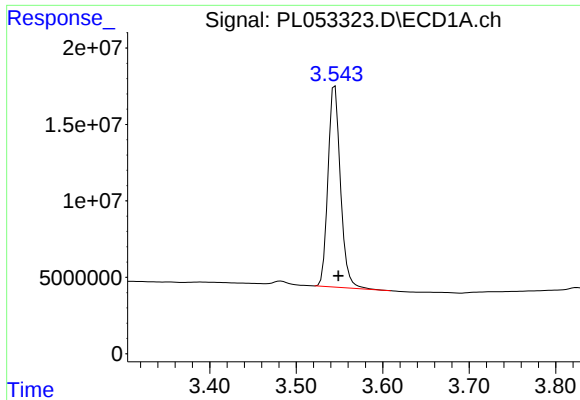

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: -0.004 min
Response: 131736901
Conc: 13.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-20A-D

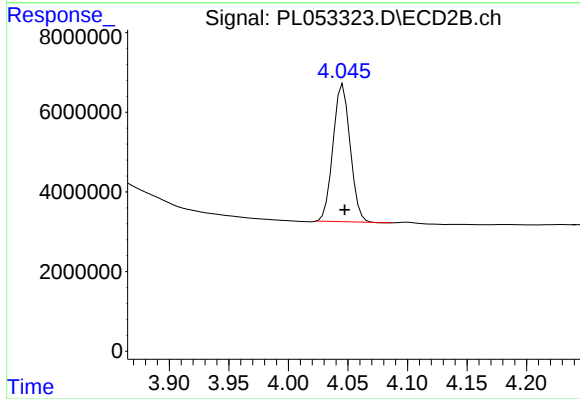


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: -0.001 min
Response: 34580171
Conc: 12.88 ng/ml

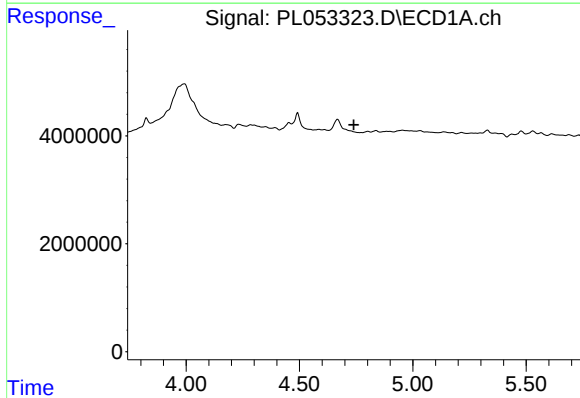


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.740 min
Response: 0
Conc: N.D.

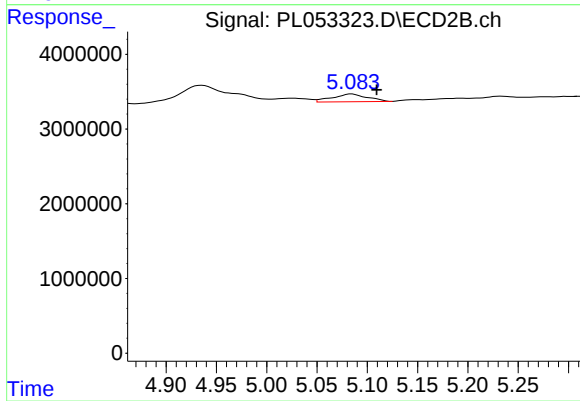

#7 delta-BHC


R.T.: 5.085 min
Delta R.T.: -0.025 min
Response: 2508131
Conc: 0.69 ng/ml

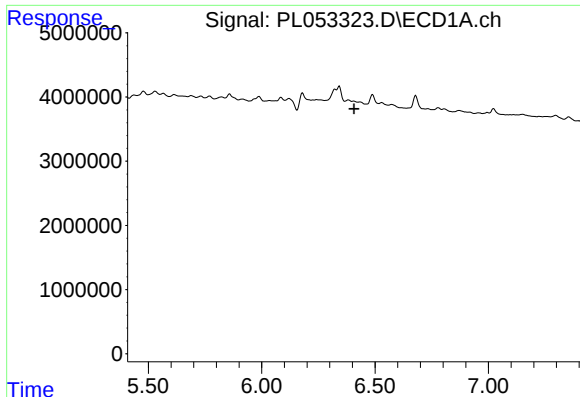

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-20A-D

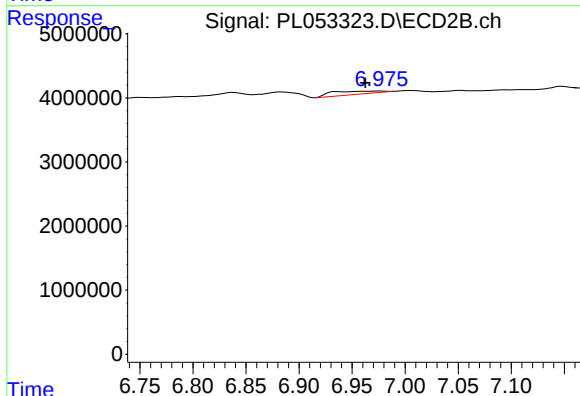


#15 Endosulfan II

R.T.: 6.977 min
Delta R.T.: 0.014 min
Response: 1583250
Conc: 0.53 ng/ml

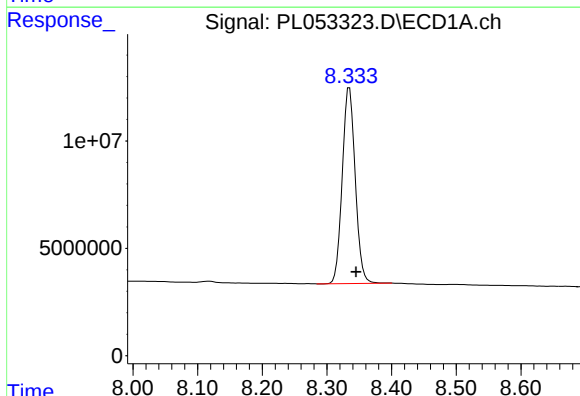

#28 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: -0.010 min
Response: 127163184
Conc: 12.70 ng/ml

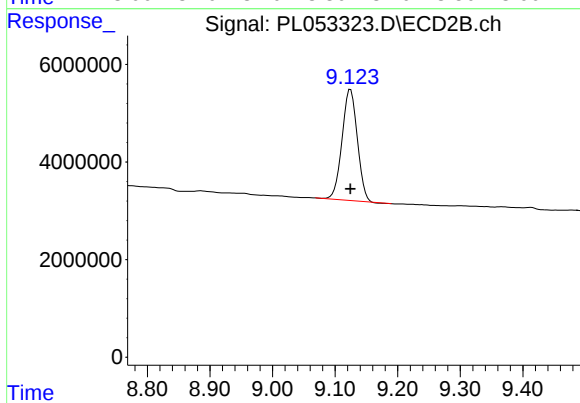

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.000 min
Response: 38675442
Conc: 13.18 ng/ml