

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101519\
 Data File : PL053328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2019 20:32
 Operator : SG\AJ
 Sample : K5337-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HHT-WATER

Manual Integrations
 APPROVED

Ankita
 10/15/2019 11:38:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 00:57:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.545	4.046	140.8E6	36593583	14.158	13.628
28) SA Decachlor...	8.334	9.125	137.5E6	41517793	13.725	14.152
Target Compounds						
3) MA gamma-BHC...	4.290	4.729	20518070	2773270	1.409m	0.766 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101519\
Data File : PL053328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2019 20:32
Operator : SG\AJ
Sample : K5337-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HHT-WATER


Manual Integrations
APPROVED

Ankita
10/15/2019 11:38:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 00:57:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

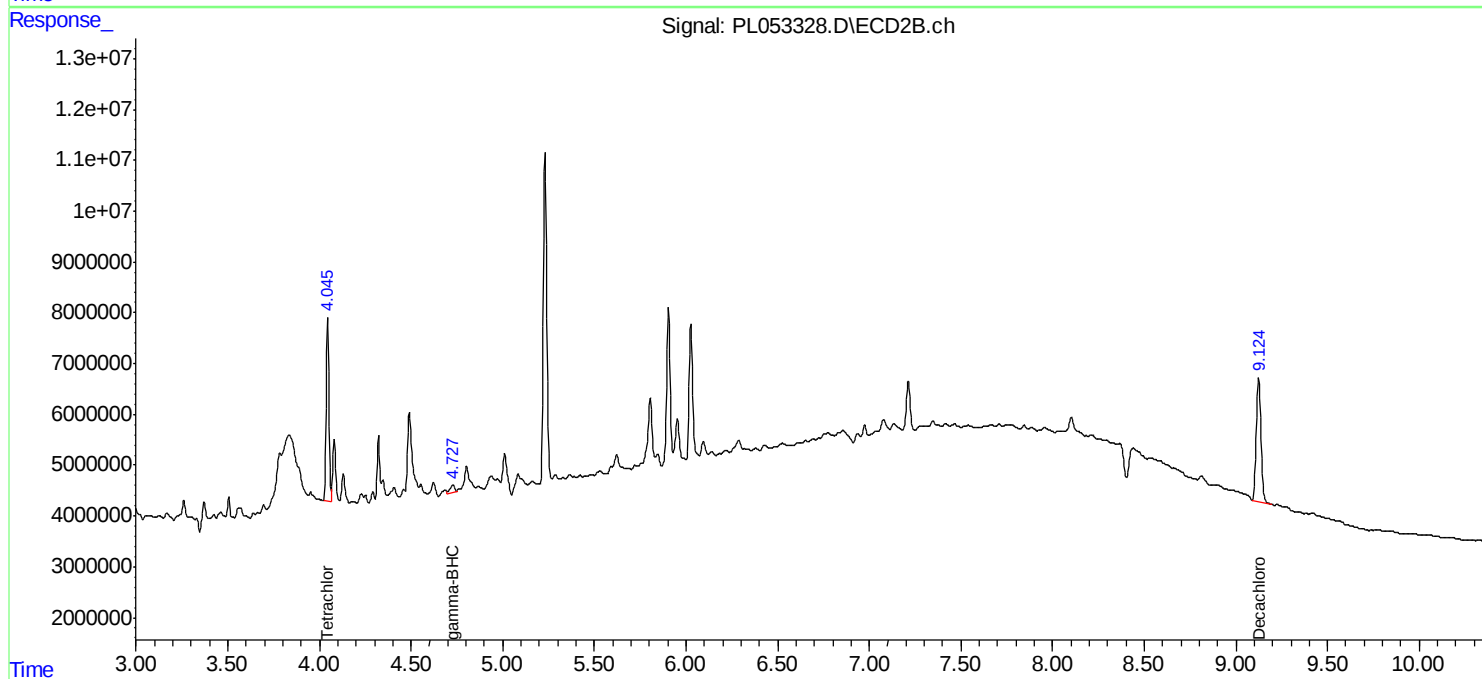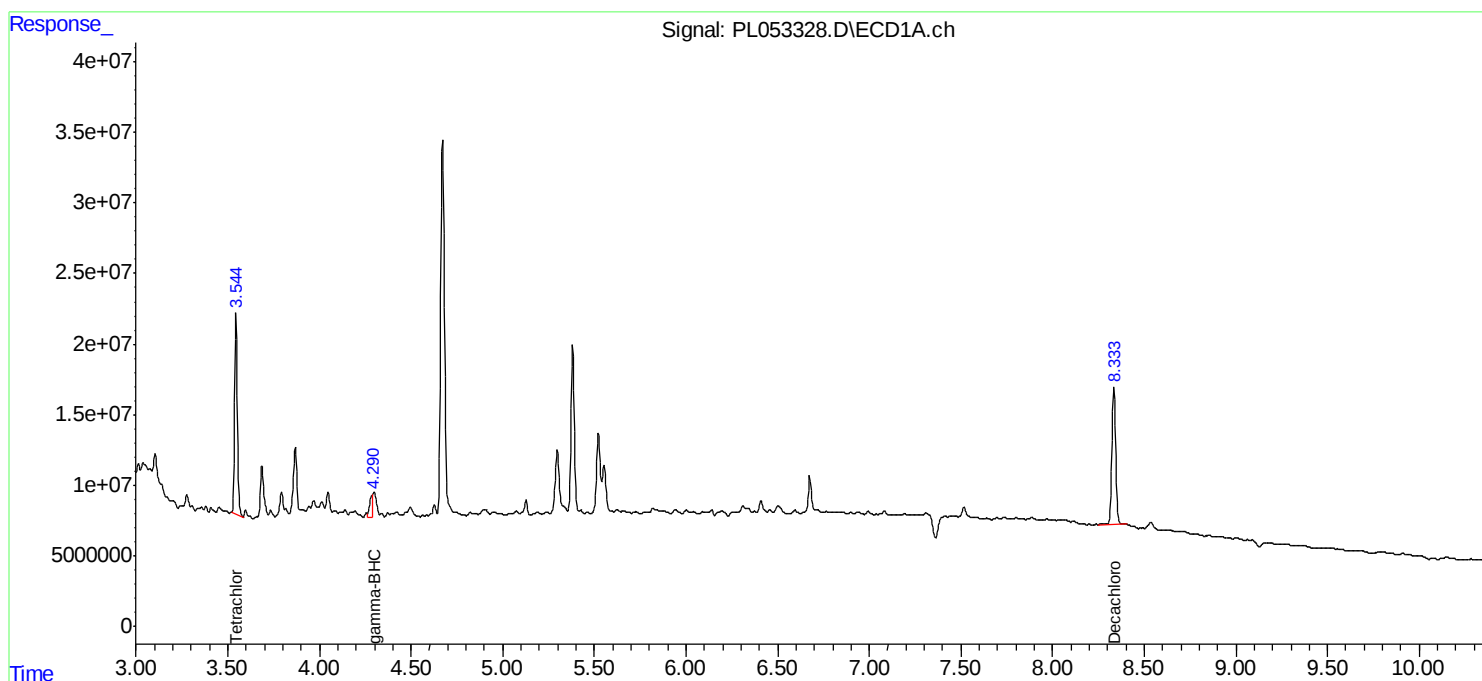

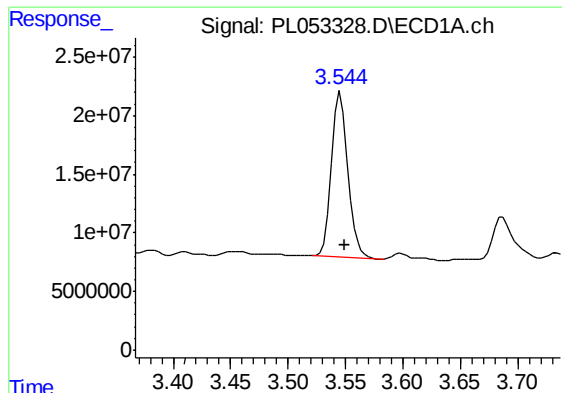


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: -0.004 min
Response: 140826731
Conc: 14.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
HHT-WATER


Manual Integrations
APPROVED

Ankita
10/15/2019 11:38:09 AM

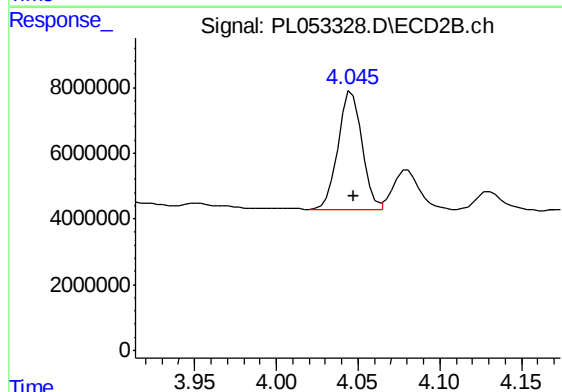


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 36593583
Conc: 13.63 ng/ml

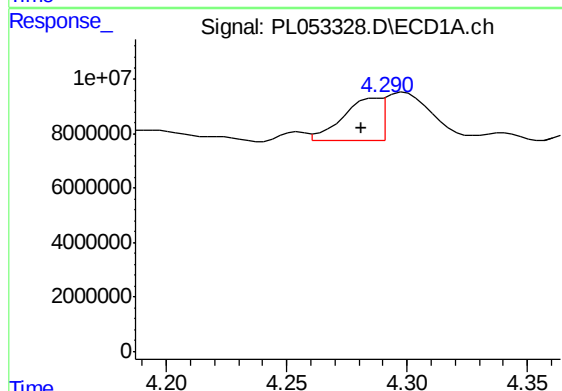


#3 gamma-BHC (Lindane)

R.T.: 4.290 min
Delta R.T.: 0.010 min
Response: 20518070
Conc: 1.41 ng/ml m

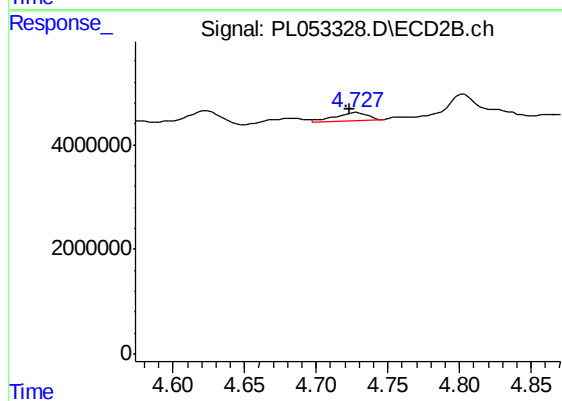

#3 gamma-BHC (Lindane)

R.T.: 4.729 min
Delta R.T.: 0.006 min
Response: 2773270
Conc: 0.77 ng/ml

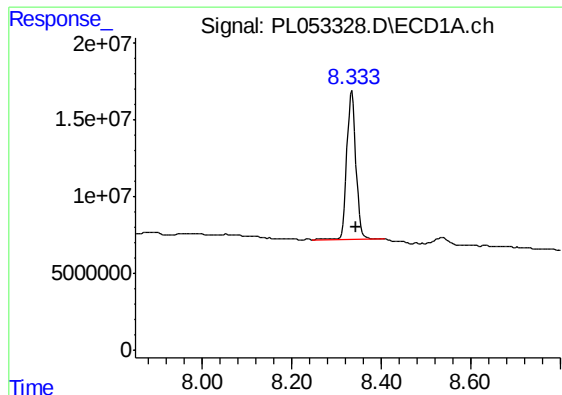


#28 Decachlorobiphenyl

R.T.: 8.334 min
Delta R.T.: -0.011 min
Response: 137472322
Conc: 13.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
HHT-WATER

Manual Integrations
APPROVED

Ankita
10/15/2019 11:38:09 AM

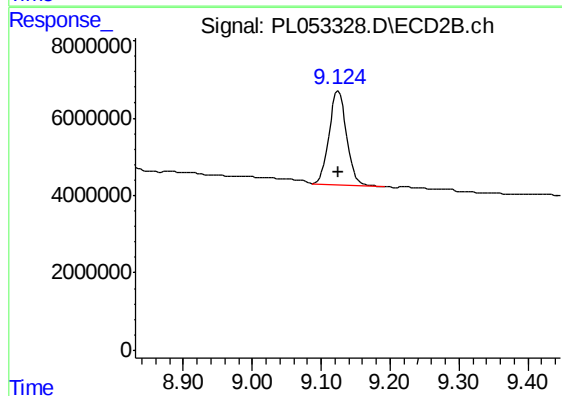

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.000 min
Response: 41517793
Conc: 14.15 ng/ml