

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101520\
 Data File : PL062294.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2020 14:51
 Operator : DD\AJ
 Sample : L4226-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 16:58:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 13 05:04:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.951	21170165	24325862	12.163	8.631 #
28)	SA Decachlor...	8.125	8.992	17206014	26684632	9.406	9.722
Target Compounds							
2)	A alpha-BHC	0.000	4.359f	0	6485069	N.D.	1.546 #
23)	Chlordane-1	0.000	4.955	0	1309070	N.D.	13.219 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101520\
Data File : PL062294.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2020 14:51
Operator : DD\AJ
Sample : L4226-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 16:58:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
Quant Title : GC Extractables
QLast Update : Tue Oct 13 05:04:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

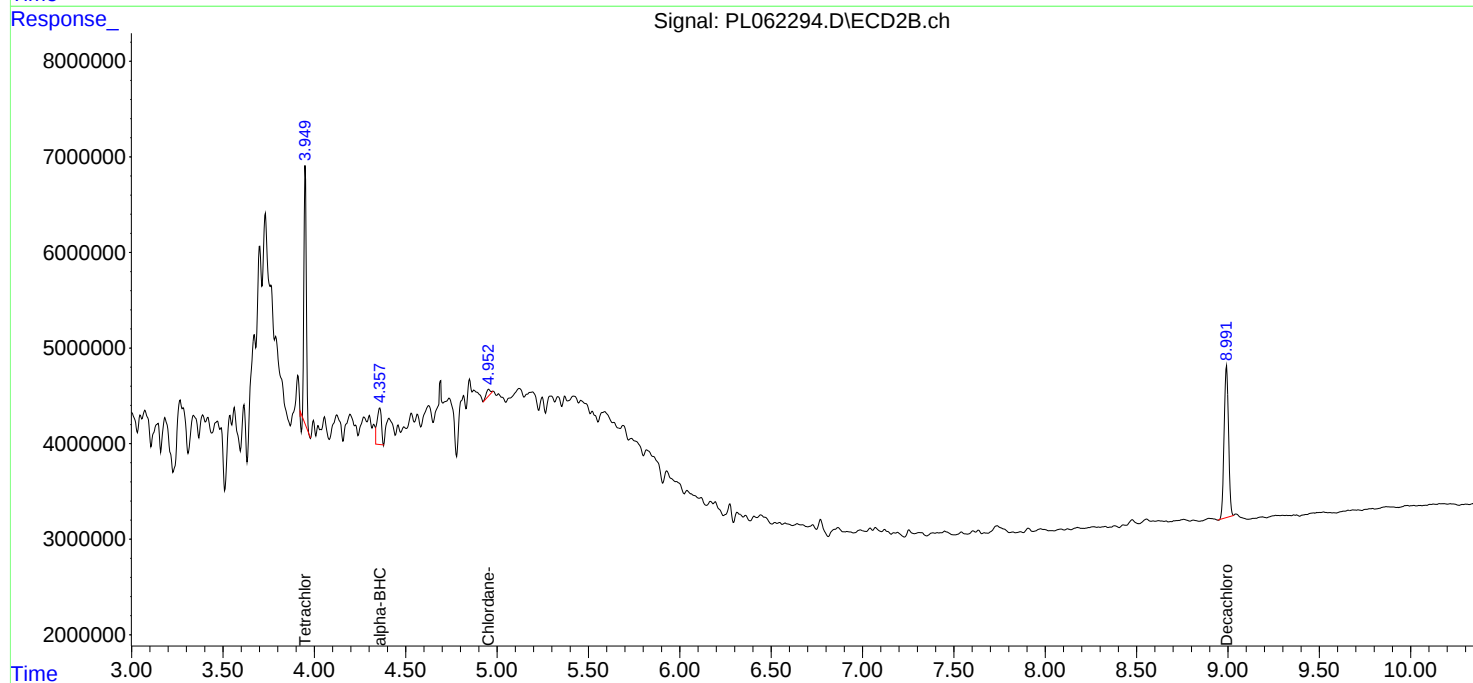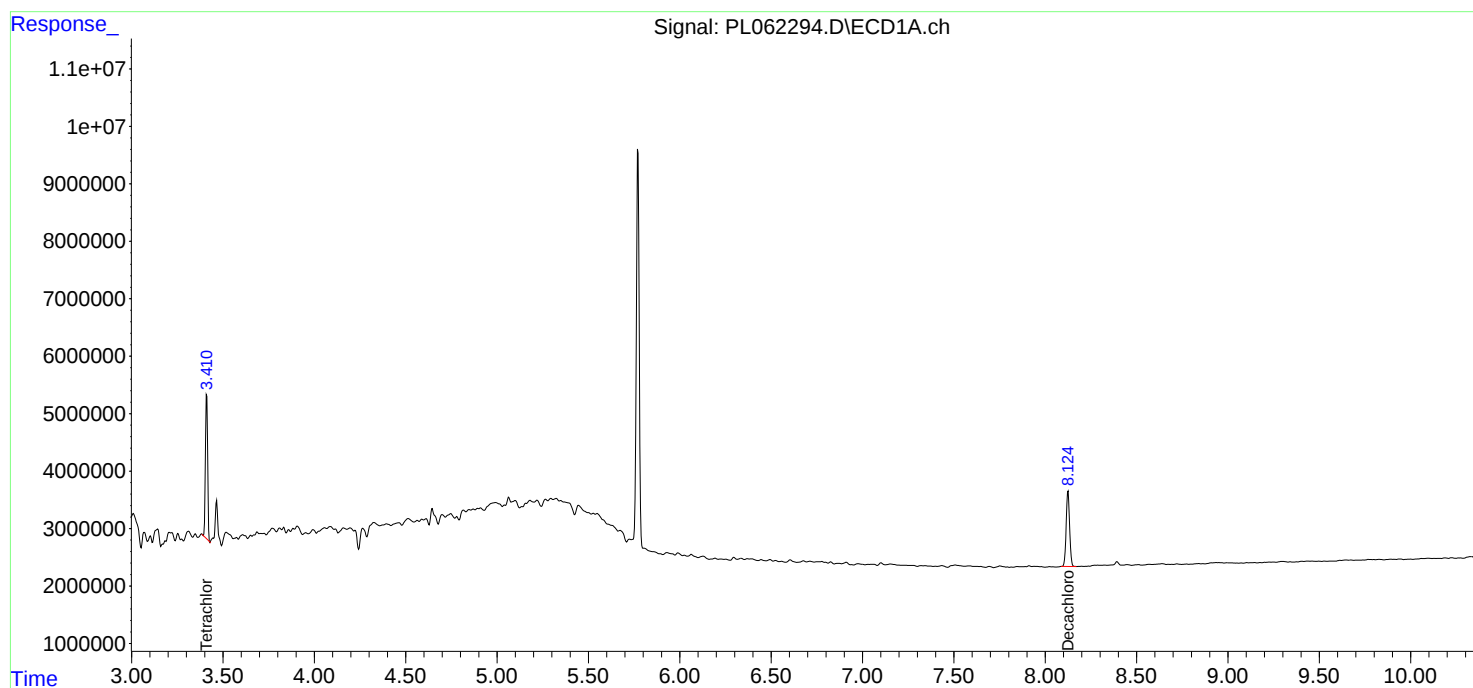


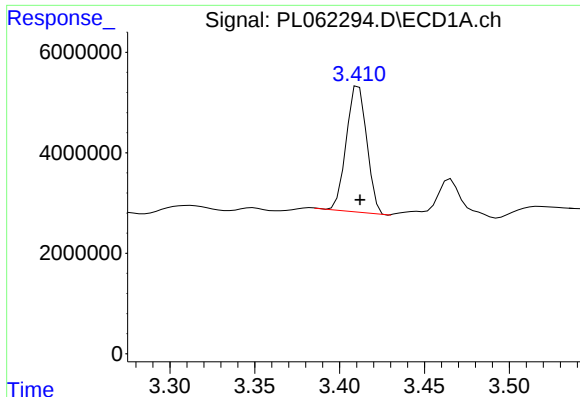

#1 Tetrachloro-m-xylene


R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 21170165
Conc: 12.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

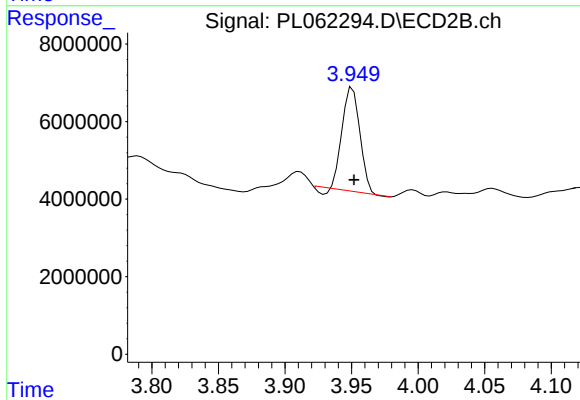


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: -0.001 min
Response: 24325862
Conc: 8.63 ng/ml

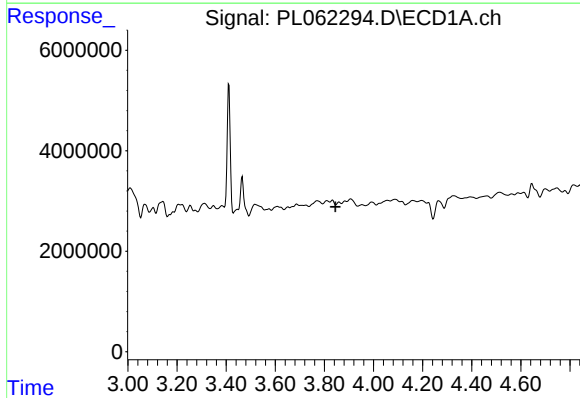


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.845 min
Response: 0
Conc: N.D.

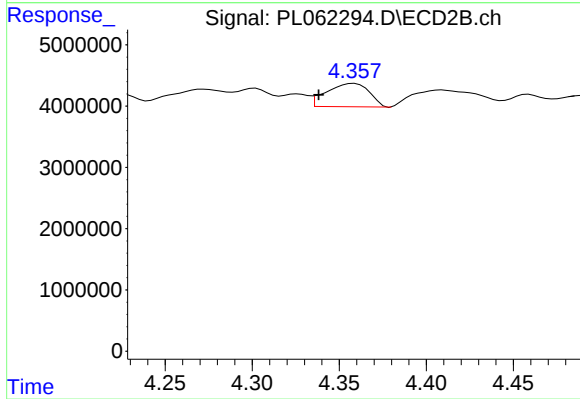

#2 alpha-BHC


R.T.: 4.359 min
Delta R.T.: 0.020 min
Response: 6485069
Conc: 1.55 ng/ml

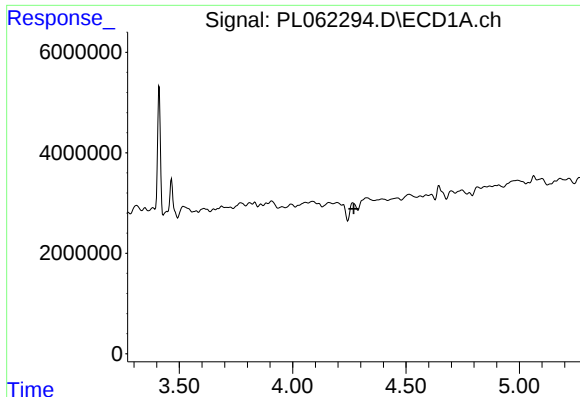

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.270 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

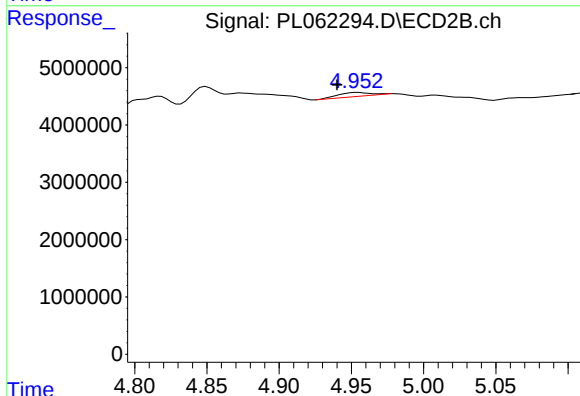


#23 Chlordane-1

R.T.: 4.955 min
Delta R.T.: 0.014 min
Response: 1309070
Conc: 13.22 ng/ml

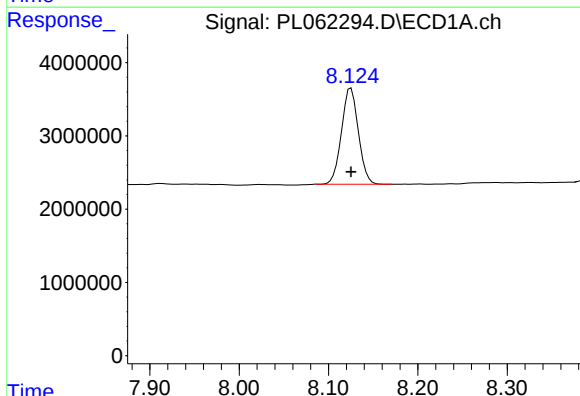

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: 0.000 min
Response: 17206014
Conc: 9.41 ng/ml

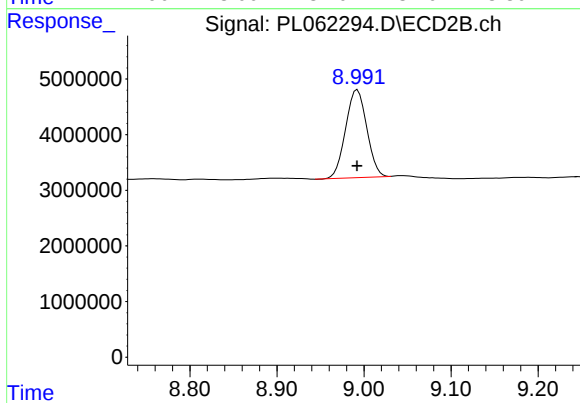

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 26684632
Conc: 9.72 ng/ml