

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101520\
 Data File : PL062303.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2020 16:59
 Operator : DD\AJ
 Sample : PB132372BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 02:11:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 13 05:04:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.952	37791701	61049030	21.712	21.661
28)	SA Decachlor...	8.125	8.993	37483510	54222519	20.491	19.755
Target Compounds							
2)	A alpha-BHC	3.853	0.000	1429087	0	0.558	N.D. #
23)	Chlordane-1	4.298f	0.000	2612900	0	50.206	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101520\
Data File : PL062303.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2020 16:59
Operator : DD\AJ
Sample : PB132372BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 02:11:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
Quant Title : GC Extractables
QLast Update : Tue Oct 13 05:04:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

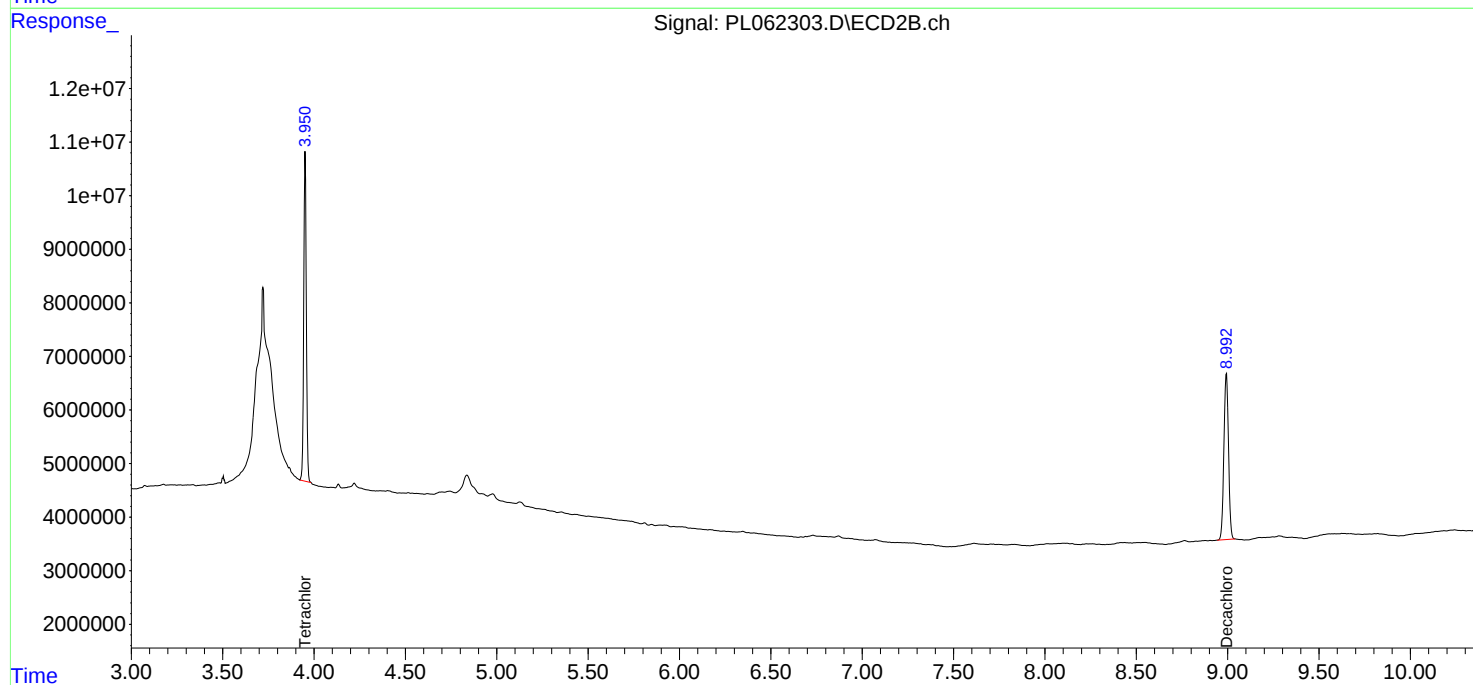


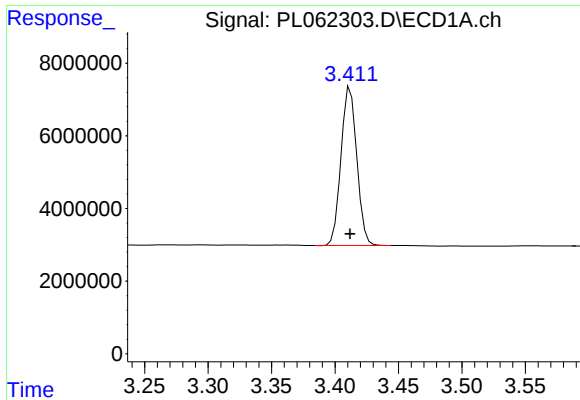

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 37791701
Conc: 21.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

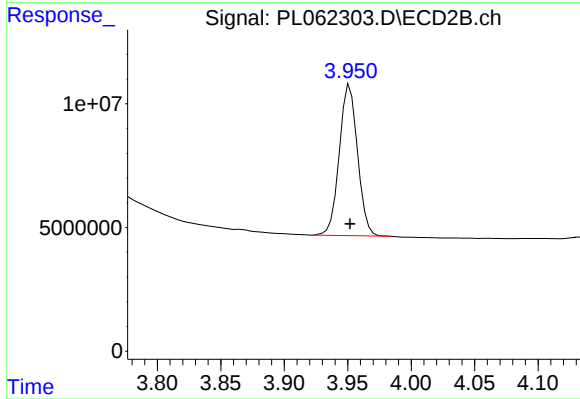


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 61049030
Conc: 21.66 ng/ml

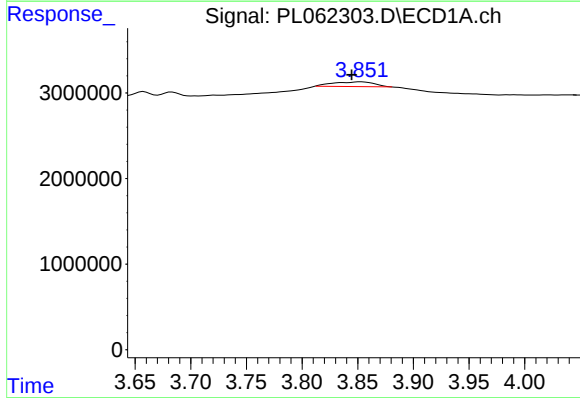


#2 alpha-BHC

R.T.: 3.853 min
Delta R.T.: 0.008 min
Response: 1429087
Conc: 0.56 ng/ml

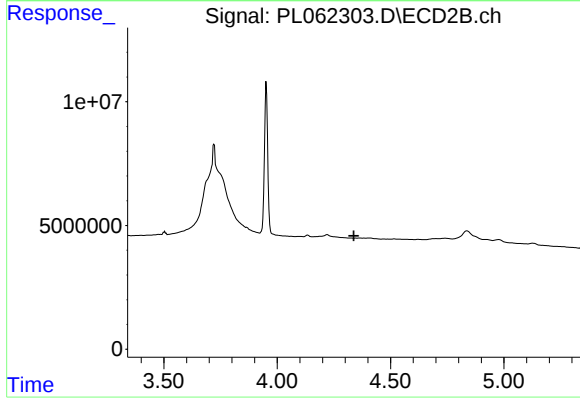

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.338 min
Response: 0
Conc: N.D.

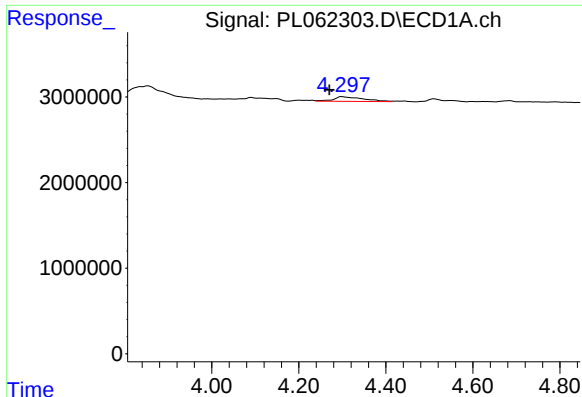

#23 Chlordane-1


R.T.: 4.298 min
Delta R.T.: 0.028 min
Response: 2612900
Conc: 50.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

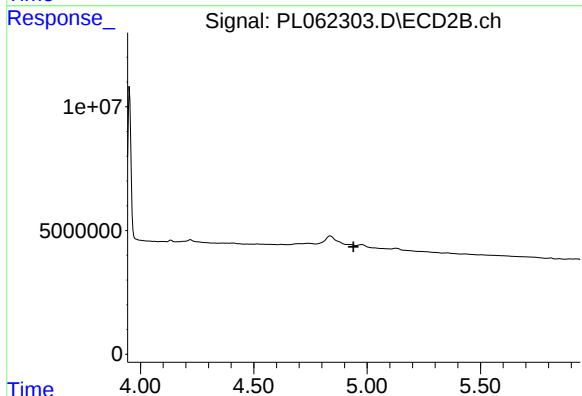


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.940 min
Response: 0
Conc: N.D.

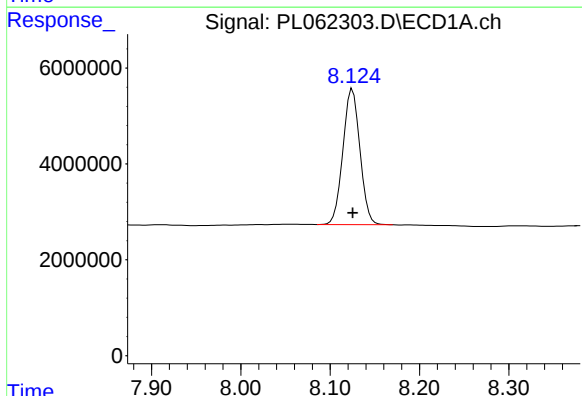

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: 0.000 min
Response: 37483510
Conc: 20.49 ng/ml

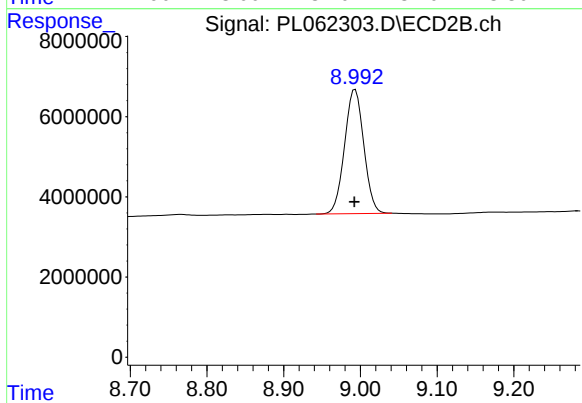

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.001 min
Response: 54222519
Conc: 19.75 ng/ml