

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101520\
 Data File : PL062293.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2020 14:37
 Operator : DD\AJ
 Sample : L4226-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-08-101320

Manual Integrations
 APPROVED

Ankita
 10/15/2020 11:25:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 16:58:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 13 05:04:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.950	24733117	37071801	14.210	13.154
28)	SA Decachlor...	8.125	8.992	22392767	33044483	12.241	12.039
Target Compounds							
17)	MA 4,4'-DDT	6.296	7.067	1459685	1287963	1.132m	0.563m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101520\
Data File : PL062293.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2020 14:37
Operator : DD\AJ
Sample : L4226-07
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TR-08-101320


Manual Integrations
APPROVED

Ankita
10/15/2020 11:25:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 16:58:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
Quant Title : GC Extractables
QLast Update : Tue Oct 13 05:04:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

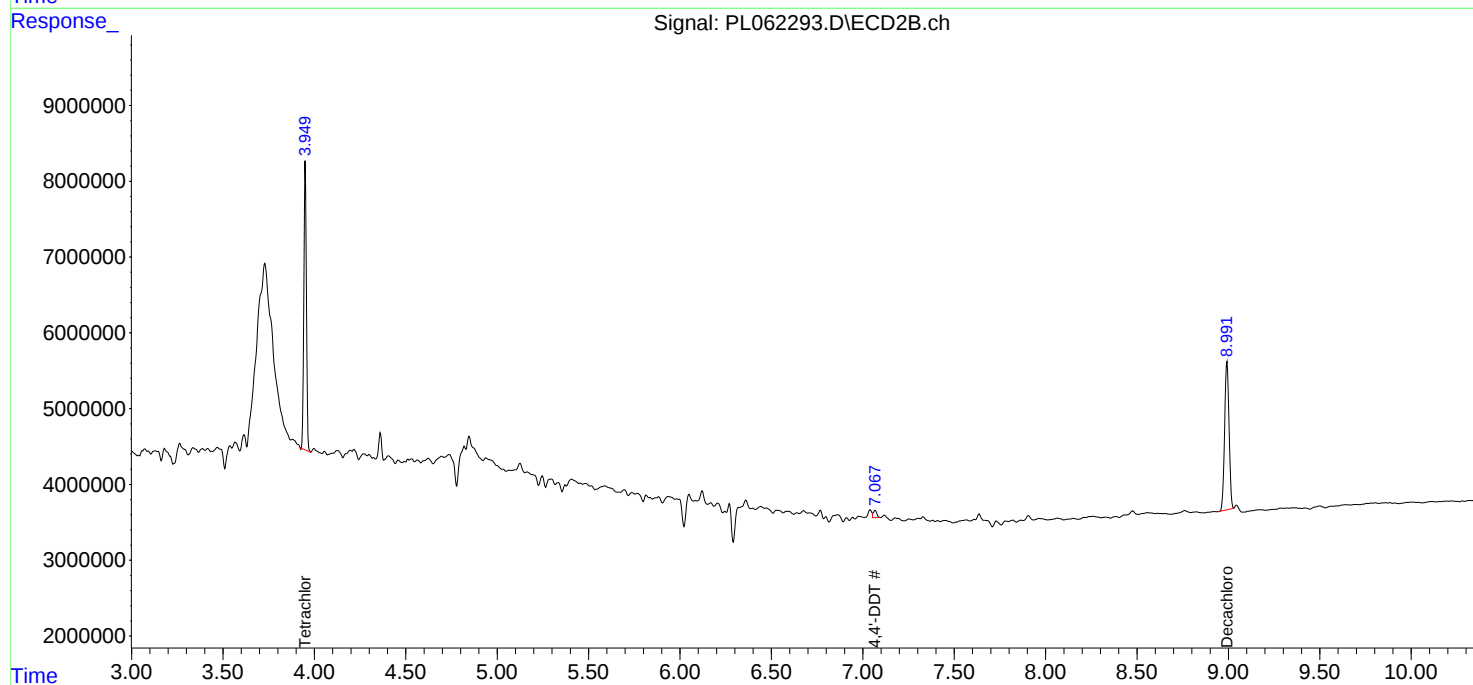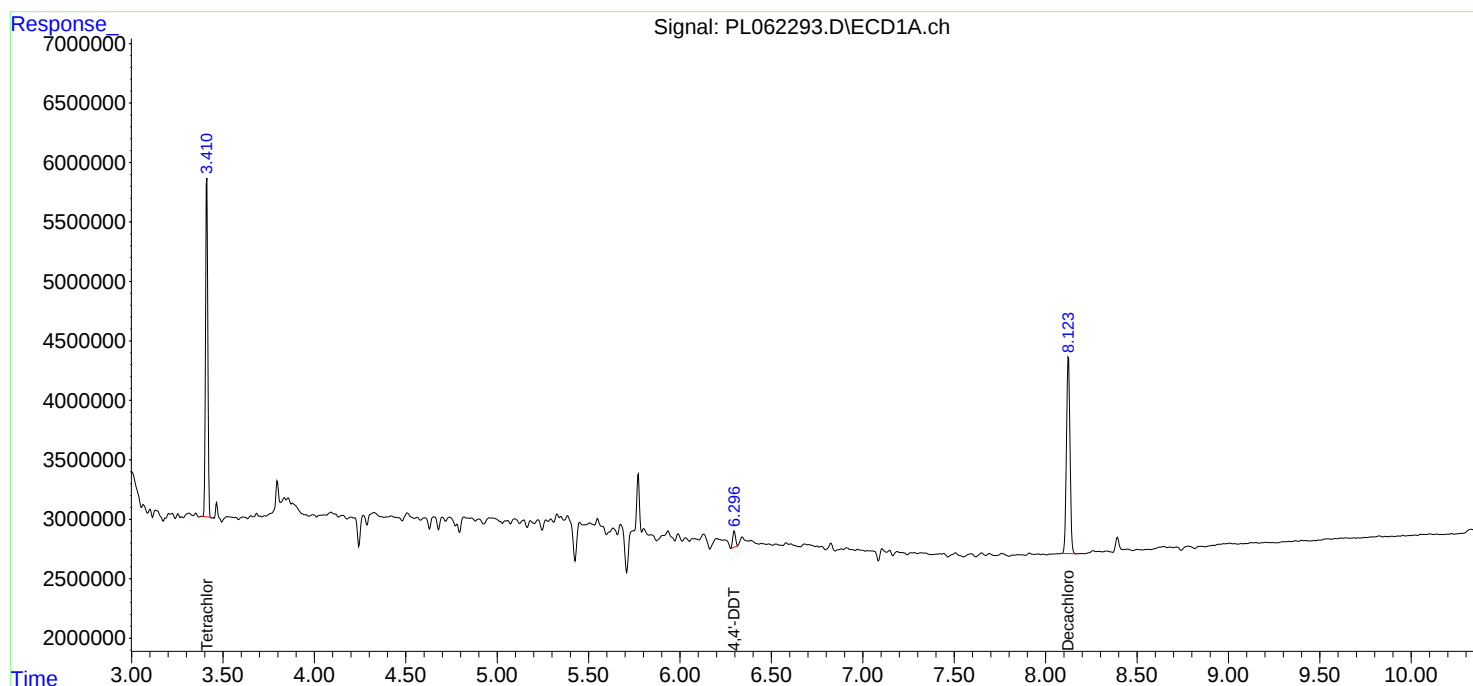

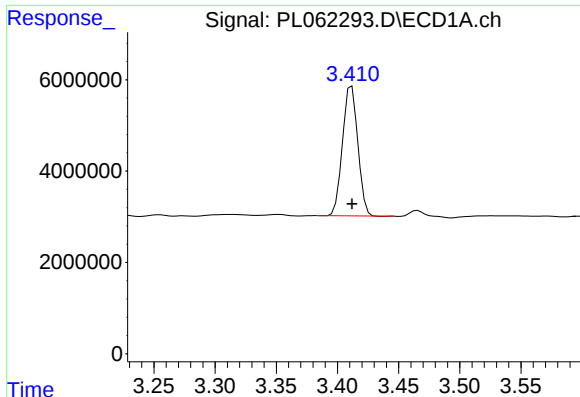


#1 Tetrachloro-m-xylene

R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 24733117
Conc: 14.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-08-101320


Manual Integrations
APPROVED

Ankita
10/15/2020 11:25:27 AM

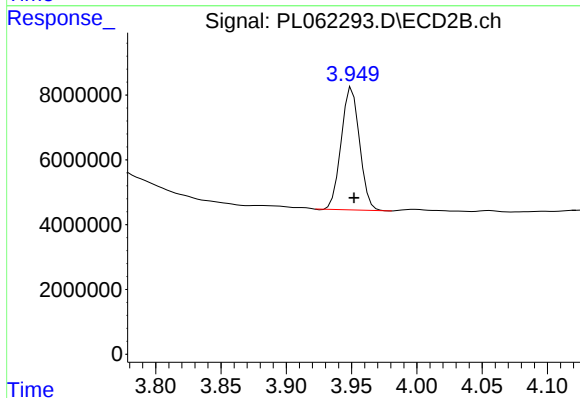


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 37071801
Conc: 13.15 ng/ml

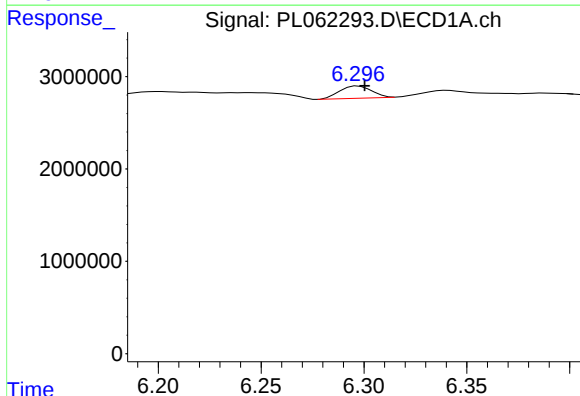


#17 4,4'-DDT

R.T.: 6.296 min
Delta R.T.: -0.005 min
Response: 1459685
Conc: 1.13 ng/ml m

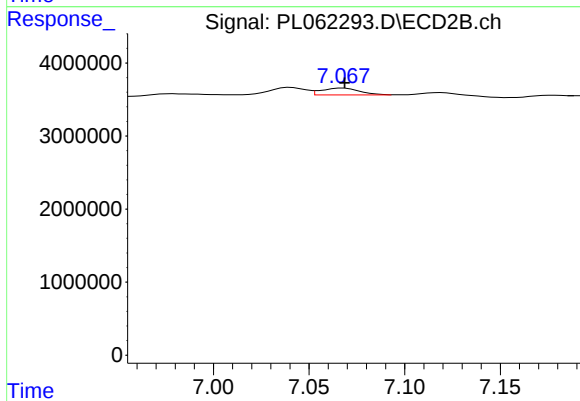

#17 4,4'-DDT

R.T.: 7.067 min
Delta R.T.: -0.002 min
Response: 1287963
Conc: 0.56 ng/ml m

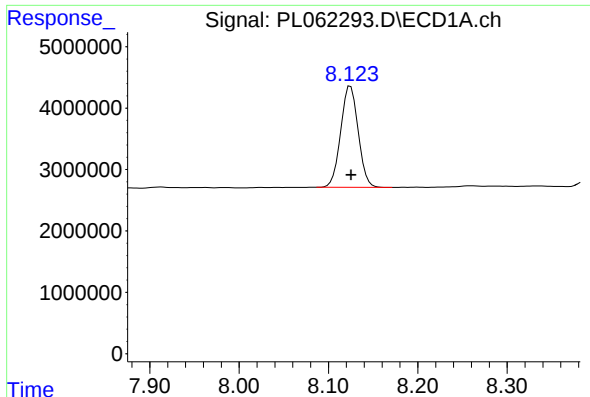


#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: 0.000 min
Response: 22392767
Conc: 12.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-08-101320

Manual Integrations
APPROVED

Ankita
10/15/2020 11:25:27 AM

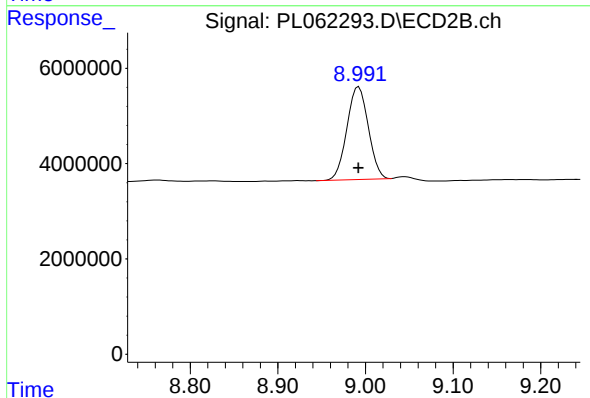

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 33044483
Conc: 12.04 ng/ml