

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101618\
 Data File : PL041057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2018 23:11
 Operator : AJ\SJ
 Sample : J5527-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-STONE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 02:00:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.477	4.104	140.1E6	75550863	25.566	27.096
28)	SA Decachlor...	8.226	9.234	144.7E6	66603780	27.832	25.757
Target Compounds							
6)	B beta-BHC	4.425f	4.997f	2820542	7126431	0.889	4.446 #
8)	B Heptachlo...	5.264f	5.991	3319873	6818593	0.506	2.377 #
9)	A Endosulfan I	5.557	0.000	2020778	0	0.337	N.D. #
14)	MA Endrin	6.039	0.000	3811236	0	0.664	N.D. #
15)	B Endosulfa...	0.000	7.043	0	3531869	N.D.	1.487 #
16)	A 4,4'-DDD	0.000	6.915f	0	6574286	N.D.	3.139 #
19)	B Endosulfa...	6.698	0.000	3596466	0	0.707	N.D. #
23)	Chlordane-1	4.356	0.000	3756751	0	14.720	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101618\
Data File : PL041057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2018 23:11
Operator : AJ\SJ
Sample : J5527-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
SP-STONE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 02:00:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

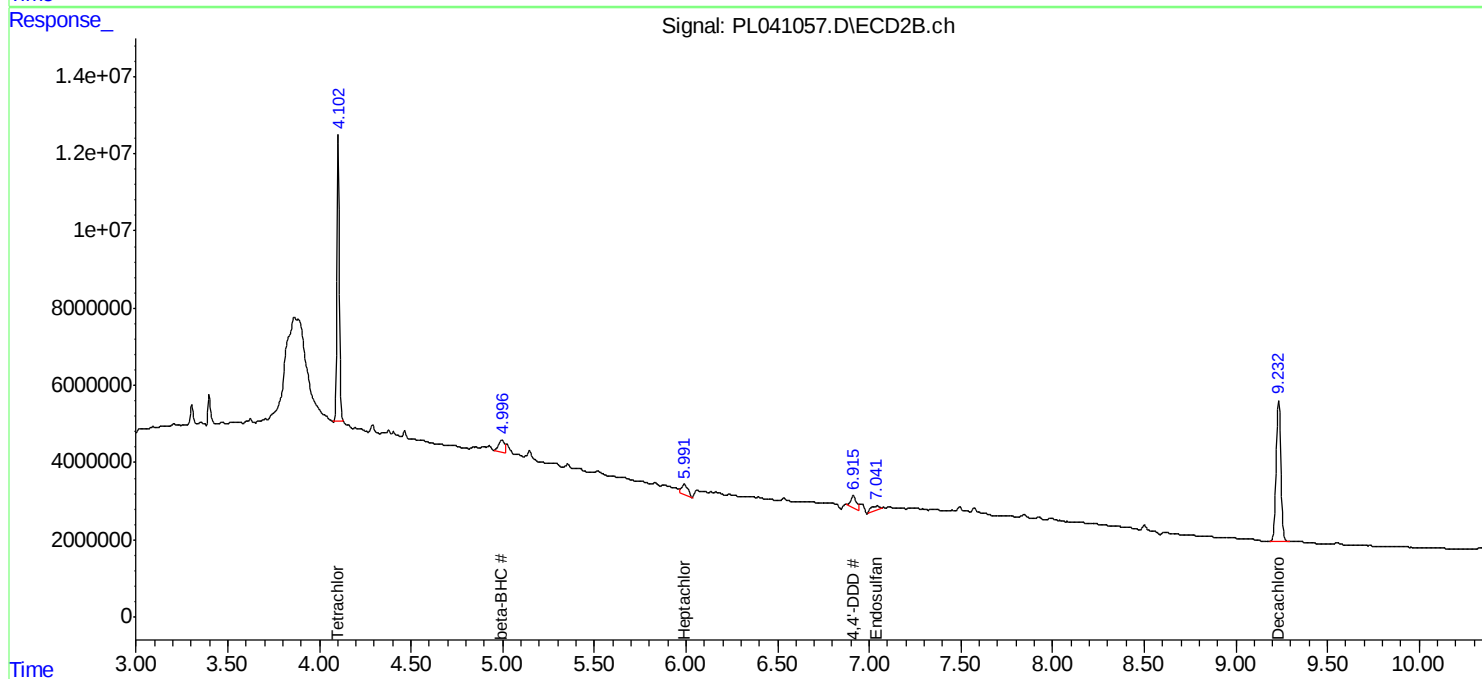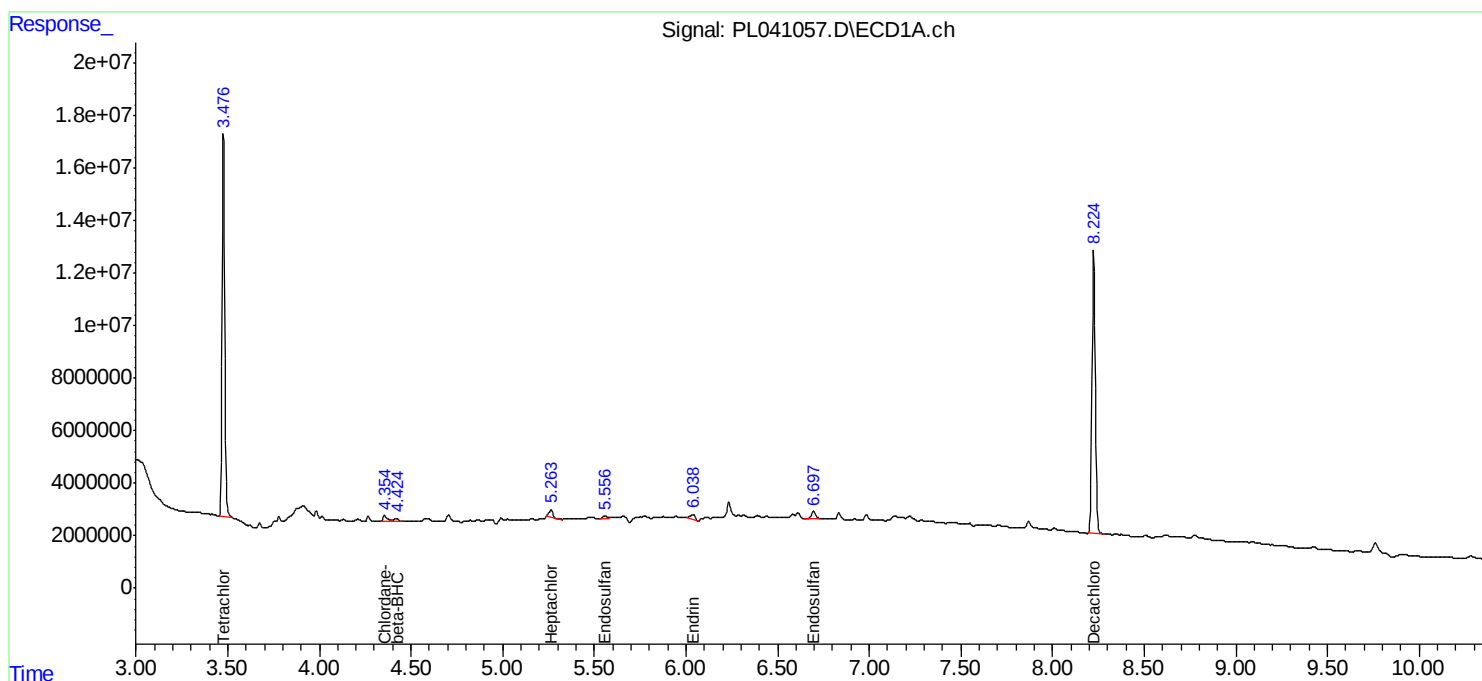


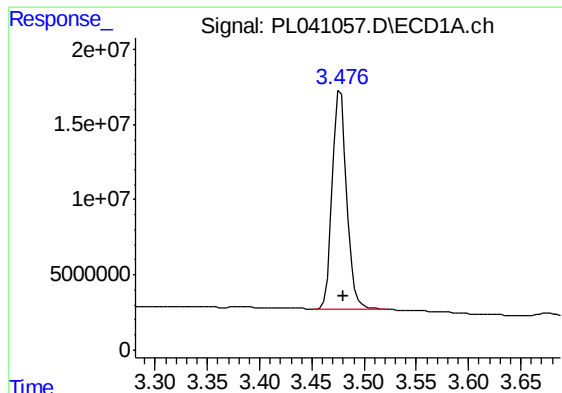

#1 Tetrachloro-m-xylene


R.T.: 3.477 min
Delta R.T.: -0.003 min
Response: 140118927
Conc: 25.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-STONE

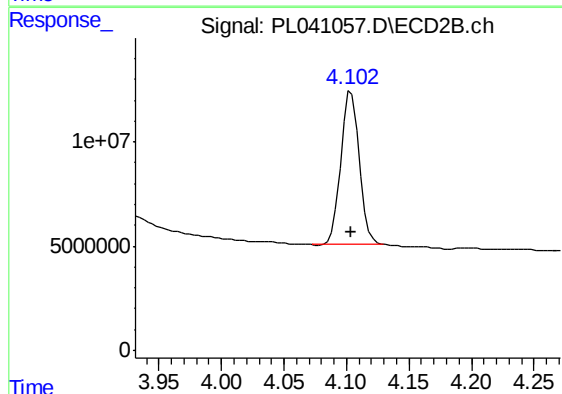


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 75550863
Conc: 27.10 ng/ml

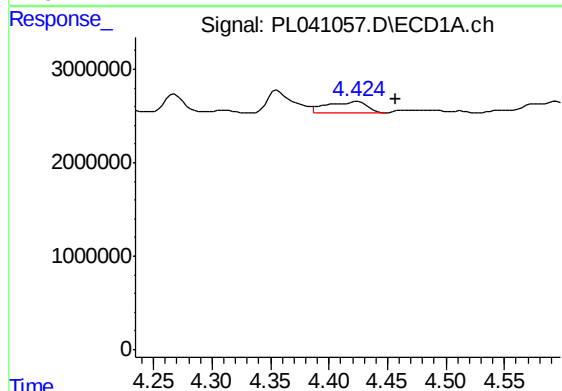


#6 beta-BHC

R.T.: 4.425 min
Delta R.T.: -0.033 min
Response: 2820542
Conc: 0.89 ng/ml

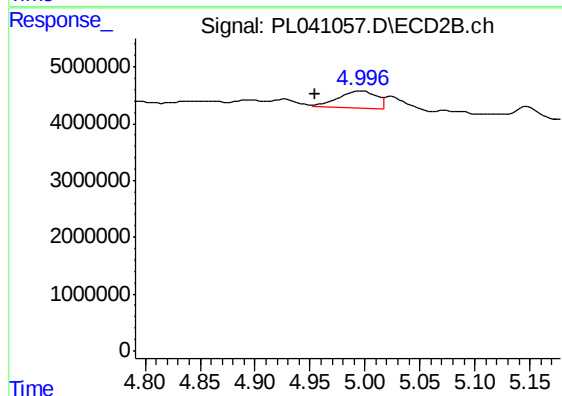

#6 beta-BHC


R.T.: 4.997 min
Delta R.T.: 0.042 min
Response: 7126431
Conc: 4.45 ng/ml

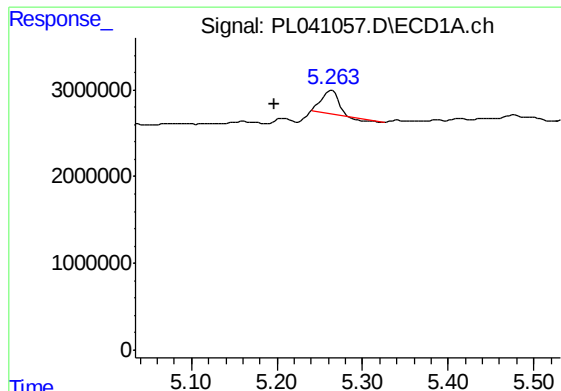

#8 Heptachlor epoxide


R.T.: 5.264 min
Delta R.T.: 0.068 min
Response: 3319873
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-STONE

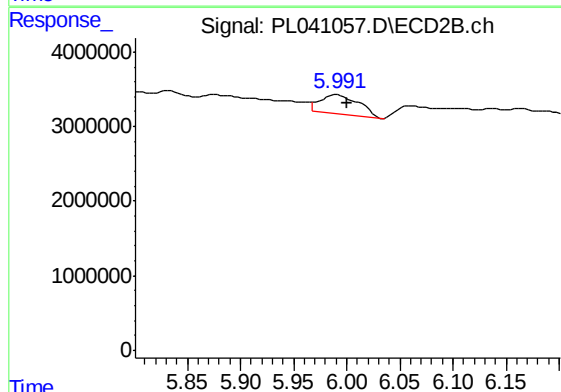


#8 Heptachlor epoxide

R.T.: 5.991 min
Delta R.T.: -0.009 min
Response: 6818593
Conc: 2.38 ng/ml

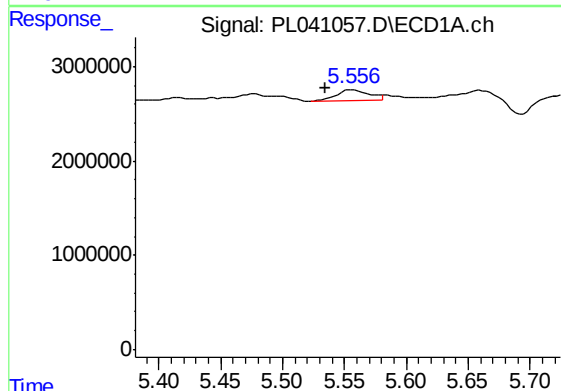


#9 Endosulfan I

R.T.: 5.557 min
Delta R.T.: 0.023 min
Response: 2020778
Conc: 0.34 ng/ml

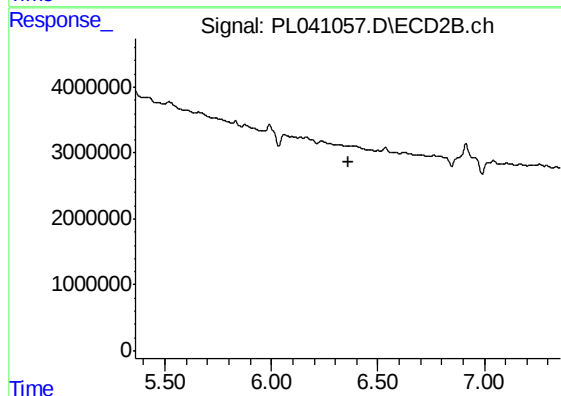

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.360 min
Response: 0
Conc: N.D.

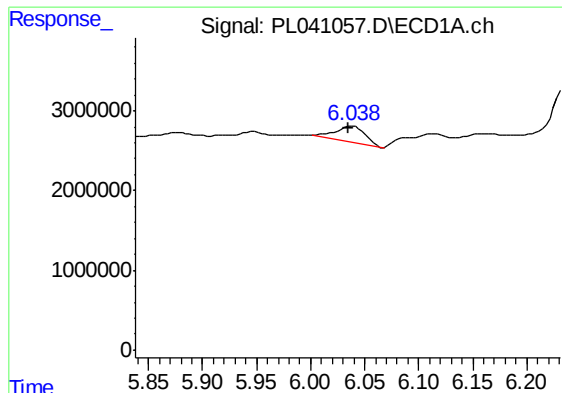

#14 Endrin


R.T.: 6.039 min
Delta R.T.: 0.004 min
Response: 3811236
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-STONE

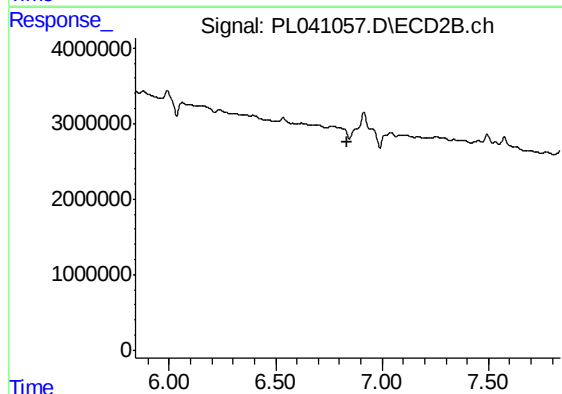


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.838 min
Response: 0
Conc: N.D.

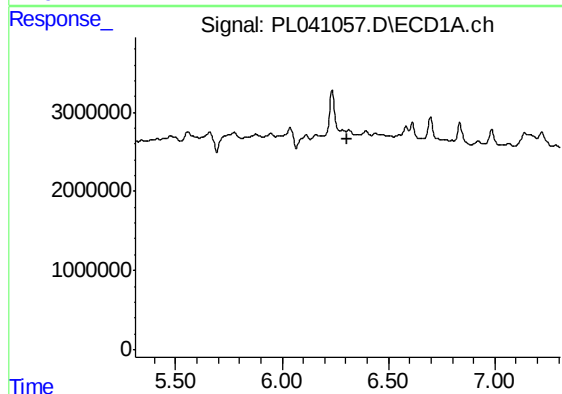


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.309 min
Response: 0
Conc: N.D.

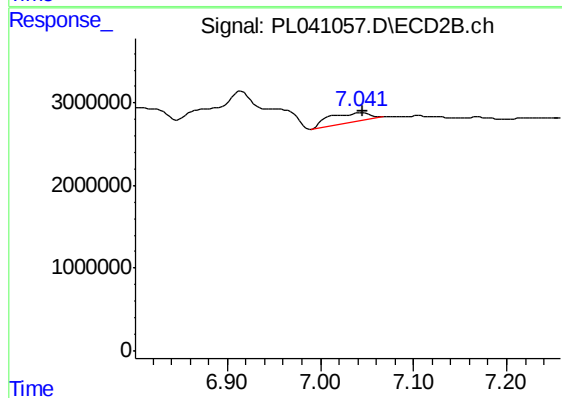

#15 Endosulfan II


R.T.: 7.043 min
Delta R.T.: -0.002 min
Response: 3531869
Conc: 1.49 ng/ml

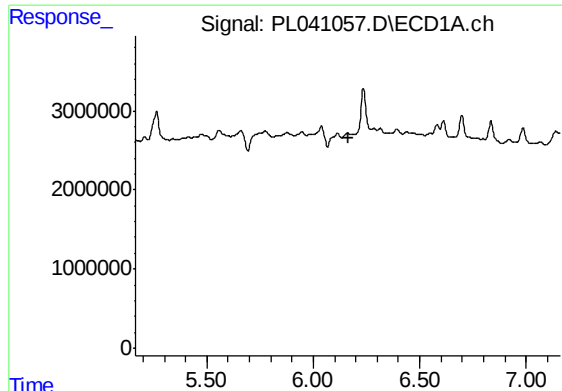

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SP-STONE

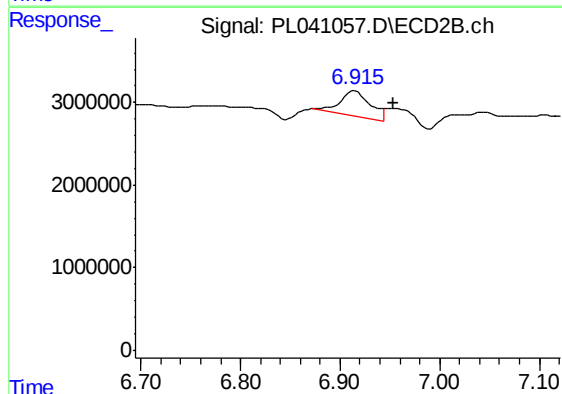


#16 4,4'-DDD

R.T.: 6.915 min
Delta R.T.: -0.039 min
Response: 6574286
Conc: 3.14 ng/ml

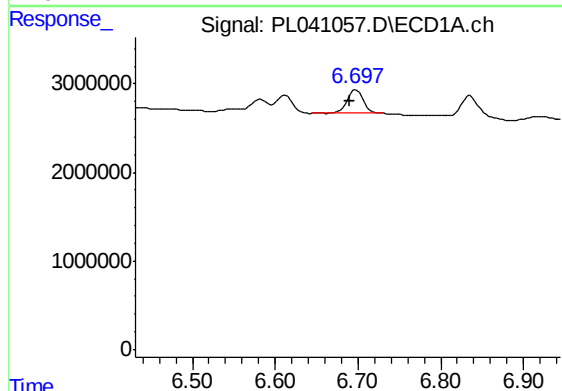


#19 Endosulfan Sulfate

R.T.: 6.698 min
Delta R.T.: 0.008 min
Response: 3596466
Conc: 0.71 ng/ml

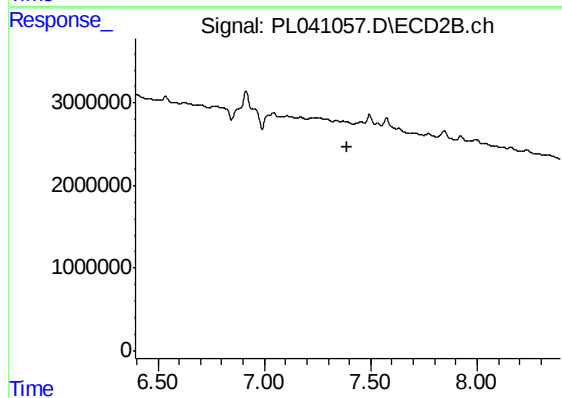

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

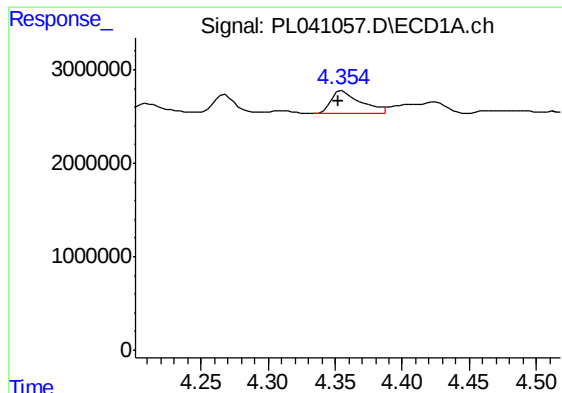

#23 Chlordane-1


R.T.: 4.356 min
Delta R.T.: 0.003 min
Response: 3756751
Conc: 14.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-STONE

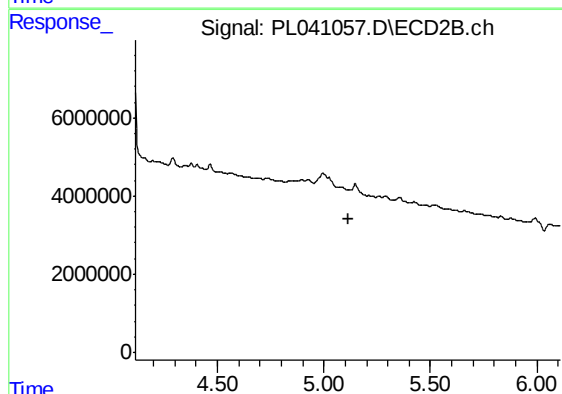


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

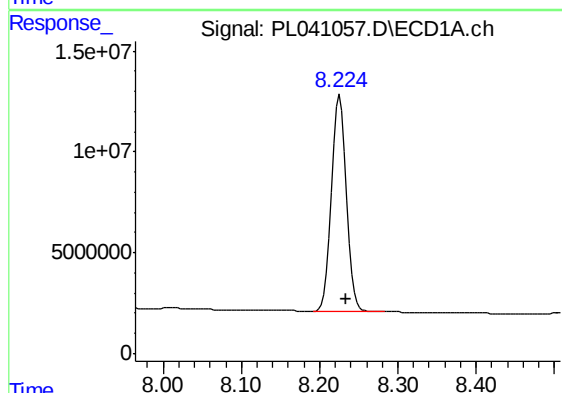

#28 Decachlorobiphenyl

R.T.: 8.226 min
Delta R.T.: -0.009 min
Response: 144711125
Conc: 27.83 ng/ml

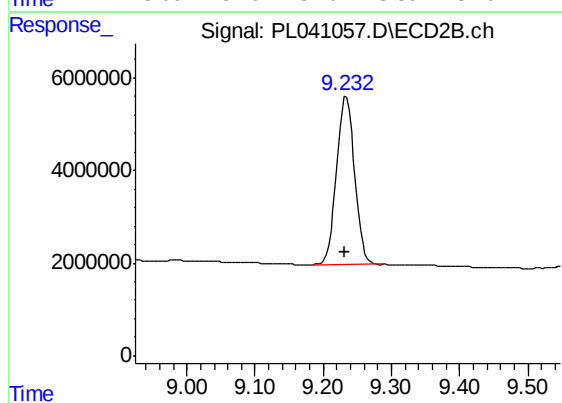

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.002 min
Response: 66603780
Conc: 25.76 ng/ml