

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101618\
 Data File : PL041040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2018 15:54
 Operator : AJ\SJ
 Sample : J5516-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SSSI-1011-S-DH-30

Manual Integrations
 APPROVED

Sohil
 10/17/2018 1:31:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 01:54:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.477	4.102	76042260	36783114	13.874	13.192m
28)	SA Decachlor...	8.226	9.233	90823015	40893820	17.468	15.814
Target Compounds							
17)	MA 4,4'-DDT	6.396	7.254	6858708	3535805	1.506	1.700

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101618\
Data File : PL041040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2018 15:54
Operator : AJ\SJ
Sample : J5516-06
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SSSI-1011-S-DH-30


Manual Integrations
APPROVED

Sohil
10/17/2018 1:31:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 01:54:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

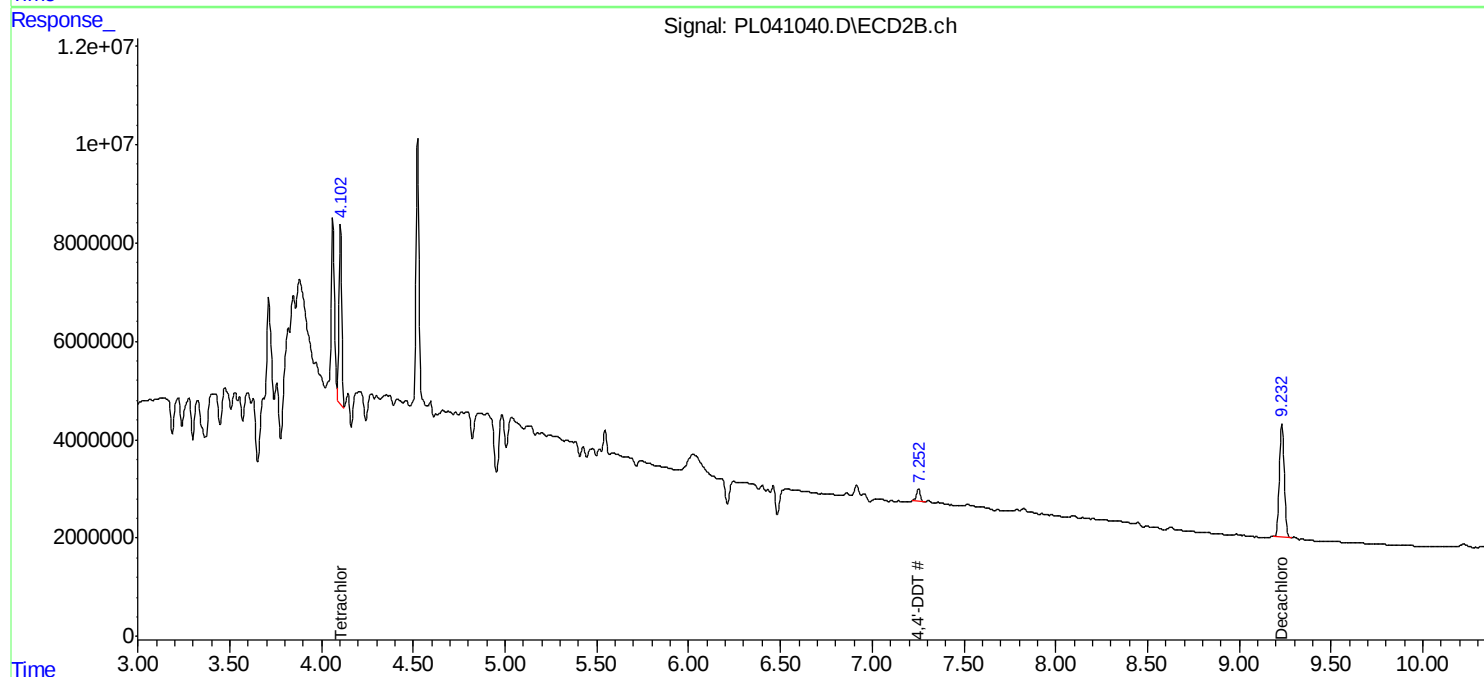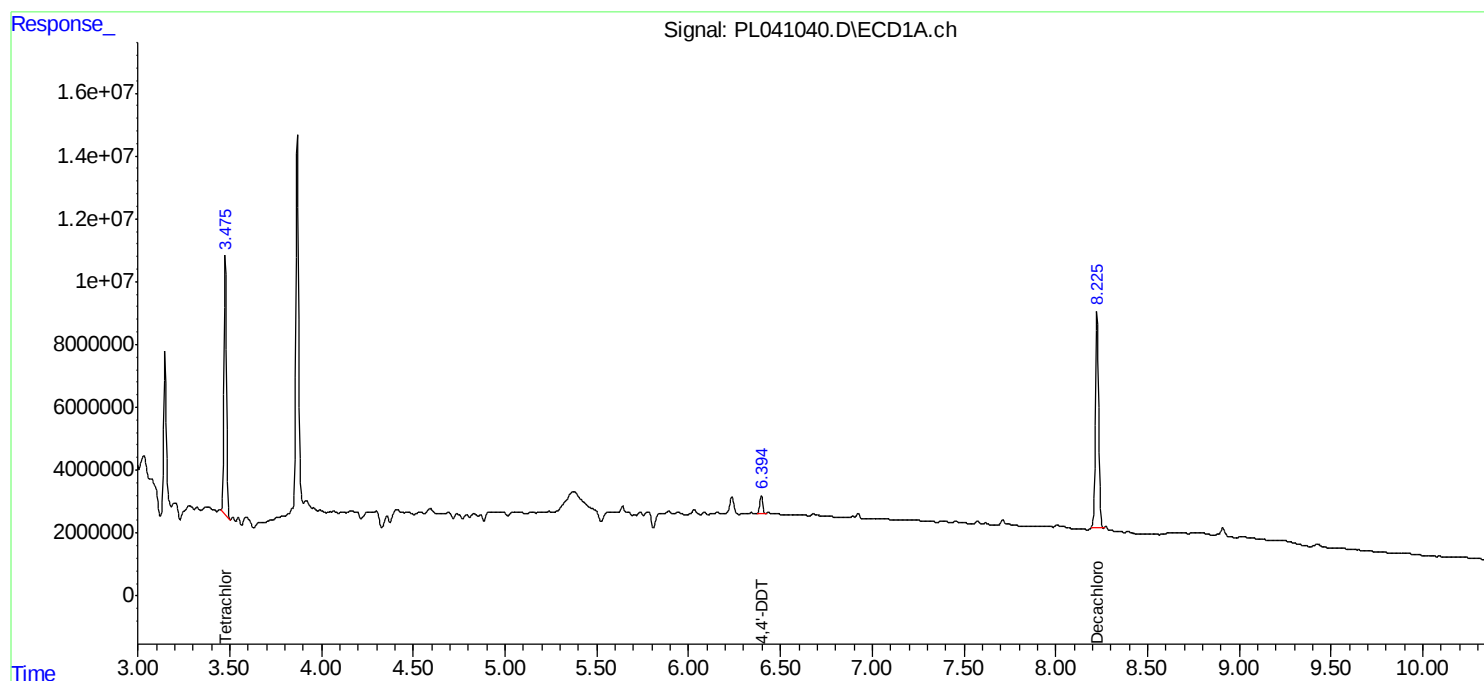

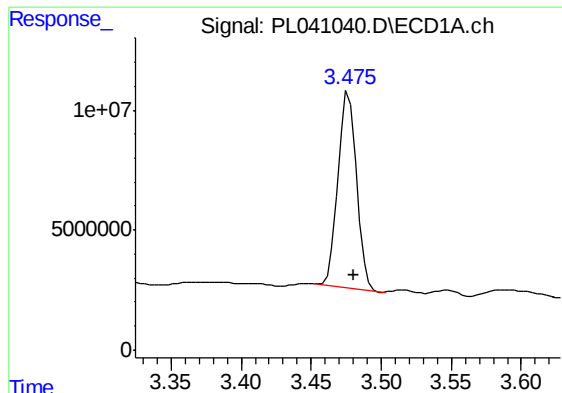


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: -0.003 min
Response: 76042260
Conc: 13.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1011-S-DH-30


Manual Integrations
APPROVED

Sohil
10/17/2018 1:31:42 PM

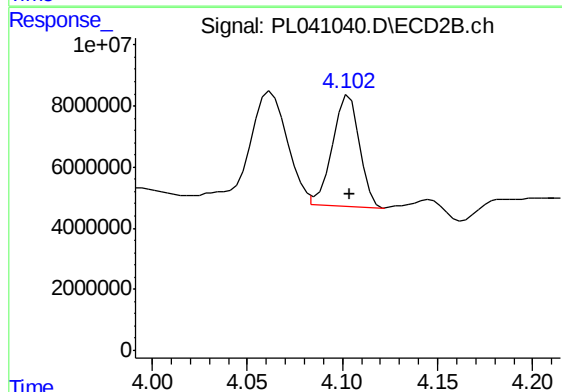


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: -0.002 min
Response: 36783114
Conc: 13.19 ng/ml m

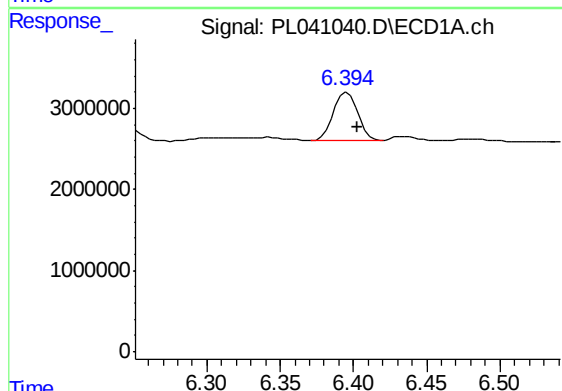


#17 4,4'-DDT

R.T.: 6.396 min
Delta R.T.: -0.007 min
Response: 6858708
Conc: 1.51 ng/ml

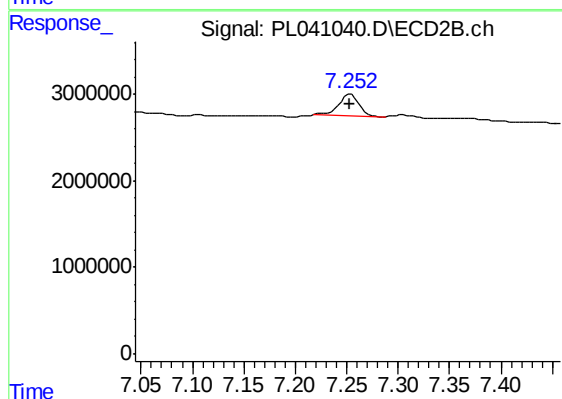

#17 4,4'-DDT

R.T.: 7.254 min
Delta R.T.: 0.000 min
Response: 3535805
Conc: 1.70 ng/ml

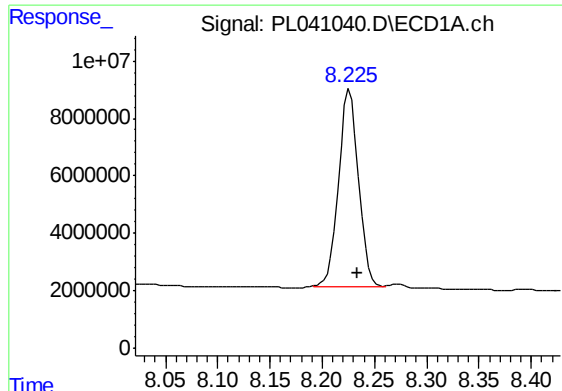


#28 Decachlorobiphenyl

R.T.: 8.226 min
Delta R.T.: -0.008 min
Response: 90823015
Conc: 17.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1011-S-DH-30

Manual Integrations
APPROVED

Sohil
10/17/2018 1:31:42 PM

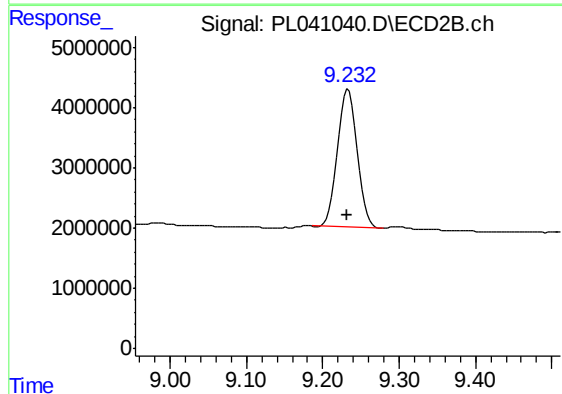

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.002 min
Response: 40893820
Conc: 15.81 ng/ml