

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101619\
 Data File : PL053332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2019 11:29
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 00:41:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	4.046	230.1E6	52361062	23.137	19.500
28)	SA Decachlor...	8.332	9.122	225.1E6	61294741	22.473	20.893
Target Compounds							
4)	MA Heptachlor	0.000	5.238	0	925287	N.D.	0.243 #
7)	B delta-BHC	0.000	5.084f	0	2665524	N.D.	0.736 #
8)	B Heptachlo...	0.000	5.917	0	1514681	N.D.	0.452 #
9)	A Endosulfan I	0.000	6.282	0	9491993	N.D.	3.037 #
14)	MA Endrin	0.000	6.758	0	2265259	N.D.	0.816 #
15)	B Endosulfa...	0.000	6.973	0	663249	N.D.	0.224 #
16)	A 4,4'-DDD	0.000	6.866	0	868220	N.D.	0.354 #
27)	Chlordane-5	0.000	7.011f	0	247797	N.D.	2.809 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101619\
Data File : PL053332.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 11:29
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 00:41:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

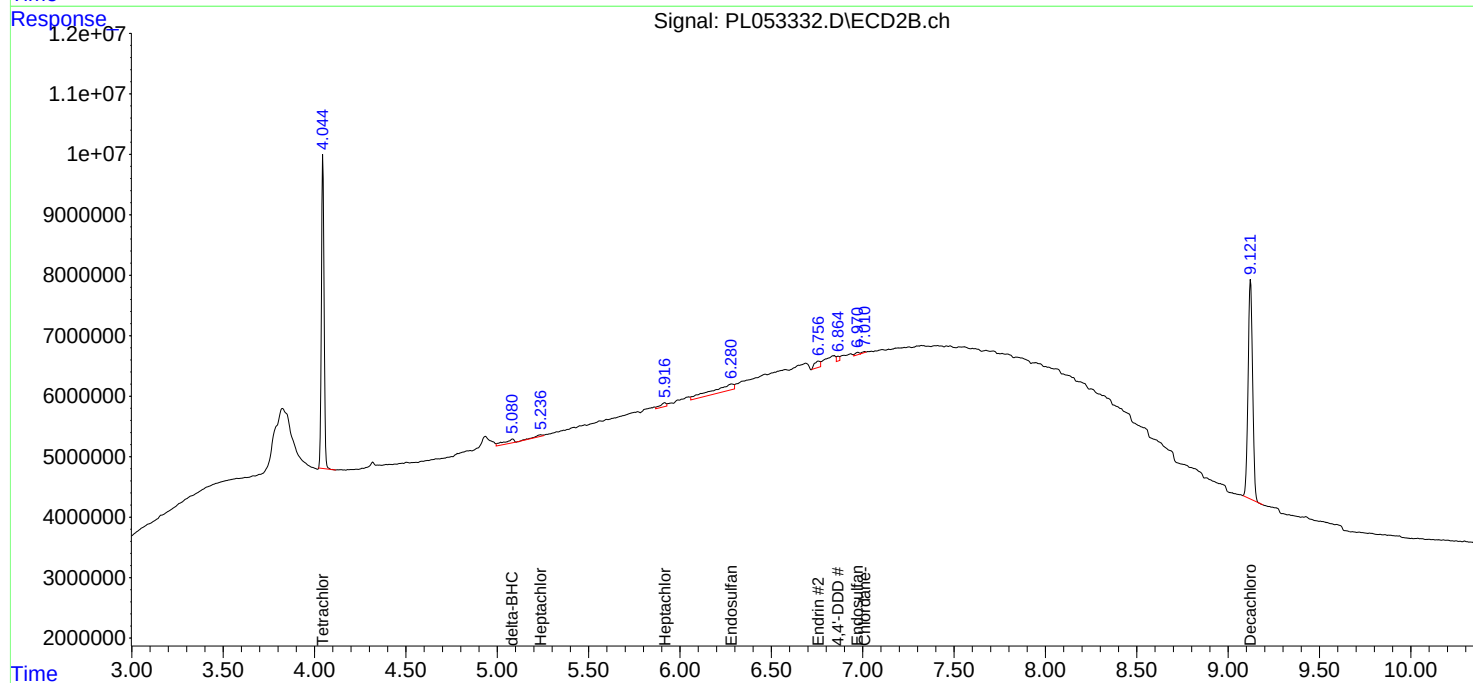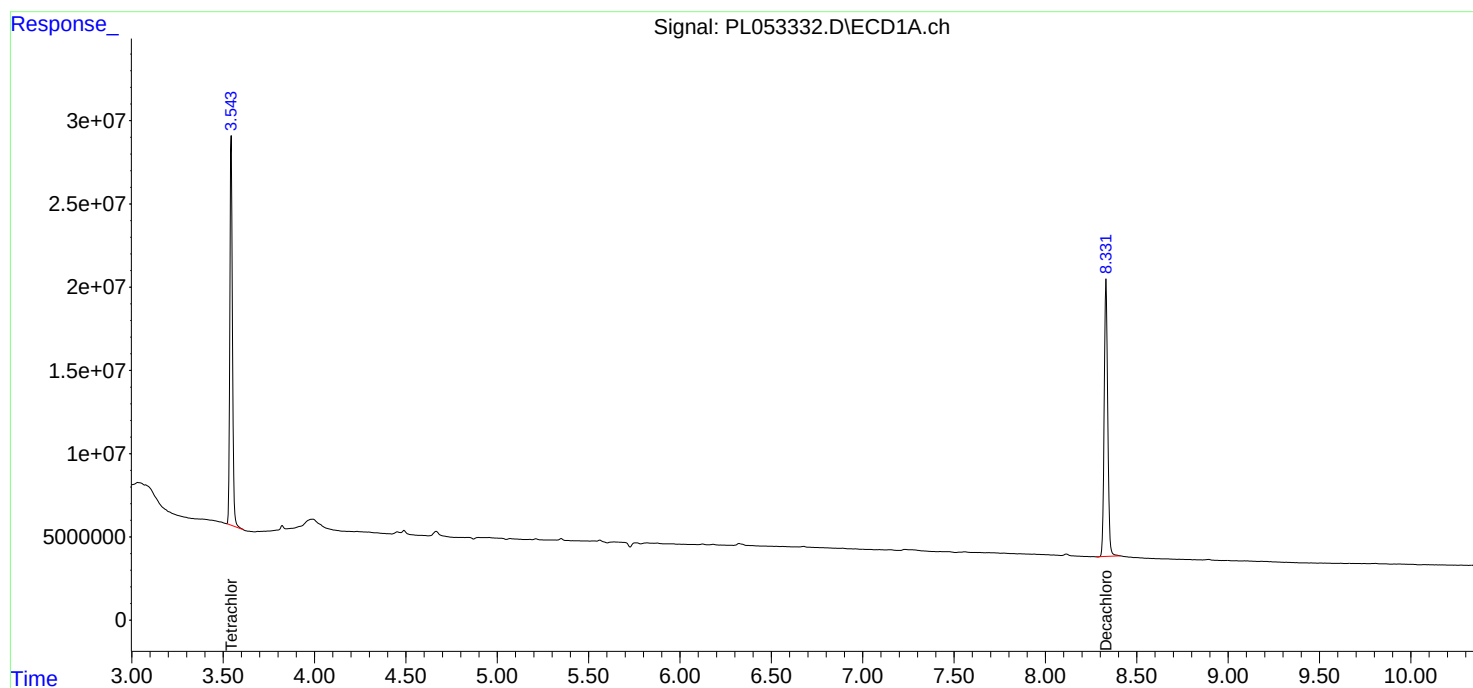


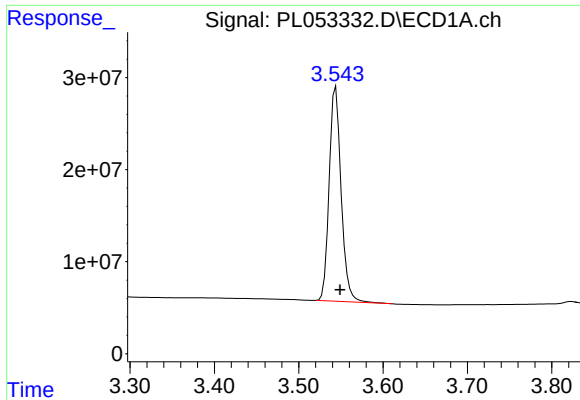

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: -0.005 min
Response: 230140048
Conc: 23.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

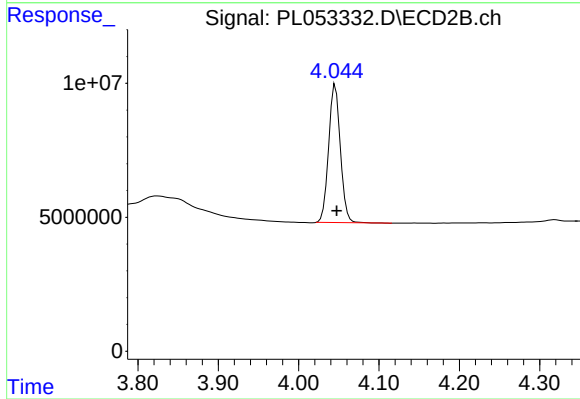


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: -0.001 min
Response: 52361062
Conc: 19.50 ng/ml

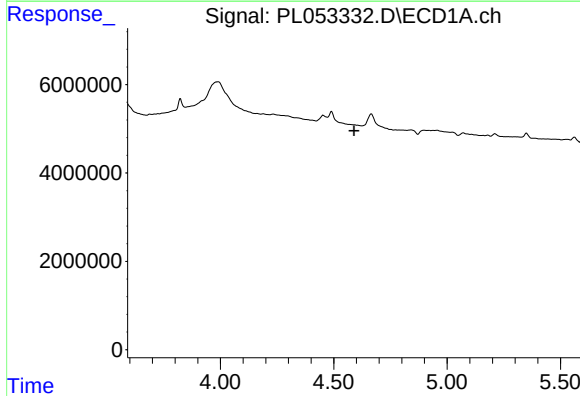


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.590 min
Response: 0
Conc: N.D.

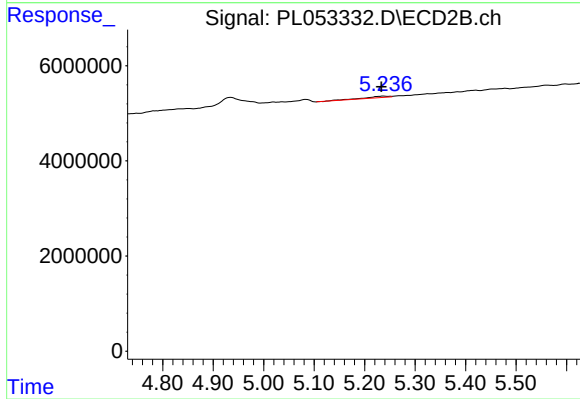

#4 Heptachlor


R.T.: 5.238 min
Delta R.T.: 0.004 min
Response: 925287
Conc: 0.24 ng/ml

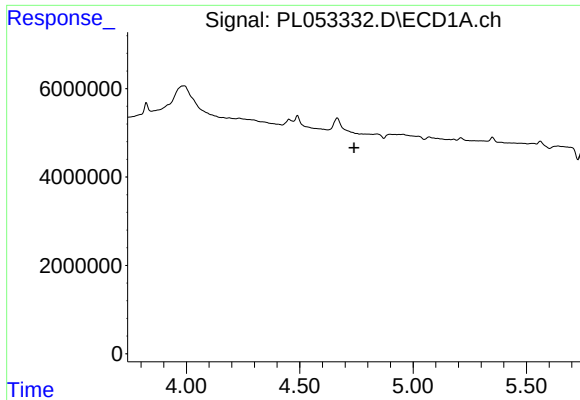

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.740 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

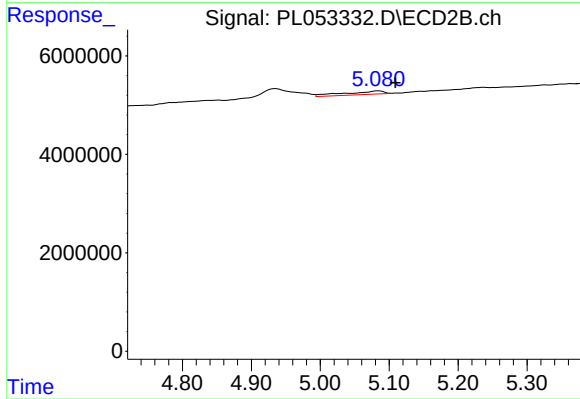


#7 delta-BHC

R.T.: 5.084 min
Delta R.T.: -0.025 min
Response: 2665524
Conc: 0.74 ng/ml

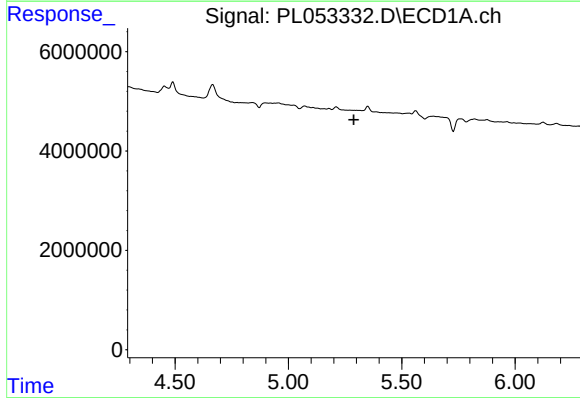


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.289 min
Response: 0
Conc: N.D.

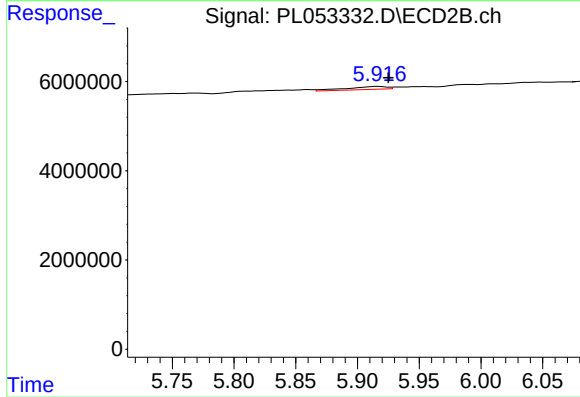

#8 Heptachlor epoxide


R.T.: 5.917 min
Delta R.T.: -0.008 min
Response: 1514681
Conc: 0.45 ng/ml

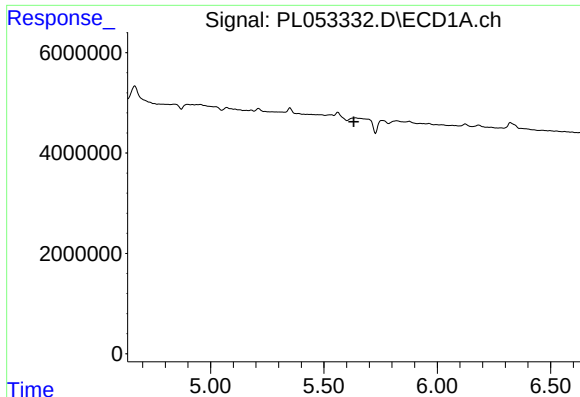

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.632 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

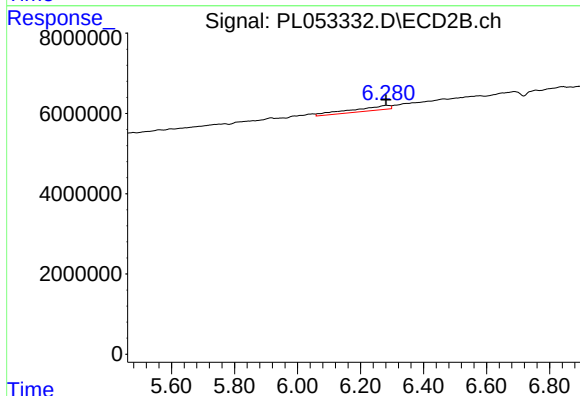


#9 Endosulfan I

R.T.: 6.282 min
Delta R.T.: 0.000 min
Response: 9491993
Conc: 3.04 ng/ml

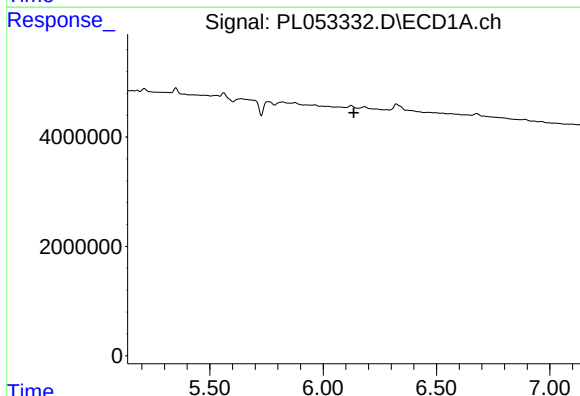


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.135 min
Response: 0
Conc: N.D.

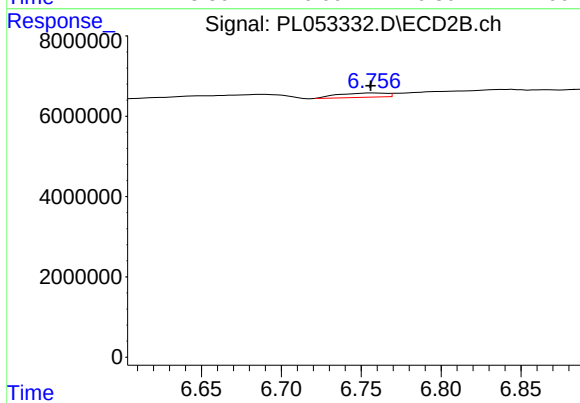

#14 Endrin


R.T.: 6.758 min
Delta R.T.: 0.002 min
Response: 2265259
Conc: 0.82 ng/ml

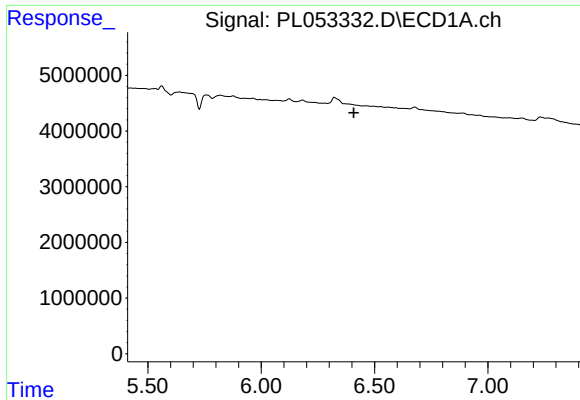

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

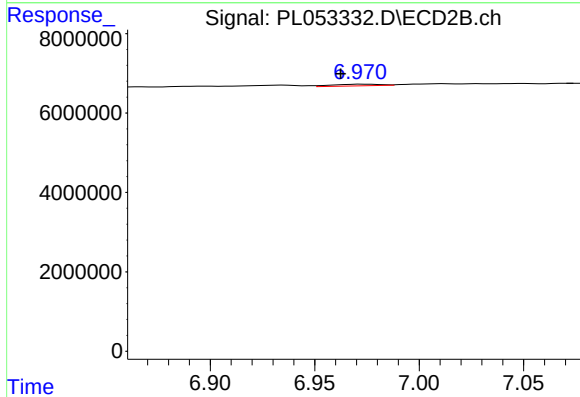


#15 Endosulfan II

R.T.: 6.973 min
Delta R.T.: 0.011 min
Response: 663249
Conc: 0.22 ng/ml

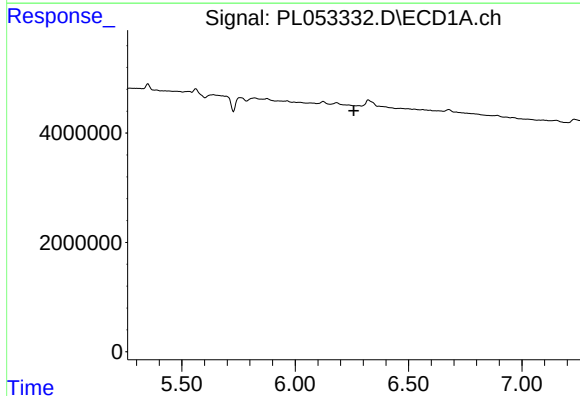


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.258 min
Response: 0
Conc: N.D.

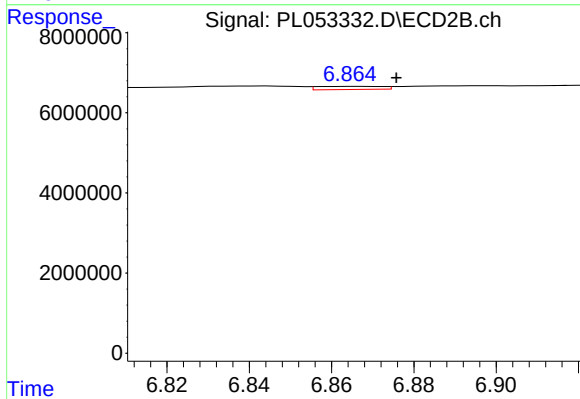

#16 4,4'-DDD


R.T.: 6.866 min
Delta R.T.: -0.010 min
Response: 868220
Conc: 0.35 ng/ml

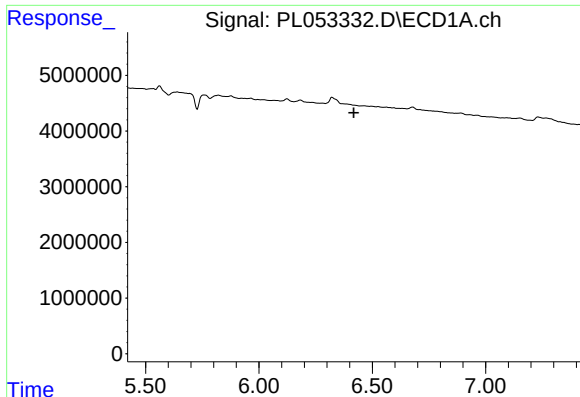

#27 Chlorodane-5


R.T.: 0.000 min
Exp R.T.: 6.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

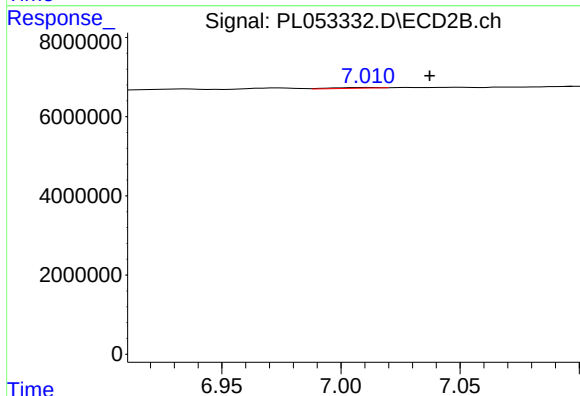


#27 Chlorodane-5

R.T.: 7.011 min
Delta R.T.: -0.026 min
Response: 247797
Conc: 2.81 ng/ml

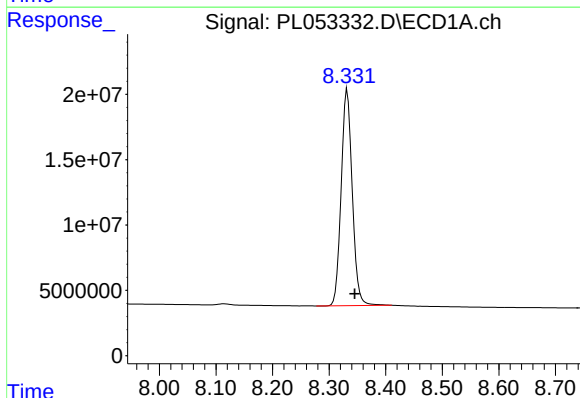

#28 Decachlorobiphenyl

R.T.: 8.332 min
Delta R.T.: -0.013 min
Response: 225088162
Conc: 22.47 ng/ml

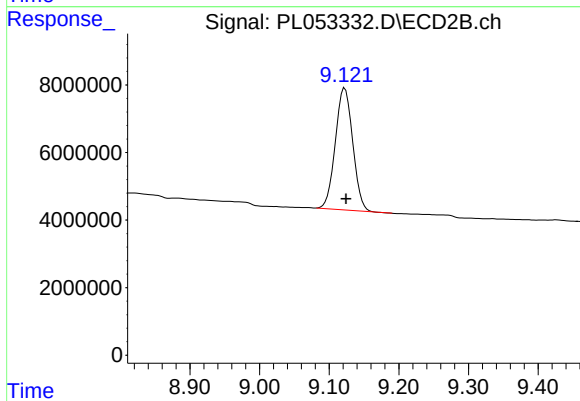

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.002 min
Response: 61294741
Conc: 20.89 ng/ml