

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101619\
 Data File : PL053345.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2019 15:46
 Operator : SG\AJ
 Sample : PB123986BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 00:44:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	4.046	182.4E6	39935124	18.339	14.872
28)	SA Decachlor...	8.334	9.124	173.6E6	49619557	17.330	16.914
Target Compounds							
4)	MA Heptachlor	0.000	5.234	0	4270390	N.D.	1.121 #
7)	B delta-BHC	0.000	5.084f	0	2309943	N.D.	0.638 #
8)	B Heptachlo...	0.000	5.907f	0	1274377	N.D.	0.380 #
10)	B gamma-Chl...	0.000	6.131f	0	5503167	N.D.	1.627 #
12)	B 4,4'-DDE	0.000	6.357f	0	5873604	N.D.	1.798 #
15)	B Endosulfa...	0.000	6.973	0	612018	N.D.	0.206 #
24)	Chlordane-2	0.000	5.502	0	815524	N.D.	7.287 #
25)	Chlordane-3	0.000	6.131f	0	5503167	N.D.	12.636 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101619\
Data File : PL053345.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 15:46
Operator : SG\AJ
Sample : PB123986BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 00:44:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

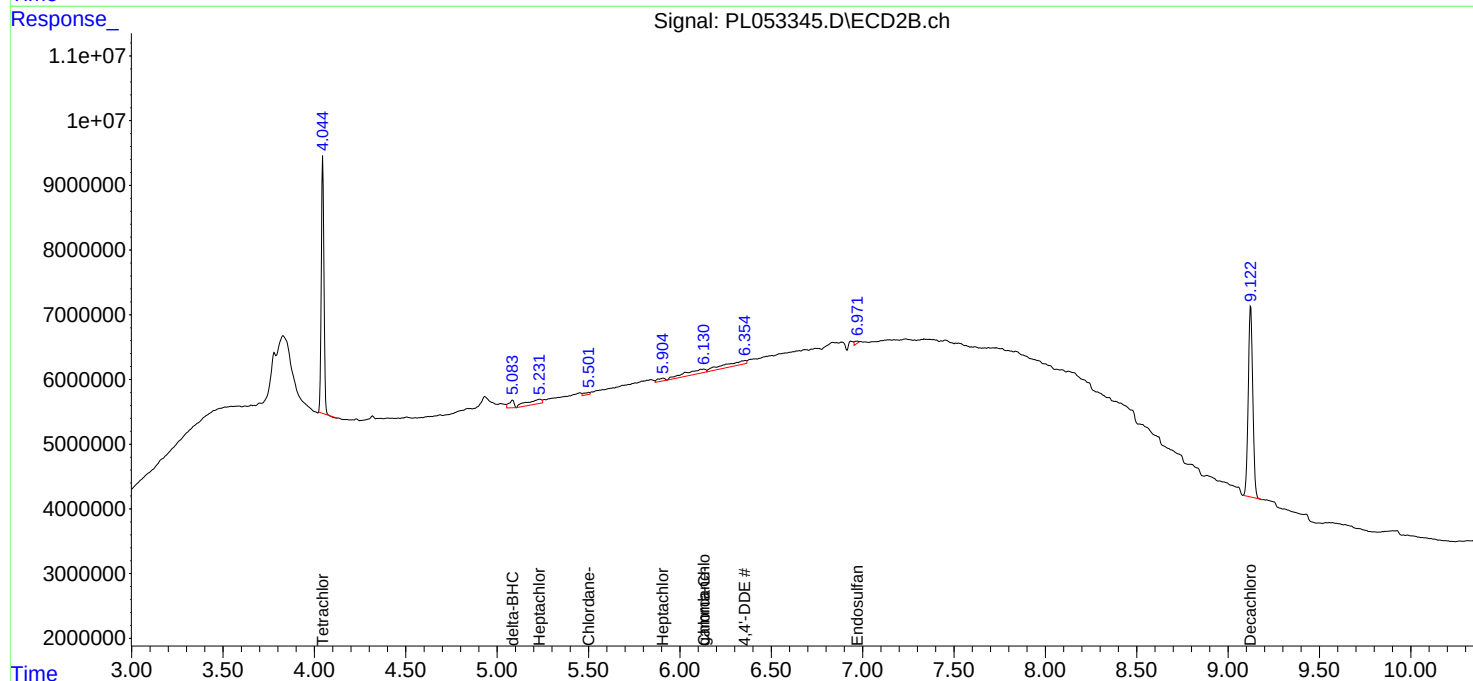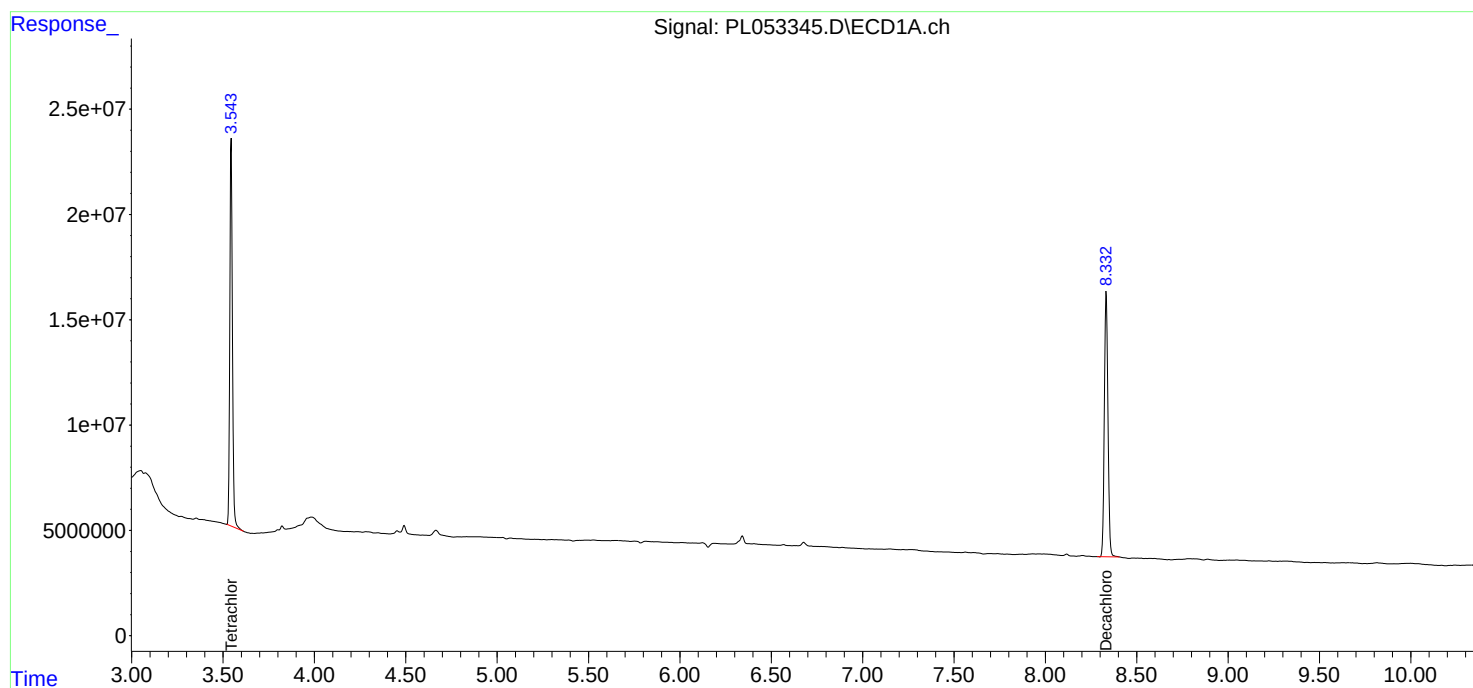


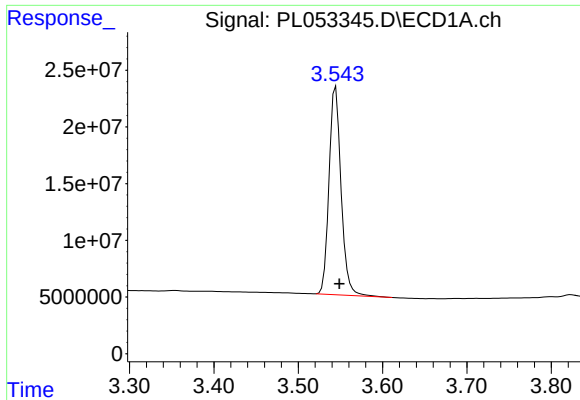

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: -0.004 min
Response: 182408637
Conc: 18.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

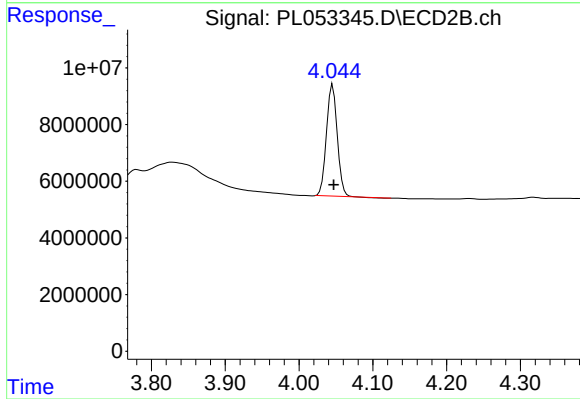


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: -0.002 min
Response: 39935124
Conc: 14.87 ng/ml

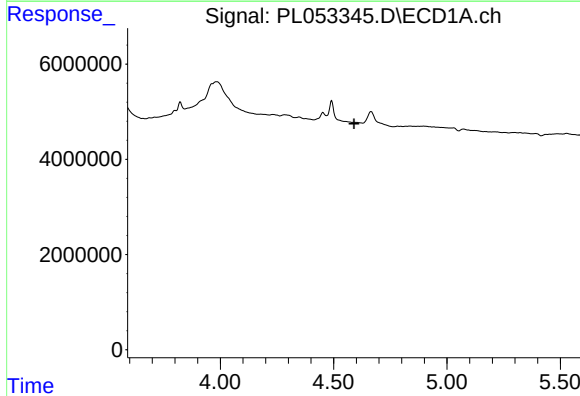


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.590 min
Response: 0
Conc: N.D.

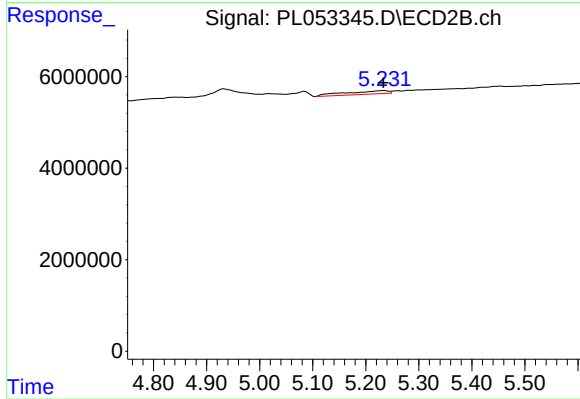

#4 Heptachlor


R.T.: 5.234 min
Delta R.T.: 0.000 min
Response: 4270390
Conc: 1.12 ng/ml

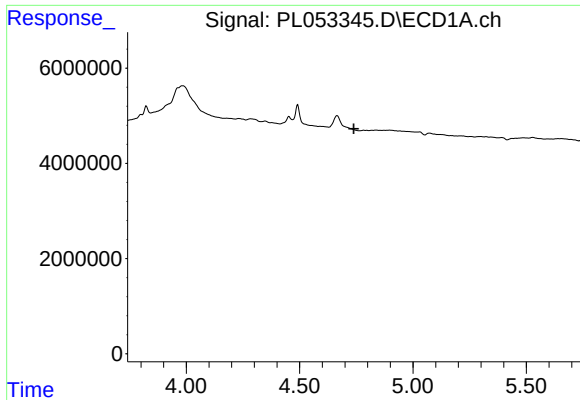

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.740 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

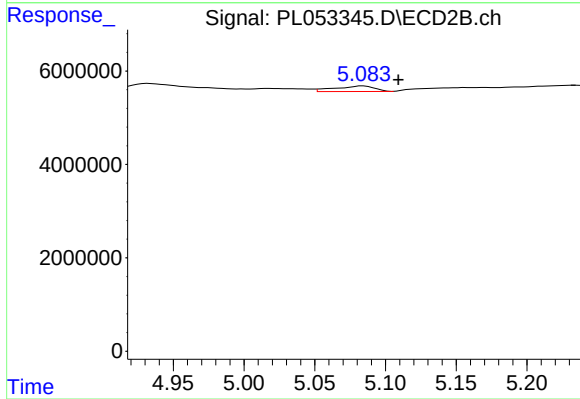


#7 delta-BHC

R.T.: 5.084 min
Delta R.T.: -0.025 min
Response: 2309943
Conc: 0.64 ng/ml

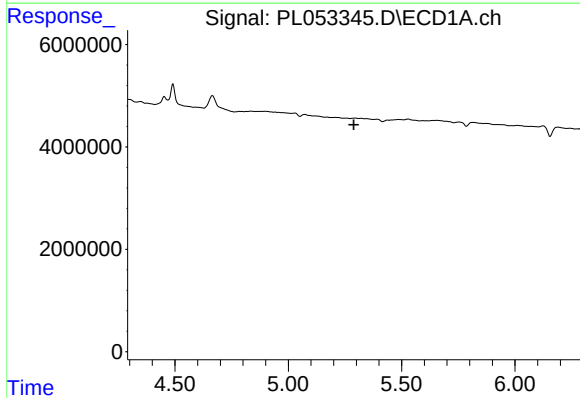


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.289 min
Response: 0
Conc: N.D.

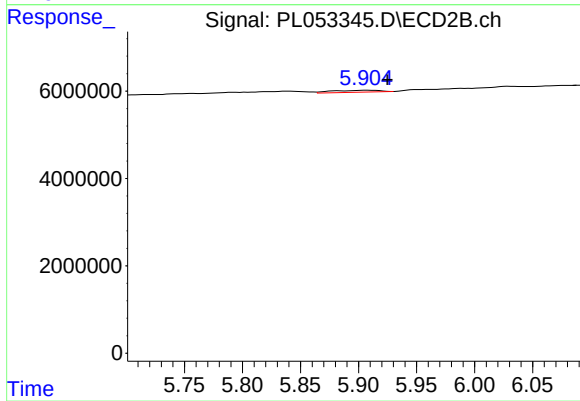

#8 Heptachlor epoxide


R.T.: 5.907 min
Delta R.T.: -0.018 min
Response: 1274377
Conc: 0.38 ng/ml

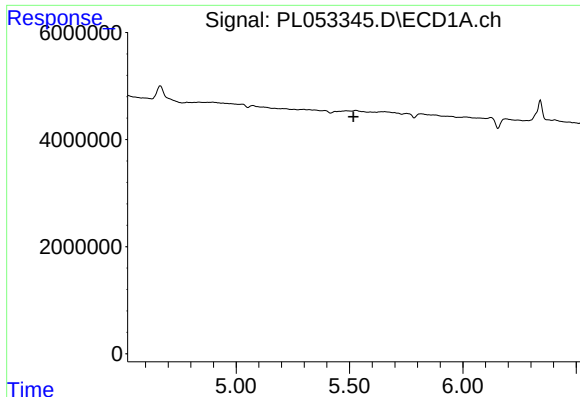

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

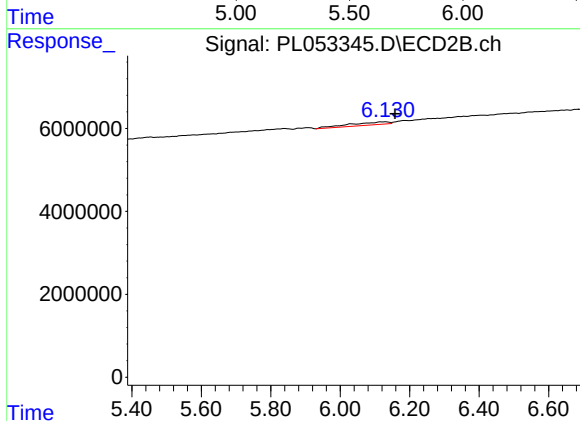


#10 gamma-Chlordane

R.T.: 6.131 min
Delta R.T.: -0.027 min
Response: 5503167
Conc: 1.63 ng/ml

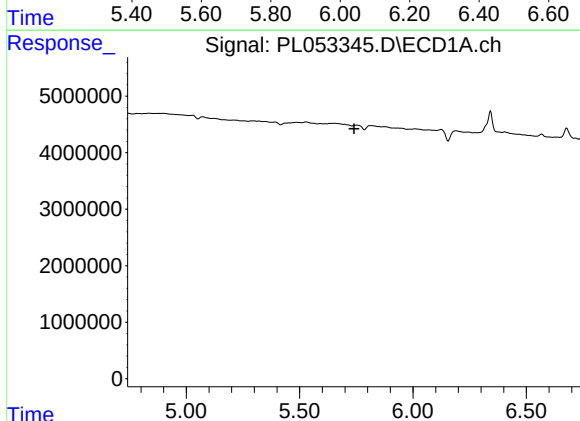


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.740 min
Response: 0
Conc: N.D.

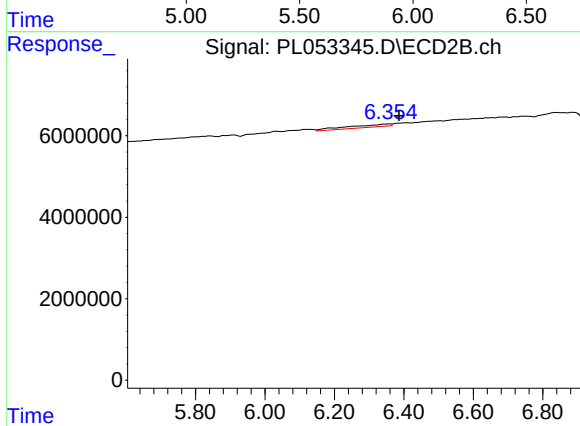

#12 4,4'-DDE


R.T.: 6.357 min
Delta R.T.: -0.029 min
Response: 5873604
Conc: 1.80 ng/ml

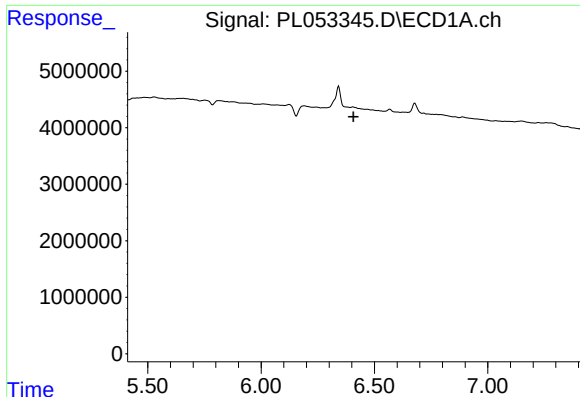

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

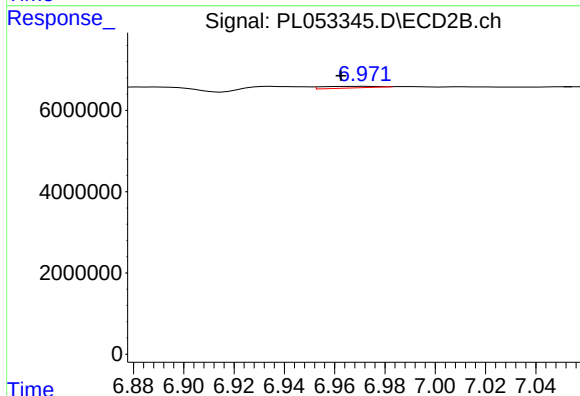


#15 Endosulfan II

R.T.: 6.973 min
Delta R.T.: 0.010 min
Response: 612018
Conc: 0.21 ng/ml

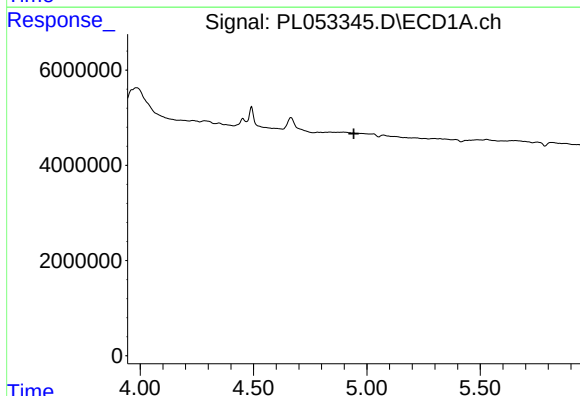


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

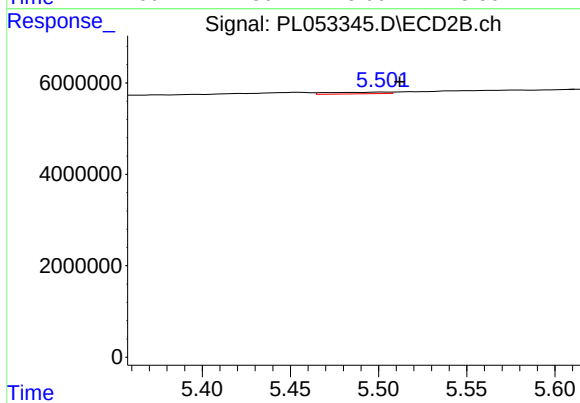

#24 Chlordane-2


R.T.: 5.502 min
Delta R.T.: -0.010 min
Response: 815524
Conc: 7.29 ng/ml

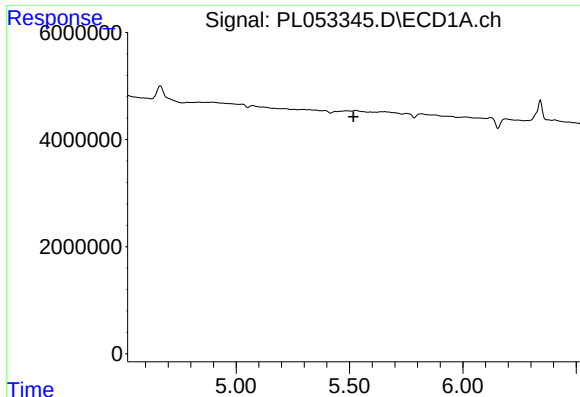

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

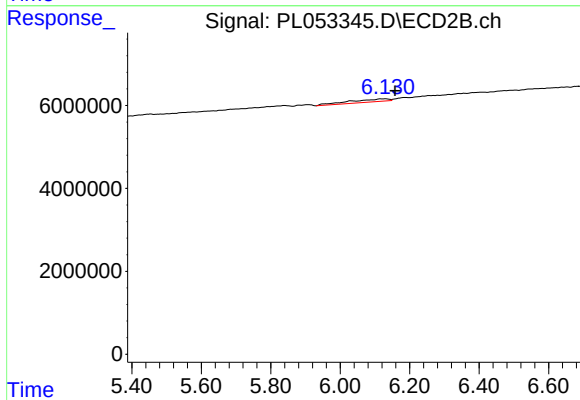


#25 Chlordane-3

R.T.: 6.131 min
Delta R.T.: -0.027 min
Response: 5503167
Conc: 12.64 ng/ml

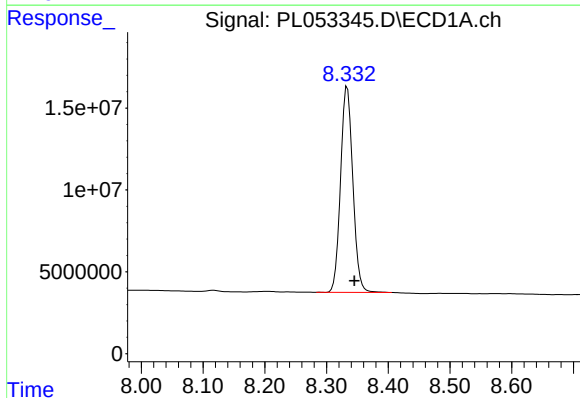

#28 Decachlorobiphenyl

R.T.: 8.334 min
Delta R.T.: -0.011 min
Response: 173573732
Conc: 17.33 ng/ml

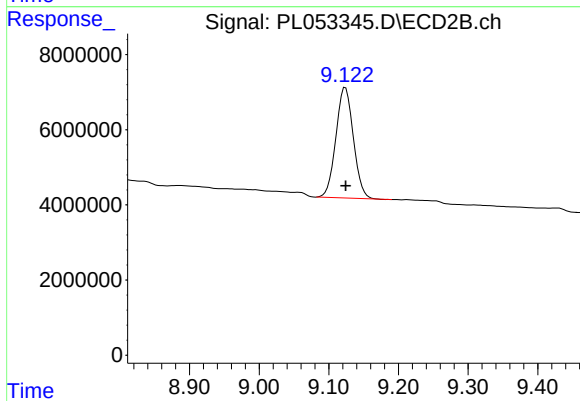

#28 Decachlorobiphenyl

R.T.: 9.124 min
Delta R.T.: 0.000 min
Response: 49619557
Conc: 16.91 ng/ml