

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101620\
 Data File : PL062342.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2020 16:12
 Operator : DD\AJ
 Sample : L4406-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 05:21:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 13 05:04:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.951	24827948	37835727	14.264	13.425
28)	SA Decachlor...	8.124	8.992	21128452	30559144	11.550	11.134
Target Compounds							
8)	B Heptachlo...	5.100	5.810	830550	1396788	0.454	0.430
10)	B gamma-Chl...	5.327	6.049	3062054	3506384	1.698	1.068 #
11)	B alpha-Chl...	5.383	6.123	2771813	5819800	1.531	1.781
12)	B 4,4'-DDE	5.548	6.279	1393650	2236653	0.845	0.735
16)	A 4,4'-DDD	0.000	6.773	0	2084316	N.D.	0.854 #
17)	MA 4,4'-DDT	6.297	7.069	1359241	1630111	1.054	0.713 #
25)	Chlordane-3	5.327	6.049	3062054	3506384	19.217	8.562 #
26)	Chlordane-4	5.383	6.123	2771813	5819800	20.832	11.777 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101620\
Data File : PL062342.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2020 16:12
Operator : DD\AJ
Sample : L4406-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 05:21:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
Quant Title : GC Extractables
QLast Update : Tue Oct 13 05:04:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

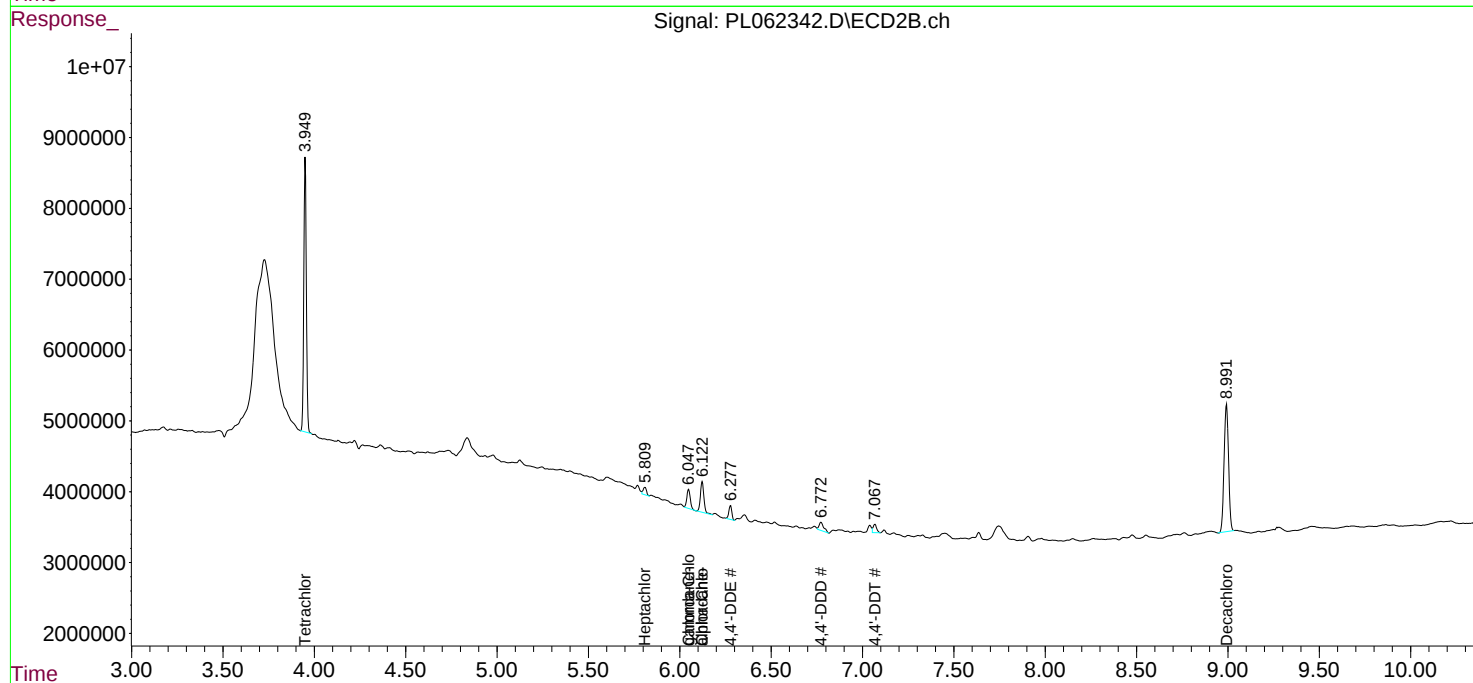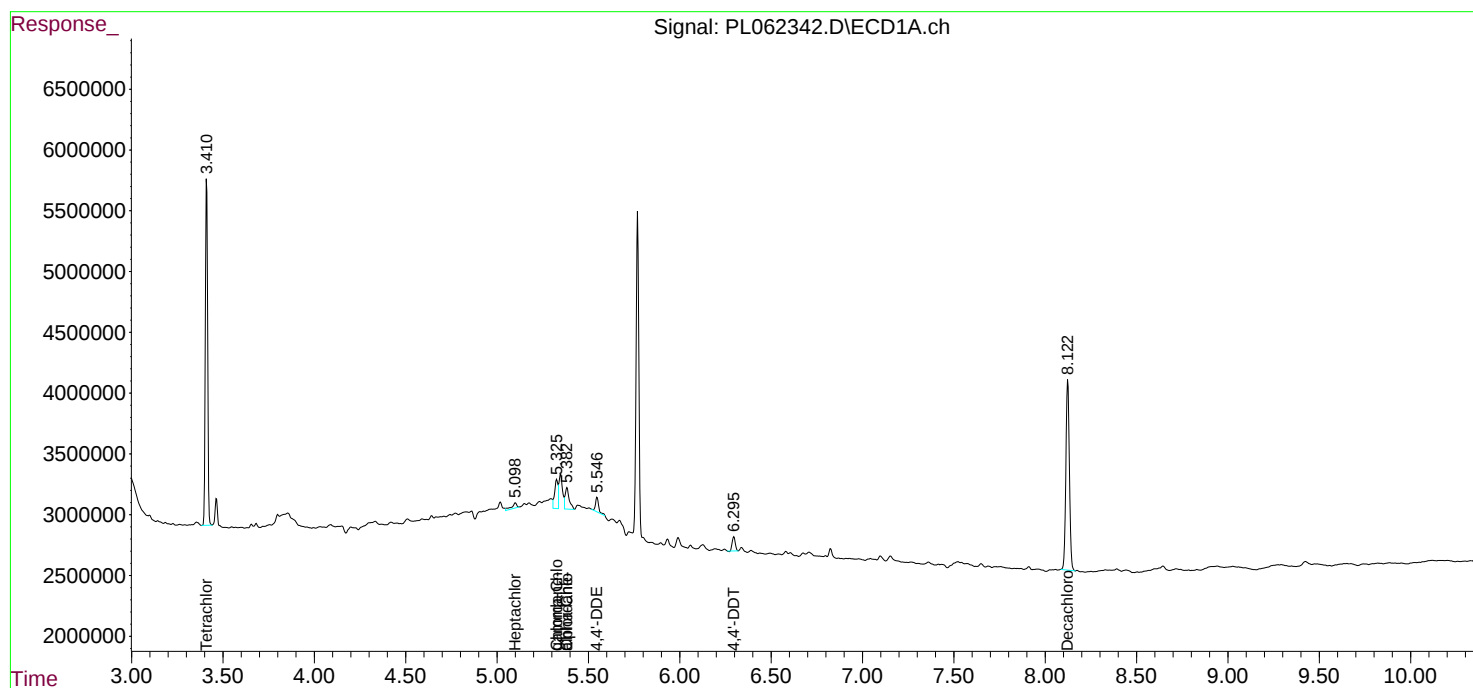


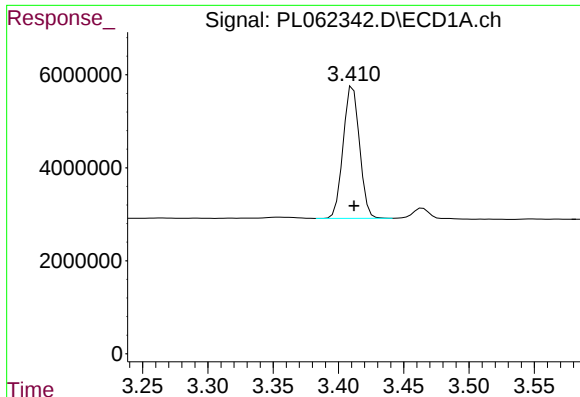

#1 Tetrachloro-m-xylene


R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 24827948
Conc: 14.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

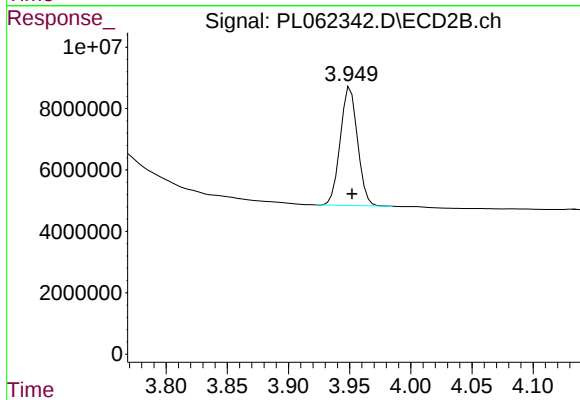


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: -0.001 min
Response: 37835727
Conc: 13.42 ng/ml

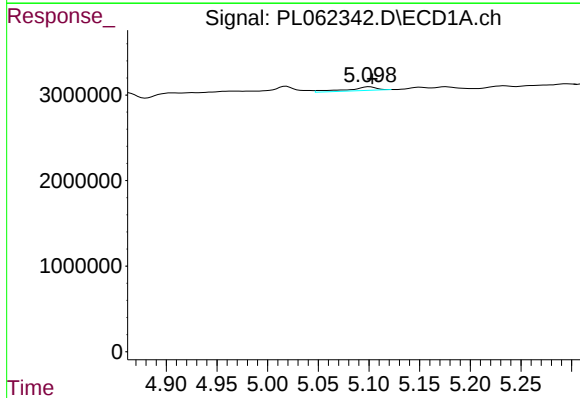


#8 Heptachlor epoxide

R.T.: 5.100 min
Delta R.T.: -0.003 min
Response: 830550
Conc: 0.45 ng/ml

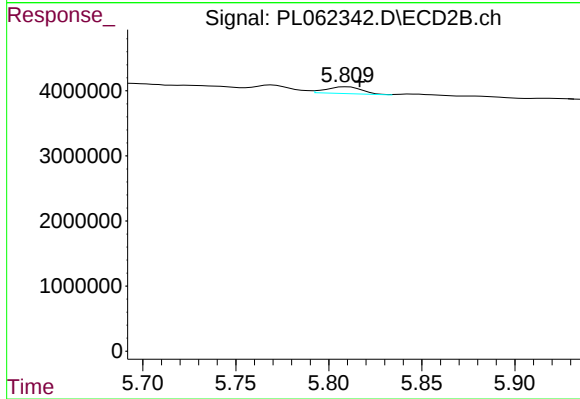

#8 Heptachlor epoxide


R.T.: 5.810 min
Delta R.T.: -0.007 min
Response: 1396788
Conc: 0.43 ng/ml

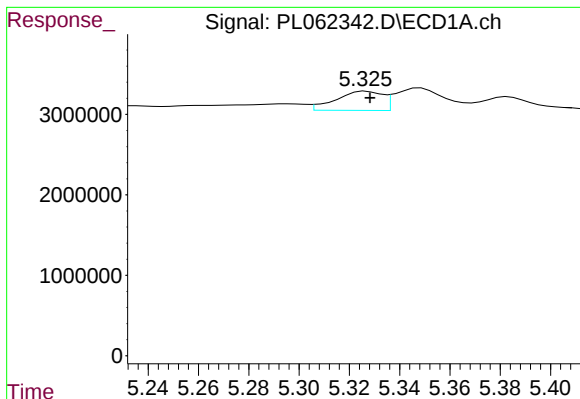

#10 gamma-Chlordane


R.T.: 5.327 min
Delta R.T.: -0.002 min
Response: 3062054
Conc: 1.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

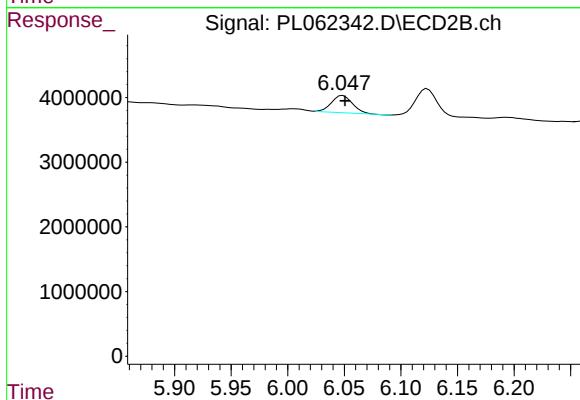


#10 gamma-Chlordane

R.T.: 6.049 min
Delta R.T.: -0.002 min
Response: 3506384
Conc: 1.07 ng/ml

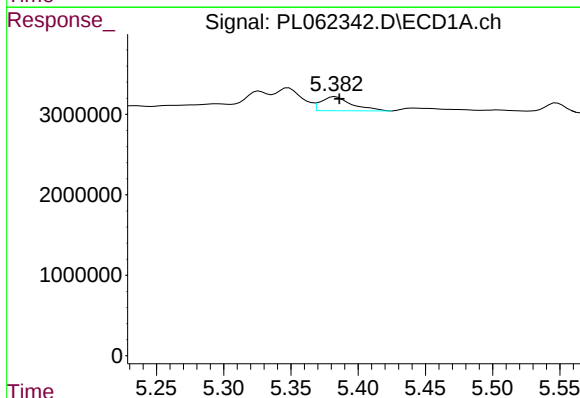


#11 alpha-Chlordane

R.T.: 5.383 min
Delta R.T.: -0.003 min
Response: 2771813
Conc: 1.53 ng/ml

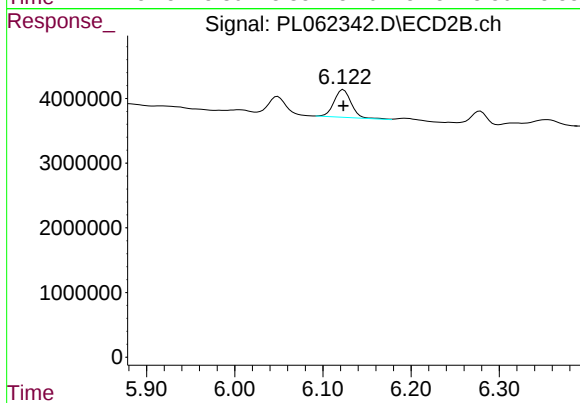

#11 alpha-Chlordane


R.T.: 6.123 min
Delta R.T.: 0.000 min
Response: 5819800
Conc: 1.78 ng/ml

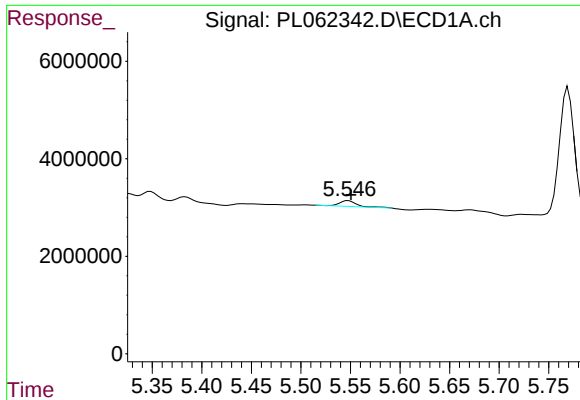

#12 4,4'-DDE


R.T.: 5.548 min
Delta R.T.: -0.003 min
Response: 1393650
Conc: 0.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

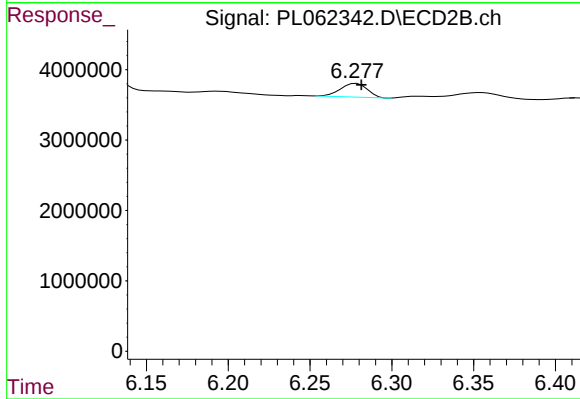


#12 4,4'-DDE

R.T.: 6.279 min
Delta R.T.: -0.003 min
Response: 2236653
Conc: 0.74 ng/ml

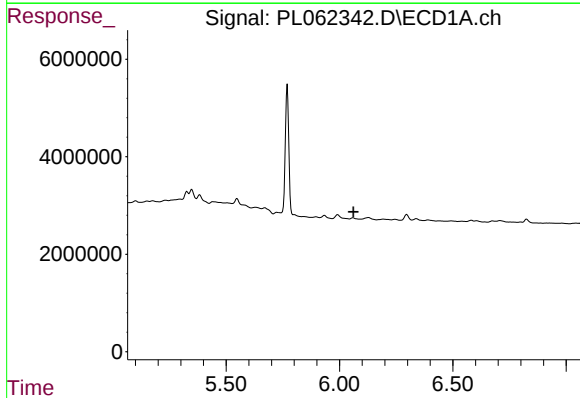


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.062 min
Response: 0
Conc: N.D.

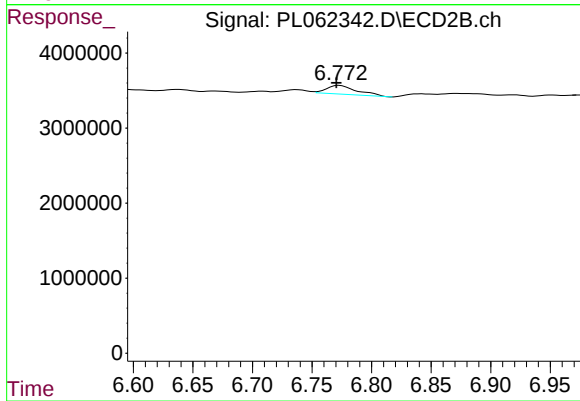

#16 4,4'-DDD


R.T.: 6.773 min
Delta R.T.: 0.003 min
Response: 2084316
Conc: 0.85 ng/ml

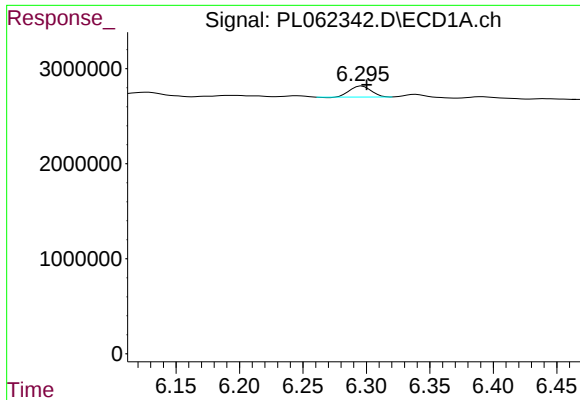

#17 4,4'-DDT


R.T.: 6.297 min
Delta R.T.: -0.004 min
Response: 1359241
Conc: 1.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

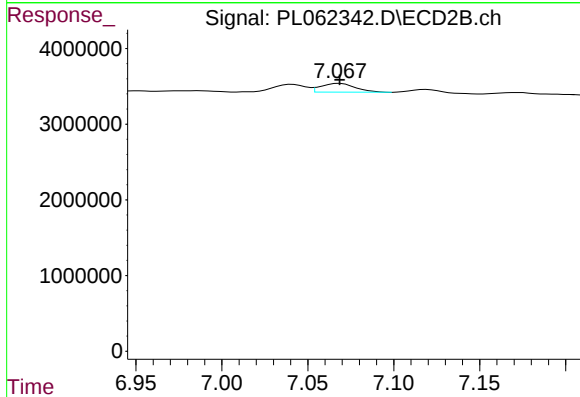


#17 4,4'-DDT

R.T.: 7.069 min
Delta R.T.: 0.000 min
Response: 1630111
Conc: 0.71 ng/ml

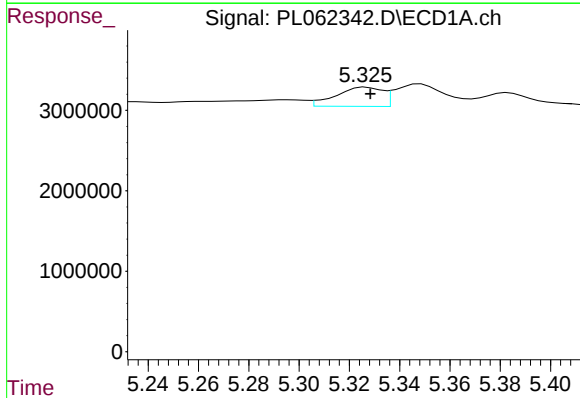


#25 Chlordane-3

R.T.: 5.327 min
Delta R.T.: -0.002 min
Response: 3062054
Conc: 19.22 ng/ml

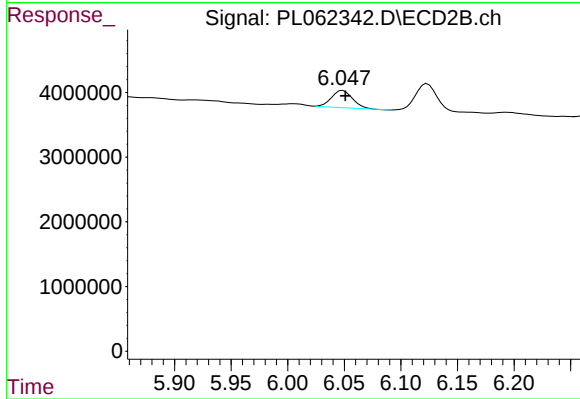

#25 Chlordane-3


R.T.: 6.049 min
Delta R.T.: -0.002 min
Response: 3506384
Conc: 8.56 ng/ml

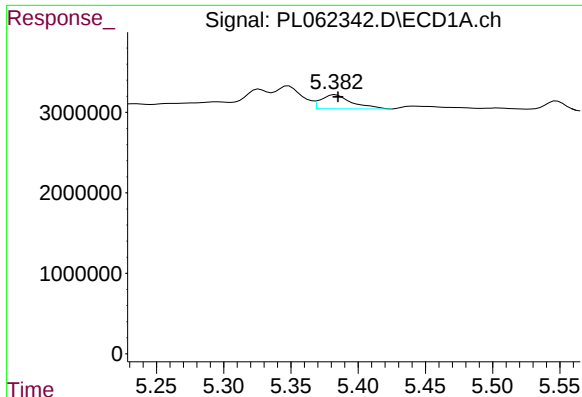

#26 Chlordane-4


R.T.: 5.383 min
Delta R.T.: -0.002 min
Response: 2771813
Conc: 20.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

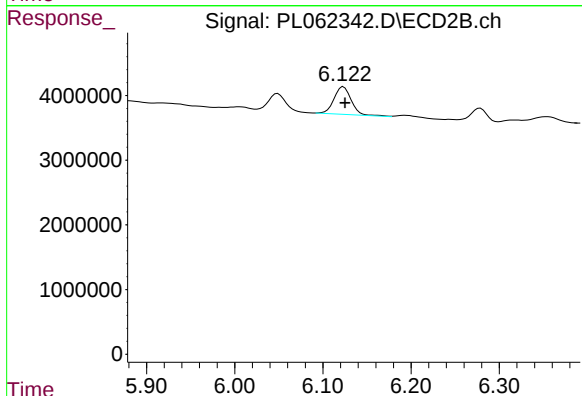


#26 Chlordane-4

R.T.: 6.123 min
Delta R.T.: -0.002 min
Response: 5819800
Conc: 11.78 ng/ml

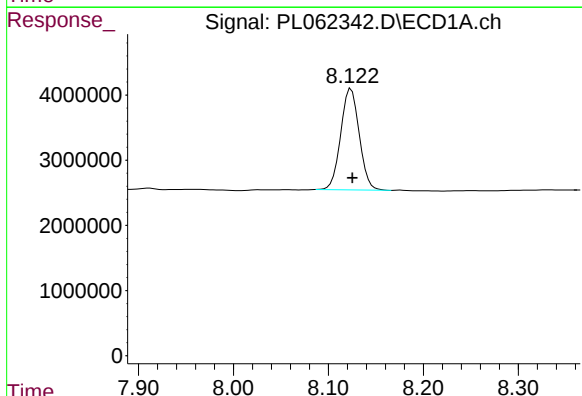

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.002 min
Response: 21128452
Conc: 11.55 ng/ml

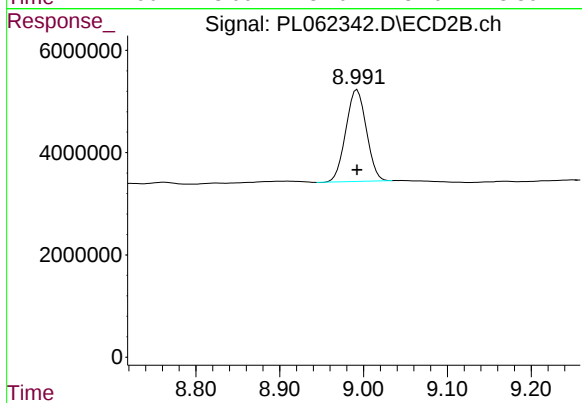

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 30559144
Conc: 11.13 ng/ml