

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101620\
 Data File : PL062352.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2020 18:34
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 05:24:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 13 05:04:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	38927967	61606628	22.365	21.859
28)	SA Decachlor...	8.124	8.994	38792304	56378827	21.207	20.541
Target Compounds							
8)	B Heptachlo...	0.000	5.811	0	5960455	N.D.	1.834 #
10)	B gamma-Chl...	0.000	6.057	0	765408	N.D.	0.233 #
25)	Chlordane-3	0.000	6.057	0	765408	N.D.	1.869 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101620\
Data File : PL062352.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2020 18:34
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 05:24:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
Quant Title : GC Extractables
QLast Update : Tue Oct 13 05:04:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

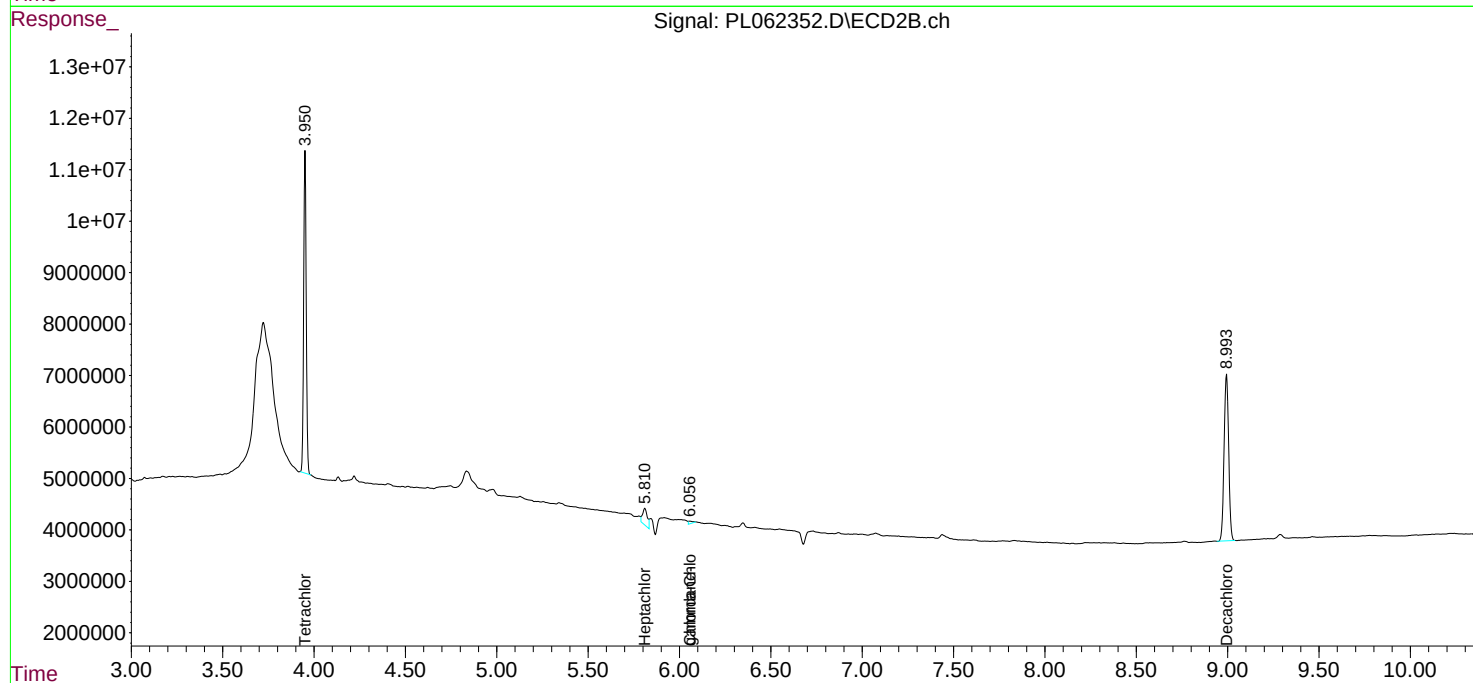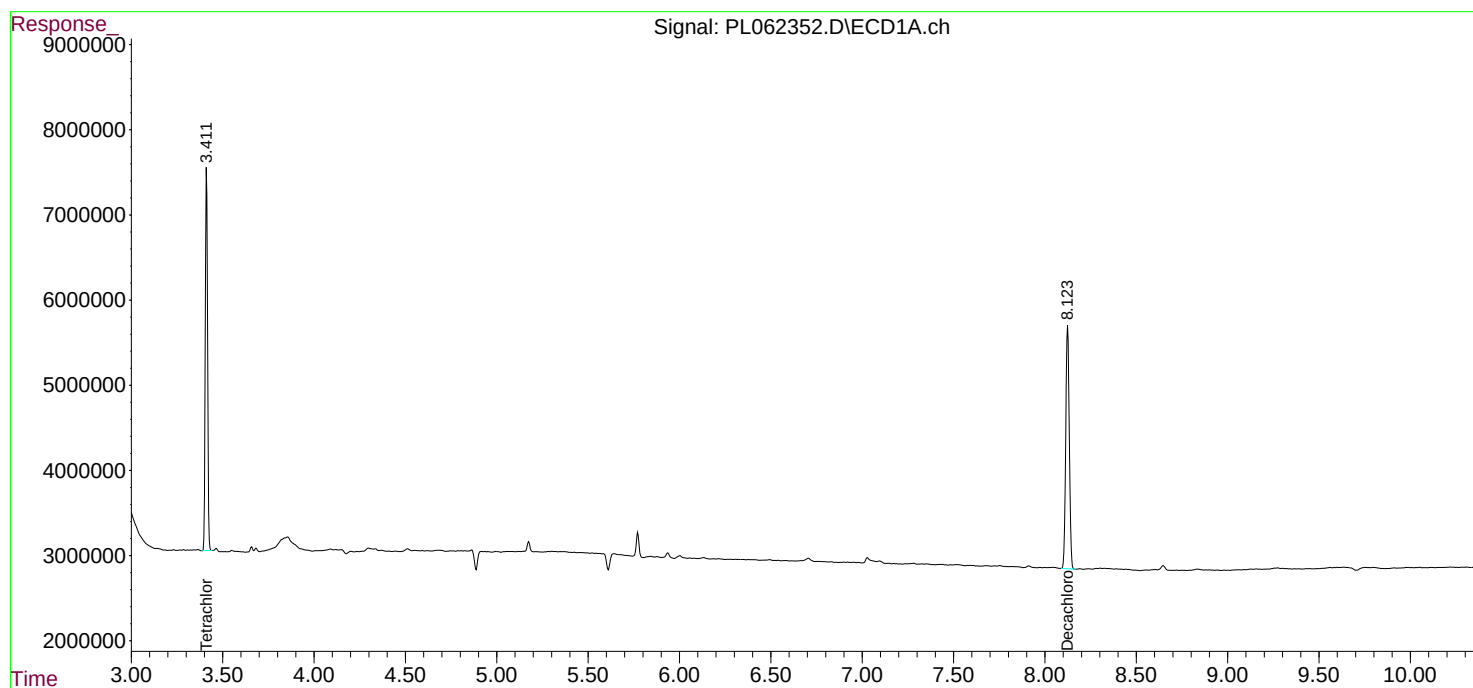


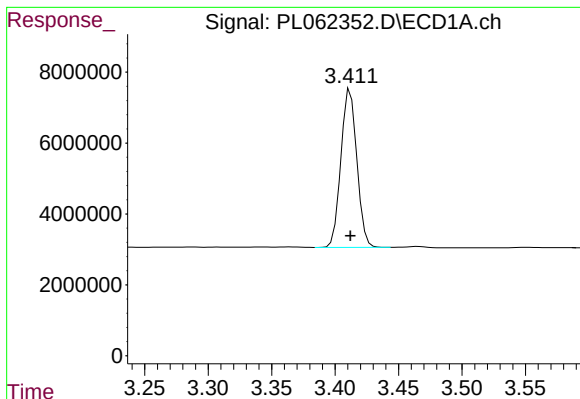

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 38927967
Conc: 22.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

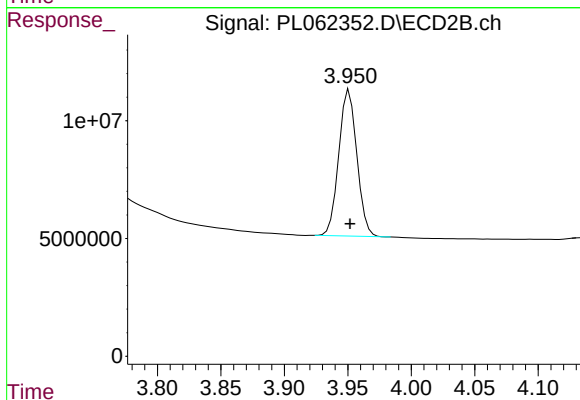


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 61606628
Conc: 21.86 ng/ml

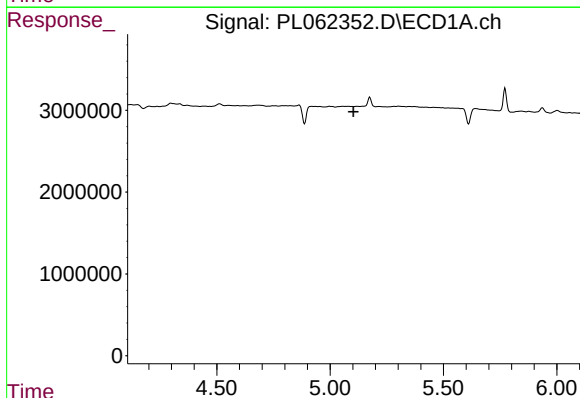


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.103 min
Response: 0
Conc: N.D.

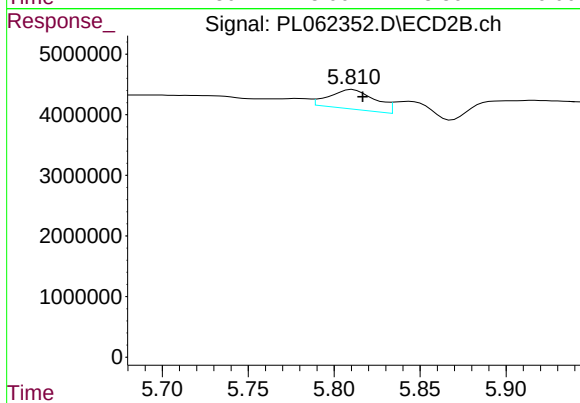

#8 Heptachlor epoxide


R.T.: 5.811 min
Delta R.T.: -0.006 min
Response: 5960455
Conc: 1.83 ng/ml

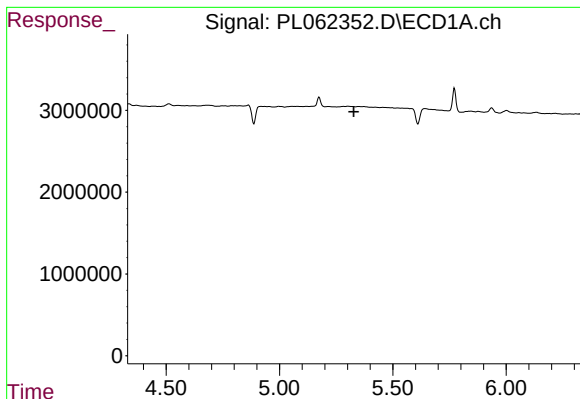

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

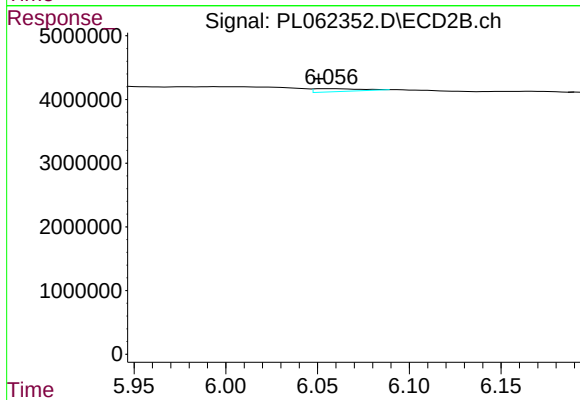


#10 gamma-Chlordane

R.T.: 6.057 min
Delta R.T.: 0.007 min
Response: 765408
Conc: 0.23 ng/ml

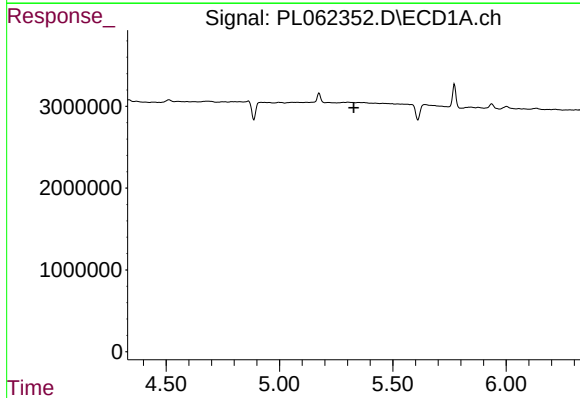


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

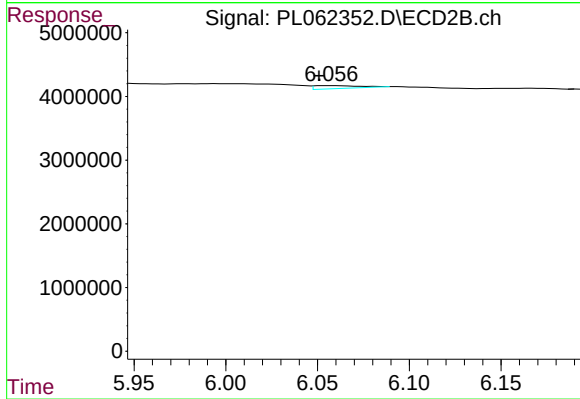

#25 Chlordane-3


R.T.: 6.057 min
Delta R.T.: 0.007 min
Response: 765408
Conc: 1.87 ng/ml

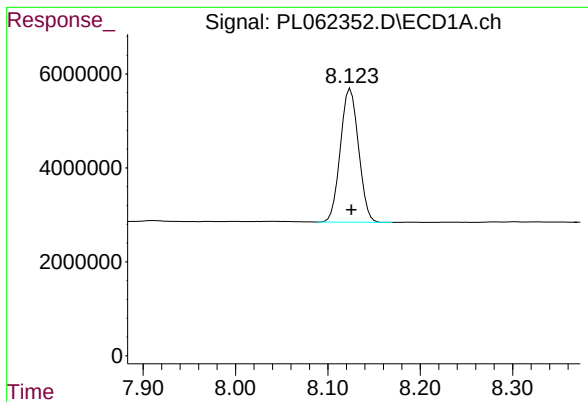

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: 0.000 min
Response: 38792304
Conc: 21.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

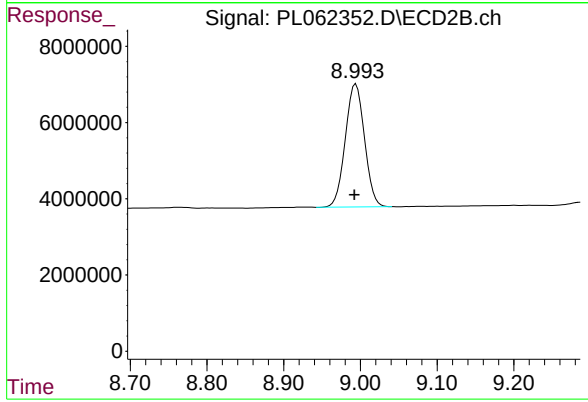

#28 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: 0.002 min
Response: 56378827
Conc: 20.54 ng/ml