

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101620\
 Data File : PL062331.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2020 13:35
 Operator : DD\AJ
 Sample : L4227-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BU-01-101420

Manual Integrations
 APPROVED

Ankita
 10/16/2020 11:51:04 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 18:05:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 13 05:04:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.950	23935276	35798183	13.751	12.702
28)	SA Decachlor...	8.125	8.990	19496592	29582550	10.658	10.778m
Target Compounds							
17)	MA 4,4'-DDT	6.296	7.068	1669060	1350473	1.294m	0.590 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101620\
Data File : PL062331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2020 13:35
Operator : DD\AJ
Sample : L4227-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
BU-01-101420


Manual Integrations
APPROVED

Ankita
10/16/2020 11:51:04 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 18:05:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
Quant Title : GC Extractables
QLast Update : Tue Oct 13 05:04:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

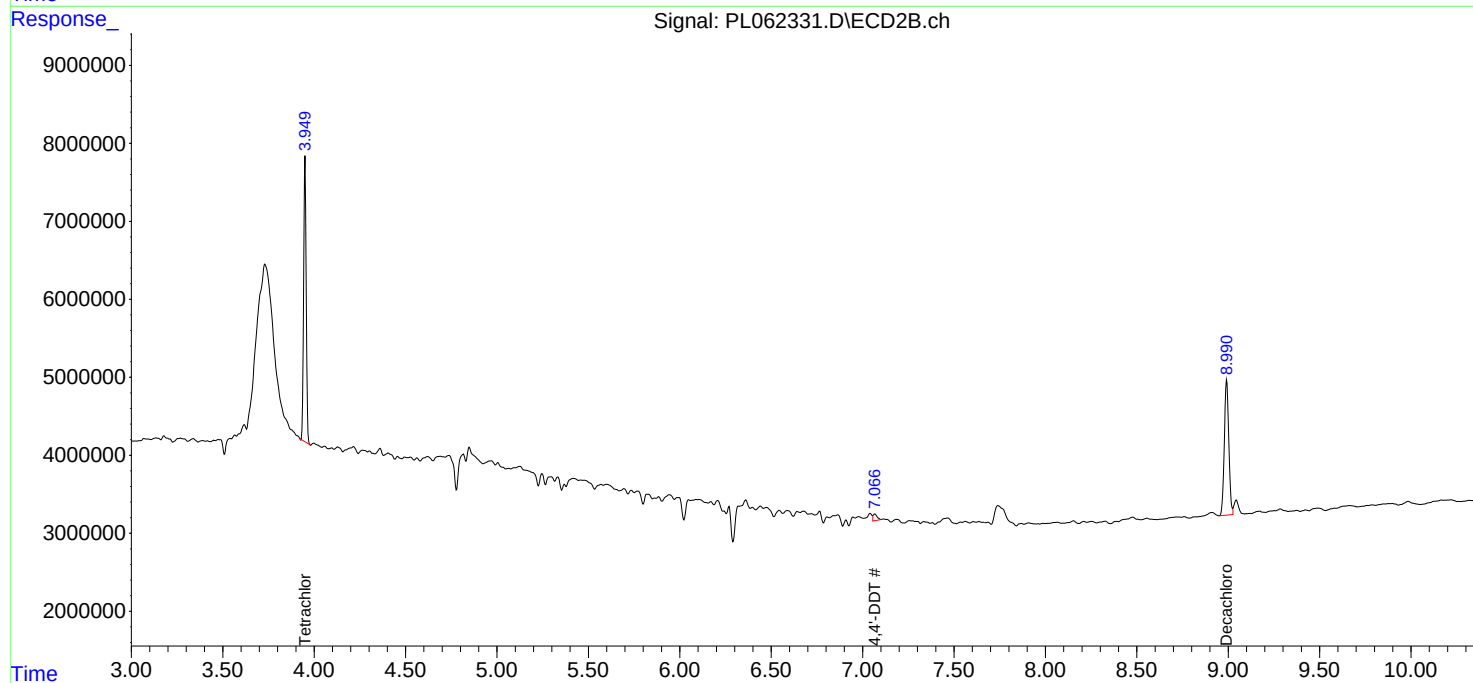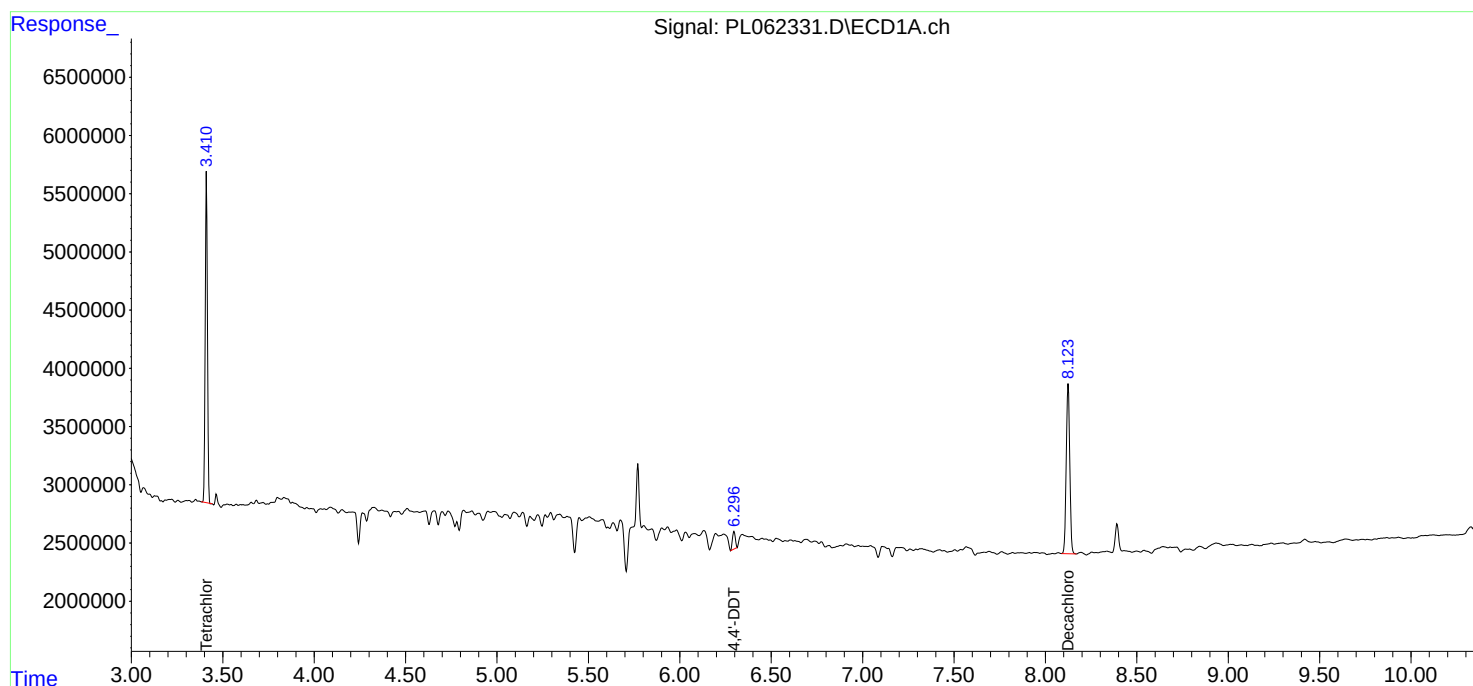

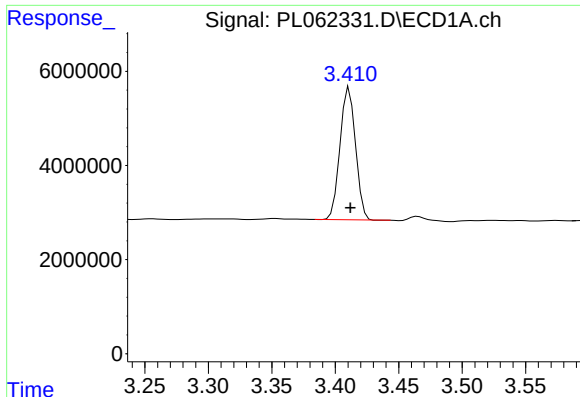


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 23935276
Conc: 13.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
BU-01-101420


Manual Integrations
APPROVED

Ankita
10/16/2020 11:51:04 AM

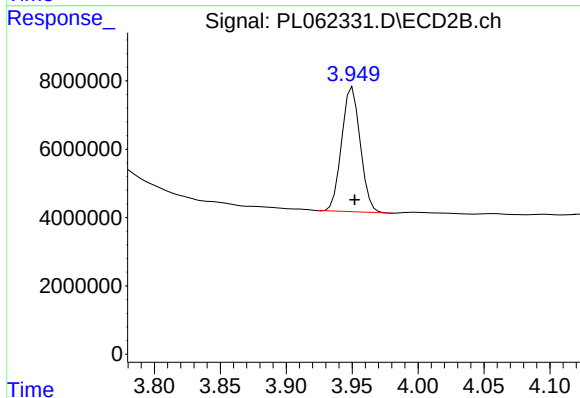


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 35798183
Conc: 12.70 ng/ml

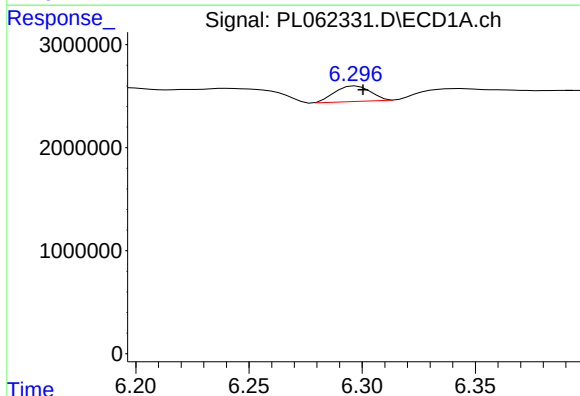


#17 4,4'-DDT

R.T.: 6.296 min
Delta R.T.: -0.004 min
Response: 1669060
Conc: 1.29 ng/ml m

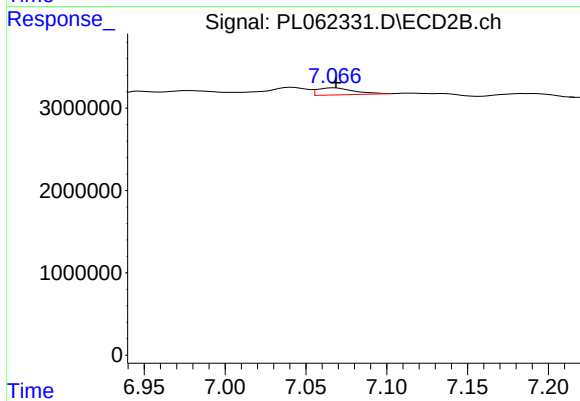

#17 4,4'-DDT

R.T.: 7.068 min
Delta R.T.: 0.000 min
Response: 1350473
Conc: 0.59 ng/ml

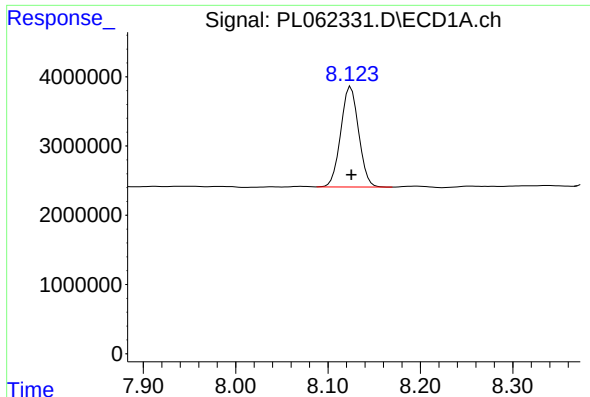

#28 Decachlorobiphenyl

R.T.: 8.125 min

Delta R.T.: 0.000 min


Response: 19496592

Conc: 10.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
BU-01-101420

Manual Integrations
APPROVED

Ankita
10/16/2020 11:51:04 AM

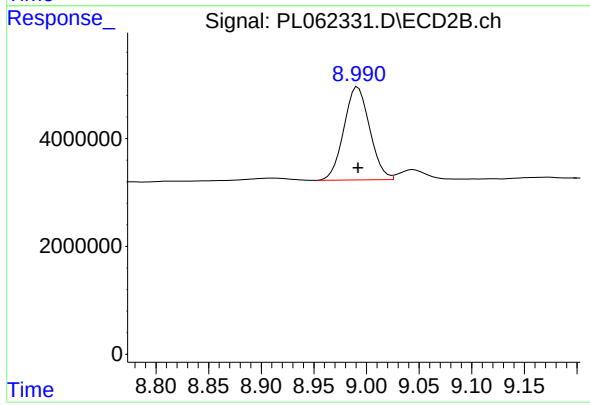

#28 Decachlorobiphenyl

R.T.: 8.990 min

Delta R.T.: -0.002 min

Response: 29582550

Conc: 10.78 ng/ml m