

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101620\
 Data File : PL062336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2020 14:46
 Operator : DD\AJ
 Sample : L4393-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-COMP

Manual Integrations
 APPROVED

Ankita
 10/16/2020 11:51:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 18:06:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 13 05:04:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.951	36090839	52864049	20.735	18.757
28)	SA Decachlor...	8.124	8.992	23286950	33659508	12.730	12.263
Target Compounds							
12)	B 4,4'-DDE	5.550	6.280	12022934	19450142	7.291	6.392
13)	MA Dieldrin	5.676	6.427	7429139	13174451	4.226m	4.266
17)	MA 4,4'-DDT	6.300	7.067	7636439	11045564	5.920	4.829

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101620\
Data File : PL062336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2020 14:46
Operator : DD\AJ
Sample : L4393-04
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SP-COMP


Manual Integrations
APPROVED

Ankita
10/16/2020 11:51:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 18:06:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
Quant Title : GC Extractables
QLast Update : Tue Oct 13 05:04:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

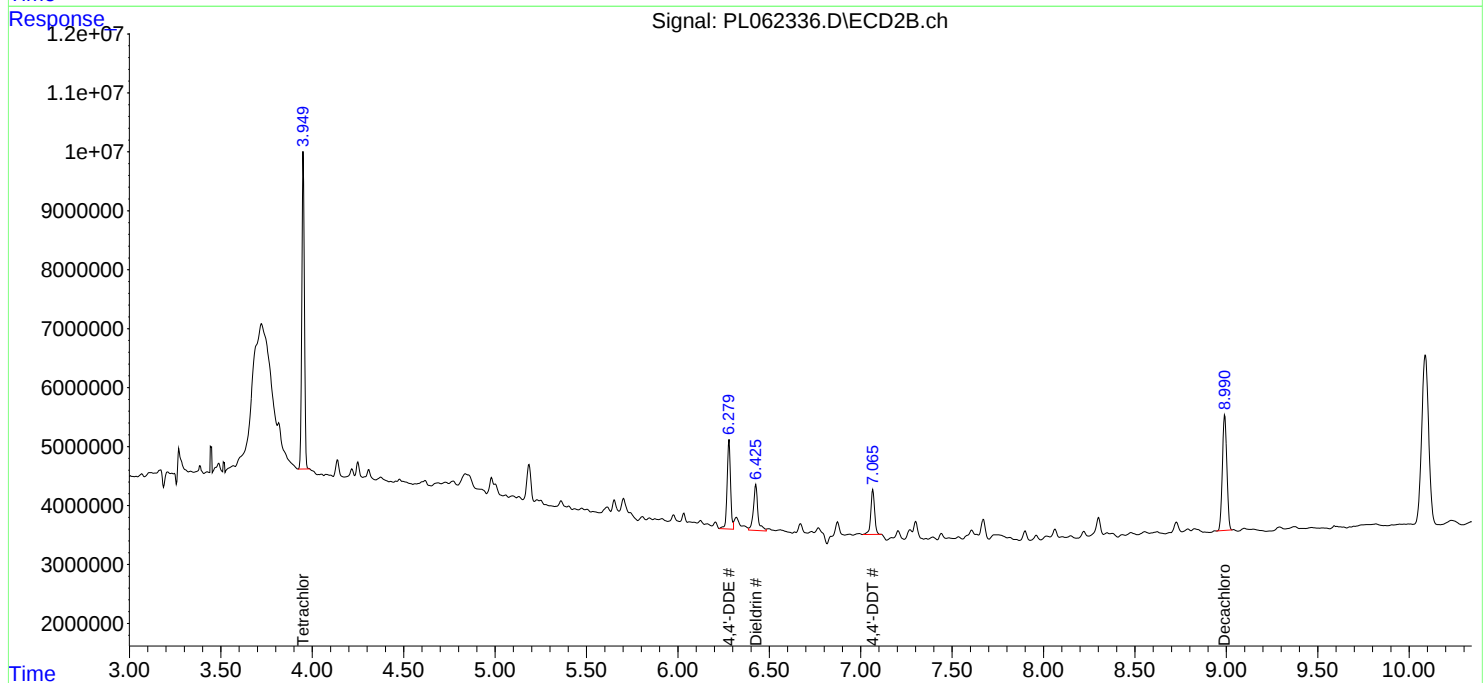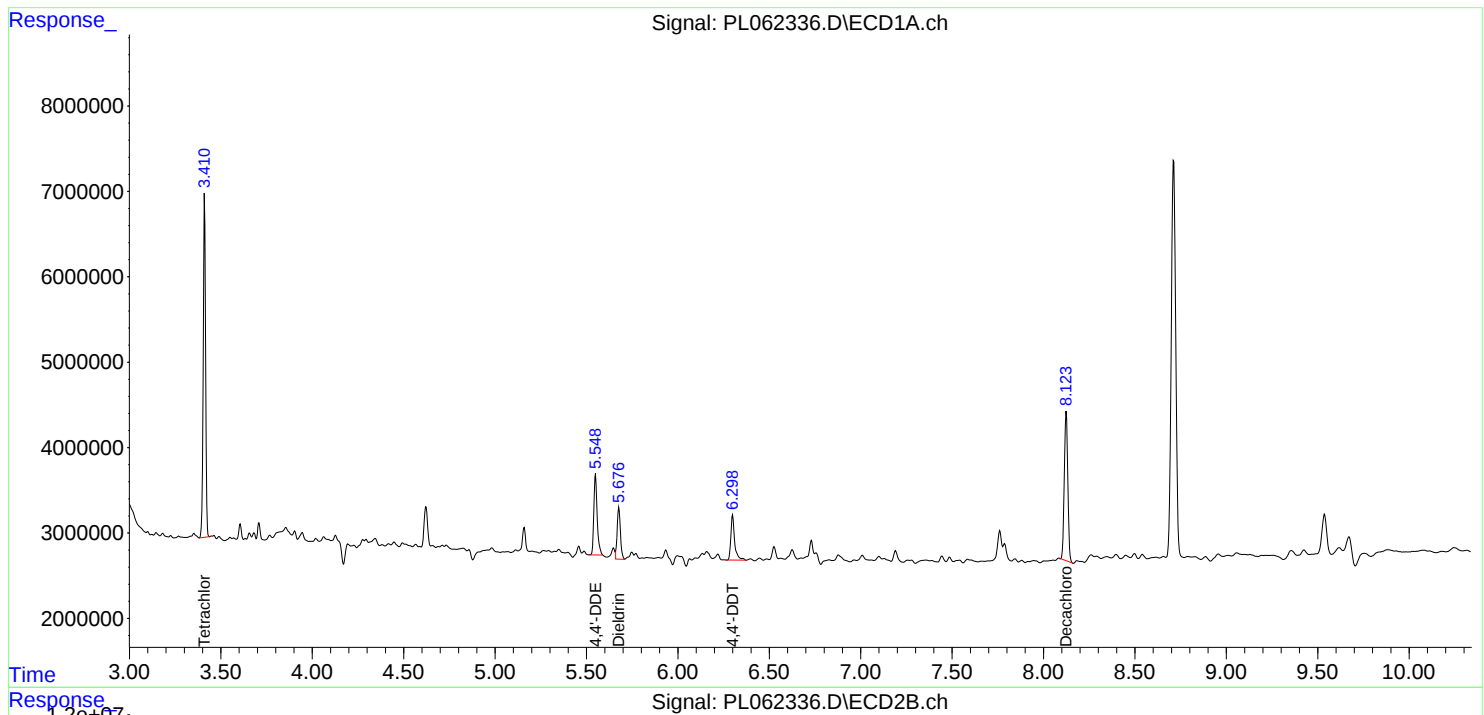

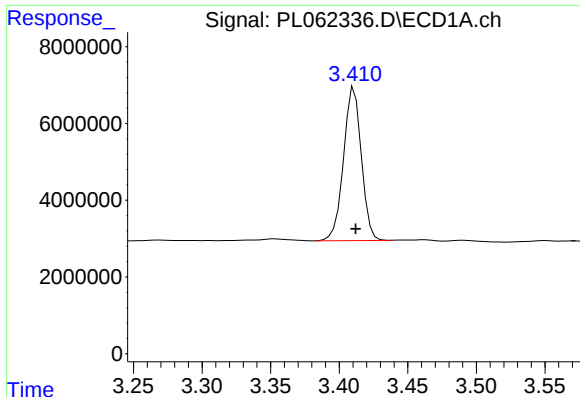


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 36090839
Conc: 20.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-COMP


Manual Integrations
APPROVED

Ankita
10/16/2020 11:51:12 AM

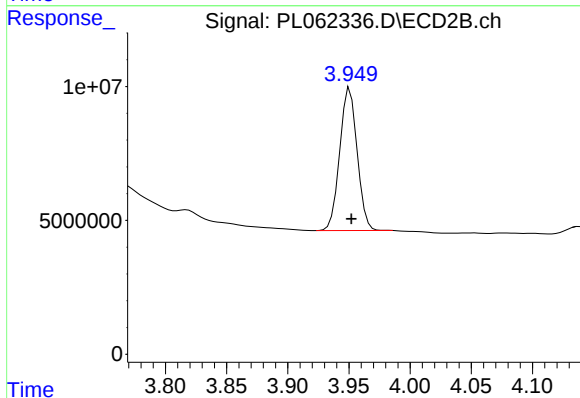


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: -0.001 min
Response: 52864049
Conc: 18.76 ng/ml

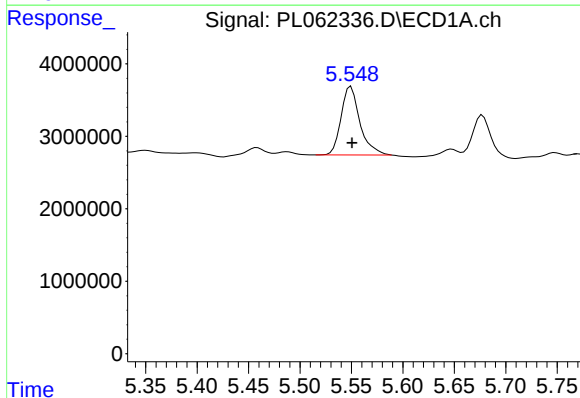


#12 4,4'-DDE

R.T.: 5.550 min
Delta R.T.: -0.001 min
Response: 12022934
Conc: 7.29 ng/ml

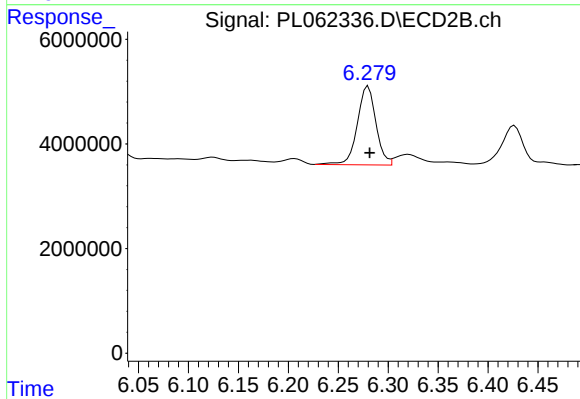

#12 4,4'-DDE

R.T.: 6.280 min
Delta R.T.: -0.001 min
Response: 19450142
Conc: 6.39 ng/ml

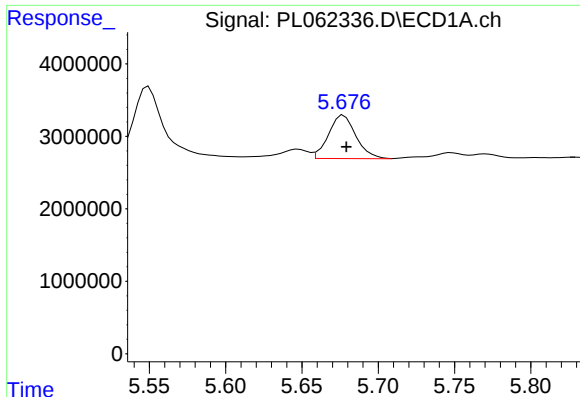


#13 Dieldrin

R.T.: 5.676 min
Delta R.T.: -0.003 min
Response: 7429139
Conc: 4.23 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SP-COMP


Manual Integrations
APPROVED

Ankita
10/16/2020 11:51:12 AM

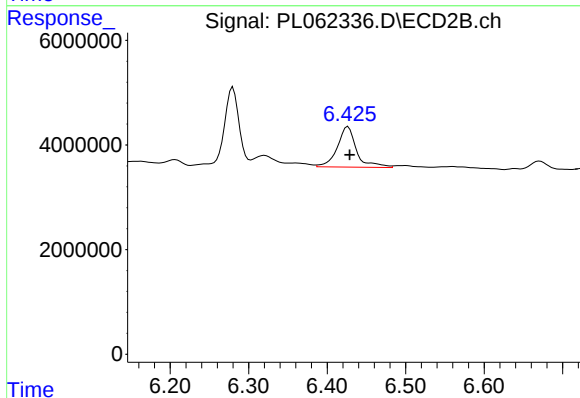


#13 Dieldrin

R.T.: 6.427 min
Delta R.T.: -0.002 min
Response: 13174451
Conc: 4.27 ng/ml

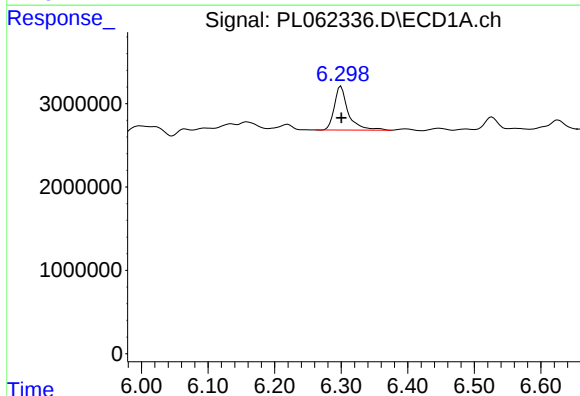


#17 4,4'-DDT

R.T.: 6.300 min
Delta R.T.: 0.000 min
Response: 7636439
Conc: 5.92 ng/ml

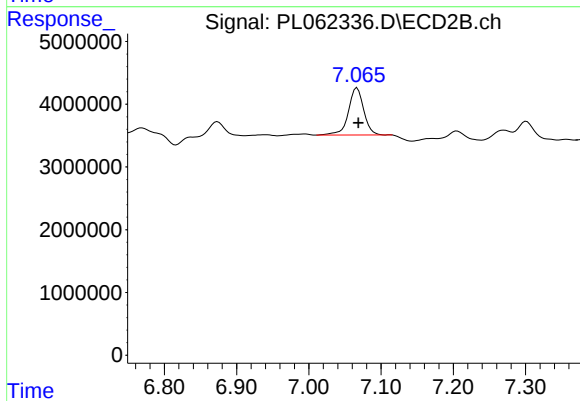

#17 4,4'-DDT

R.T.: 7.067 min
Delta R.T.: -0.002 min
Response: 11045564
Conc: 4.83 ng/ml

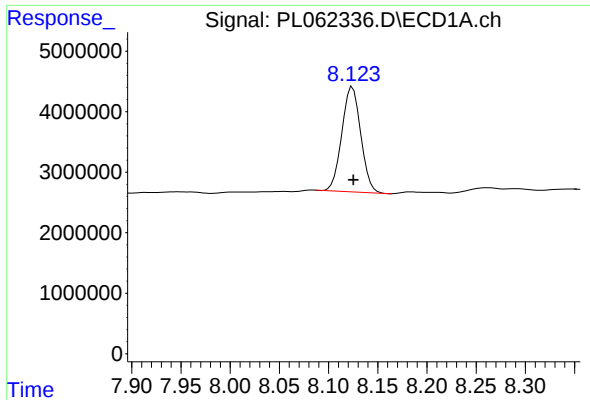


#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.001 min
Response: 23286950
Conc: 12.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-COMP

Manual Integrations
APPROVED

Ankita
10/16/2020 11:51:12 AM

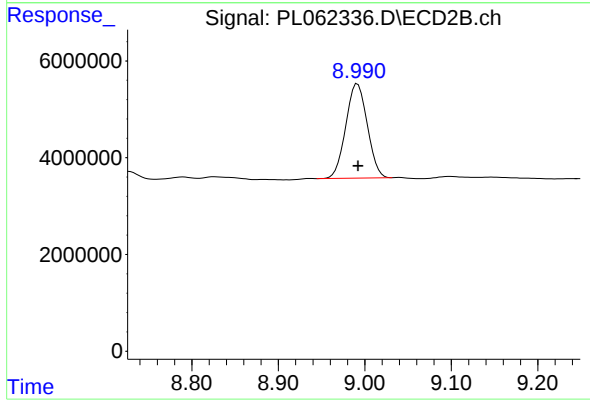

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 33659508
Conc: 12.26 ng/ml