

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101621\
 Data File : PL070348.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2021 16:58
 Operator : AR\AJ
 Sample : M4222-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TEST-A(1)

Manual Integrations
 APPROVED

Ankita
 10/18/2021 12:07:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 09:18:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.624	5.561	7530482	21443620	15.049	16.213
28)	SA Decachlor...	10.389	11.482	10953490	21241415	15.829	17.552
Target Compounds							
10)	B gamma-Chl...	7.339	8.294	1646899	4161723	2.274m	2.602m
11)	B alpha-Chl...	7.408	8.376	2088992	7518797	2.868m	4.767m#
17)	MA 4,4'-DDT	8.468	9.419	1250599	1490652	2.044	1.141m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101621\
Data File : PL070348.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2021 16:58
Operator : AR\AJ
Sample : M4222-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TEST-A(1)


Manual Integrations
APPROVED

Ankita
10/18/2021 12:07:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 09:18:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

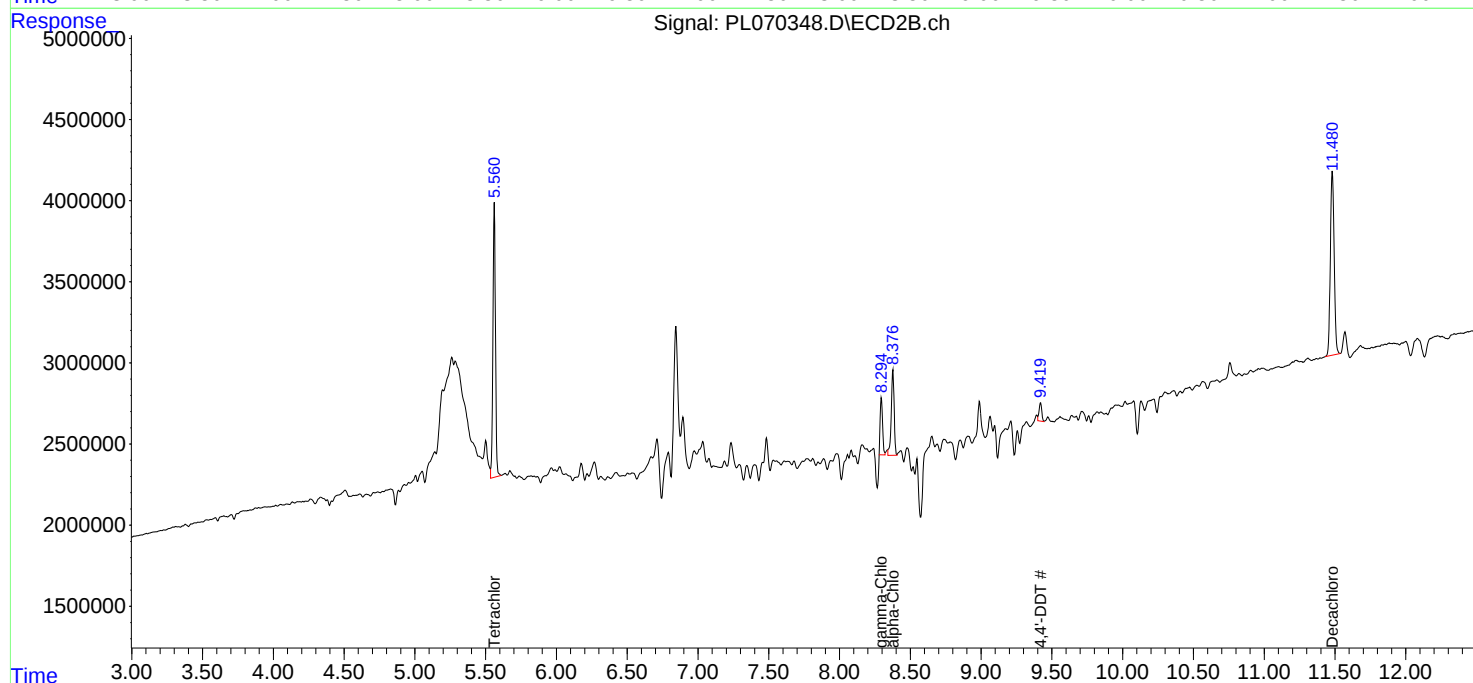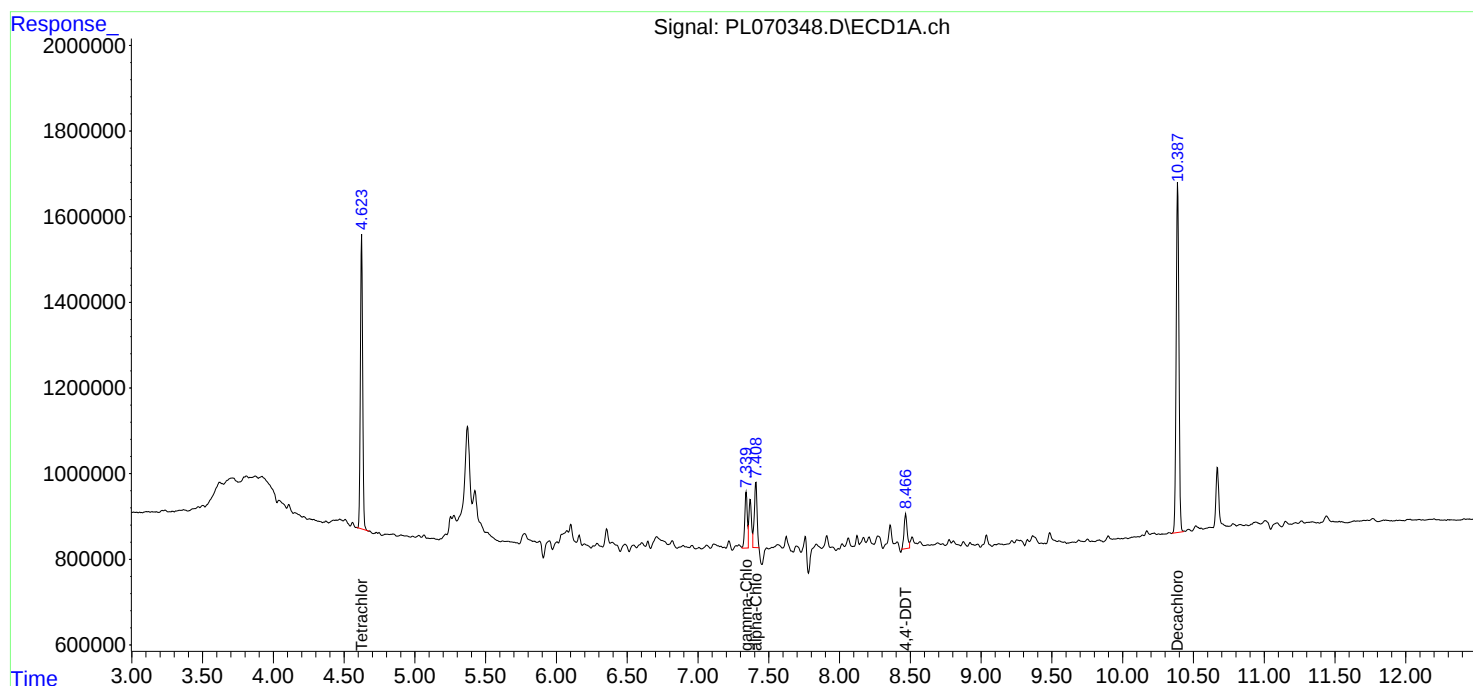

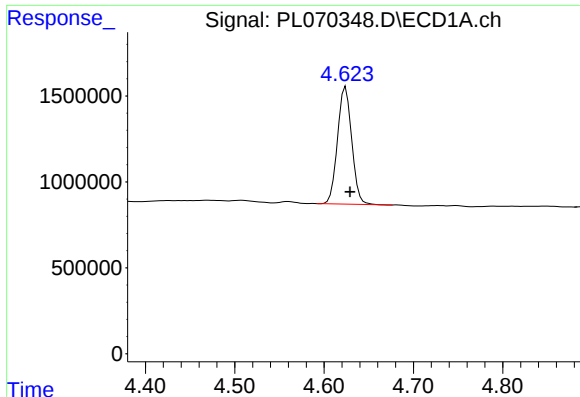


#1 Tetrachloro-m-xylene

R.T.: 4.624 min
Delta R.T.: -0.005 min
Response: 7530482
Conc: 15.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-A(1)


Manual Integrations
APPROVED

Ankita
10/18/2021 12:07:30 PM

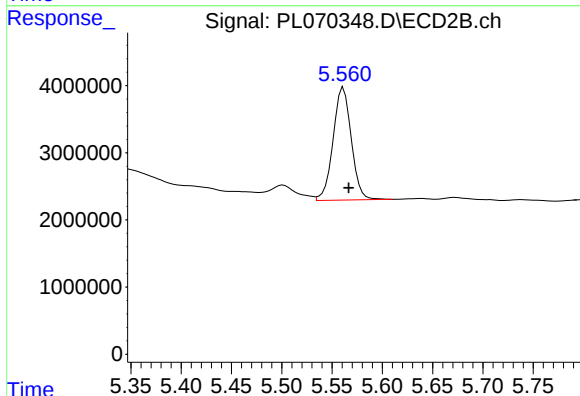


#1 Tetrachloro-m-xylene

R.T.: 5.561 min
Delta R.T.: -0.005 min
Response: 21443620
Conc: 16.21 ng/ml

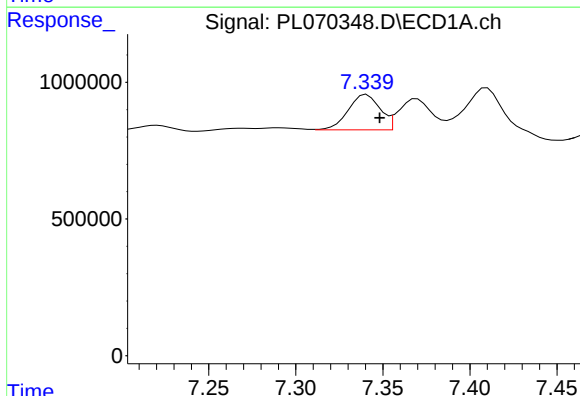


#10 gamma-Chlordane

R.T.: 7.339 min
Delta R.T.: -0.009 min
Response: 1646899
Conc: 2.27 ng/ml m

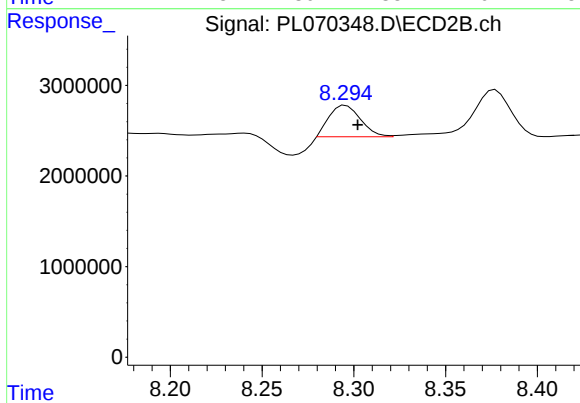

#10 gamma-Chlordane

R.T.: 8.294 min
Delta R.T.: -0.008 min
Response: 4161723
Conc: 2.60 ng/ml m

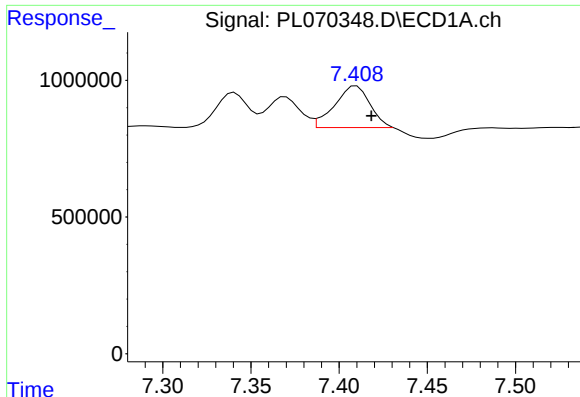


#11 alpha-Chlordane

R.T.: 7.408 min
Delta R.T.: -0.010 min
Response: 2088992
Conc: 2.87 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TEST-A(1)


Manual Integrations
APPROVED

Ankita
10/18/2021 12:07:30 PM

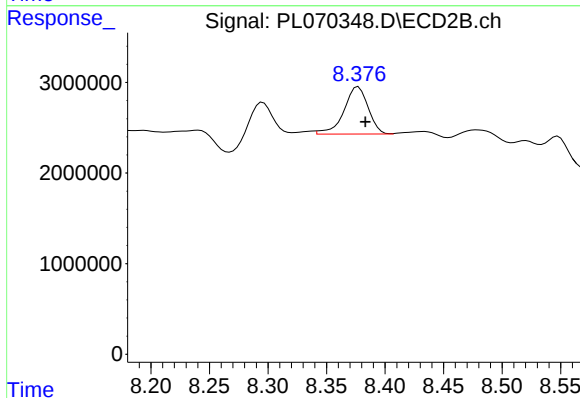


#11 alpha-Chlordane

R.T.: 8.376 min
Delta R.T.: -0.007 min
Response: 7518797
Conc: 4.77 ng/ml m

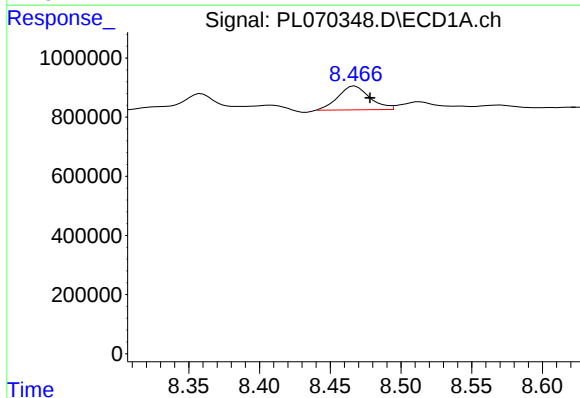


#17 4,4'-DDT

R.T.: 8.468 min
Delta R.T.: -0.011 min
Response: 1250599
Conc: 2.04 ng/ml

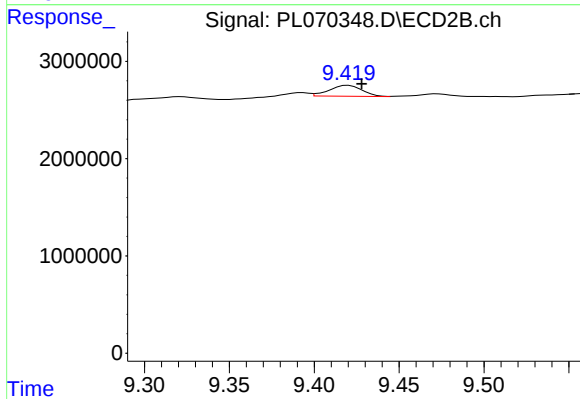

#17 4,4'-DDT

R.T.: 9.419 min
Delta R.T.: -0.009 min
Response: 1490652
Conc: 1.14 ng/ml m

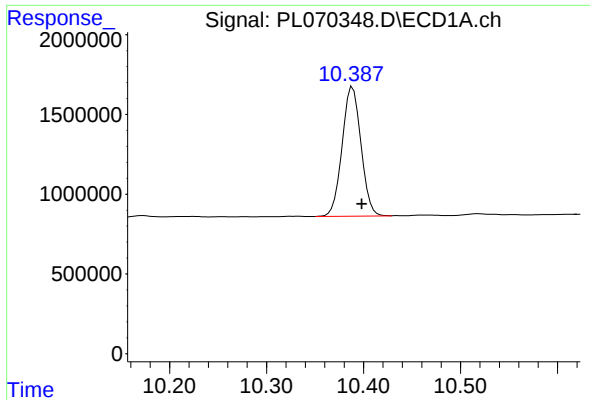


#28 Decachlorobiphenyl

R.T.: 10.389 min
Delta R.T.: -0.009 min
Response: 10953490
Conc: 15.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-A(1)

Manual Integrations
APPROVED

Ankita
10/18/2021 12:07:30 PM

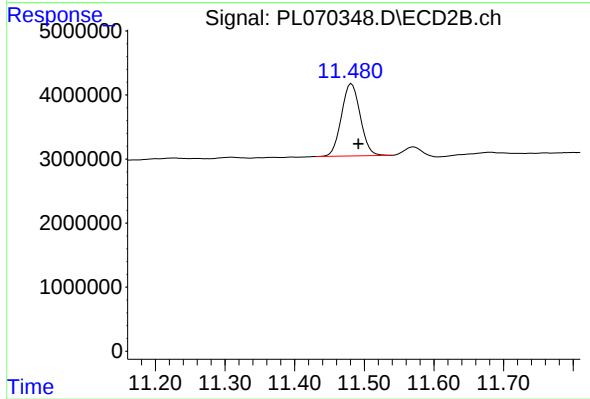

#28 Decachlorobiphenyl

R.T.: 11.482 min
Delta R.T.: -0.010 min
Response: 21241415
Conc: 17.55 ng/ml