

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101623\
 Data File : PL085959.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2023 18:14
 Operator : AR\AJ
 Sample : 04895-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 A-3

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/17/2023
 Supervised By :Ankita Jodhani 10/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 22:19:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.356	2.622	52408633	17014915	17.621	18.215
2) SA Decachlor...	8.860	7.776	44281414	19584440	20.331	21.219
Target Compounds						
16) A 4,4'-DDD	6.538	5.633	2632629	716311	1.307	1.029m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101623\
Data File : PL085959.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2023 18:14
Operator : AR\AJ
Sample : 04895-03
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
A-3


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/17/2023
Supervised By : Ankita Jodhani 10/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 22:19:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

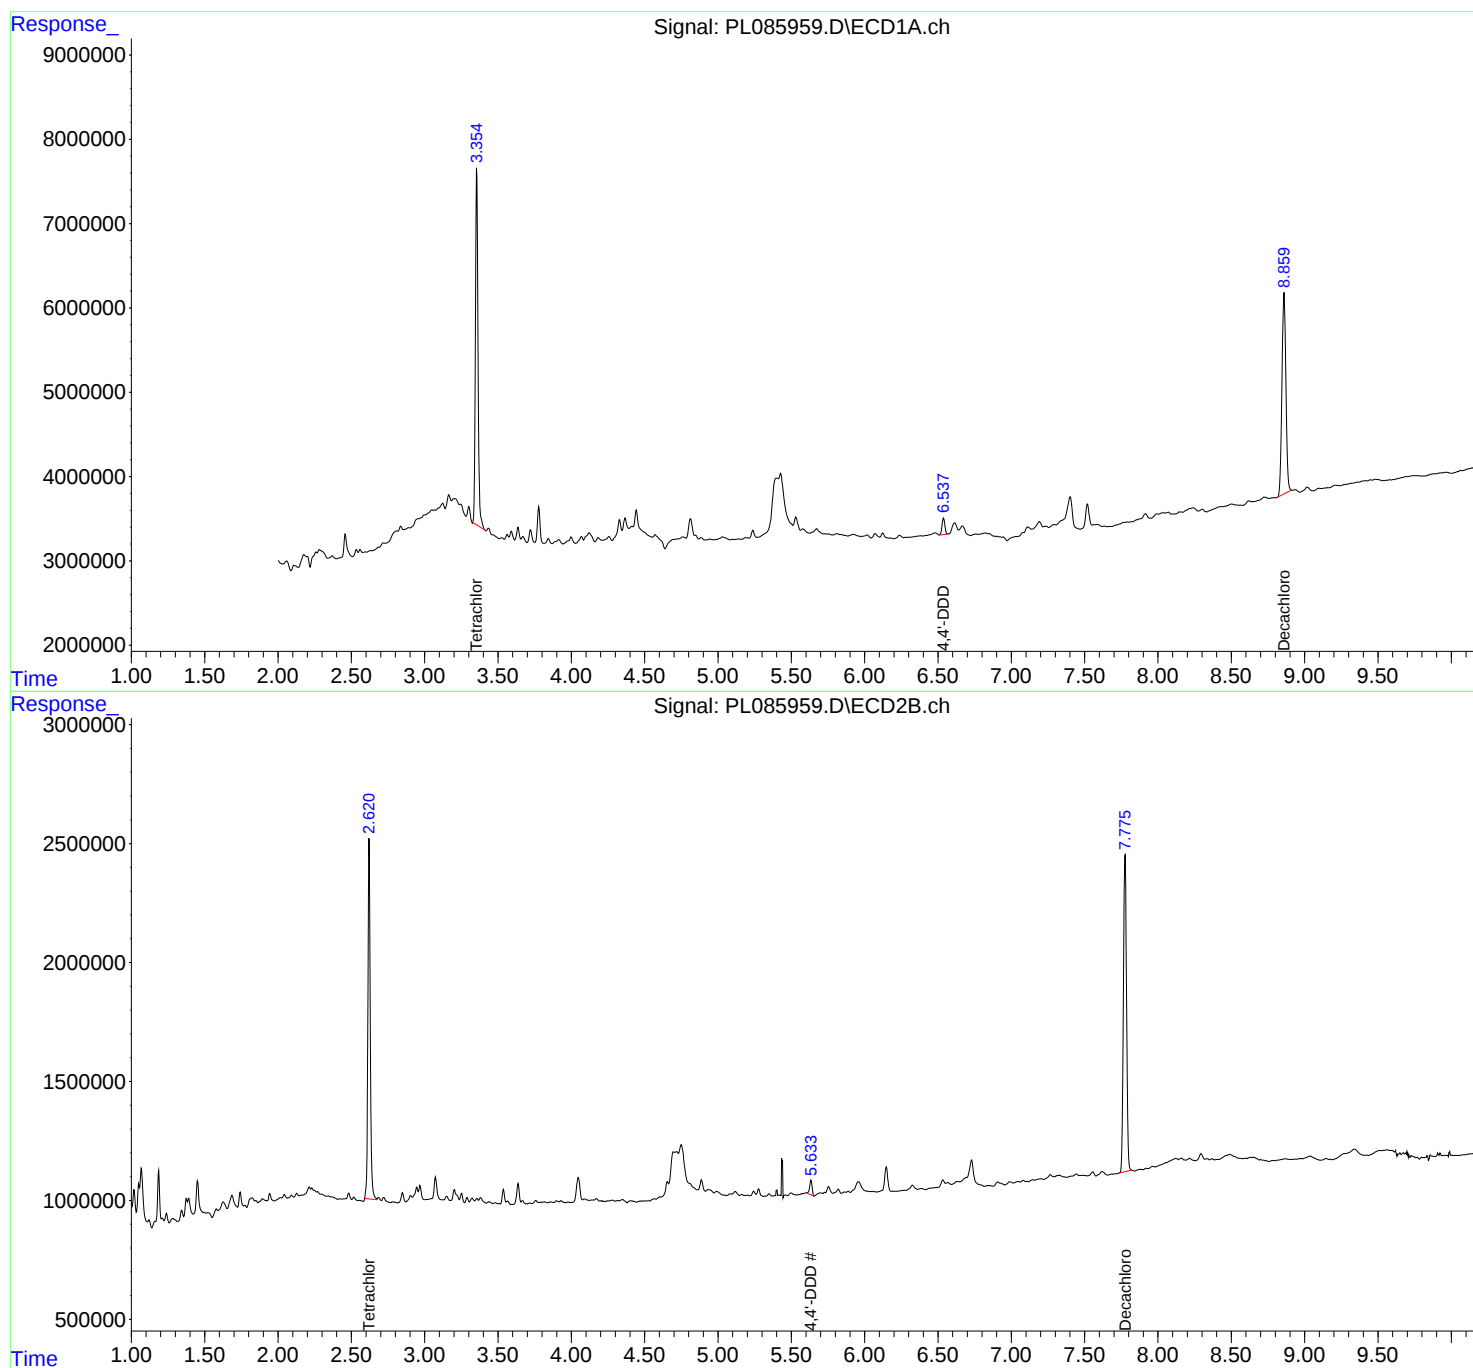

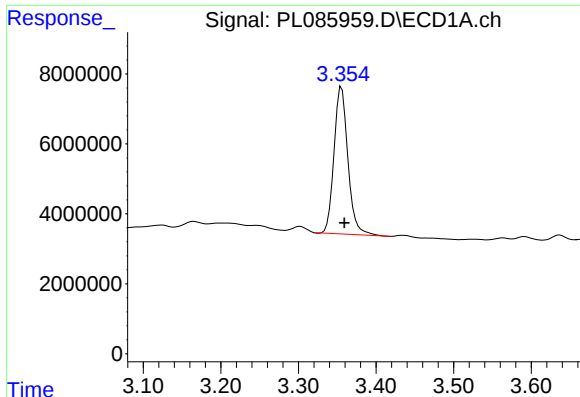


#1 Tetrachloro-m-xylene

R.T.: 3.356 min
Delta R.T.: -0.003 min
Response: 52408633
Conc: 17.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
A-3


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/17/2023
Supervised By :Ankita Jodhani 10/17/2023

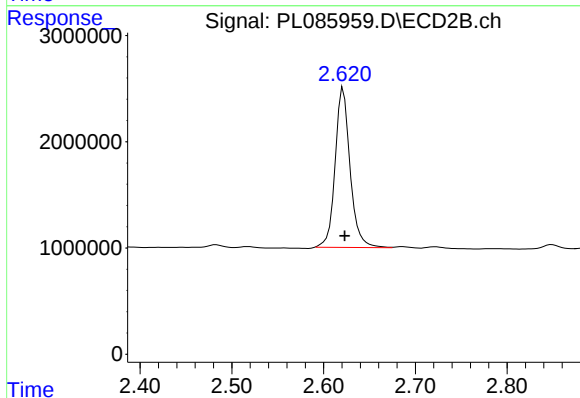


#1 Tetrachloro-m-xylene

R.T.: 2.622 min
Delta R.T.: -0.001 min
Response: 17014915
Conc: 18.22 ng/ml

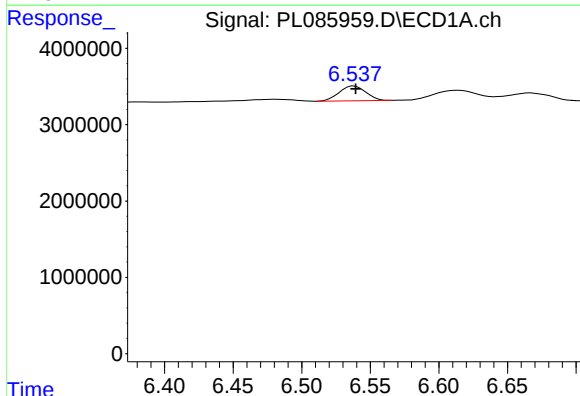


#16 4,4'-DDD

R.T.: 6.538 min
Delta R.T.: -0.001 min
Response: 2632629
Conc: 1.31 ng/ml

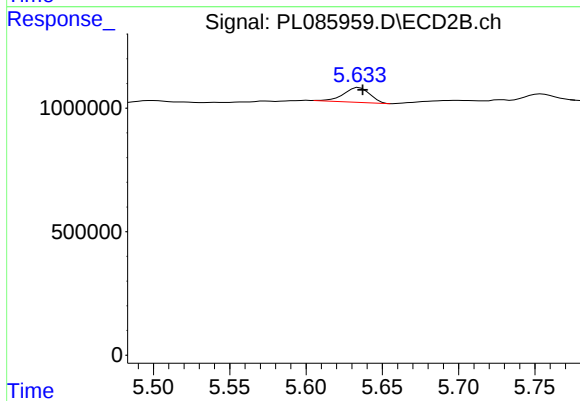

#16 4,4'-DDD

R.T.: 5.633 min
Delta R.T.: -0.004 min
Response: 716311
Conc: 1.03 ng/ml m

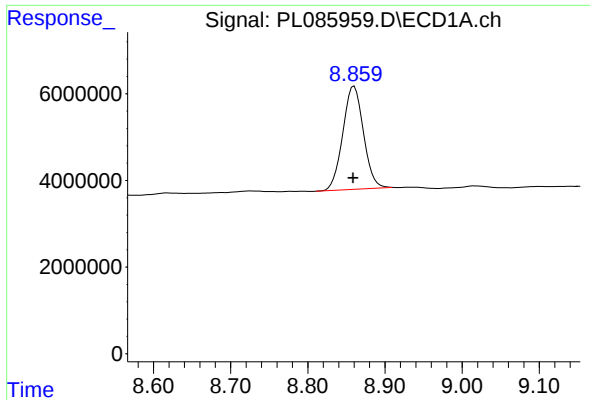


#28 Decachlorobiphenyl

R.T.: 8.860 min
Delta R.T.: 0.001 min
Response: 44281414
Conc: 20.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
A-3

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/17/2023
Supervised By :Ankita Jodhani 10/17/2023

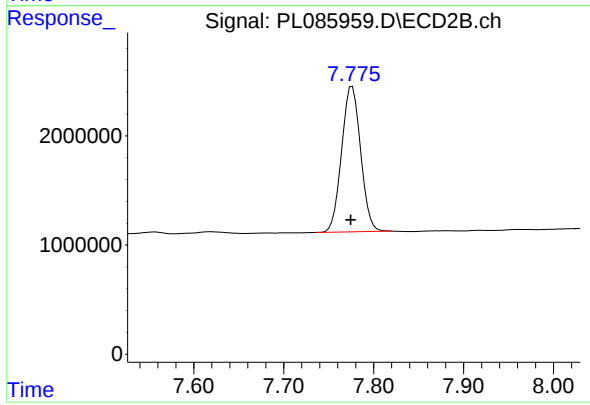

#28 Decachlorobiphenyl

R.T.: 7.776 min
Delta R.T.: 0.002 min
Response: 19584440
Conc: 21.22 ng/ml