

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101624\
 Data File : PL092403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 13:22
 Operator : AR\AJ
 Sample : P4346-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EOAW5

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/18/2024
 Supervised By : Ankita Jodhani 10/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 02:38:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 07:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.546	2.780	24065272	29489069	13.779m	13.854
27) SA Decachlor...	9.061	7.922	18846176	28425491	14.026m	13.359
Target Compounds						
3) MA gamma-BHC...	4.309	3.621	8983267	3482523	3.654m	1.247 #
10) B trans-Chl...	5.947	5.013	4178080	2282704	2.145m	0.948m#
14) MA Endrin	6.577	5.656	1945484	3328237	1.222m	1.547 #
16) A 4,4'-DDD	6.714	5.793	6959601	2711332	4.882m	1.484m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101624\
Data File : PL092403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 13:22
Operator : AR\AJ
Sample : P4346-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 02:38:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 07:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

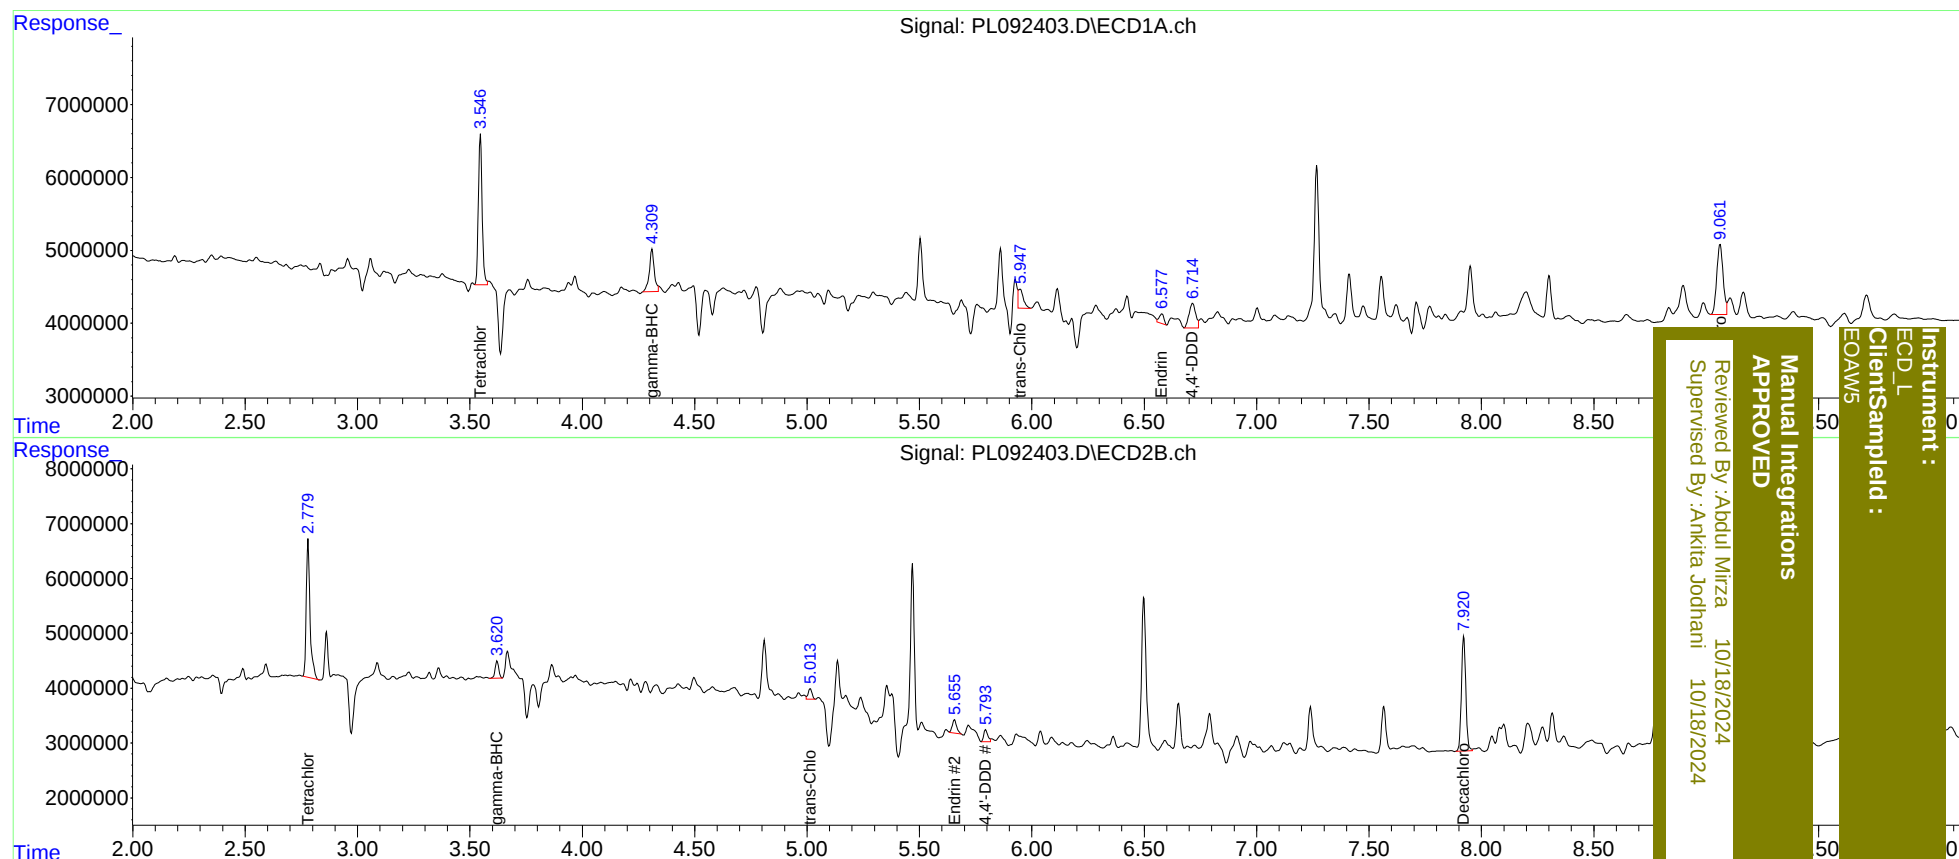

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/18/2024
Supervised By: Ankita Jodhani 10/18/2024

Instrument :
ECD_L
ClientSampled :
EOAW/S