

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101624\
 Data File : PL092408.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 14:29
 Operator : AR\AJ
 Sample : P4346-08MS
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EOAW9MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/18/2024
 Supervised By :Ankita Jodhani 10/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 02:40:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 07:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.779	26598149	28626454	15.229	13.449
2) SA Decachlor...	9.057	7.918	16830087	24968353	12.525m	11.735m
Target Compounds						
2) A alpha-BHC	3.996	3.283	155.2E6	187.2E6	61.078m	62.555
3) MA gamma-BHC...	4.330	3.613	146.3E6	171.6E6	59.489	61.448
4) MA Heptachlor	4.919	3.952	133.3E6	172.0E6	58.611	61.422
5) MB Aldrin	5.261	4.232	126.8E6	164.3E6	56.487	62.764
6) B beta-BHC	4.528	3.912	61260937	69428958	52.916	53.585
7) B delta-BHC	4.774	4.141	139.2E6	164.4E6	57.050	57.006
8) B Heptachlo...	5.687	4.735	124.1E6	145.2E6	60.902	59.253
9) A Endosulfan I	6.071	5.104	101.3E6	110.3E6	55.896m	50.830m
10) B trans-Chl...	5.942	4.983	122.9E6	150.0E6	63.109m	62.271m
11) B cis-Chlor...	6.021	5.048	116.4E6	144.7E6	57.314m	60.350
12) B 4,4'-DDE	6.195	5.237	191.9E6	293.8E6	107.106	125.033
13) MA Dieldrin	6.348	5.369	224.4E6	311.5E6	115.586	130.417
14) MA Endrin	6.578	5.645	184.7E6	263.6E6	116.054	122.549
15) B Endosulfa...	6.798	5.939	192.4E6	249.4E6	108.553	117.699
16) A 4,4'-DDD	6.713	5.792	175.5E6	225.4E6	123.090	123.316
17) MA 4,4'-DDT	7.026	6.043	165.8E6	215.4E6	112.824m	110.985
18) B Endrin al...	6.928	6.119	139.9E6	174.6E6	109.846	113.002
19) B Endosulfa...	7.162	6.341	178.4E6	232.5E6	108.293	112.774
20) A Methoxychlor	7.503	6.618	411.8E6	545.7E6	530.159	521.776
21) B Endrin ke...	7.647	6.847	194.2E6	243.7E6	107.080	105.132

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101624\
Data File : PL092408.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 14:29
Operator : AR\AJ
Sample : P4346-08MS
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 02:40:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 07:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

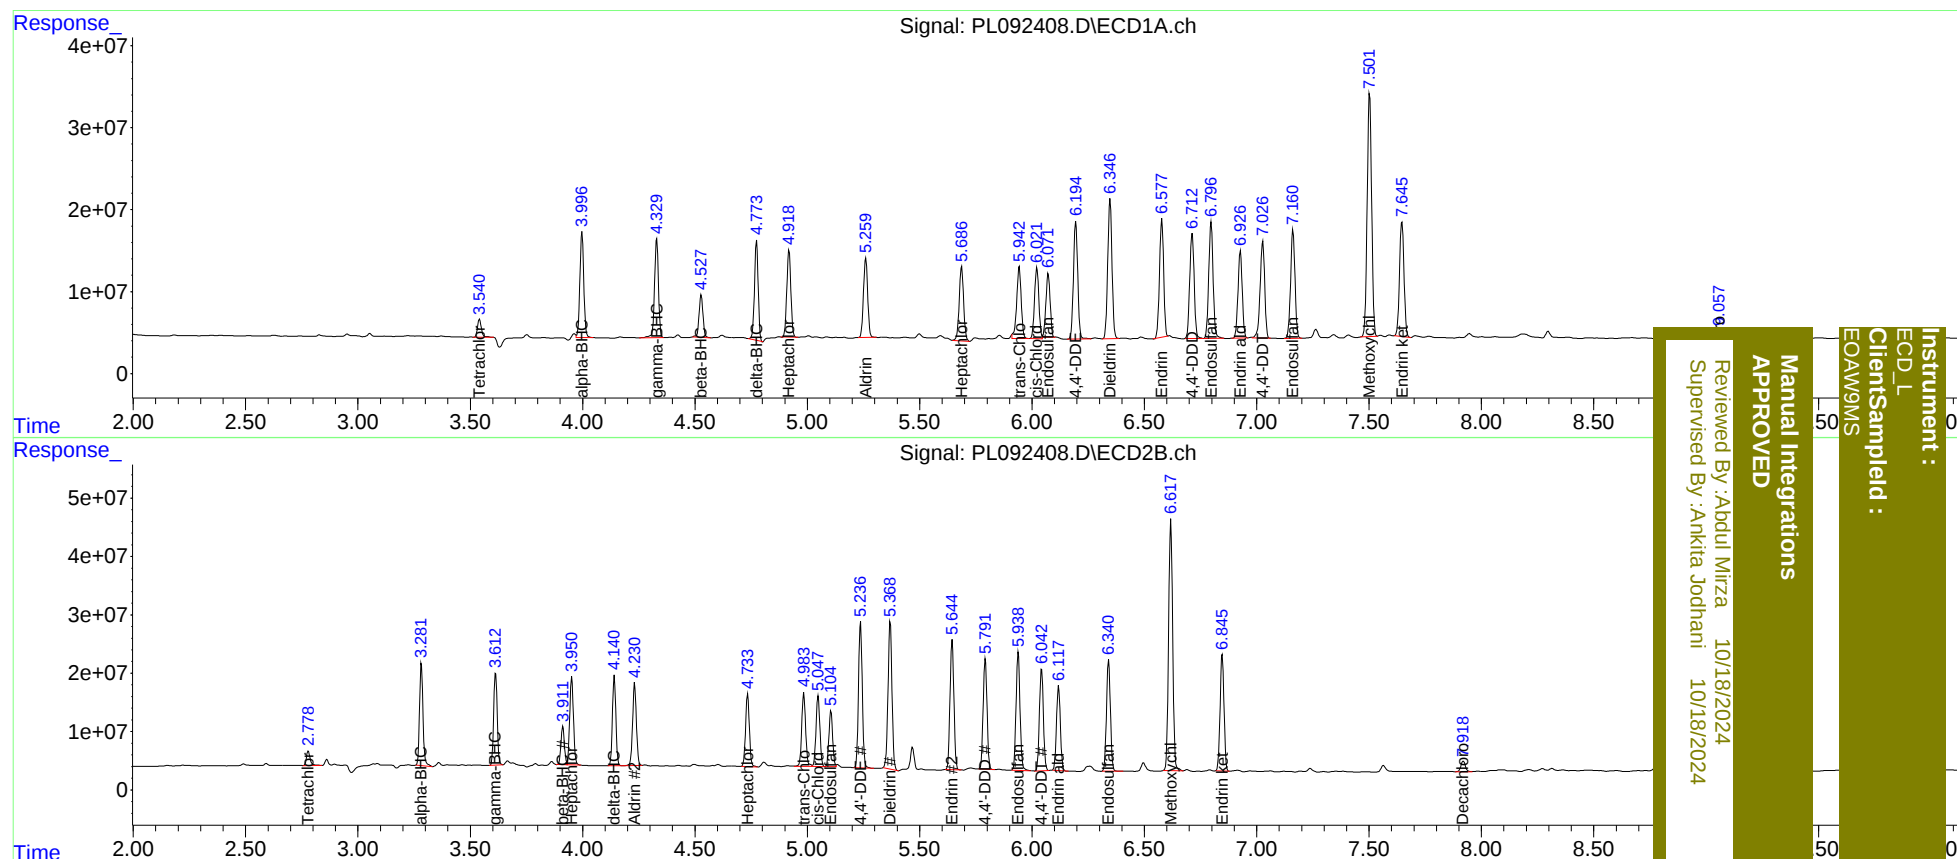

Instrument :
ECD_L
Client Sampled :
EOAW/MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 10/18/2024
Supervised By: Ankita Jodhani 10/18/2024