

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101624\
 Data File : PL092416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 17:18
 Operator : AR\AJ
 Sample : P4346-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EOAX3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/18/2024
 Supervised By : Ankita Jodhani 10/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 02:42:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 07:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.780	14833459	17082382	8.493m	8.026
2) SA Decachlor...	9.056	7.919	9972085	15237890	7.421m	7.161
Target Compounds						
10) B trans-Chl...	5.945	5.011	2180425	1386016	1.120m	0.575m#
15) B Endosulfa...	6.823	5.926	2651486	1004758	1.496m	0.474m#
16) A 4,4'-DDD	6.711	5.791	1703336	1245789	1.195m	0.682m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101624\
Data File : PL092416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 17:18
Operator : AR\AJ
Sample : P4346-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 02:42:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 07:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

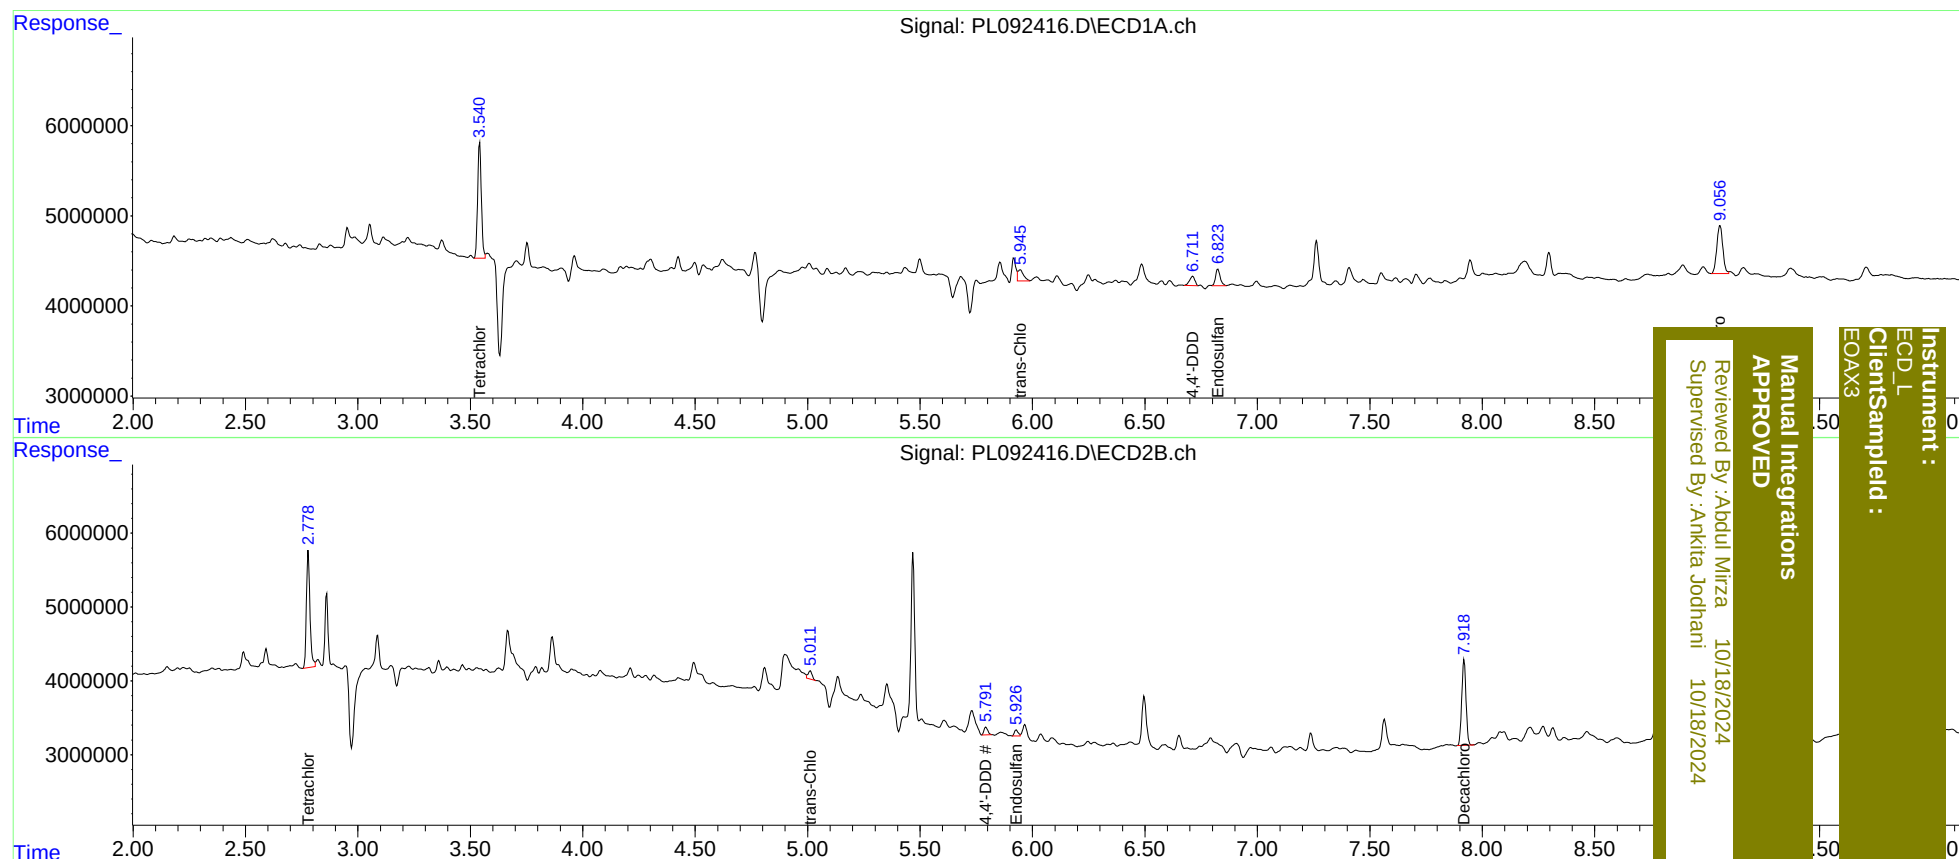

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/18/2024
Supervised By: Ankita Jodhani 10/18/2024

Instrument :
ECD_L
ClientSampled :
EOAX3