

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101719\
 Data File : PL053376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2019 14:33
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 00:55:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	4.047	270.5E6	62116478	27.198	23.133
28)	SA Decachlor...	8.338	9.130	255.5E6	72314997	25.514	24.650
Target Compounds							
4)	MA Heptachlor	0.000	5.232	0	539537	N.D.	0.142 #
7)	B delta-BHC	0.000	5.087f	0	2587264	N.D.	0.715 #
8)	B Heptachlo...	0.000	5.921	0	12574911	N.D.	3.752 #
9)	A Endosulfan I	0.000	6.281	0	5951782	N.D.	1.904 #
11)	B alpha-Chl...	0.000	6.211f	0	18439399	N.D.	5.478 #
14)	MA Endrin	0.000	6.758	0	2515060	N.D.	0.906 #
17)	MA 4,4'-DDT	0.000	7.191f	0	834215	N.D.	0.321 #
26)	Chlordane-4	0.000	6.211f	0	18439399	N.D.	34.726 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101719\
Data File : PL053376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2019 14:33
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 00:55:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

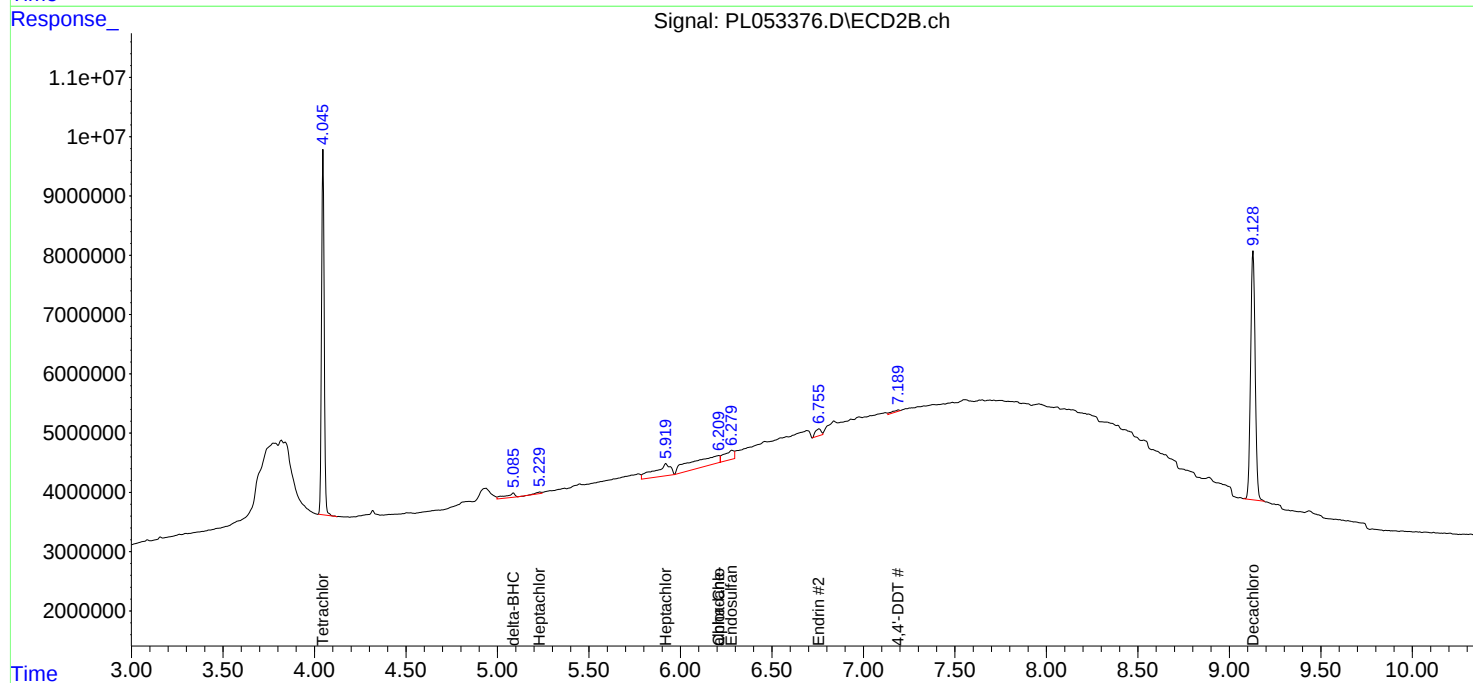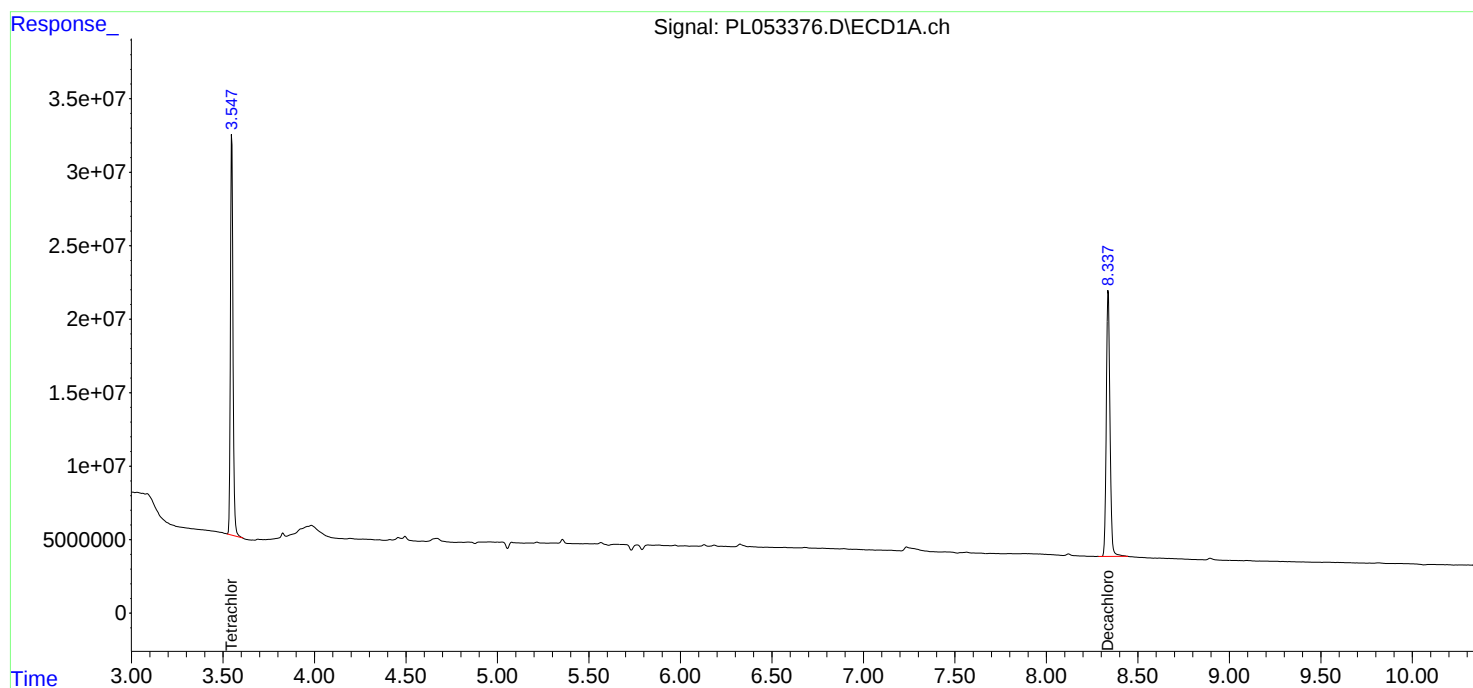


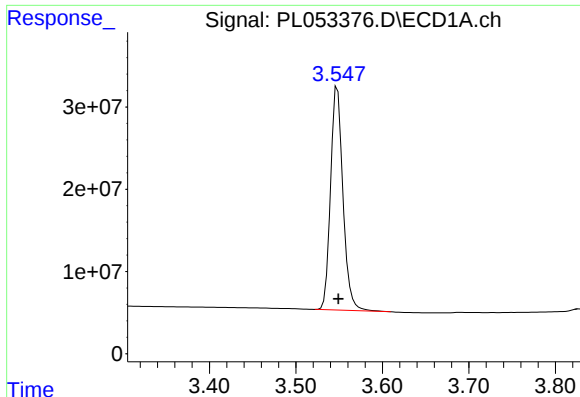

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 270530632
Conc: 27.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

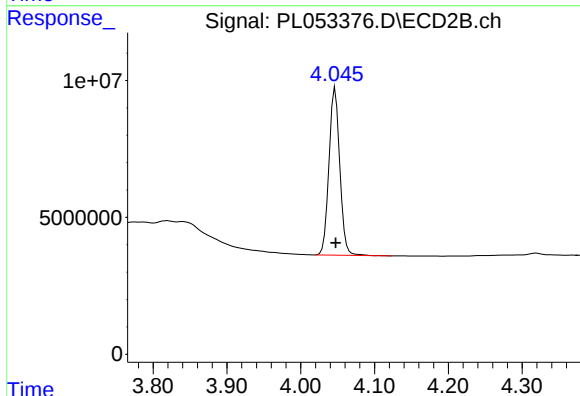


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 62116478
Conc: 23.13 ng/ml

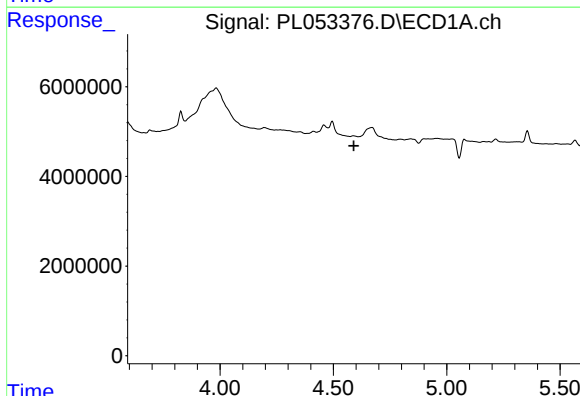


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.590 min
Response: 0
Conc: N.D.

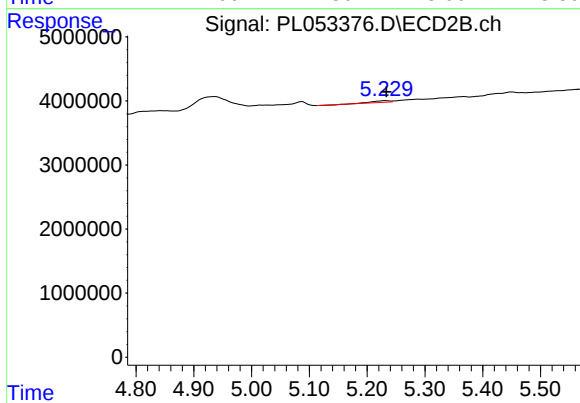

#4 Heptachlor


R.T.: 5.232 min
Delta R.T.: -0.002 min
Response: 539537
Conc: 0.14 ng/ml

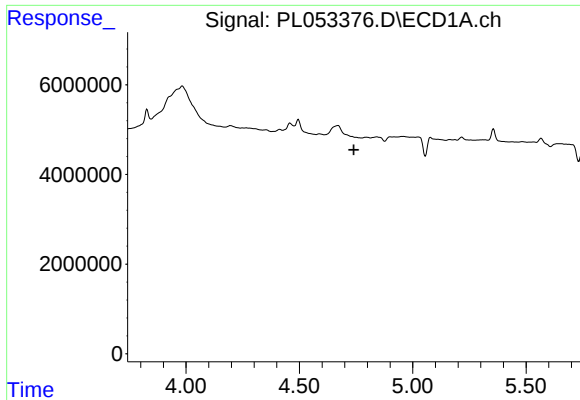

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.740 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

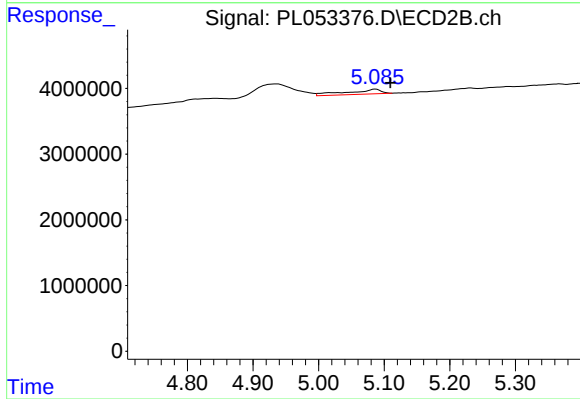


#7 delta-BHC

R.T.: 5.087 min
Delta R.T.: -0.022 min
Response: 2587264
Conc: 0.71 ng/ml

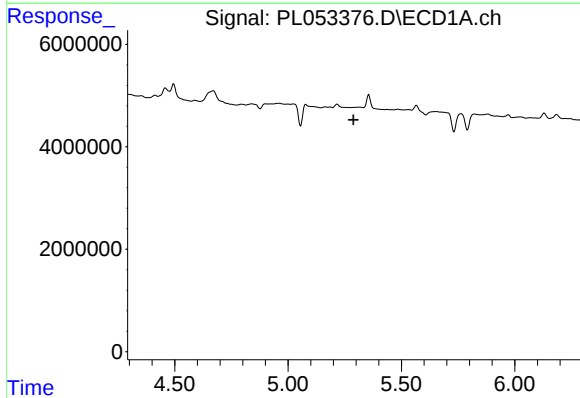


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.289 min
Response: 0
Conc: N.D.

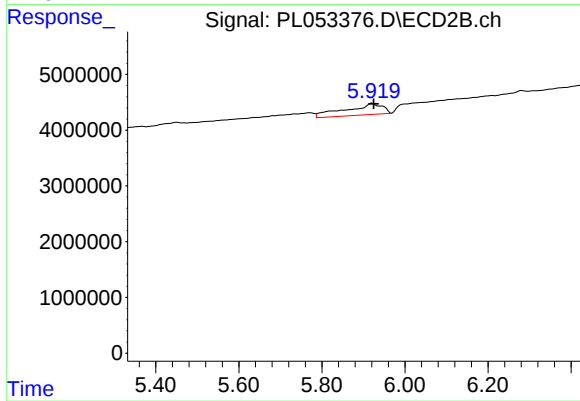

#8 Heptachlor epoxide


R.T.: 5.921 min
Delta R.T.: -0.004 min
Response: 12574911
Conc: 3.75 ng/ml

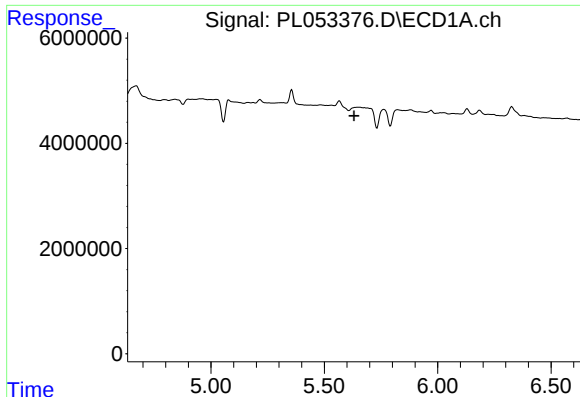

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.632 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

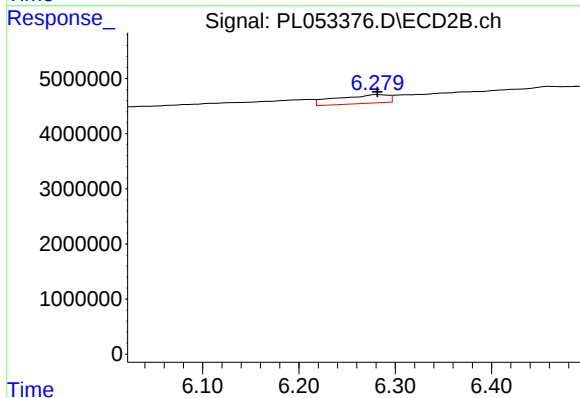


#9 Endosulfan I

R.T.: 6.281 min
Delta R.T.: 0.000 min
Response: 5951782
Conc: 1.90 ng/ml

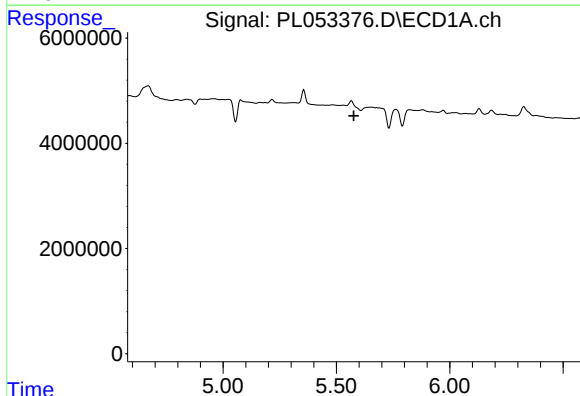


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

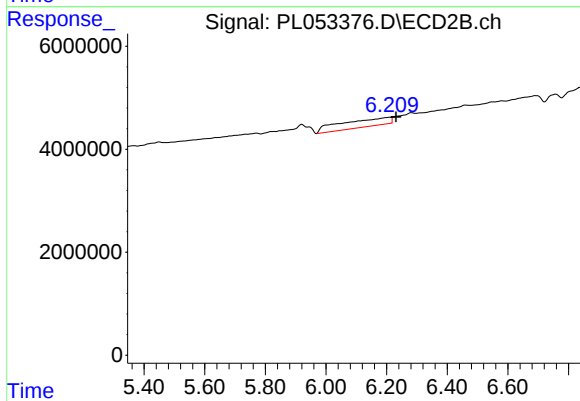

#11 alpha-Chlordane


R.T.: 6.211 min
Delta R.T.: -0.020 min
Response: 18439399
Conc: 5.48 ng/ml

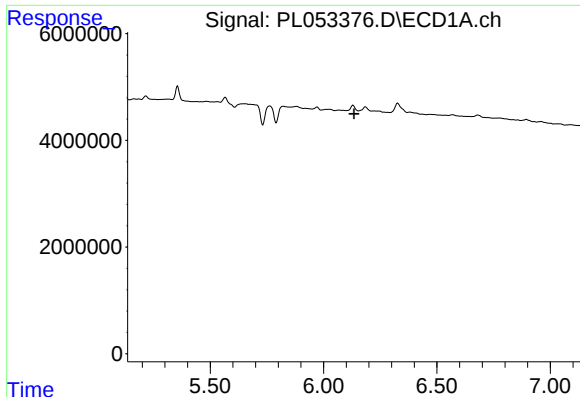

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

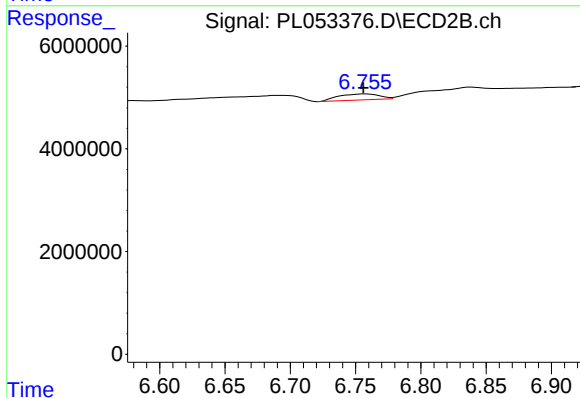


#14 Endrin

R.T.: 6.758 min
Delta R.T.: 0.002 min
Response: 2515060
Conc: 0.91 ng/ml

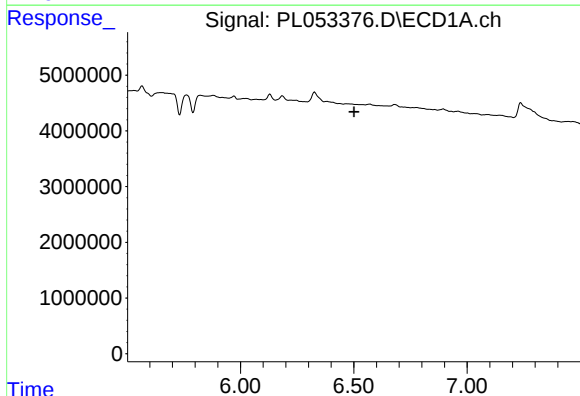


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.502 min
Response: 0
Conc: N.D.

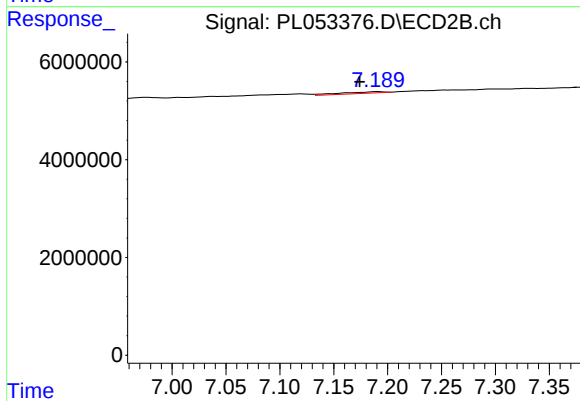

#17 4,4'-DDT


R.T.: 7.191 min
Delta R.T.: 0.016 min
Response: 834215
Conc: 0.32 ng/ml

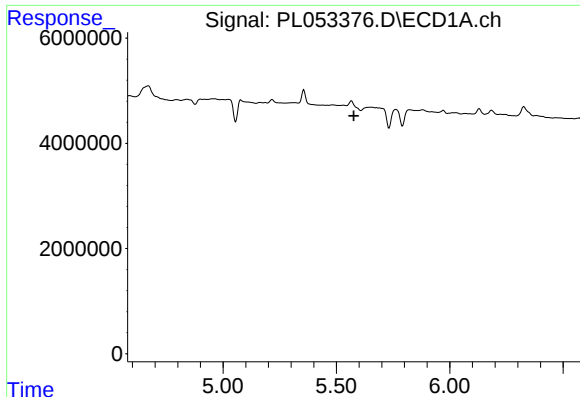

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

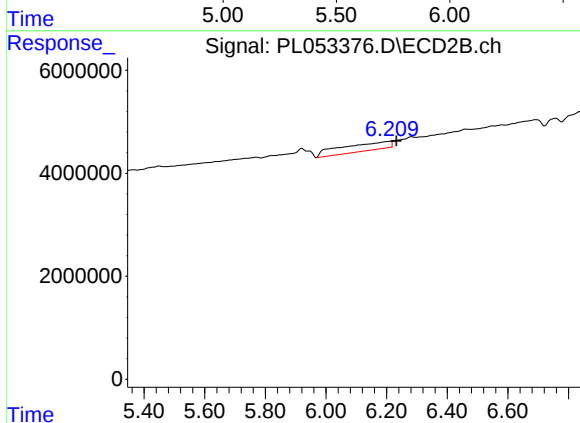


#26 Chlordane-4

R.T.: 6.211 min
Delta R.T.: -0.021 min
Response: 18439399
Conc: 34.73 ng/ml

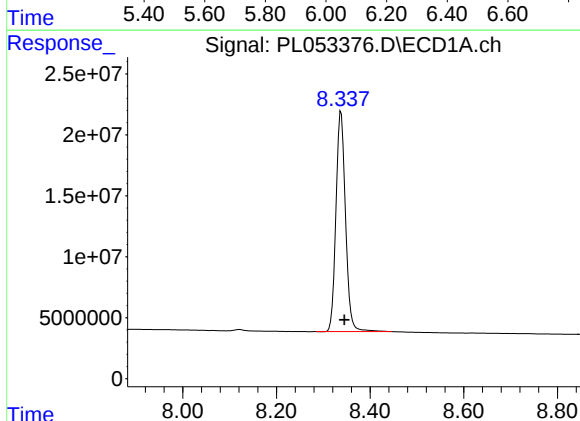

#28 Decachlorobiphenyl

R.T.: 8.338 min
Delta R.T.: -0.007 min
Response: 255546317
Conc: 25.51 ng/ml

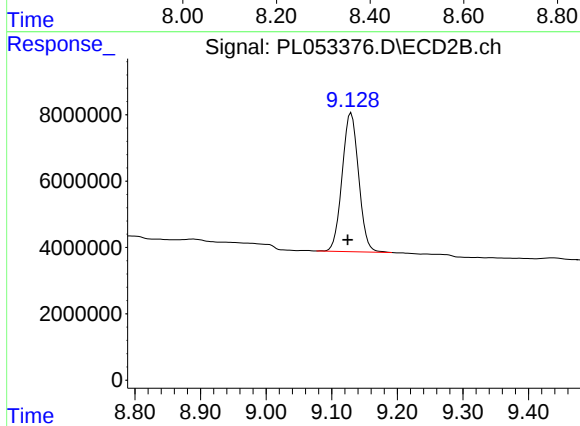

#28 Decachlorobiphenyl

R.T.: 9.130 min
Delta R.T.: 0.005 min
Response: 72314997
Conc: 24.65 ng/ml