

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101719\
 Data File : PL053381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2019 15:54
 Operator : SG\AJ
 Sample : PB124012BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 00:56:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	4.047	252.4E6	60116338	25.376	22.388
28)	SA Decachlor...	8.337	9.129	247.1E6	69402723	24.668	23.657
Target Compounds							
4)	MA Heptachlor	0.000	5.239	0	4967202	N.D.	1.303 #
6)	B beta-BHC	4.502f	0.000	13563838	0	2.185	N.D. #
7)	B delta-BHC	0.000	5.085f	0	3869415	N.D.	1.069 #
15)	B Endosulfa...	0.000	6.978f	0	1421081	N.D.	0.479 #
16)	A 4,4'-DDD	0.000	6.878	0	2391137	N.D.	0.975 #
20)	A Methoxychlor	0.000	7.657f	0	2580173	N.D.	1.833 #
21)	B Endrin ke...	0.000	7.776	0	2203680	N.D.	0.772 #
23)	Chlordane-1	0.000	5.042	0	1241075	N.D.	12.236 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101719\
Data File : PL053381.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2019 15:54
Operator : SG\AJ
Sample : PB124012BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 00:56:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

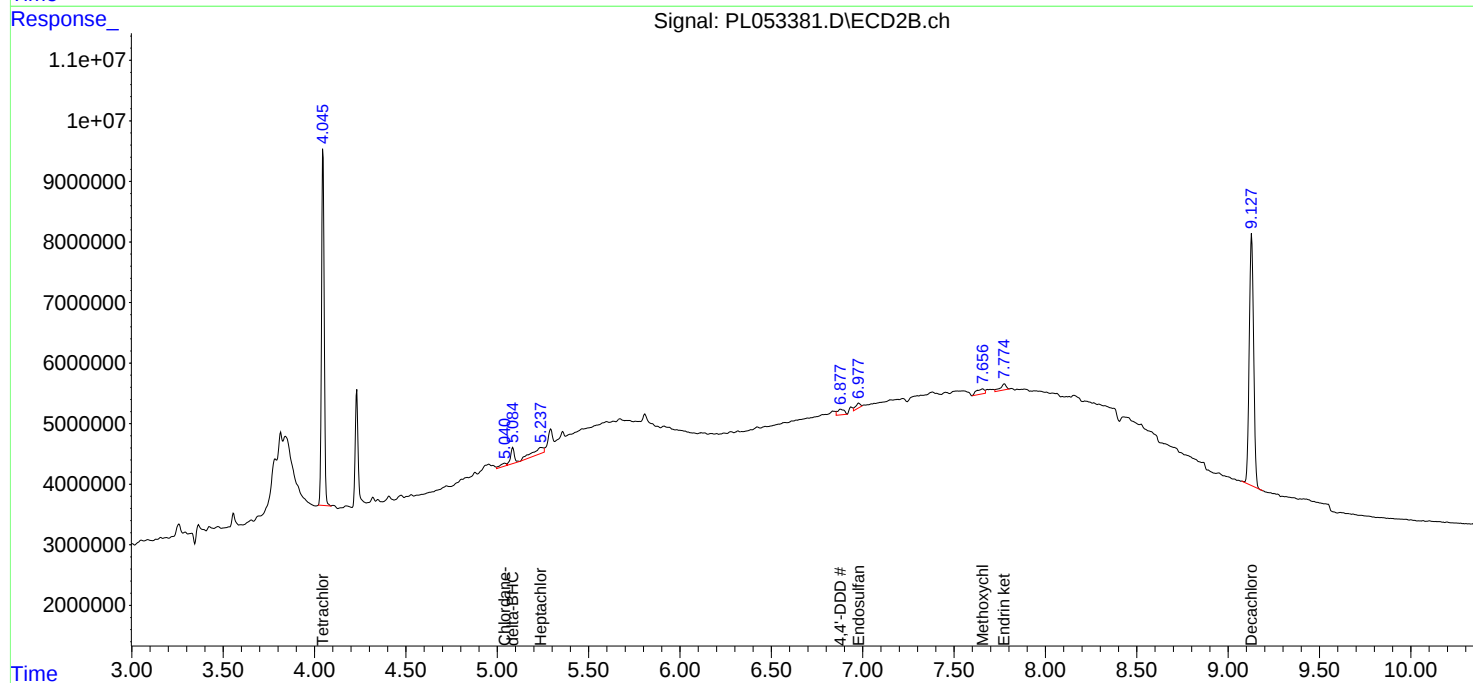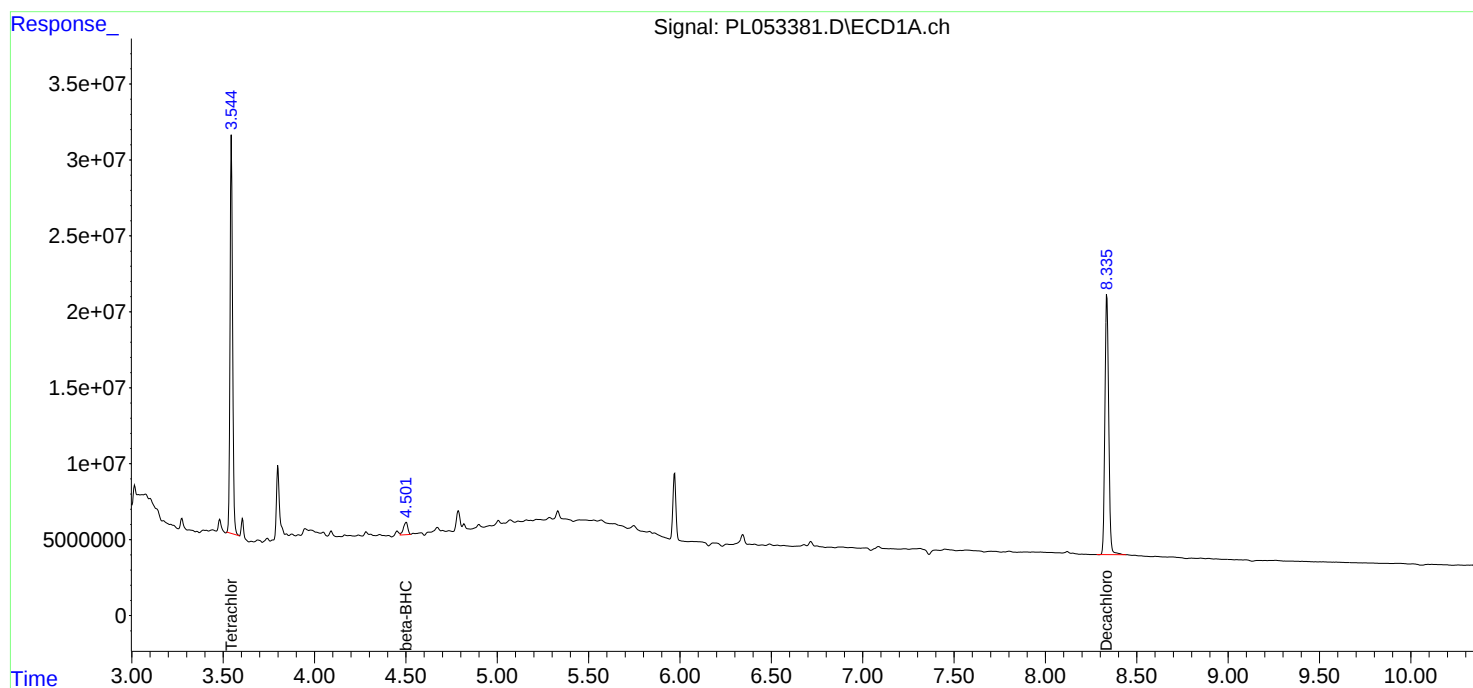


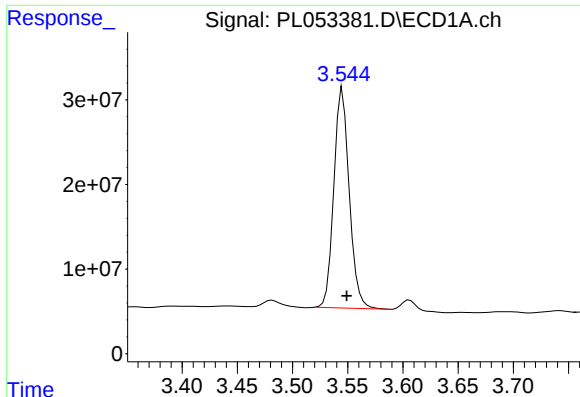

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: -0.004 min
Response: 252402643
Conc: 25.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

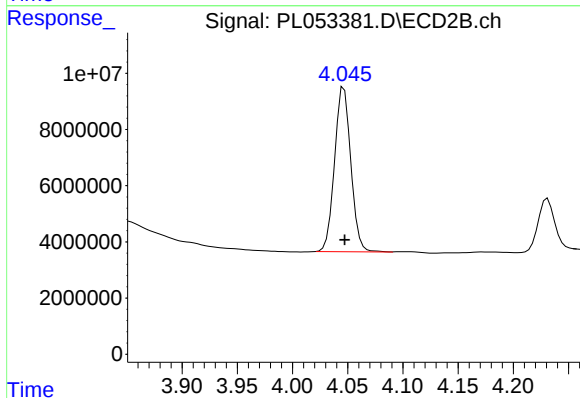


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 60116338
Conc: 22.39 ng/ml

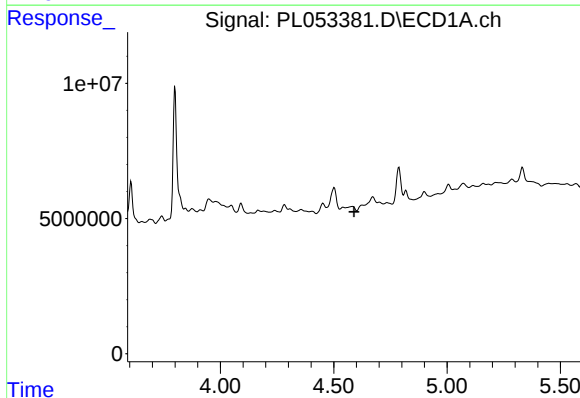


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.590 min
Response: 0
Conc: N.D.

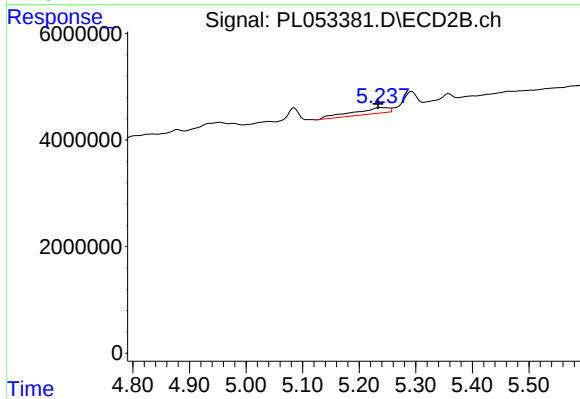

#4 Heptachlor


R.T.: 5.239 min
Delta R.T.: 0.005 min
Response: 4967202
Conc: 1.30 ng/ml

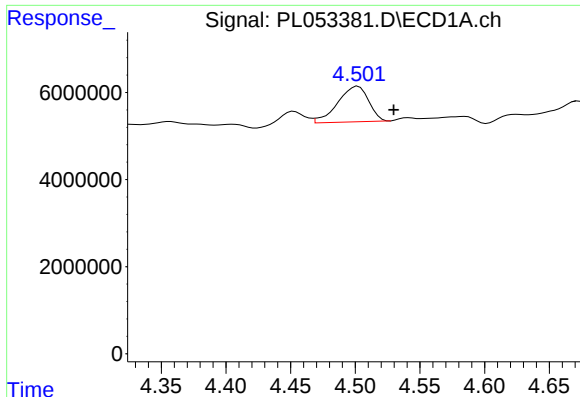

#6 beta-BHC


R.T.: 4.502 min
Delta R.T.: -0.028 min
Response: 13563838
Conc: 2.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

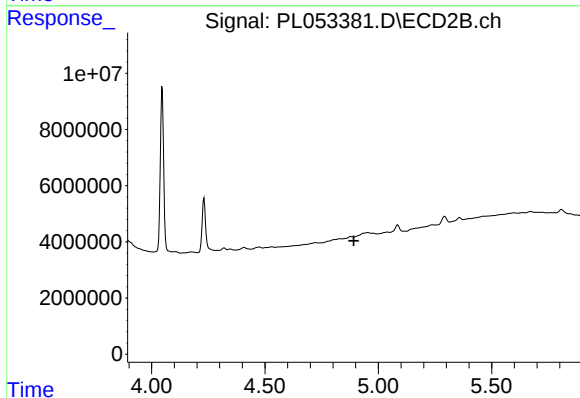


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.892 min
Response: 0
Conc: N.D.

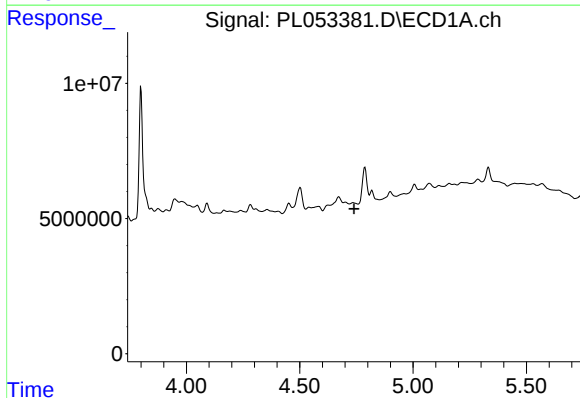


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.740 min
Response: 0
Conc: N.D.

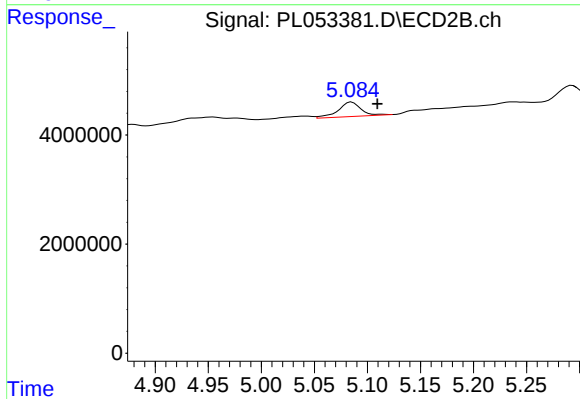

#7 delta-BHC


R.T.: 5.085 min
Delta R.T.: -0.024 min
Response: 3869415
Conc: 1.07 ng/ml

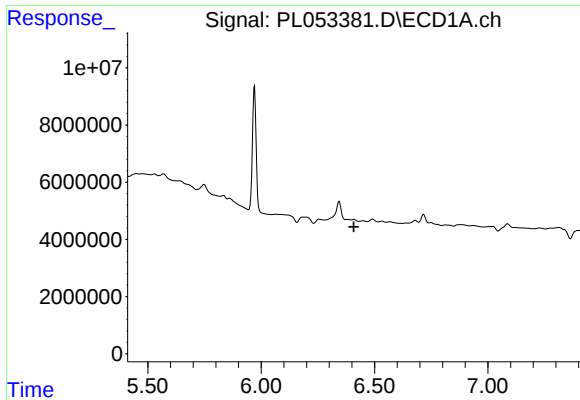

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

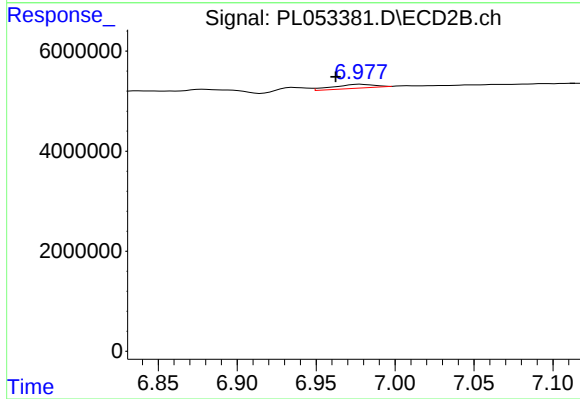


#15 Endosulfan II

R.T.: 6.978 min
Delta R.T.: 0.016 min
Response: 1421081
Conc: 0.48 ng/ml

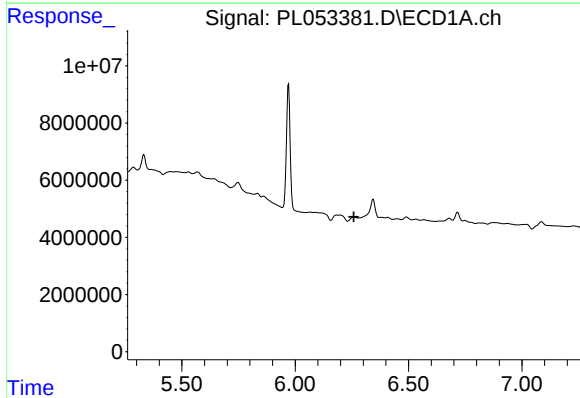


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.258 min
Response: 0
Conc: N.D.

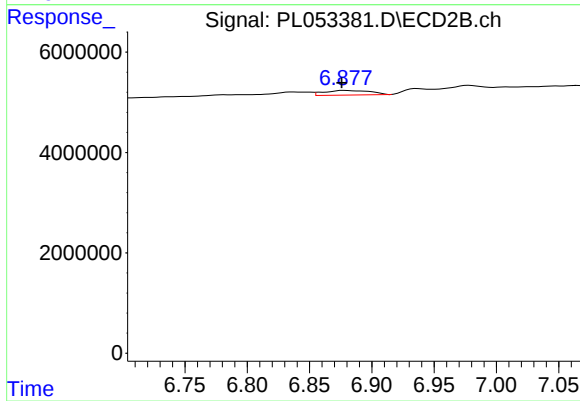

#16 4,4'-DDD


R.T.: 6.878 min
Delta R.T.: 0.003 min
Response: 2391137
Conc: 0.97 ng/ml

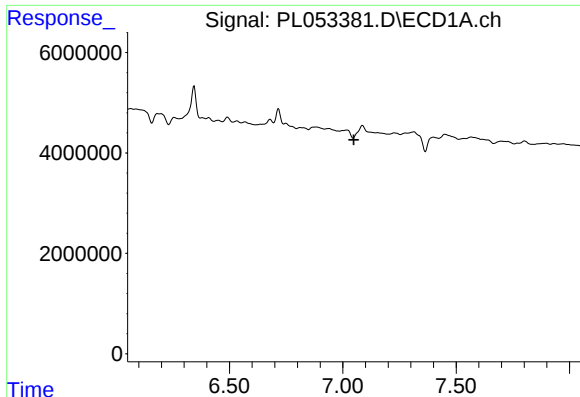

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

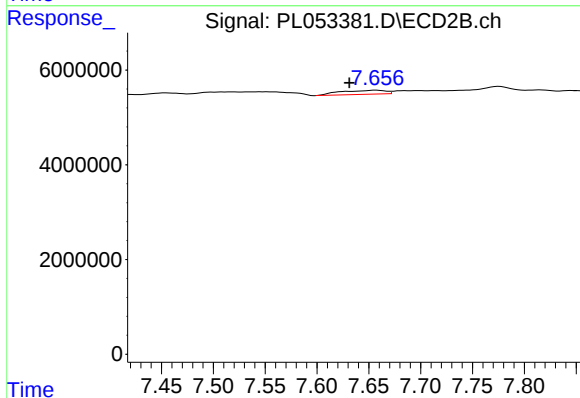


#20 Methoxychlor

R.T.: 7.657 min
Delta R.T.: 0.026 min
Response: 2580173
Conc: 1.83 ng/ml

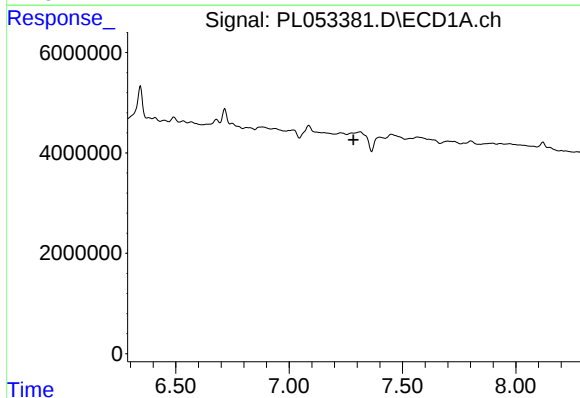


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

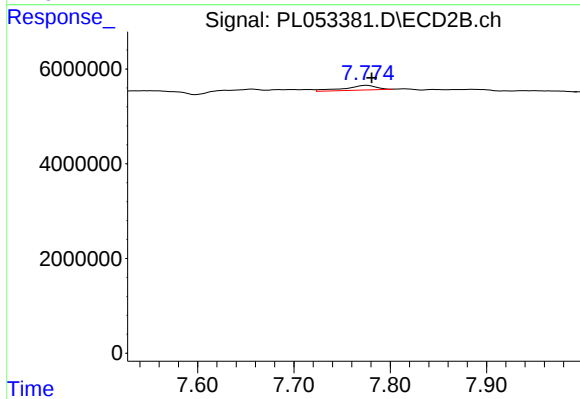

#21 Endrin ketone


R.T.: 7.776 min
Delta R.T.: -0.005 min
Response: 2203680
Conc: 0.77 ng/ml

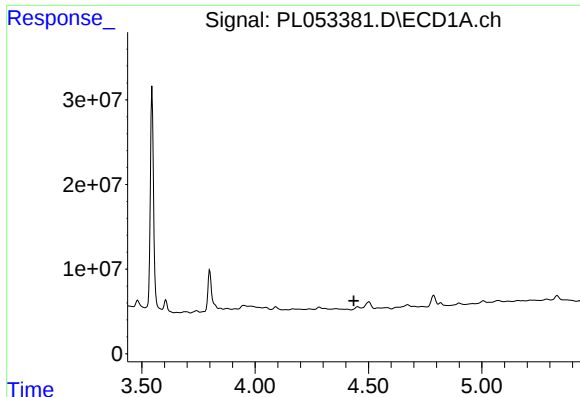

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

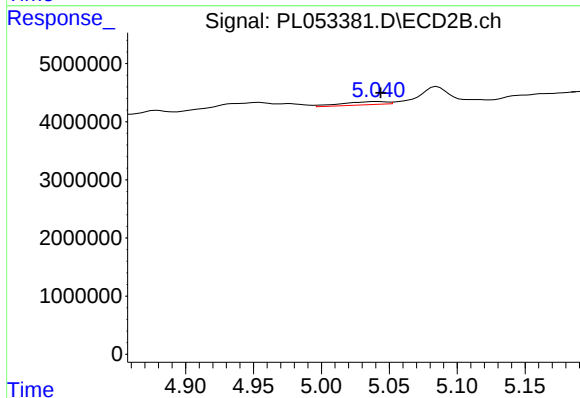


#23 Chlordane-1

R.T.: 5.042 min
Delta R.T.: -0.002 min
Response: 1241075
Conc: 12.24 ng/ml

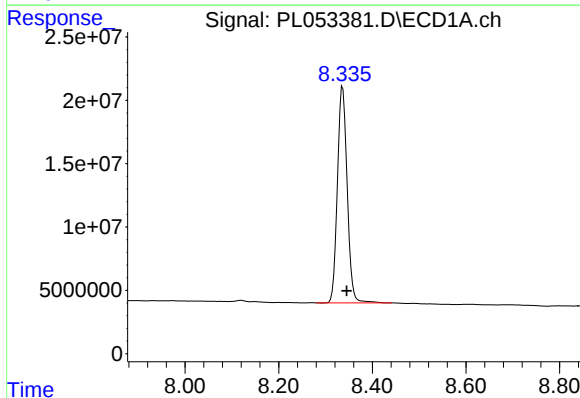

#28 Decachlorobiphenyl

R.T.: 8.337 min
Delta R.T.: -0.009 min
Response: 247080624
Conc: 24.67 ng/ml

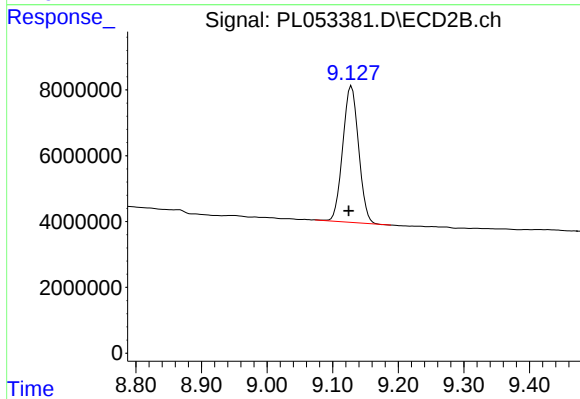

#28 Decachlorobiphenyl

R.T.: 9.129 min
Delta R.T.: 0.004 min
Response: 69402723
Conc: 23.66 ng/ml