

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101719\
 Data File : PL053388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2019 17:32
 Operator : SG\AJ
 Sample : K5392-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 00:58:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	4.047	172.4E6	42806522	17.330	15.942
28)	SA Decachlor...	8.336	9.129	146.1E6	45857367	14.588	15.631
Target Compounds							
4)	MA Heptachlor	0.000	5.233	0	1263023	N.D.	0.331 #
11)	B alpha-Chl...	0.000	6.236	0	1293725	N.D.	0.384 #
12)	B 4,4'-DDE	0.000	6.387	0	3706361	N.D.	1.135 #
15)	B Endosulfa...	0.000	6.974	0	3299600	N.D.	1.112 #
16)	A 4,4'-DDD	0.000	6.882	0	3699983	N.D.	1.509 #
26)	Chlordane-4	0.000	6.236	0	1293725	N.D.	2.436 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101719\
Data File : PL053388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2019 17:32
Operator : SG\AJ
Sample : K5392-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 00:58:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

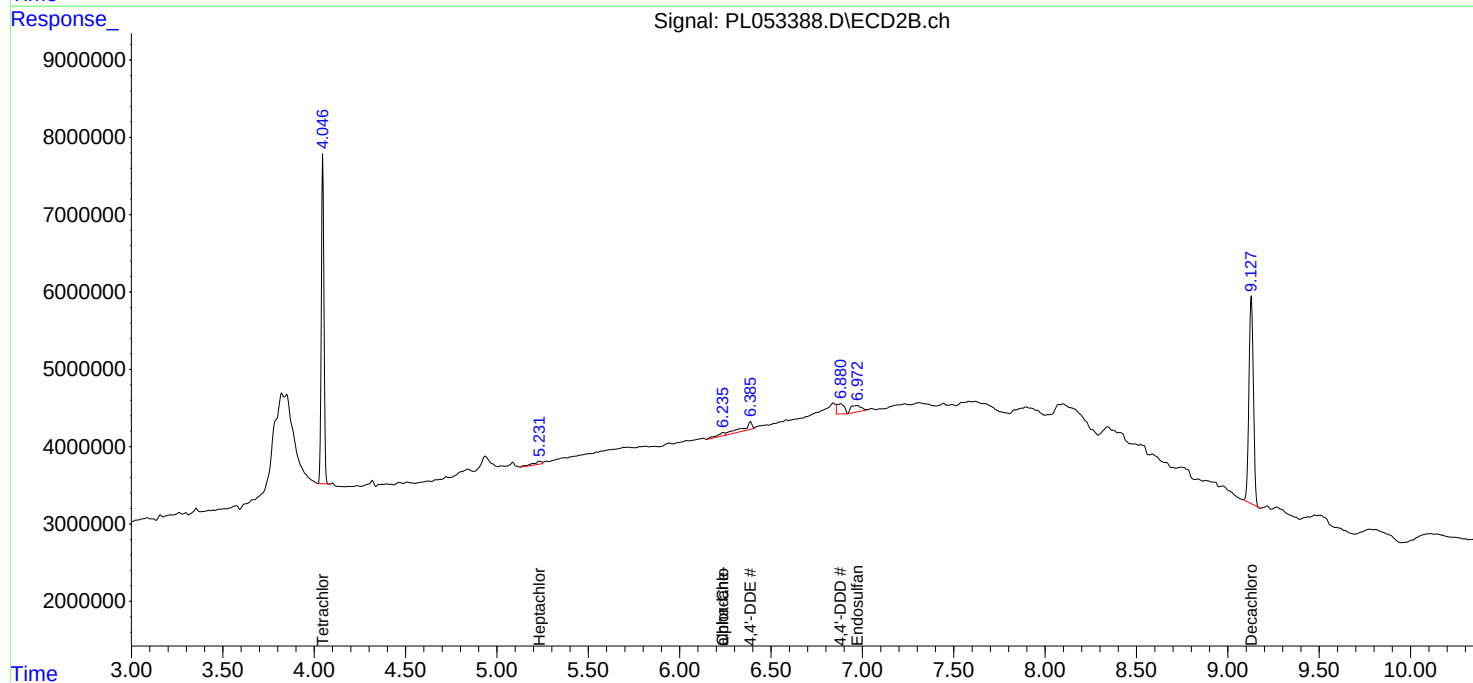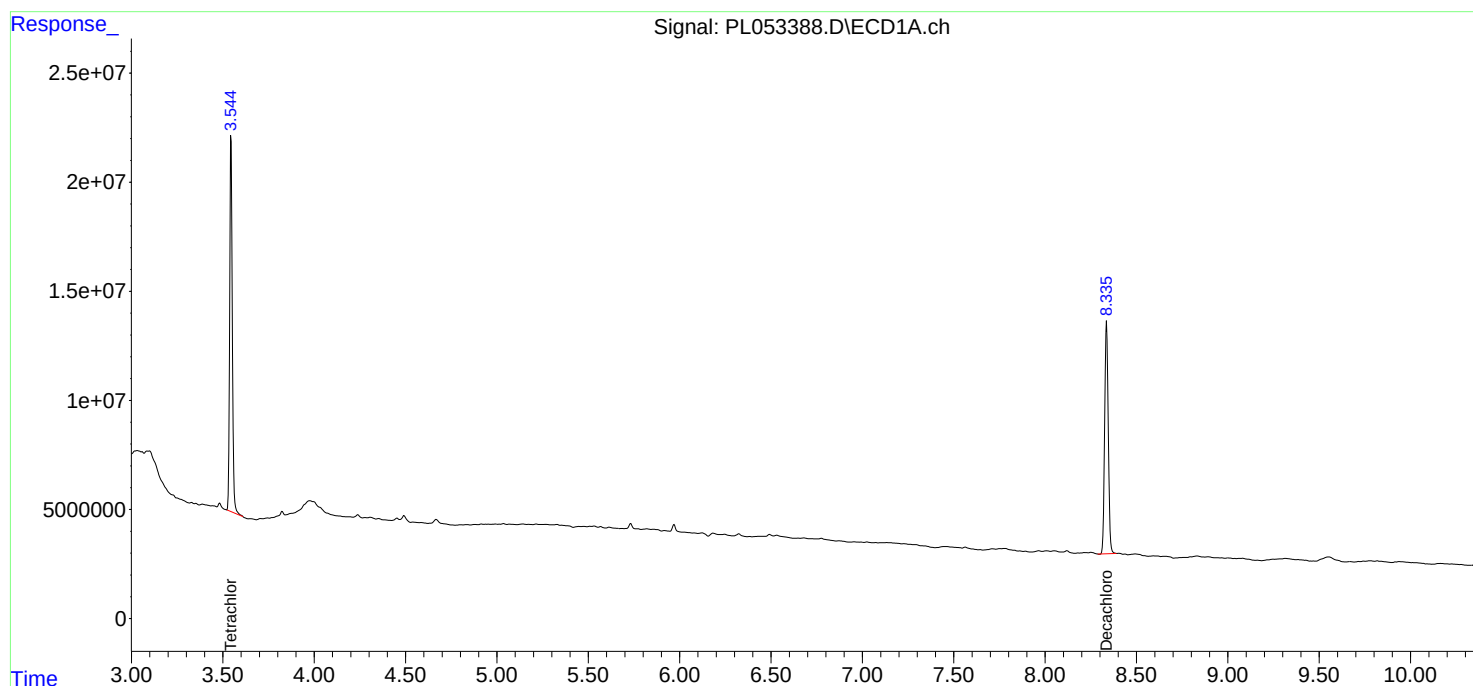


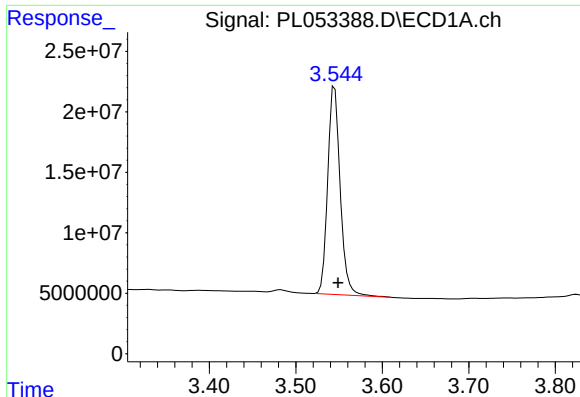

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: -0.004 min
Response: 172379325
Conc: 17.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

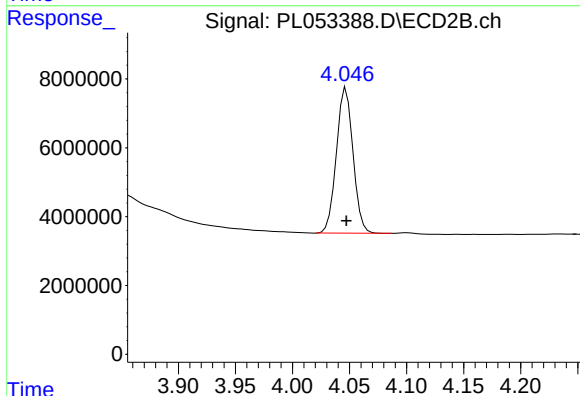


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 42806522
Conc: 15.94 ng/ml

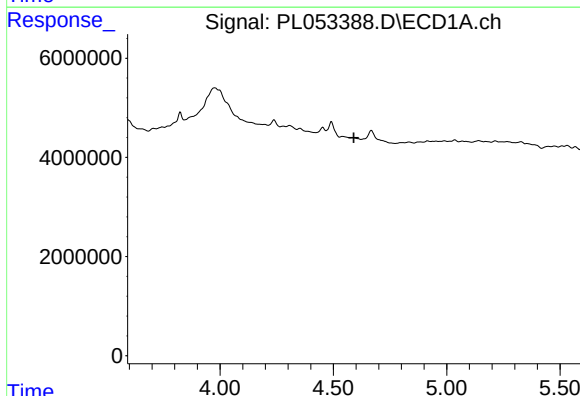


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.590 min
Response: 0
Conc: N.D.

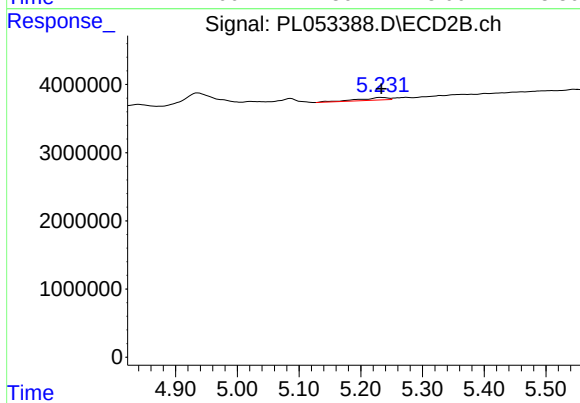

#4 Heptachlor


R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 1263023
Conc: 0.33 ng/ml

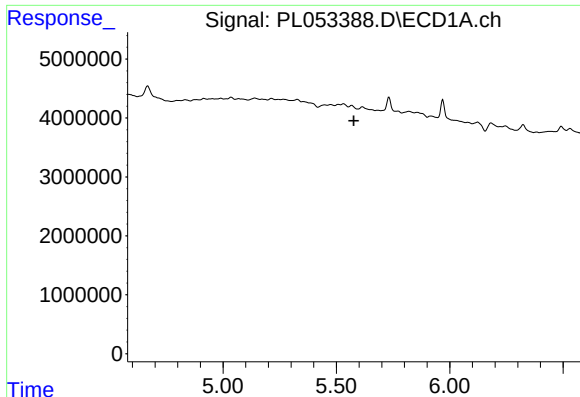

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

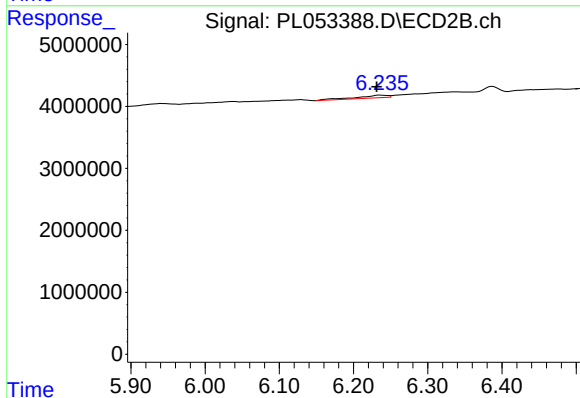


#11 alpha-Chlordane

R.T.: 6.236 min
Delta R.T.: 0.005 min
Response: 1293725
Conc: 0.38 ng/ml

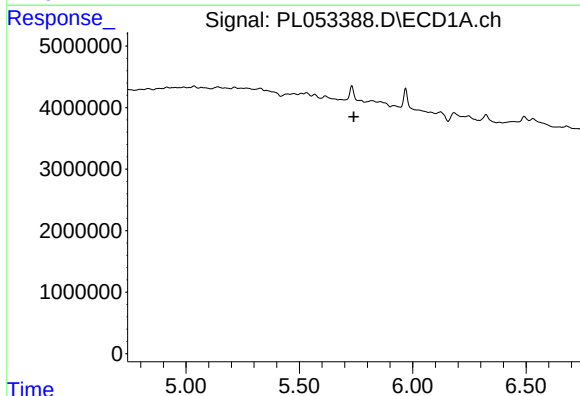


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.740 min
Response: 0
Conc: N.D.

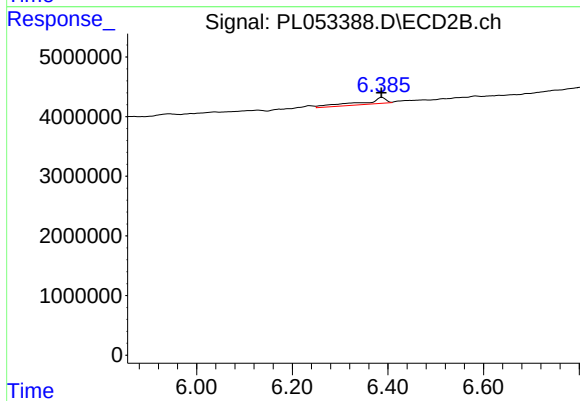

#12 4,4'-DDE


R.T.: 6.387 min
Delta R.T.: 0.000 min
Response: 3706361
Conc: 1.13 ng/ml

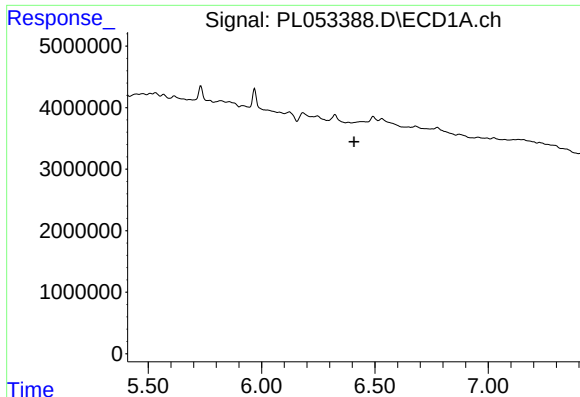

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

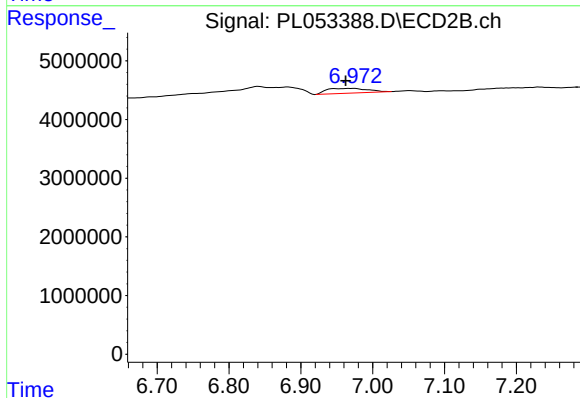


#15 Endosulfan II

R.T.: 6.974 min
Delta R.T.: 0.012 min
Response: 3299600
Conc: 1.11 ng/ml

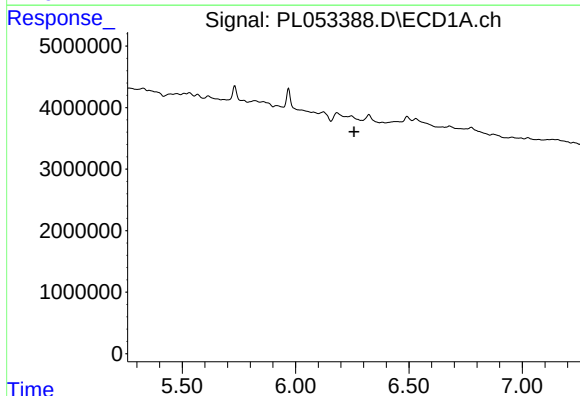


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.258 min
Response: 0
Conc: N.D.

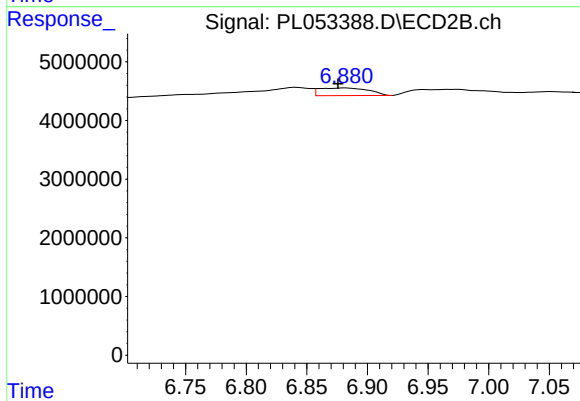

#16 4,4'-DDD


R.T.: 6.882 min
Delta R.T.: 0.006 min
Response: 3699983
Conc: 1.51 ng/ml

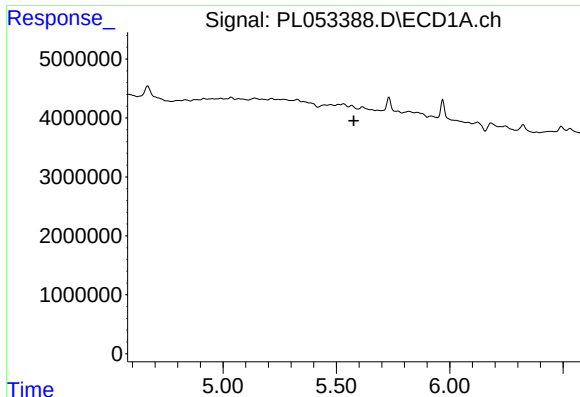

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

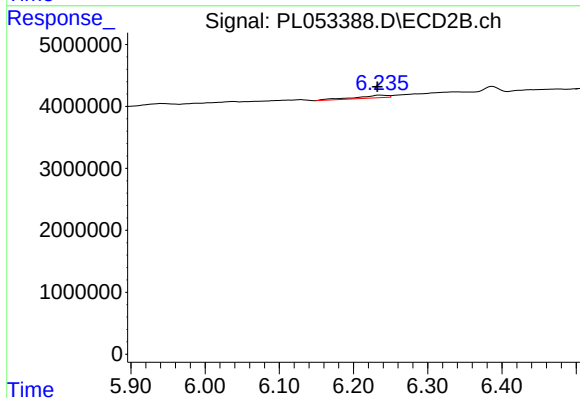


#26 Chlordane-4

R.T.: 6.236 min
Delta R.T.: 0.004 min
Response: 1293725
Conc: 2.44 ng/ml

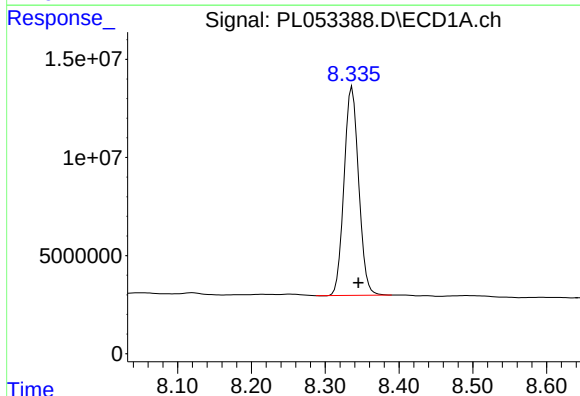

#28 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.009 min
Response: 146117788
Conc: 14.59 ng/ml

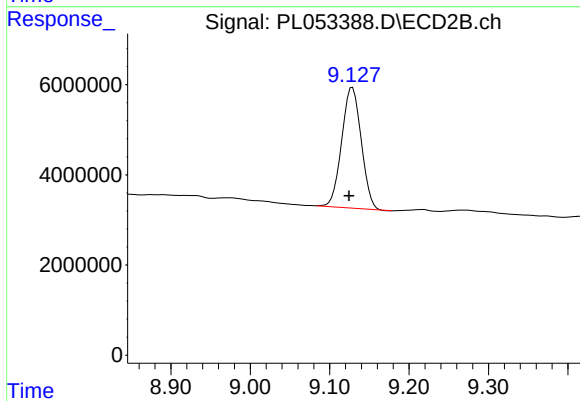

#28 Decachlorobiphenyl

R.T.: 9.129 min
Delta R.T.: 0.004 min
Response: 45857367
Conc: 15.63 ng/ml