

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101720\
 Data File : PL062373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2020 08:37
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 02:19:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 13 05:04:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	0.000	5.815	0	4480713	N.D. 1.378 #
13) MA	Dieldrin	5.665	0.000	1786624	0	1.016 N.D. #
14) MA	Endrin	0.000	6.639	0	5909872	N.D. 2.376 #
16) A	4,4'-DDD	6.064	0.000	1036569	0	0.715 N.D. #
17) MA	4,4'-DDT	6.300	0.000	6646908	0	5.153 N.D. #
18) B	Endrin al...	6.396f	6.969	4586672	684259	3.161 0.290 #
19) B	Endosulfa...	0.000	7.208	0	4392710	N.D. 1.693 #
20) A	Methoxychlor	6.853	7.550f	2485749	4309845	3.055 3.269
21) B	Endrin ke...	7.057	7.667	3075317	2615816	1.561 0.938 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101720\
Data File : PL062373.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2020 08:37
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 02:19:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
Quant Title : GC Extractables
QLast Update : Tue Oct 13 05:04:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

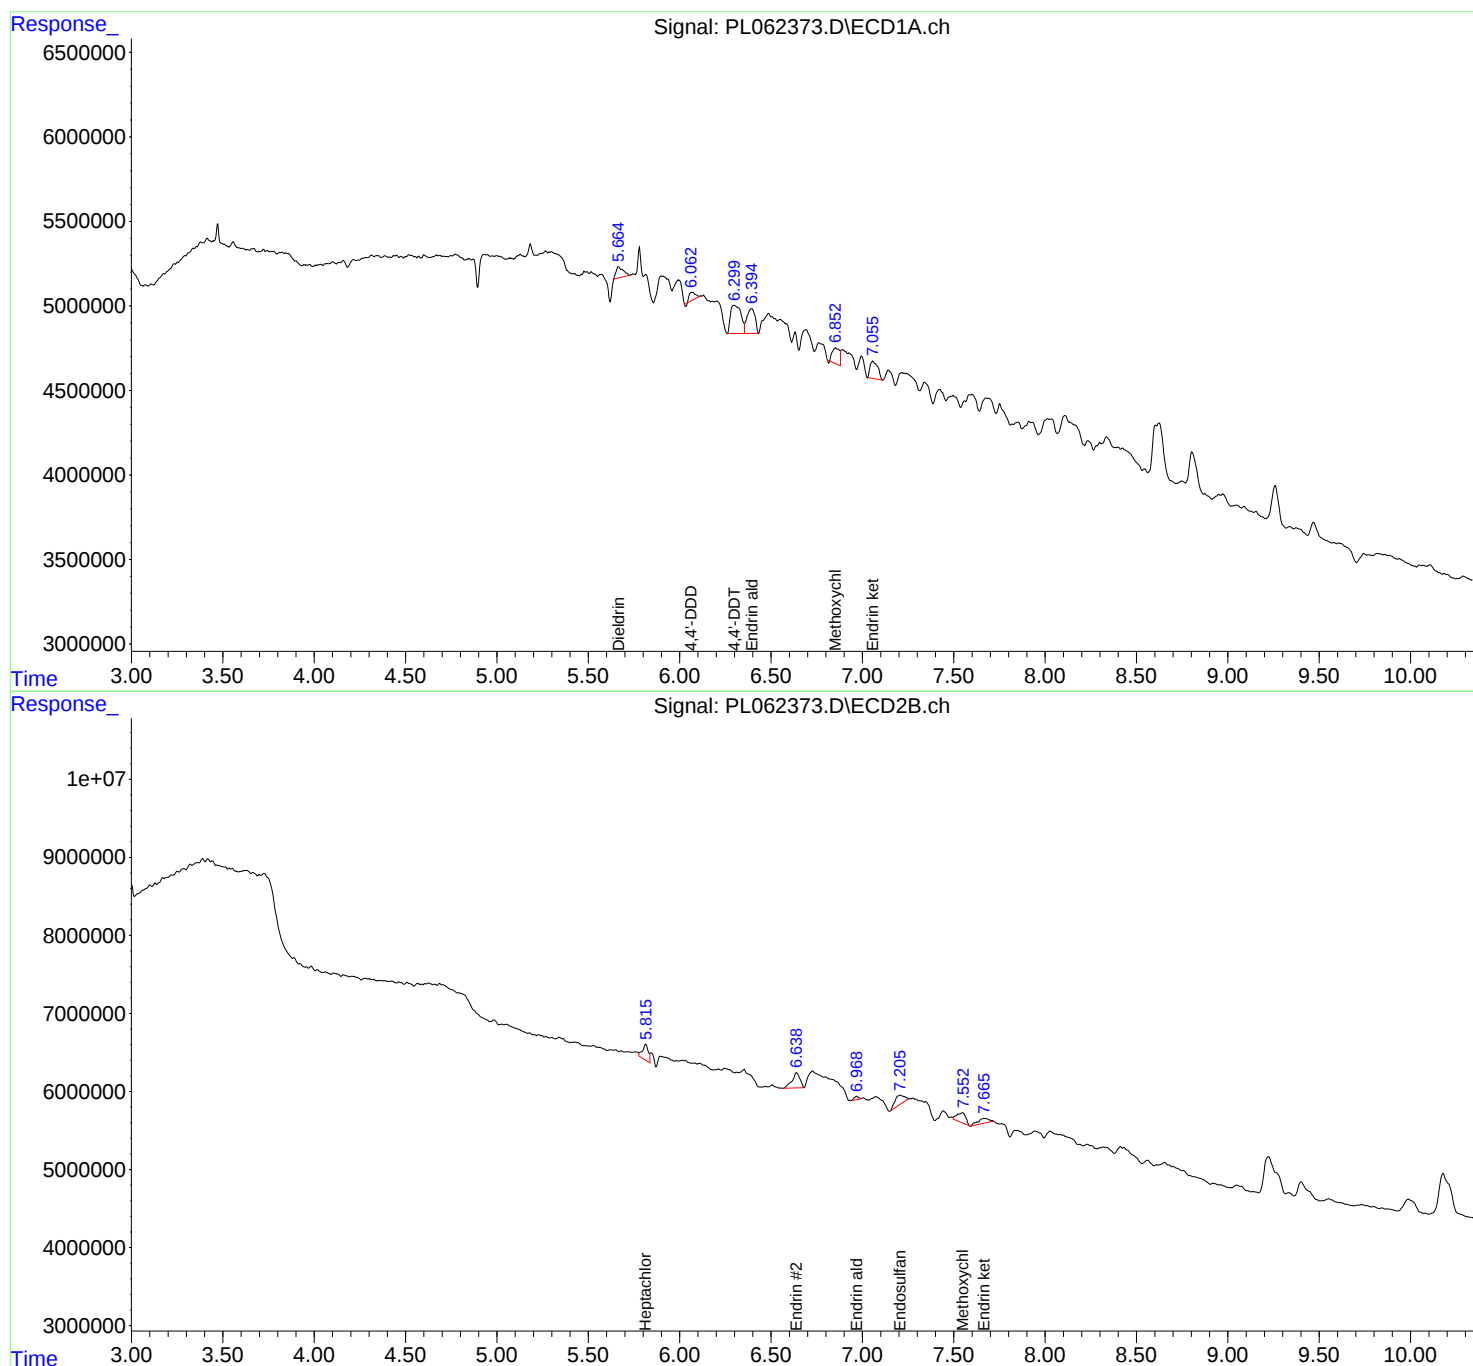


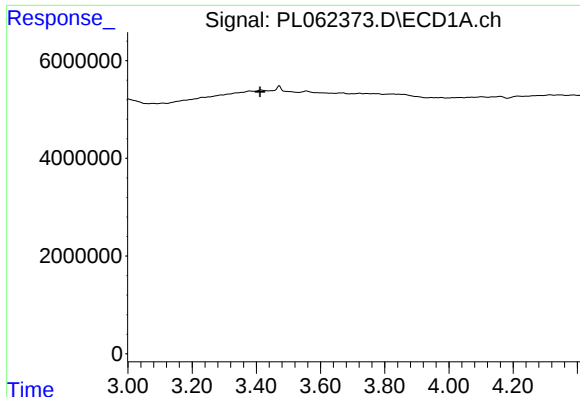

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

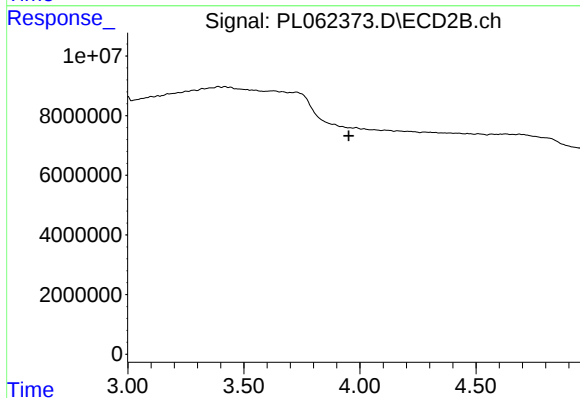


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.952 min
Response: 0
Conc: N.D.

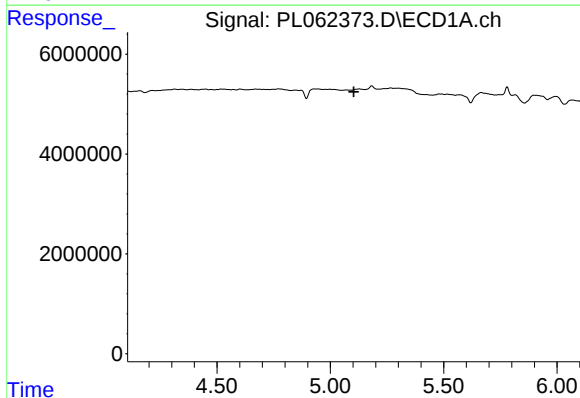


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.103 min
Response: 0
Conc: N.D.

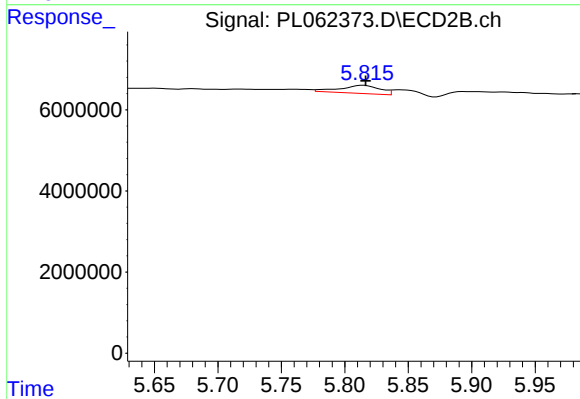

#8 Heptachlor epoxide


R.T.: 5.815 min
Delta R.T.: -0.002 min
Response: 4480713
Conc: 1.38 ng/ml

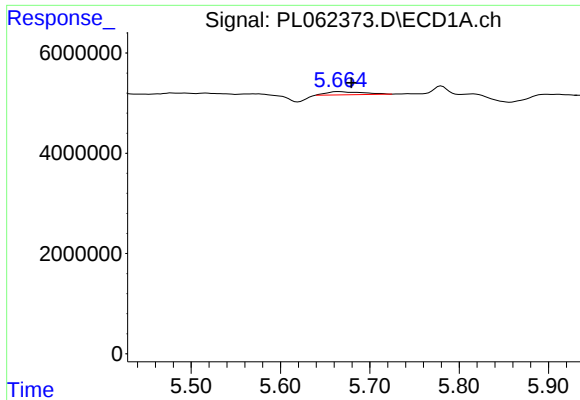

#13 Dieldrin


R.T.: 5.665 min
Delta R.T.: -0.014 min
Response: 1786624
Conc: 1.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

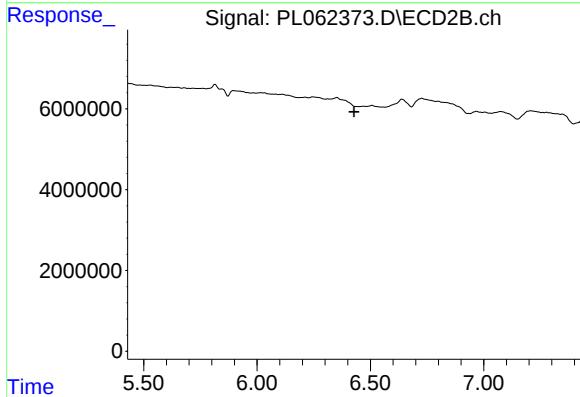


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.429 min
Response: 0
Conc: N.D.

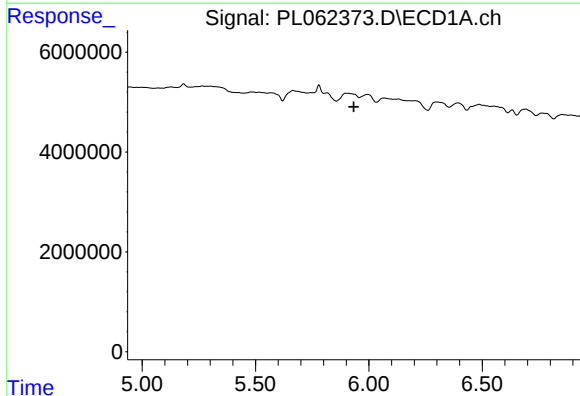


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.933 min
Response: 0
Conc: N.D.

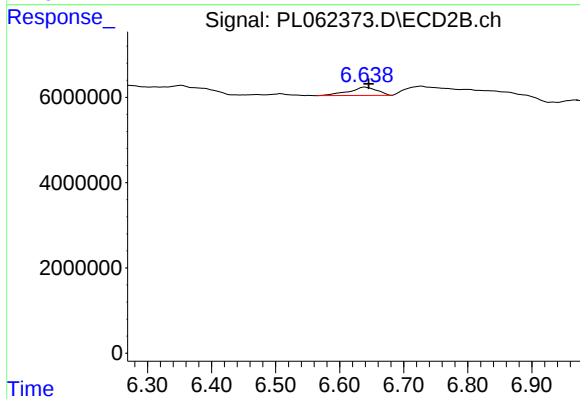

#14 Endrin


R.T.: 6.639 min
Delta R.T.: -0.006 min
Response: 5909872
Conc: 2.38 ng/ml

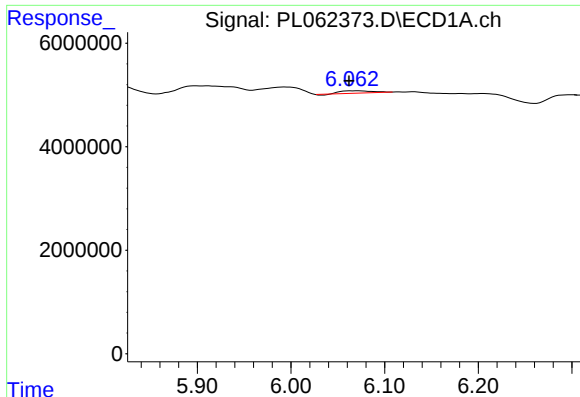

#16 4,4'-DDD


R.T.: 6.064 min
Delta R.T.: 0.002 min
Response: 1036569
Conc: 0.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

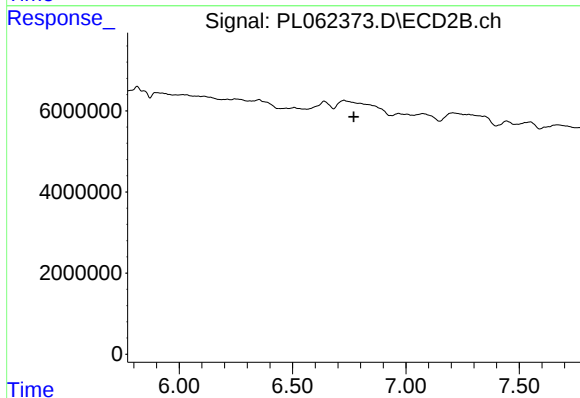


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.771 min
Response: 0
Conc: N.D.

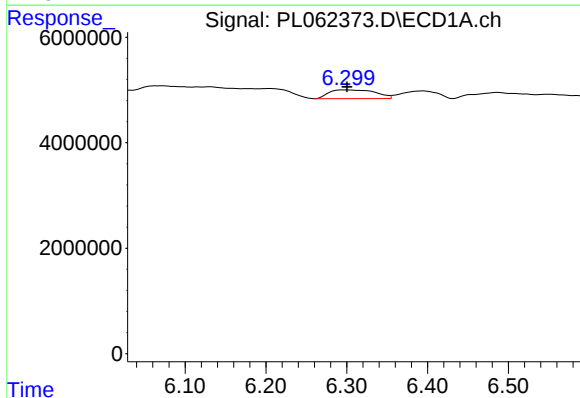


#17 4,4'-DDT

R.T.: 6.300 min
Delta R.T.: 0.000 min
Response: 6646908
Conc: 5.15 ng/ml

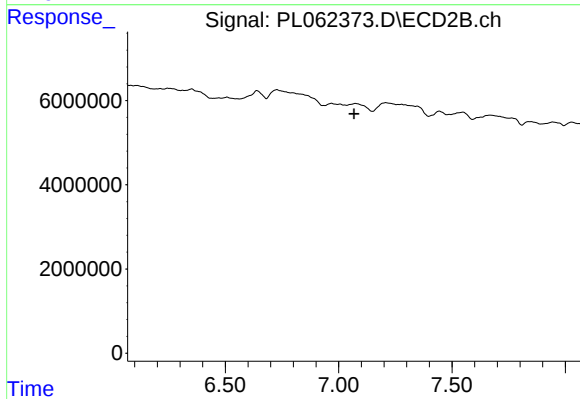

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.069 min
Response: 0
Conc: N.D.

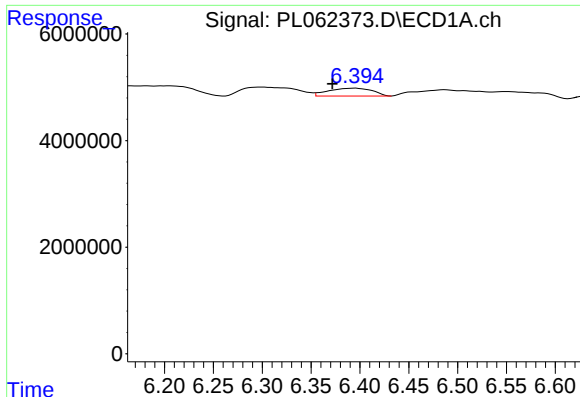

#18 Endrin aldehyde


R.T.: 6.396 min
Delta R.T.: 0.024 min
Response: 4586672
Conc: 3.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

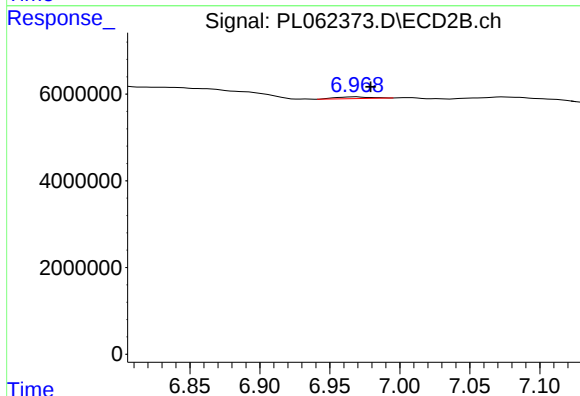


#18 Endrin aldehyde

R.T.: 6.969 min
Delta R.T.: -0.010 min
Response: 684259
Conc: 0.29 ng/ml

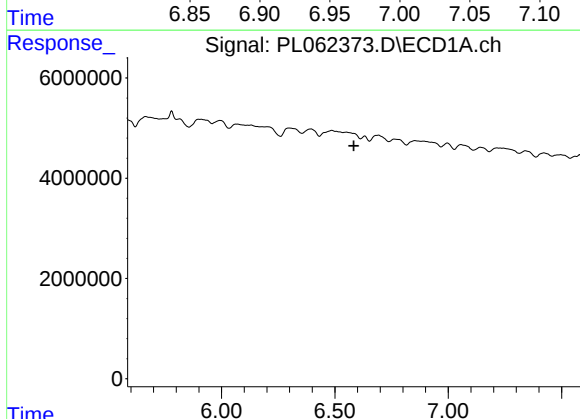


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.584 min
Response: 0
Conc: N.D.

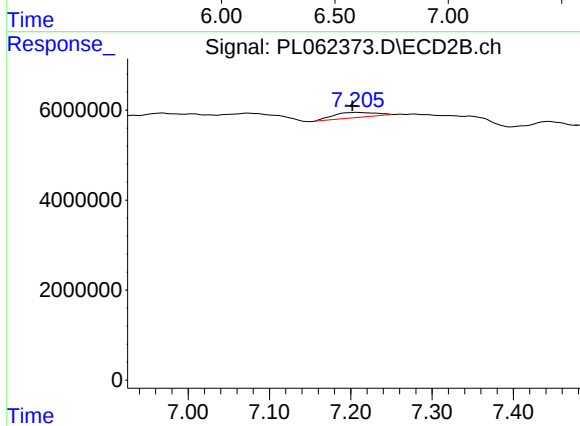

#19 Endosulfan Sulfate


R.T.: 7.208 min
Delta R.T.: 0.006 min
Response: 4392710
Conc: 1.69 ng/ml

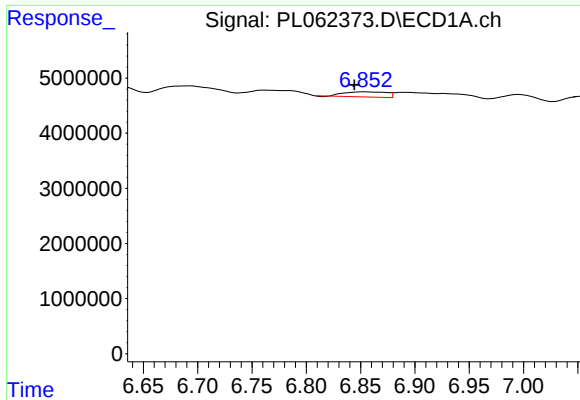

#20 Methoxychlor


R.T.: 6.853 min
Delta R.T.: 0.009 min
Response: 2485749
Conc: 3.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

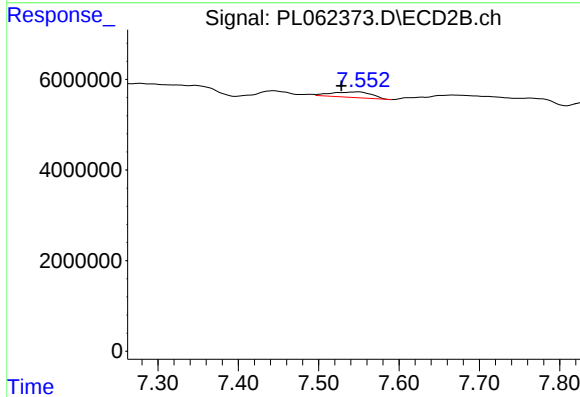


#20 Methoxychlor

R.T.: 7.550 min
Delta R.T.: 0.021 min
Response: 4309845
Conc: 3.27 ng/ml

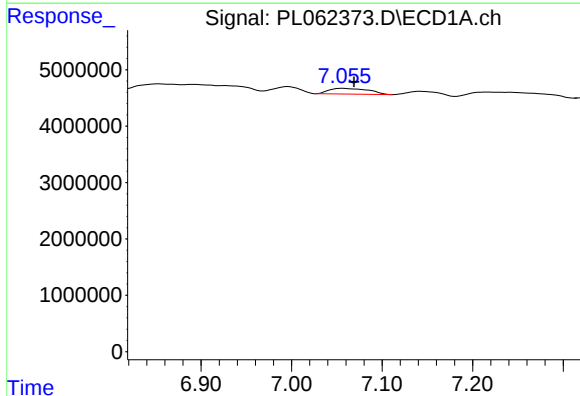


#21 Endrin ketone

R.T.: 7.057 min
Delta R.T.: -0.012 min
Response: 3075317
Conc: 1.56 ng/ml

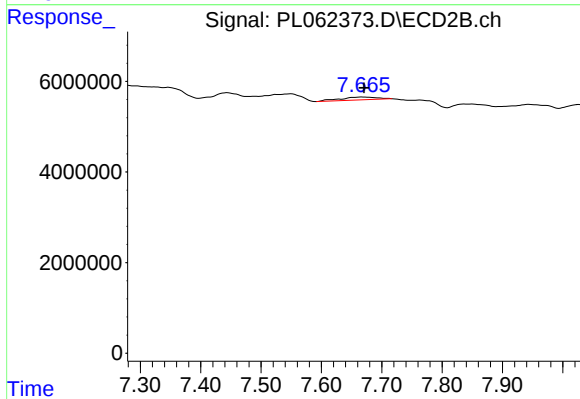

#21 Endrin ketone


R.T.: 7.667 min
Delta R.T.: -0.004 min
Response: 2615816
Conc: 0.94 ng/ml

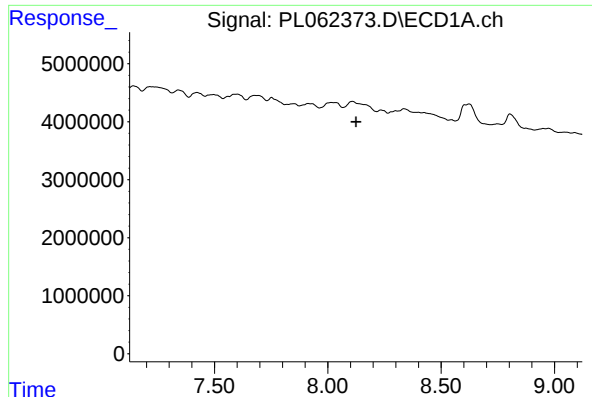

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

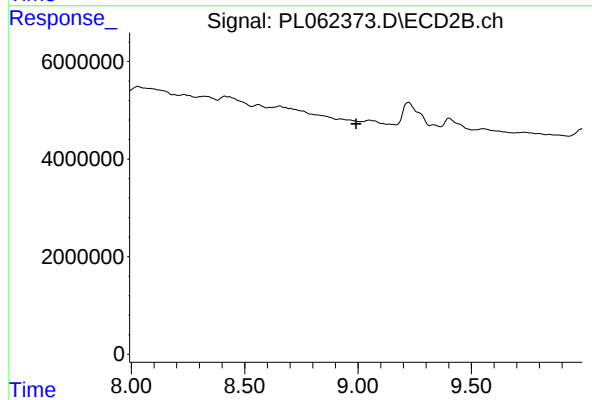

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.992 min
Response: 0
Conc: N.D.