

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101720\
 Data File : PL062377.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2020 09:55
 Operator : DD\AJ
 Sample : PB132379BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB132379BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 02:19:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 13 05:04:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.418	3.952	35252225	54967170	20.253	19.503
28)	SA Decachlor...	8.132	8.998	36567118	51775233	19.990	18.863
Target Compounds							
7)	B delta-BHC	0.000	4.991f	0	222720	N.D.	0.064 #
8)	B Heptachlo...	0.000	5.814	0	25265777	N.D.	7.773 #
9)	A Endosulfan I	0.000	6.160	0	29664796	N.D.	9.848 #
10)	B gamma-Chl...	0.000	6.076f	0	23066688	N.D.	7.024 #
14)	MA Endrin	5.944	0.000	3170767	0	2.064	N.D. #
15)	B Endosulfa...	0.000	6.870	0	6618151	N.D.	2.439 #
17)	MA 4,4'-DDT	0.000	7.074	0	3026359	N.D.	1.323 #
25)	Chlordane-3	0.000	6.076f	0	23066688	N.D.	56.327 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101720\
Data File : PL062377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2020 09:55
Operator : DD\AJ
Sample : PB132379BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB132379BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 02:19:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
Quant Title : GC Extractables
QLast Update : Tue Oct 13 05:04:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

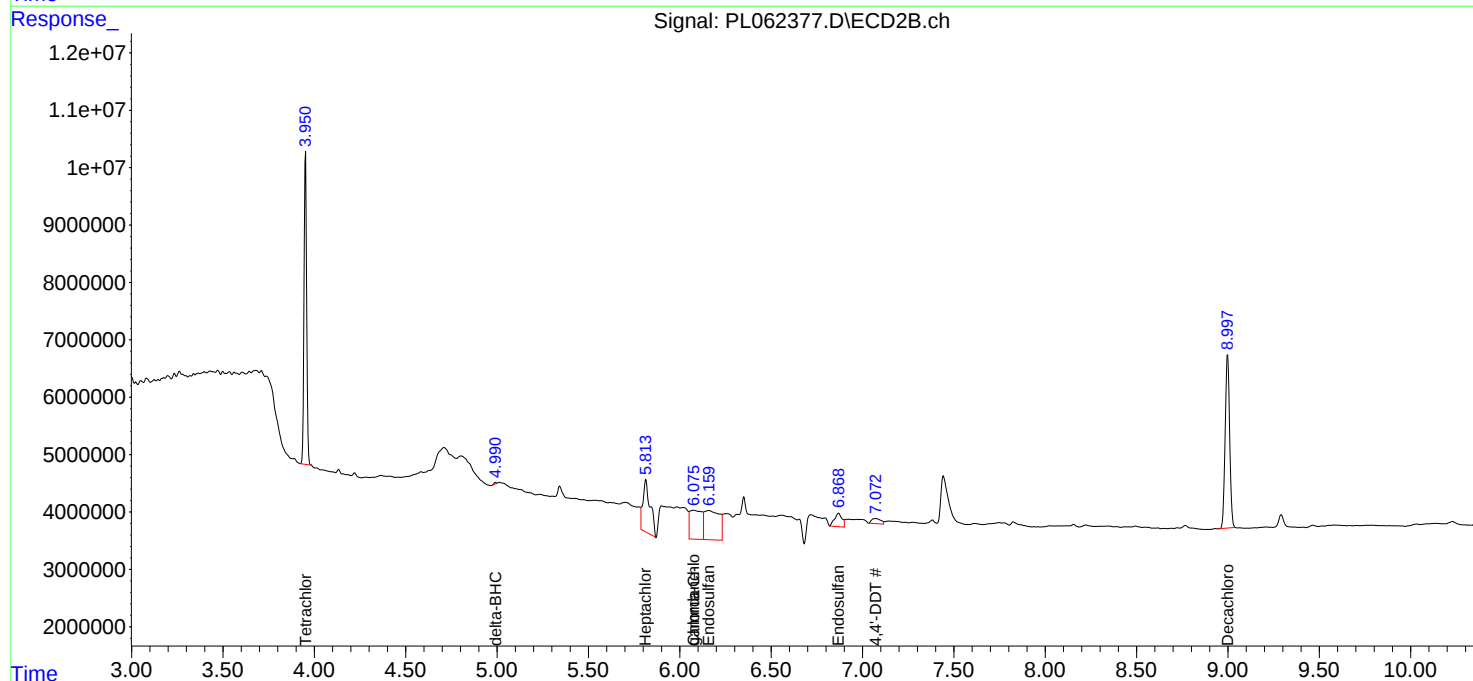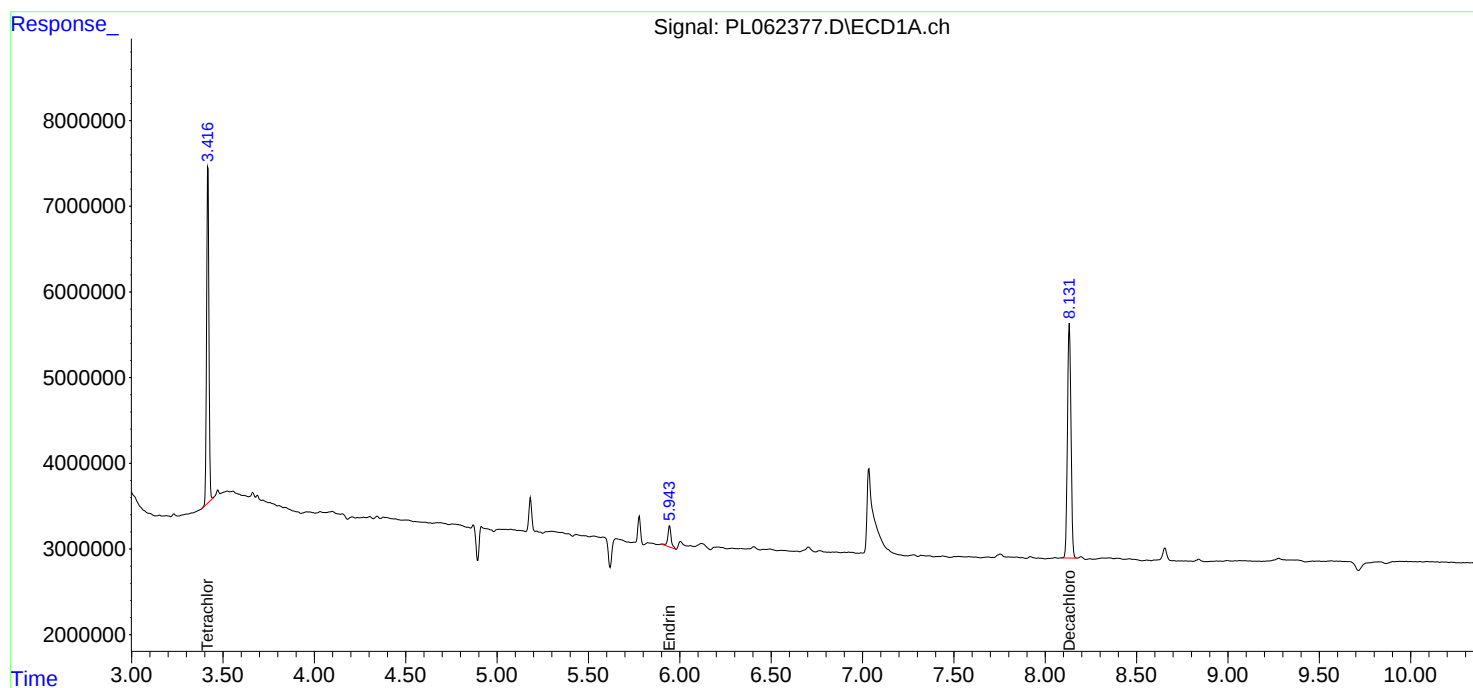


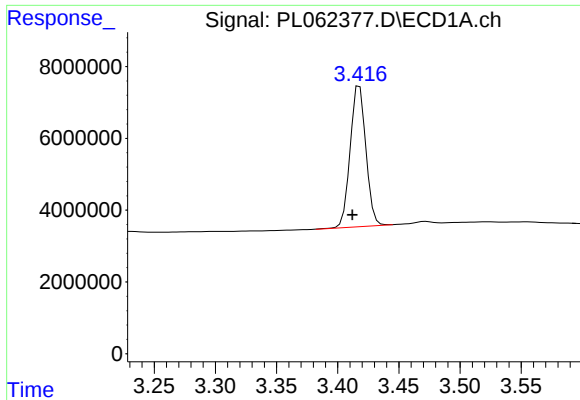

#1 Tetrachloro-m-xylene


R.T.: 3.418 min
Delta R.T.: 0.006 min
Response: 35252225
Conc: 20.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132379BL

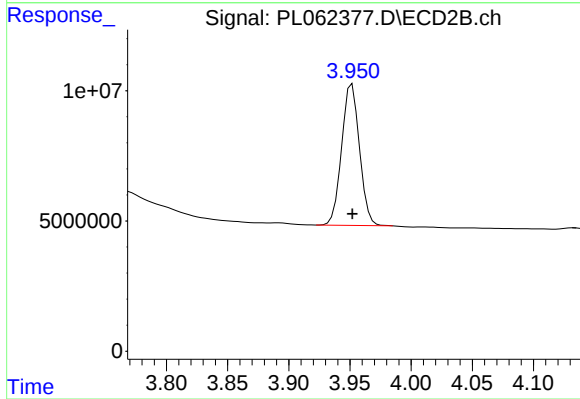


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 54967170
Conc: 19.50 ng/ml

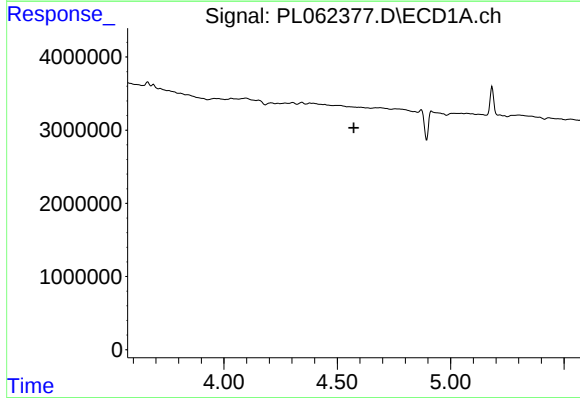


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

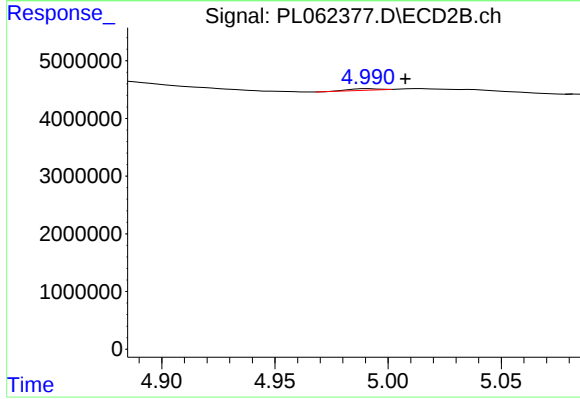

#7 delta-BHC


R.T.: 4.991 min
Delta R.T.: -0.016 min
Response: 222720
Conc: 0.06 ng/ml

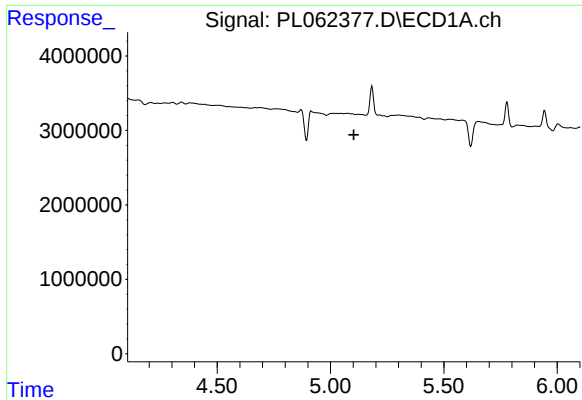

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.103 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB132379BL

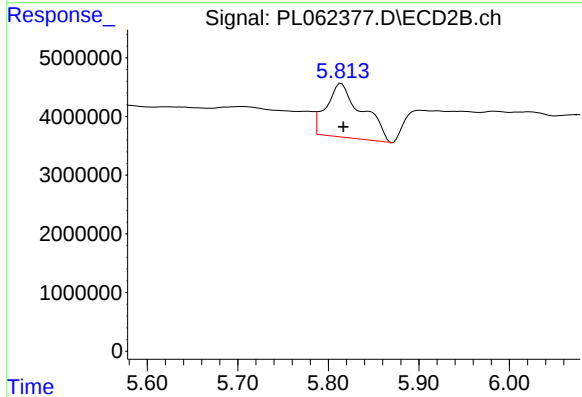


#8 Heptachlor epoxide

R.T.: 5.814 min
Delta R.T.: -0.002 min
Response: 25265777
Conc: 7.77 ng/ml

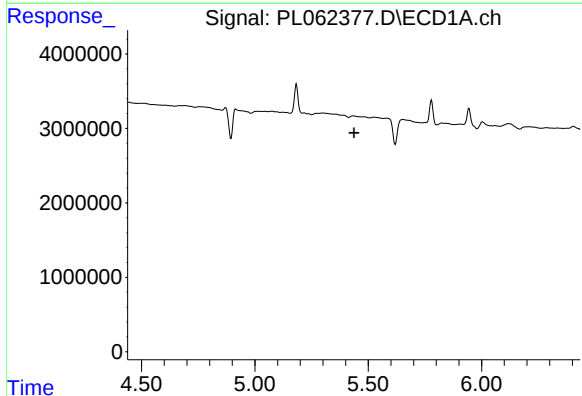


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.438 min
Response: 0
Conc: N.D.

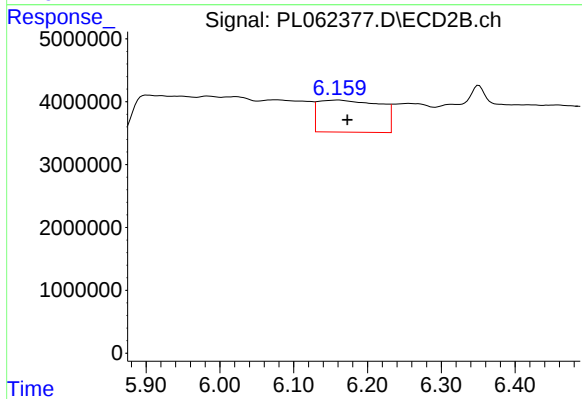

#9 Endosulfan I


R.T.: 6.160 min
Delta R.T.: -0.013 min
Response: 29664796
Conc: 9.85 ng/ml

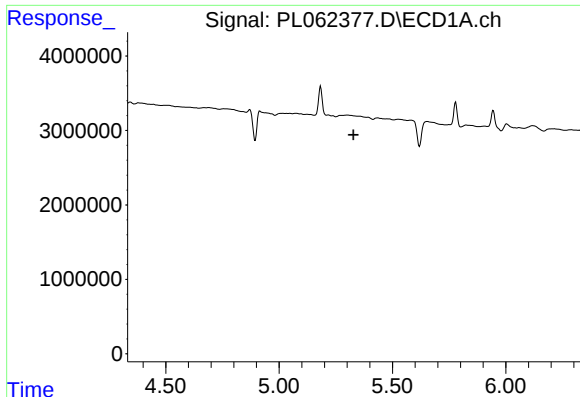

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB132379BL

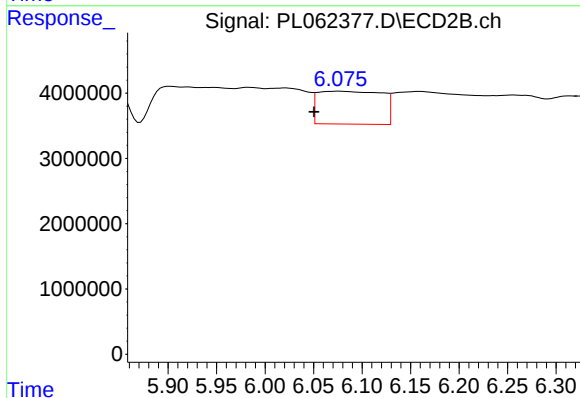


#10 gamma-Chlordane

R.T.: 6.076 min
Delta R.T.: 0.026 min
Response: 23066688
Conc: 7.02 ng/ml

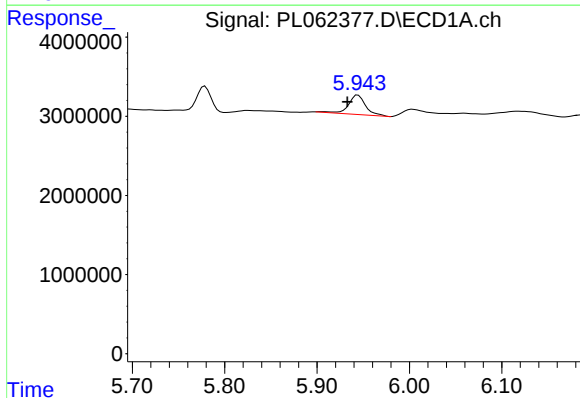


#14 Endrin

R.T.: 5.944 min
Delta R.T.: 0.011 min
Response: 3170767
Conc: 2.06 ng/ml

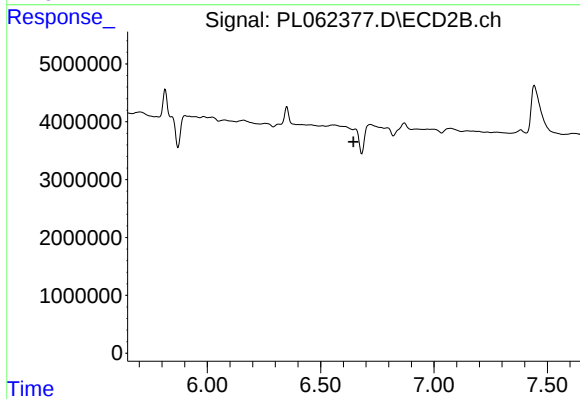

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.645 min
Response: 0
Conc: N.D.

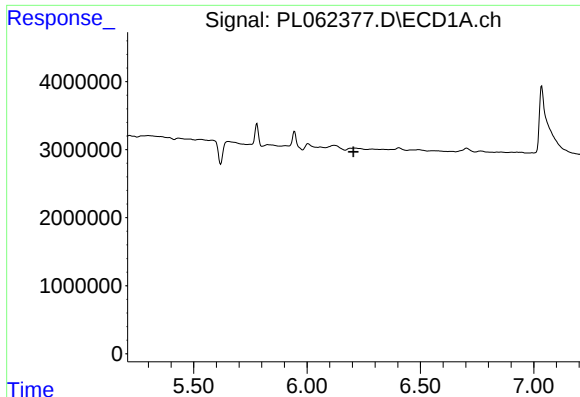

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB132379BL

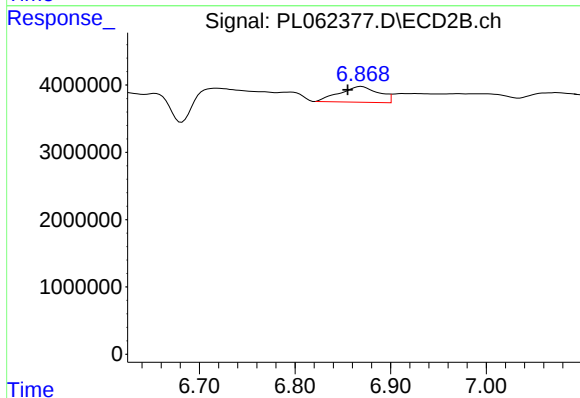


#15 Endosulfan II

R.T.: 6.870 min
Delta R.T.: 0.014 min
Response: 6618151
Conc: 2.44 ng/ml

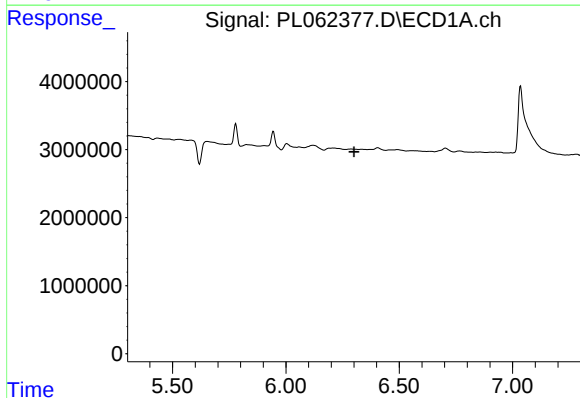


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.300 min
Response: 0
Conc: N.D.

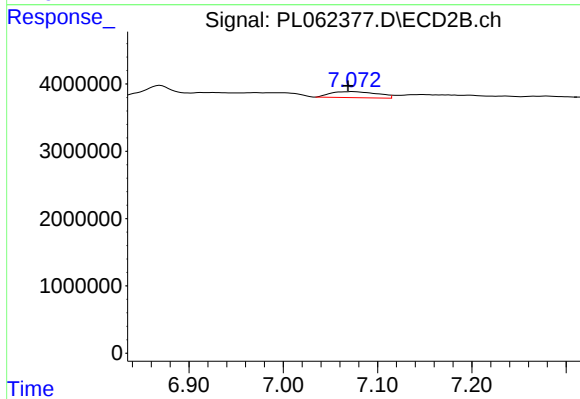

#17 4,4'-DDT


R.T.: 7.074 min
Delta R.T.: 0.005 min
Response: 3026359
Conc: 1.32 ng/ml

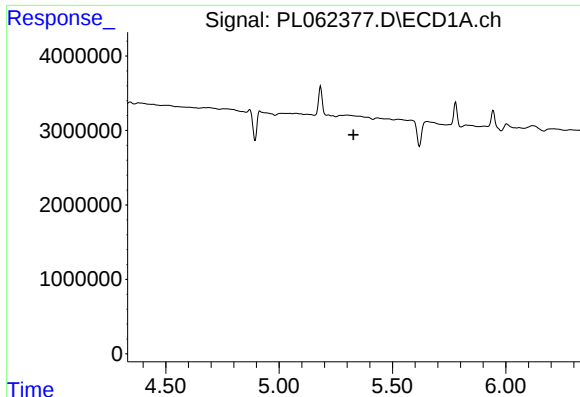

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB132379BL

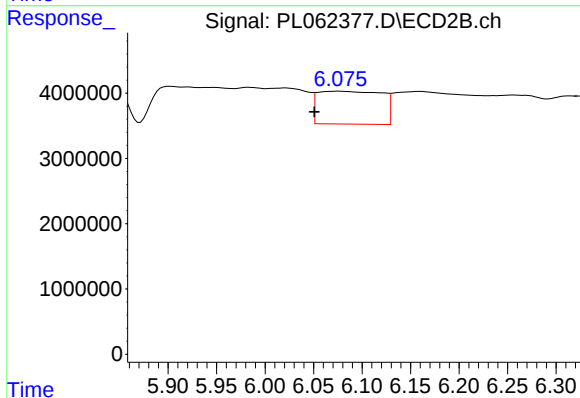


#25 Chlordane-3

R.T.: 6.076 min
Delta R.T.: 0.025 min
Response: 23066688
Conc: 56.33 ng/ml

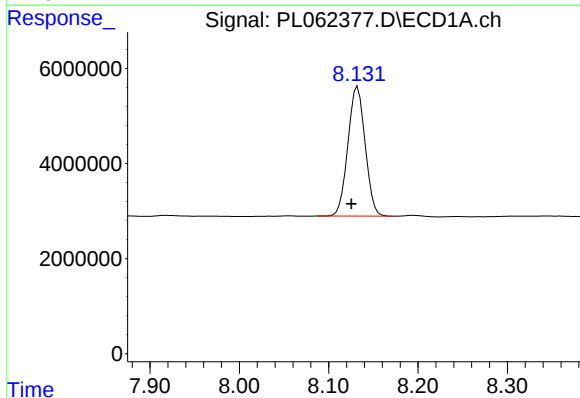

#28 Decachlorobiphenyl

R.T.: 8.132 min
Delta R.T.: 0.007 min
Response: 36567118
Conc: 19.99 ng/ml

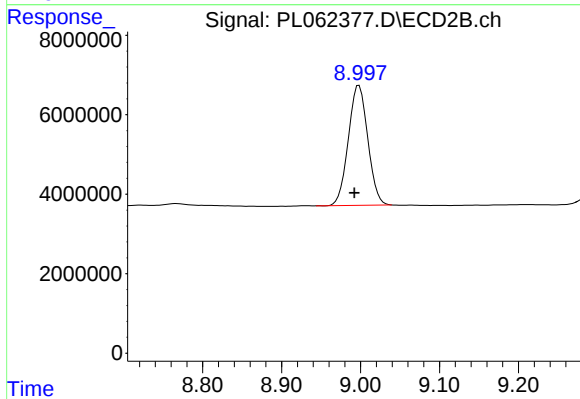

#28 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.006 min
Response: 51775233
Conc: 18.86 ng/ml