

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101720\
 Data File : PL062407.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2020 18:58
 Operator : DD\AJ
 Sample : L4223-08
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PL-01-101420

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 02:26:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 13 05:04:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	35596880	55078647	20.451	19.543
28)	SA Decachlor...	8.124	8.993	29583315	41678464	16.172	15.185
Target Compounds							
2)	A alpha-BHC	0.000	4.309f	0	875344	N.D.	0.209 #
4)	MA Heptachlor	4.446f	0.000	333108	0	0.158	N.D. #
6)	B beta-BHC	4.375	4.784	1213656	1649015	1.262	0.938 #
7)	B delta-BHC	0.000	4.984f	0	6930592	N.D.	1.998 #
10)	B gamma-Chl...	0.000	6.071f	0	226871	N.D.	0.069 #
15)	B Endosulfa...	0.000	6.871f	0	334053	N.D.	0.123 #
20)	A Methoxychlor	0.000	7.554f	0	2400986	N.D.	1.821 #
21)	B Endrin ke...	0.000	7.672	0	1141060	N.D.	0.409 #
25)	Chlordane-3	0.000	6.071f	0	226871	N.D.	0.554 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101720\
Data File : PL062407.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2020 18:58
Operator : DD\AJ
Sample : L4223-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PL-01-101420

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 02:26:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
Quant Title : GC Extractables
QLast Update : Tue Oct 13 05:04:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

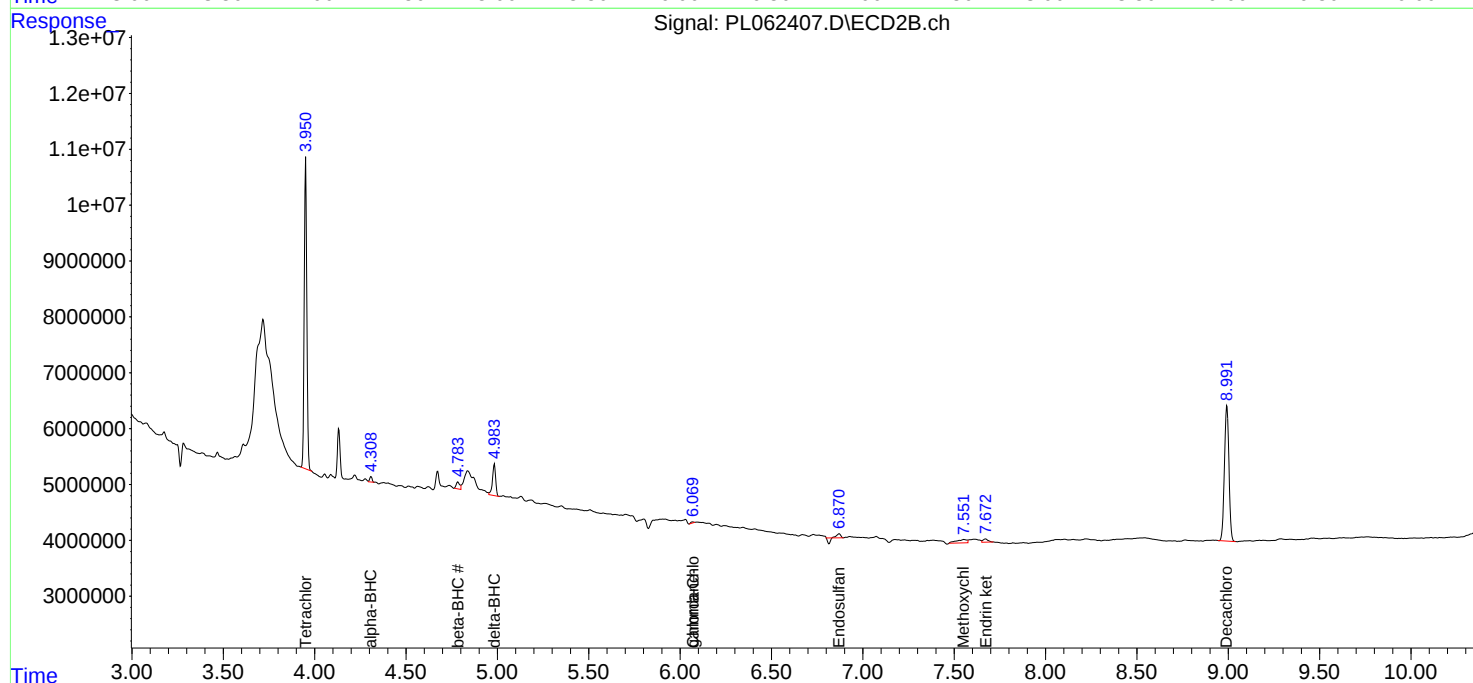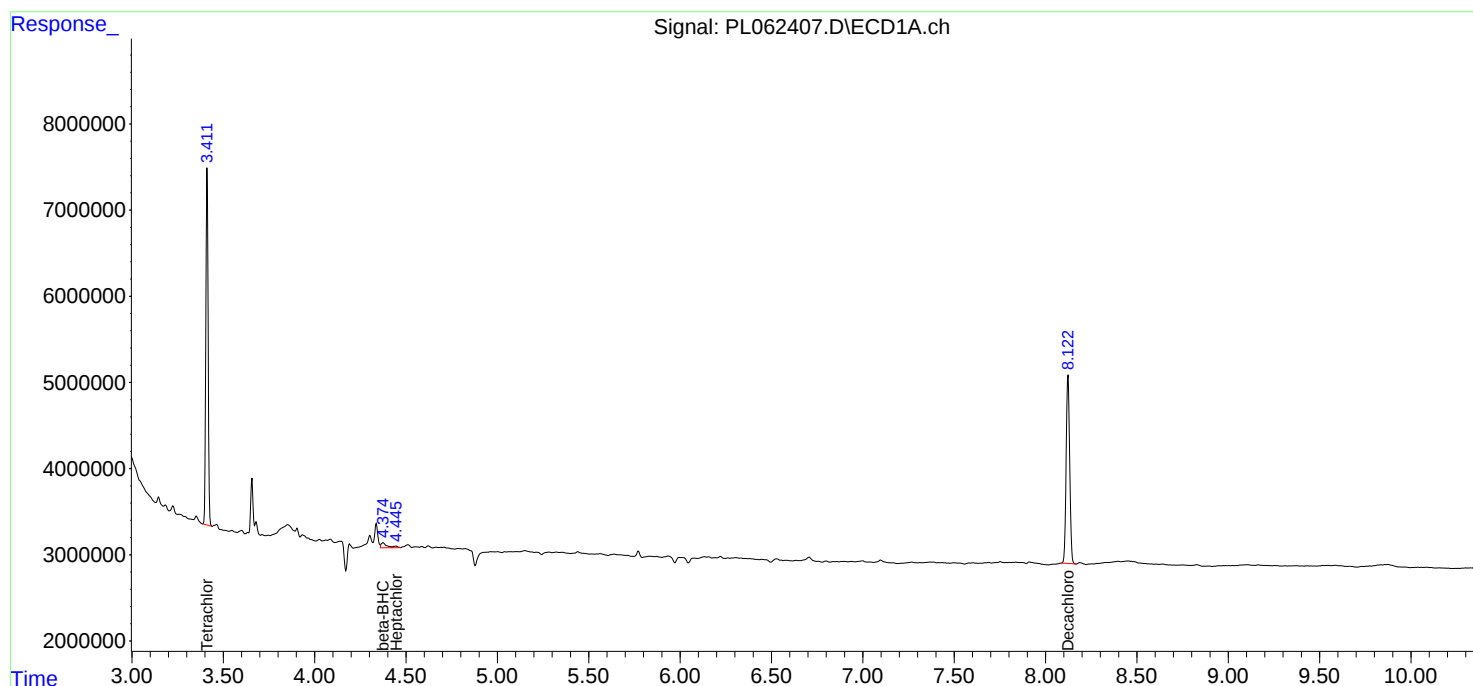


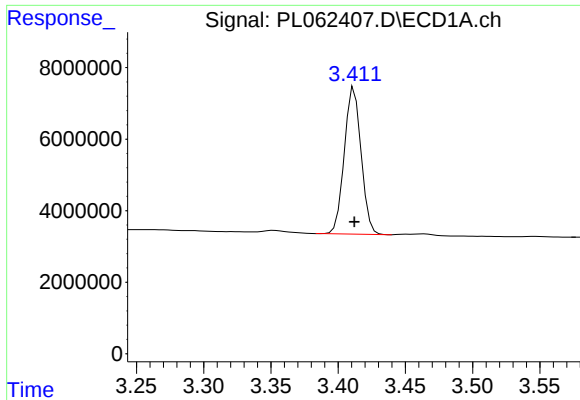

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 35596880
Conc: 20.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-01-101420

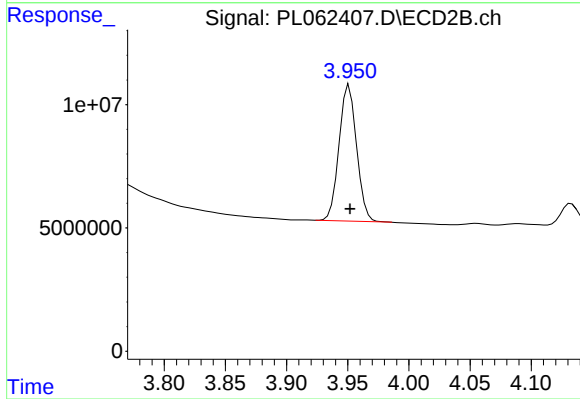


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 55078647
Conc: 19.54 ng/ml

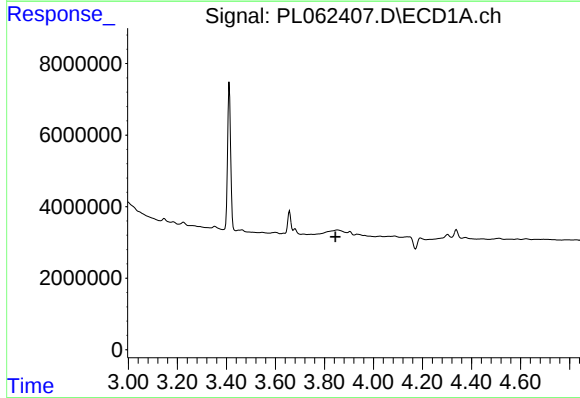


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.845 min
Response: 0
Conc: N.D.

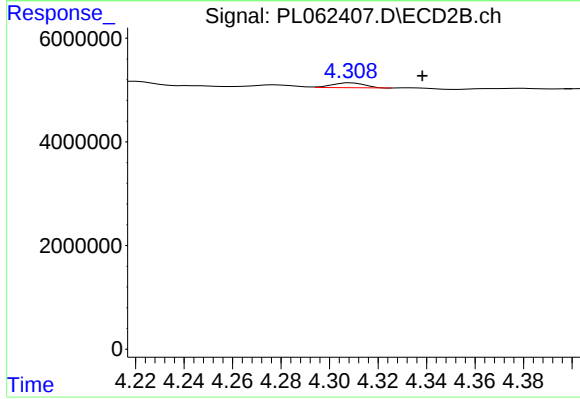

#2 alpha-BHC


R.T.: 4.309 min
Delta R.T.: -0.029 min
Response: 875344
Conc: 0.21 ng/ml

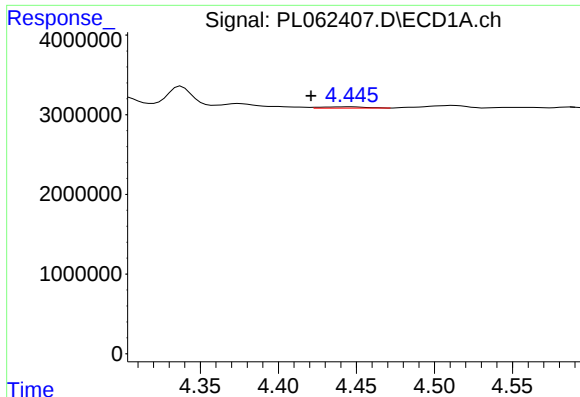

#4 Heptachlor


R.T.: 4.446 min
Delta R.T.: 0.025 min
Response: 333108
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-01-101420

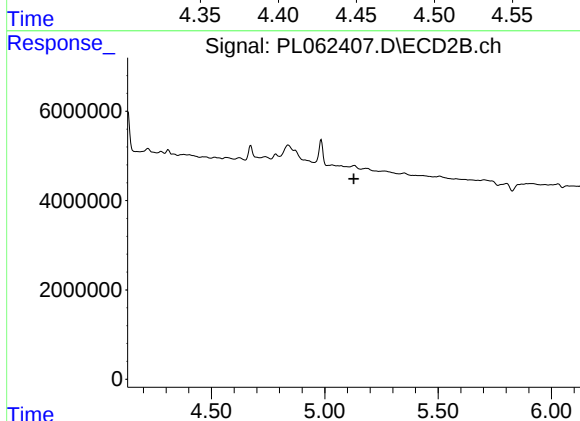


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.128 min
Response: 0
Conc: N.D.

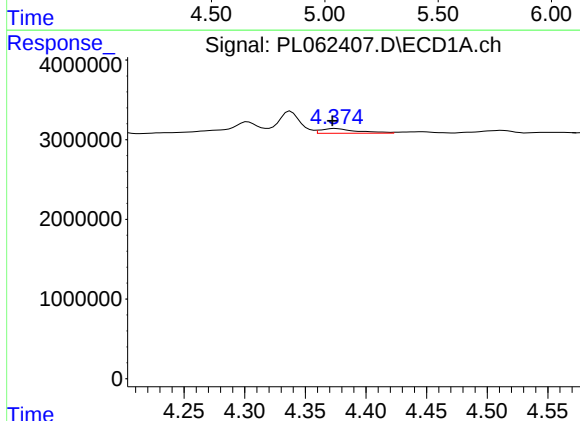


#6 beta-BHC

R.T.: 4.375 min
Delta R.T.: 0.003 min
Response: 1213656
Conc: 1.26 ng/ml

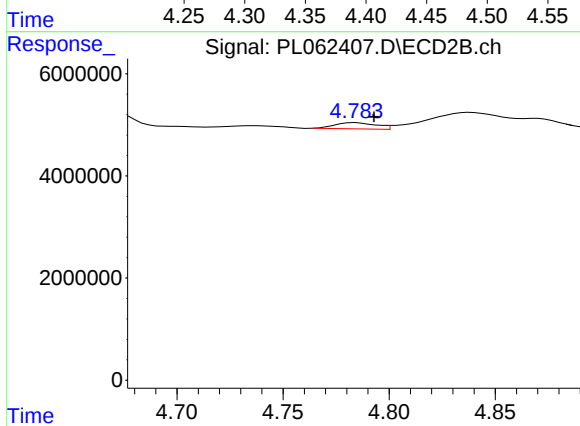

#6 beta-BHC


R.T.: 4.784 min
Delta R.T.: -0.009 min
Response: 1649015
Conc: 0.94 ng/ml

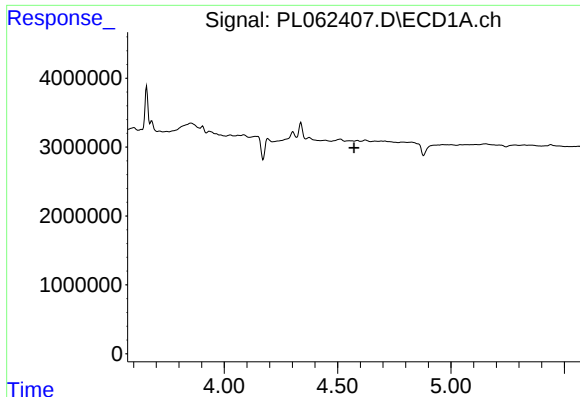

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PL-01-101420

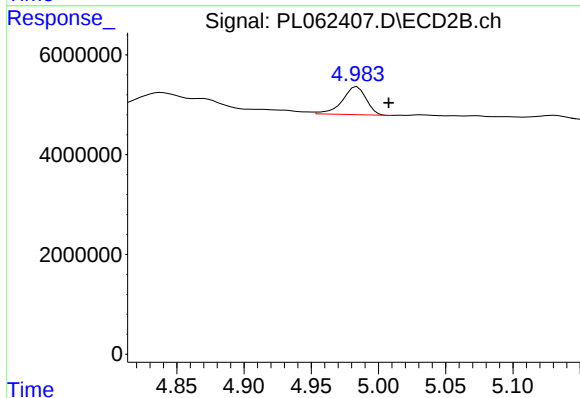


#7 delta-BHC

R.T.: 4.984 min
Delta R.T.: -0.024 min
Response: 6930592
Conc: 2.00 ng/ml

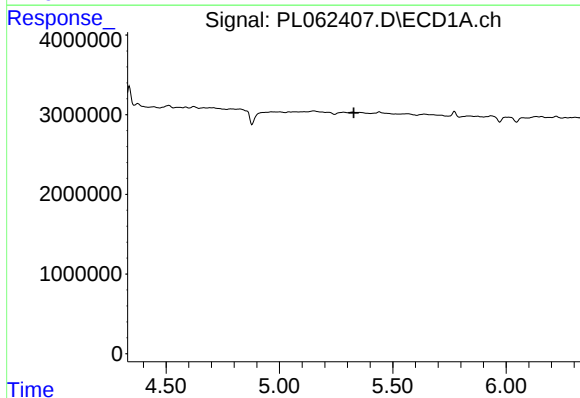


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

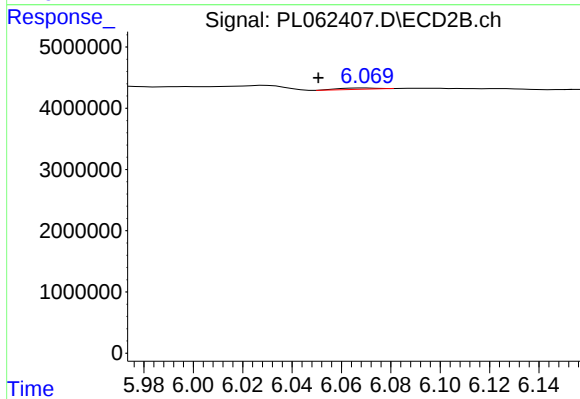

#10 gamma-Chlordane


R.T.: 6.071 min
Delta R.T.: 0.020 min
Response: 226871
Conc: 0.07 ng/ml

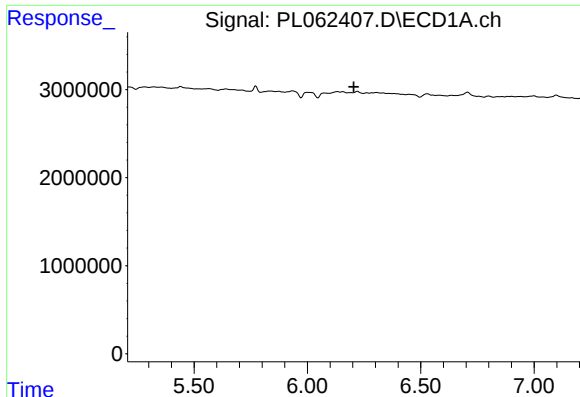

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PL-01-101420

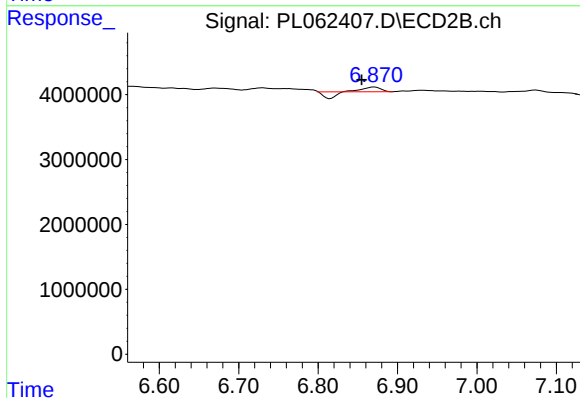


#15 Endosulfan II

R.T.: 6.871 min
Delta R.T.: 0.016 min
Response: 334053
Conc: 0.12 ng/ml

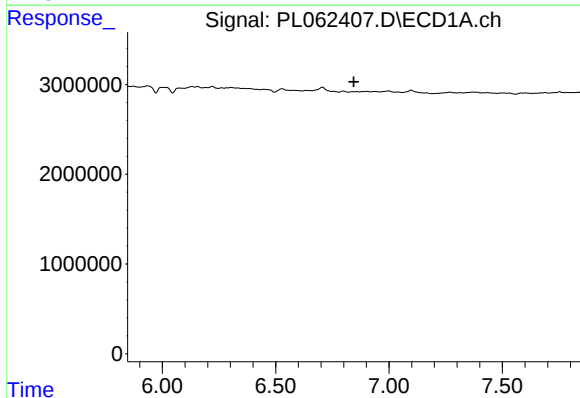


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.844 min
Response: 0
Conc: N.D.

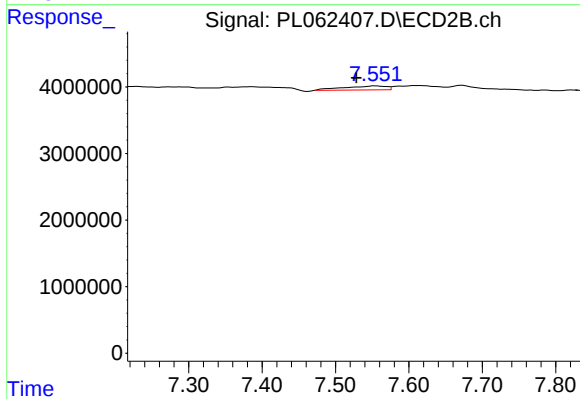

#20 Methoxychlor


R.T.: 7.554 min
Delta R.T.: 0.025 min
Response: 2400986
Conc: 1.82 ng/ml

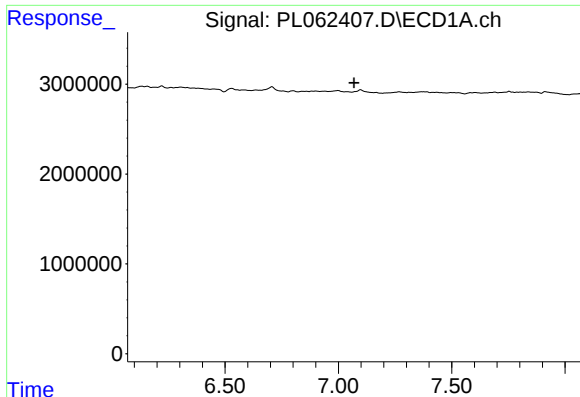

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PL-01-101420

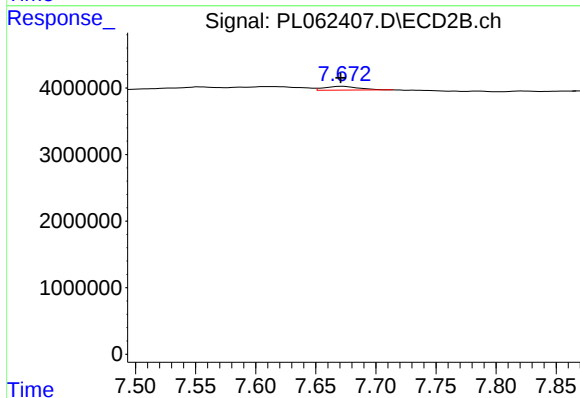


#21 Endrin ketone

R.T.: 7.672 min
Delta R.T.: 0.001 min
Response: 1141060
Conc: 0.41 ng/ml

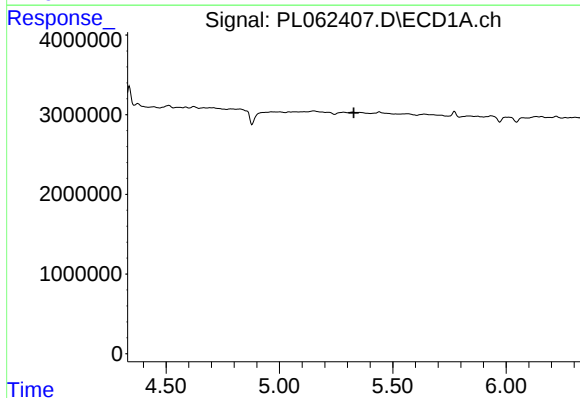


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

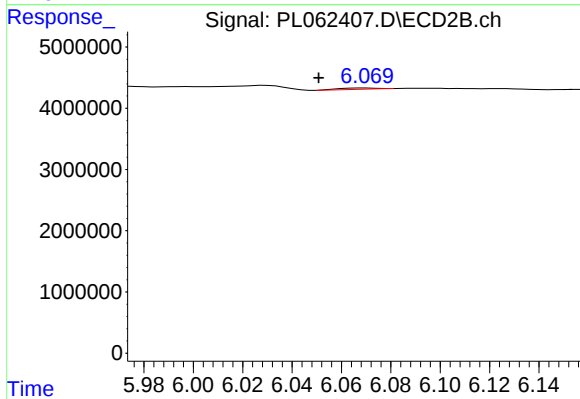

#25 Chlordane-3


R.T.: 6.071 min
Delta R.T.: 0.020 min
Response: 226871
Conc: 0.55 ng/ml

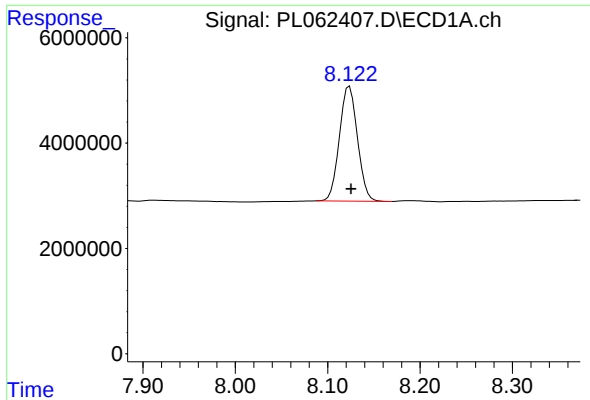

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.002 min
Response: 29583315
Conc: 16.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-01-101420

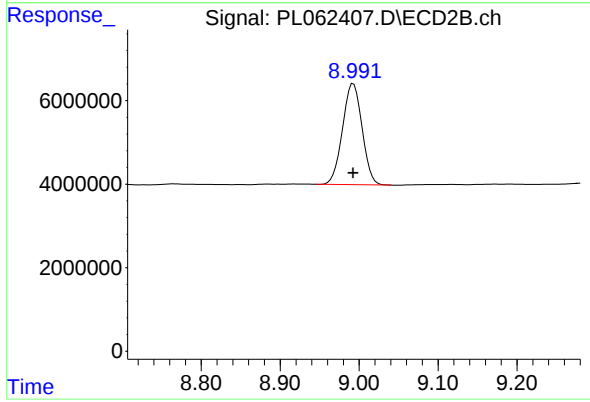

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 41678464
Conc: 15.18 ng/ml